

Date: 2026-03-16

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_260316 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.75$ S/m; $\epsilon_r = 38.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.7, 7.41, 7.62); Calibrated: 2026-02-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.39 W/kg; SAR (10g) = 1.12 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 2.48 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.3 %

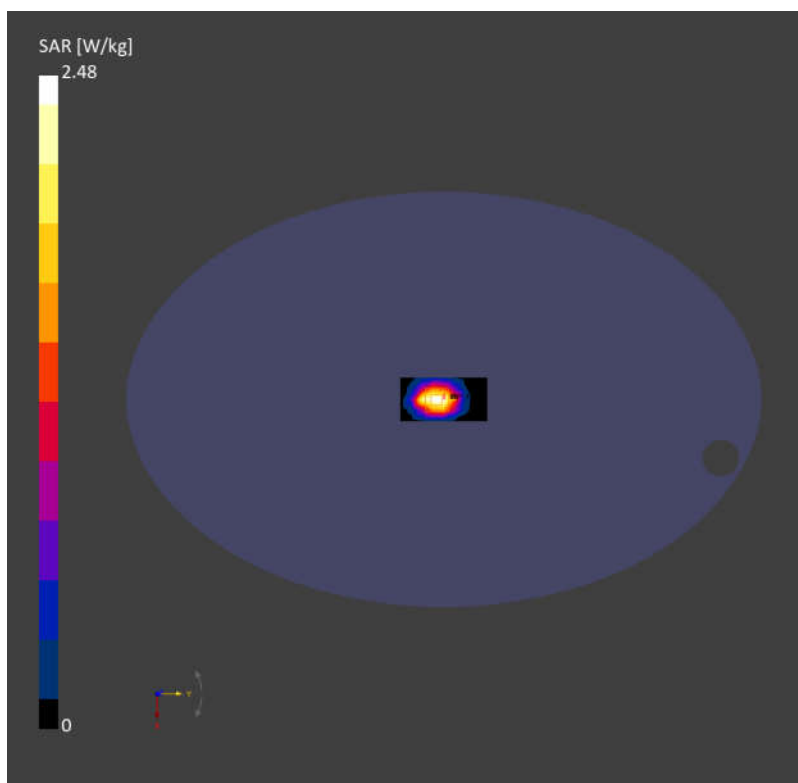

Date: 2026-03-17

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250_260317 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.61$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.83, 5.62, 5.77); Calibrated: 2026-02-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 0.976 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.76 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 6.6 mm

Ratio of SAR at M2 to SAR at M1 = 62.1 %

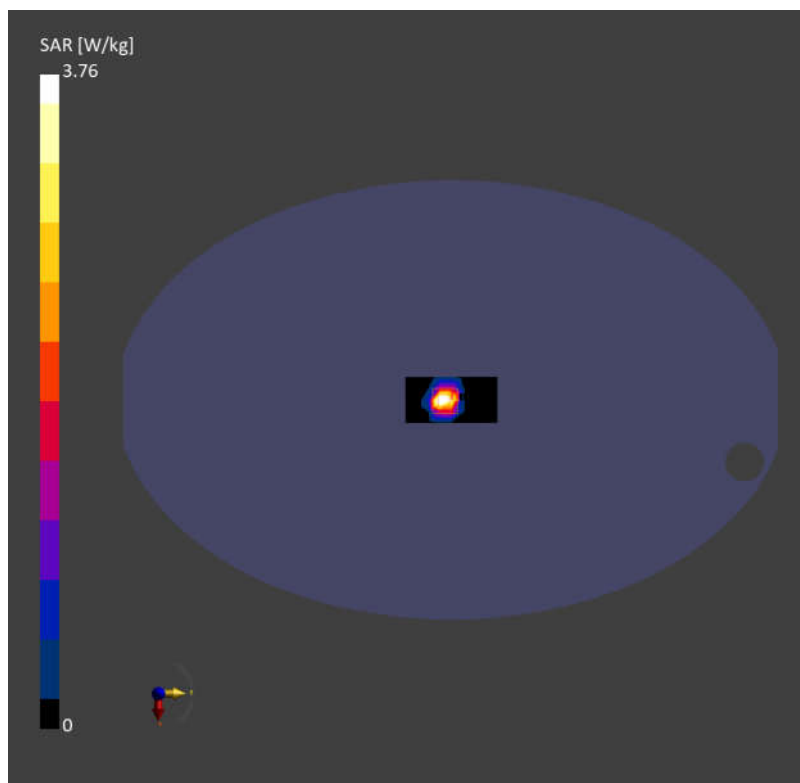

Date: 2026-03-18

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_260318 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.99$ S/m; $\epsilon_r = 35.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.33, 5.13, 5.27); Calibrated: 2026-02-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.50 W/kg; SAR (10g) = 1.06 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = 0.04 dB

SAR (1g) = 4.11 W/kg; SAR (10g) = 1.21 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.8 %

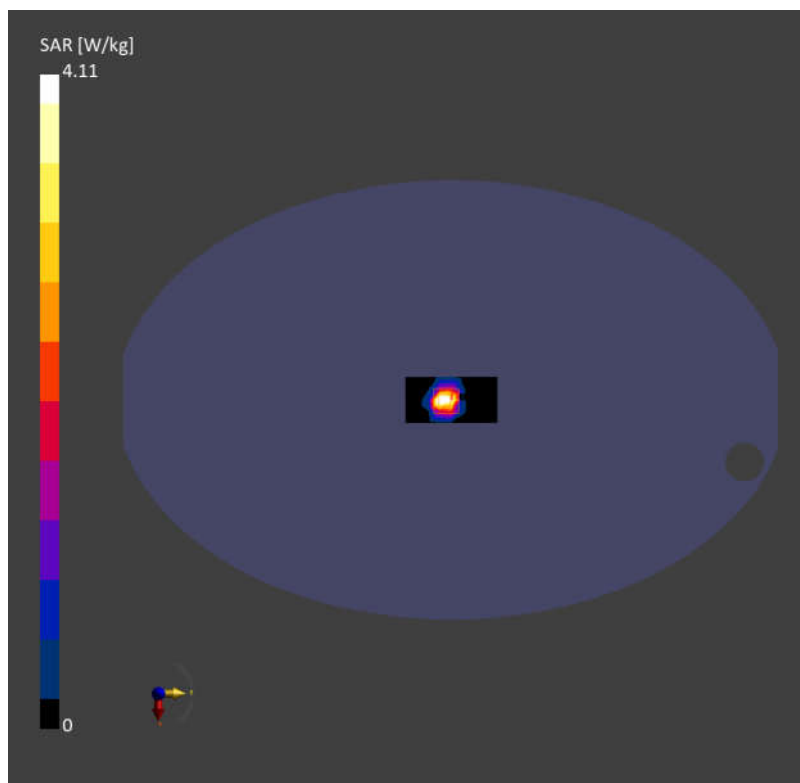

Date: 2026-03-19

System Check_Head_5800MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1

Medium: HSL_5800_260319 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.25$ S/m; $\epsilon_r = 34.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.45, 5.25, 5.39); Calibrated: 2026-02-25
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2025-07-15
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.36 W/kg; SAR (10g) = 1.01 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.91 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 7.3 mm

Ratio of SAR at M2 to SAR at M1 = 56.8 %

