



SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:08, WED

POWER: LOW
MODULATION: NONE

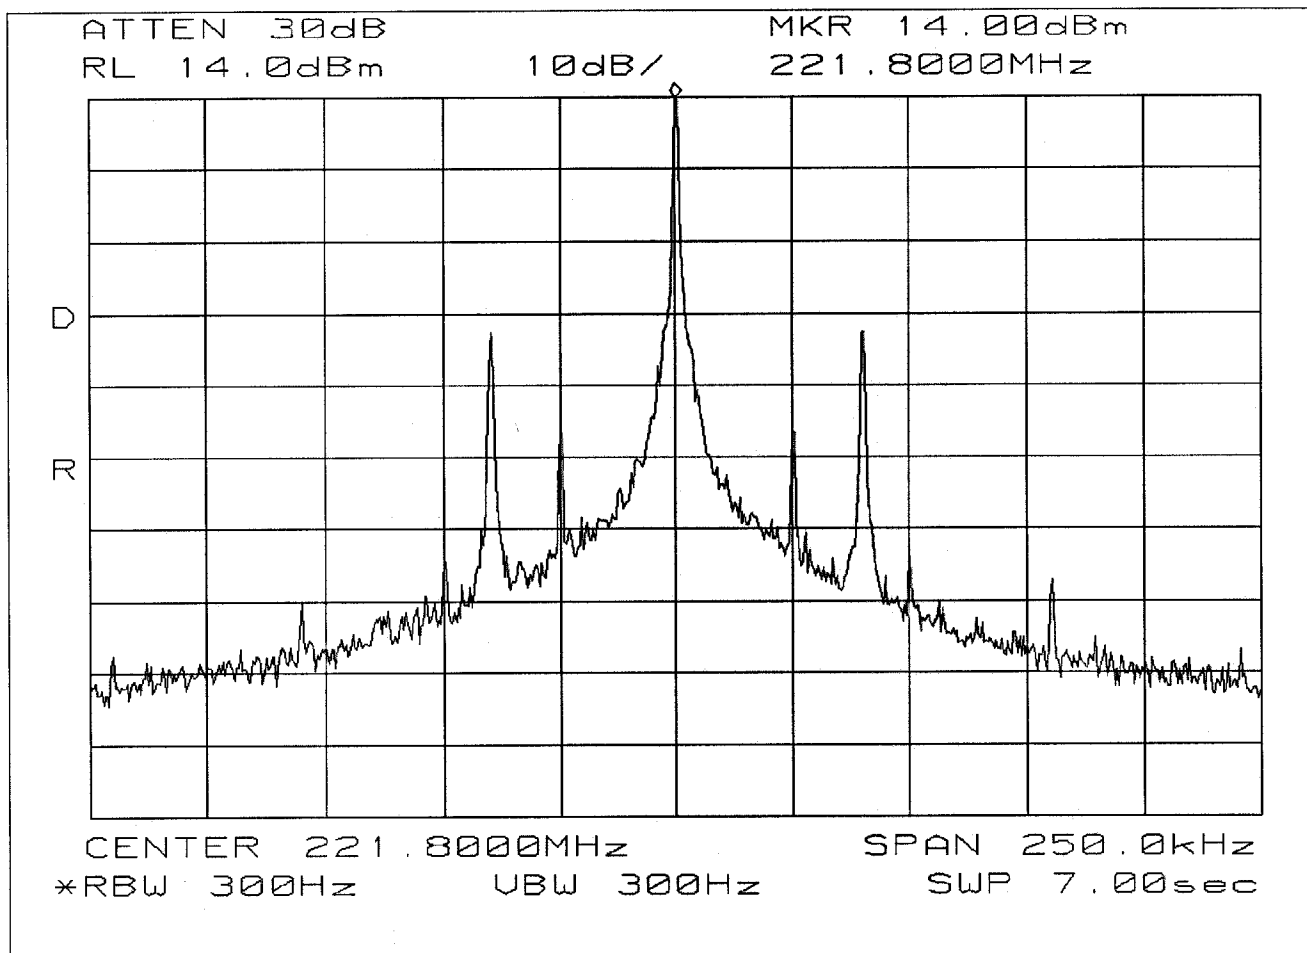


SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:10, WED

POWER: LOW
MODULATION: 5 KHZ 20 DB ABOVE REFERENCE LEVEL

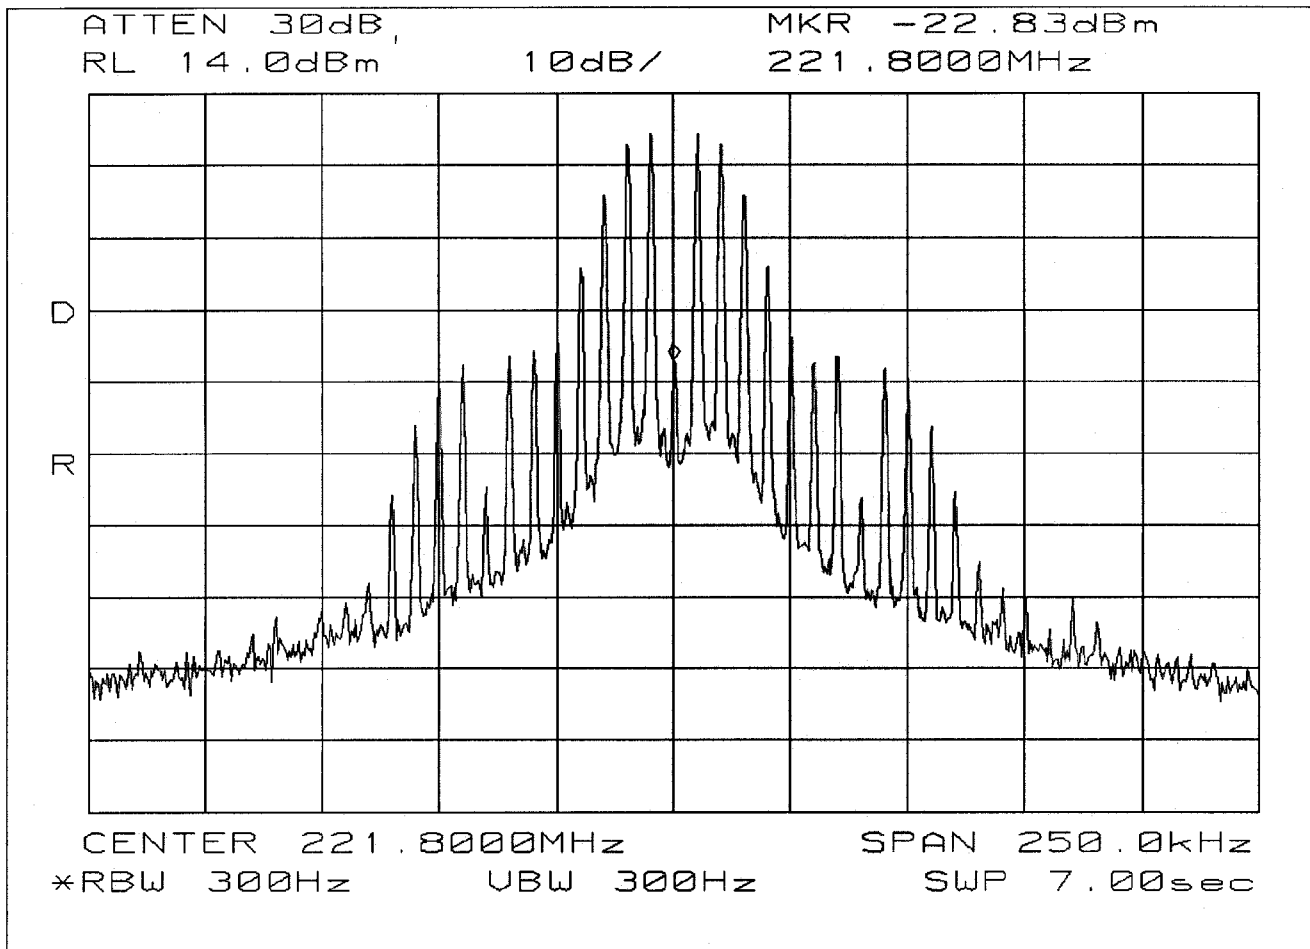


SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:15, WED

POWER: LOW
MODULATION: 15 KHZ 20 DB ABOVE REFERENCE LEVEL

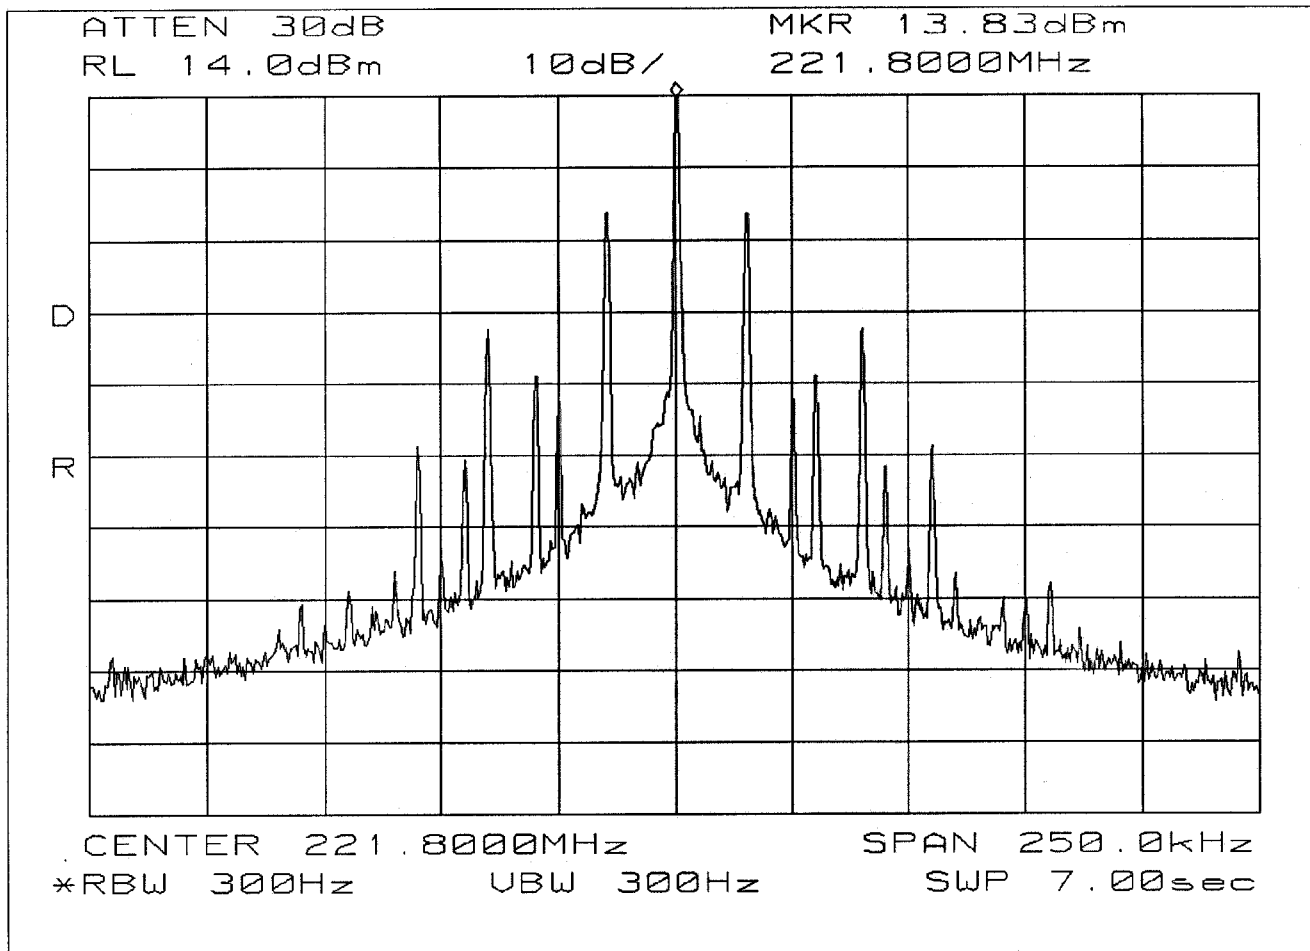


SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:04, WED

POWER: HIGH
MODULATION: NONE

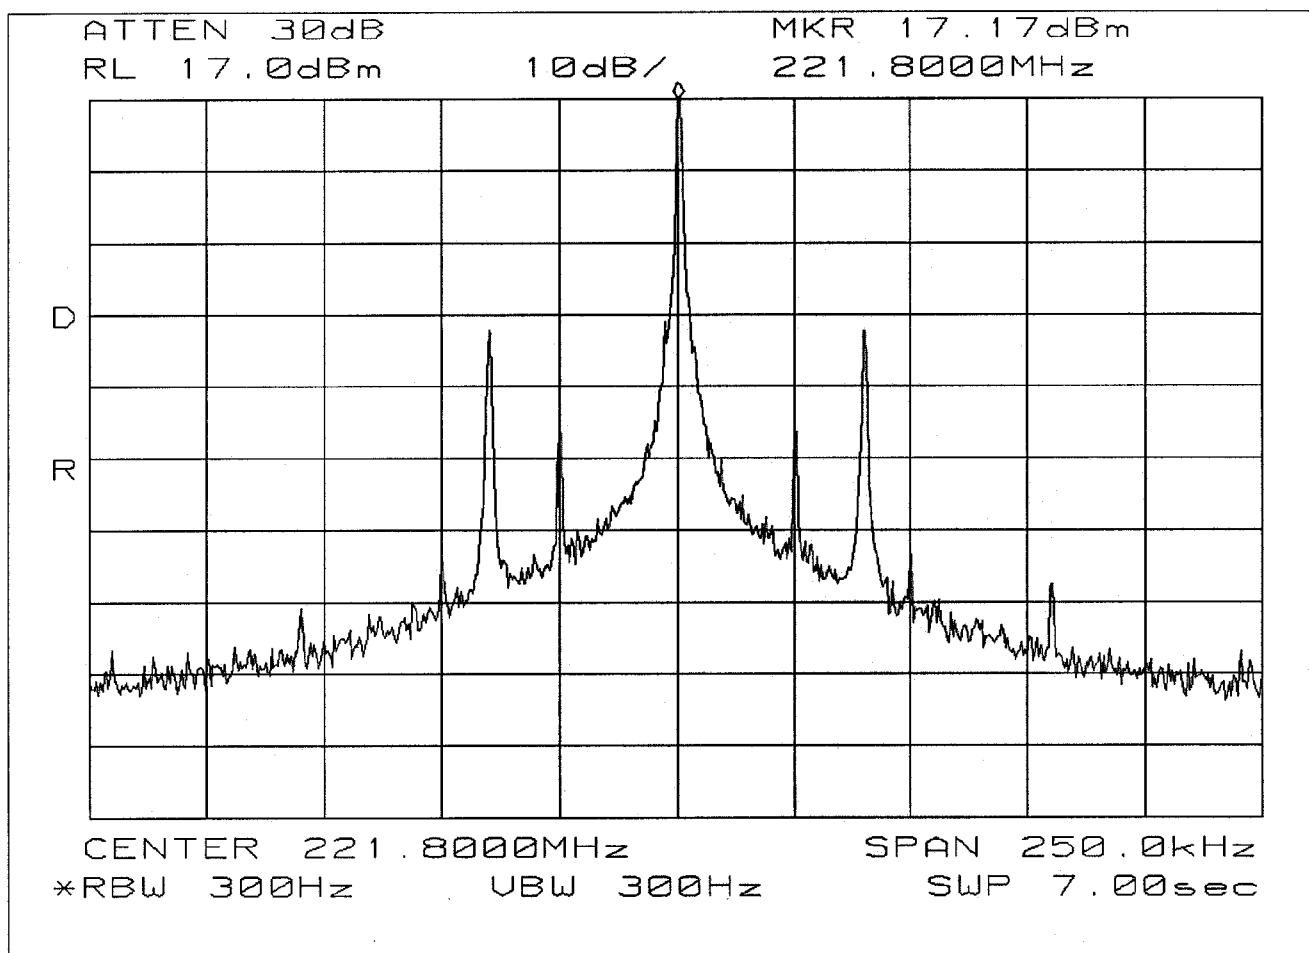

SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:12, WED

POWER: HIGH
MODULATION: 5 KHZ 20 DB ABOVE REFERENCE LEVEL

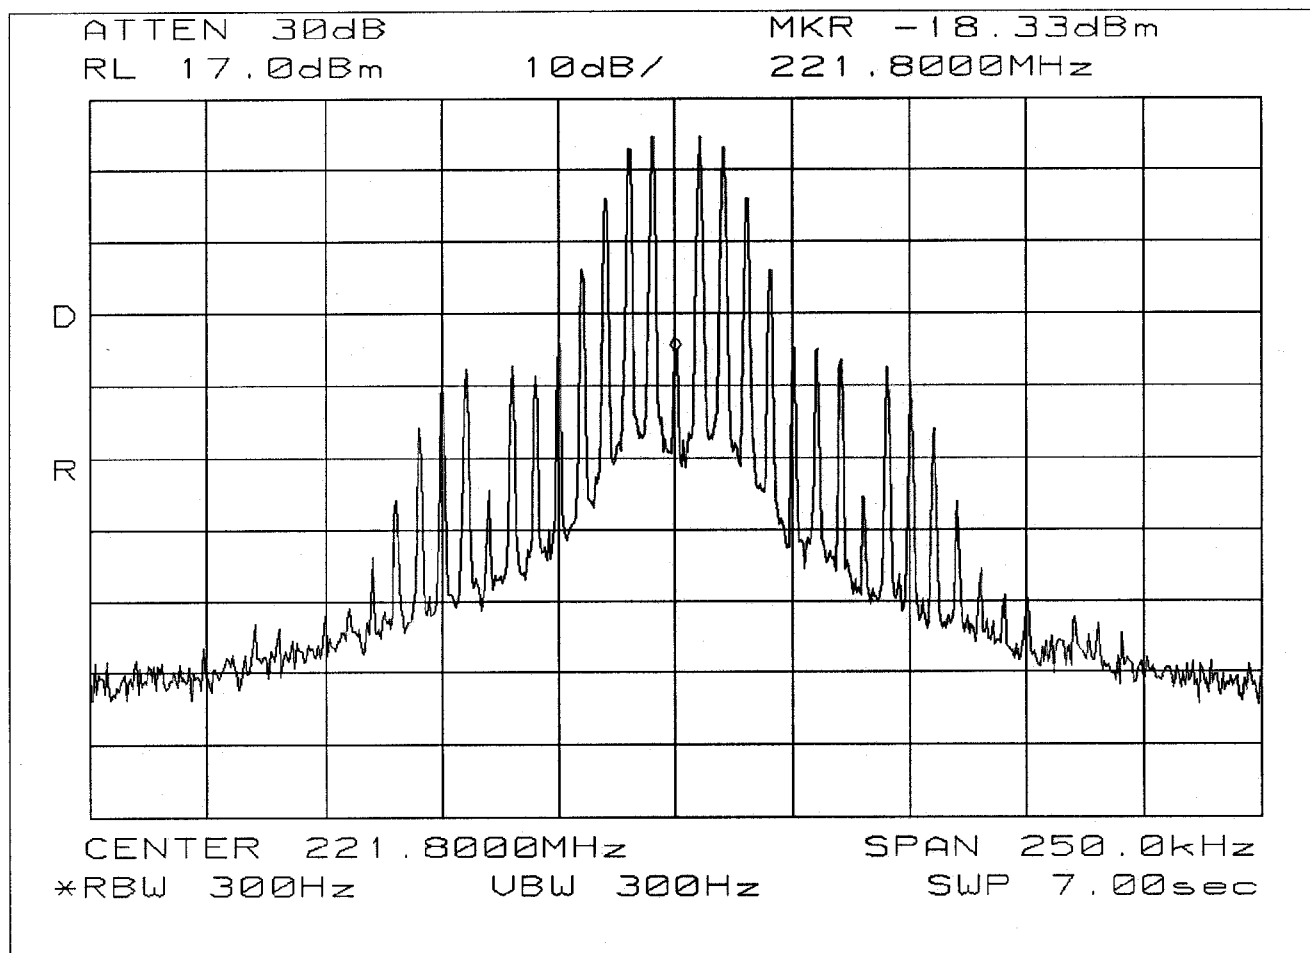

SPECTRUM ANALYZER PRESENTATION
BIO-MEDICAL, Base Station 2010
1999-OCT-20, 12:13, WED

POWER: HIGH
MODULATION: 15 KHZ 20 DB ABOVE REFERENCE LEVEL

