


MODULATION LIMITING

p9920013: BIO-MEDICAL, Base Station 2010

g99a0329: 1999-OCT-28, 11:00

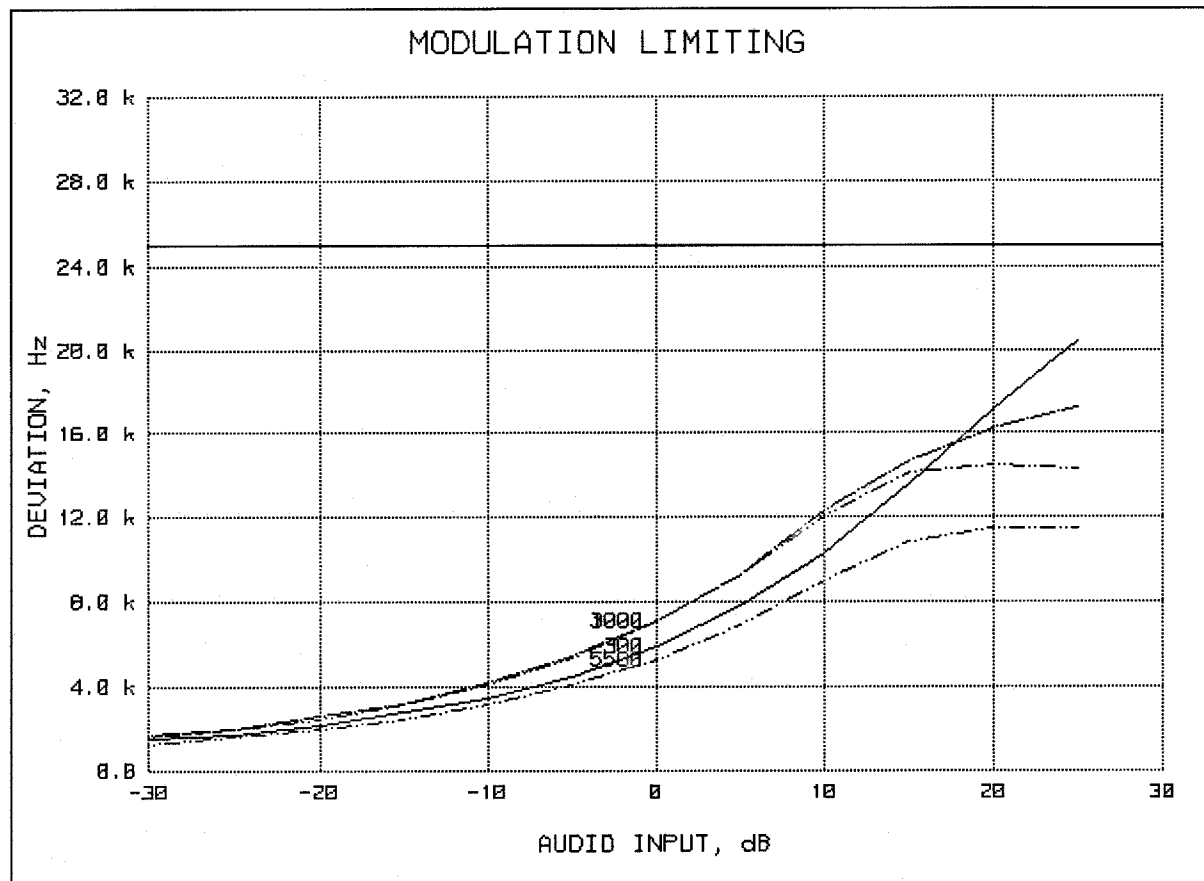

REFERENCE DEVIATION, kHz = 7

REFERENCE MODULATION, Hz = 1000


PEAKS = POSITIVE

AUDIO AMPLITUDE, mV = 233.92

MODULATION LIMITING

p9920013: BIO-MEDICAL, Base Station 2010

g99a0329: 1999-OCT-28, 11:00

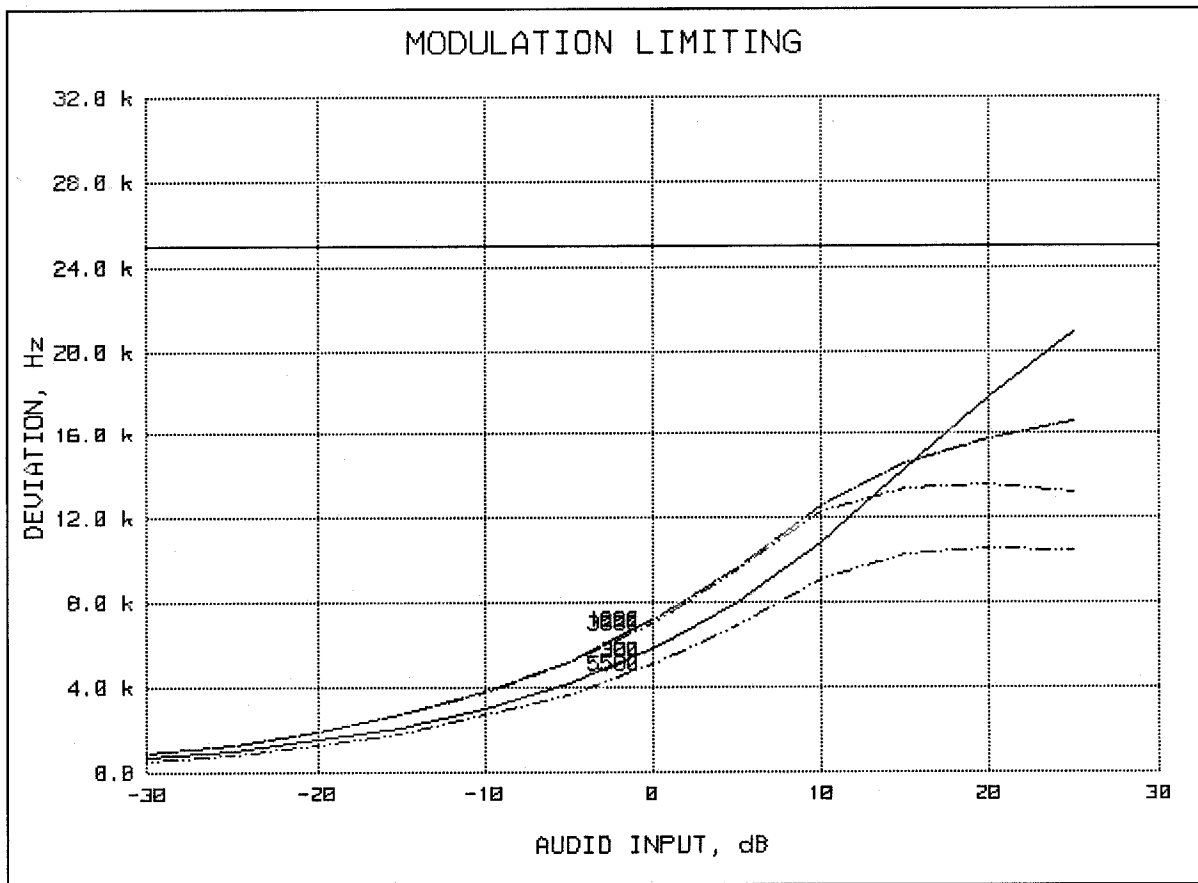

REFERENCE DEVIATION, kHz	= 7
REFERENCE MODULATION, Hz	= 1000
PEAKS	= NEGATIVE
AUDIO AMPLITUDE, mV	= 304.84