


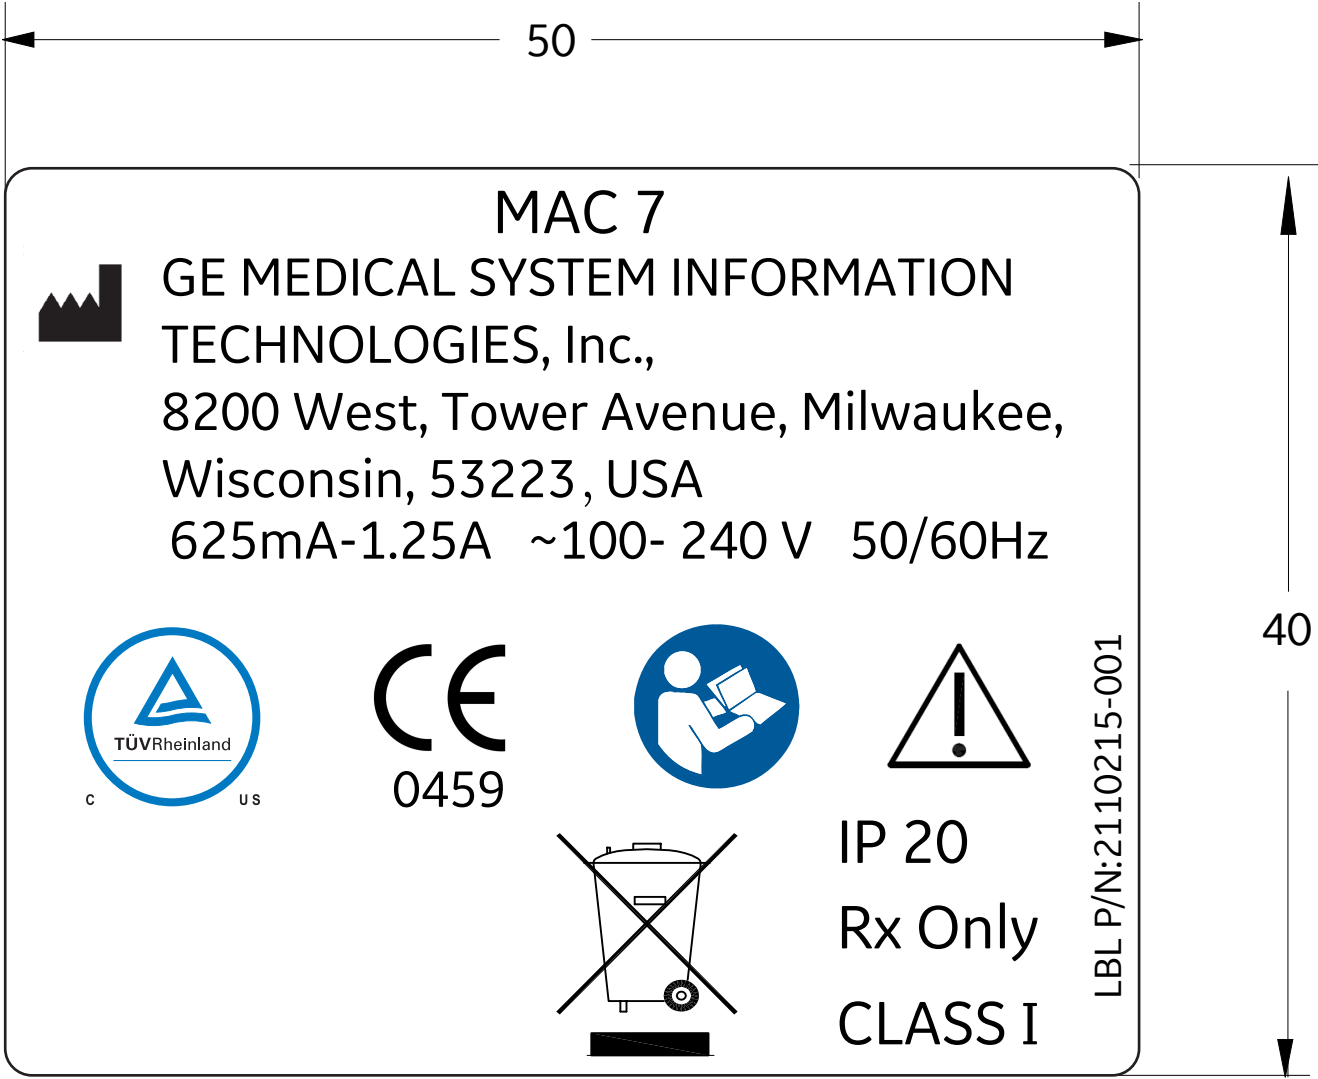

Notes :

- 1) MATERIAL: SUBSURFACE PRINTED 0.01" (10 mil) thick, VELVET / POLISHED POLYCARBONATE
- 2) ADHESIVE: 3M #9471LE OR 3M #9671LE (2mil) thick OR EQUIVALENT.
- 3) COLORS:
- a) BACKGROUND TO BE MATCHED TO : (MUNSELL No : GEHC N9)
- b) TEXT AND GRAPHICS TO BE : BLACK (EXCEPT FOR TUV AND IFU SYMBOL)
- c) TUV AND IFU SYMBOL: PANTONE 307c (BLUE) AS PER ARTWORK,
- 4) LABELS ARE TO BE DIE-CUT TO LINER WITH BREAKAWAY TAB MARKED BY VENDOR WITH GEM-IT PART NUMBER, REVISION LETTER, ARTWORK ISSUE NUMBER AND VENDOR NAME
- 5) LABELS MUST BE UL RECOGNIZED AND EACH PACKAGE MUST BE MARKED AS SPECIFIED IN THE CURRENT UL RECOGNISED COMPONENT DIRECTORY

CHECK FOR DURABILITY AS PER UL 60601-1

- 1) RUB THE LABEL BY HAND WITHOUT UNDUE PRESSURE.
- 2) WITH CLOTH RAG SOAKED IN DISTILLED WATER FOR 15 SEC.
- 3) WITH CLOTH RAG SOAKED IN METHYLATED SPIRIT FOR 15 SEC.
- 4) WITH CLOTH RAG SOCKED WITH ISOPROPYL ALCOHOL SOLUTION FOR 15 SEC.

MARKING SHOULD BE LEGIBLE AFTER TESTING AS PER ABOVE PROCEDURE.

CTQ TABLE		
QTY	FLAG	DESCRIPTION
0	#	CTQ FLAG: MEF140 QUALITY PLAN REQUIRED.

				DO NOT SCALE DRAWING		DRAWN BY		DATE		 GE Healthcare	
REV		CHANGE NO.		DATE		LIFECYCLE		CONFIDENTIAL: THIS PRINT AND THE DESIGN THEREIN REPRESENTED ARE THE PROPERTY OF GE HEALTHCARE AND MAY NOT BE USED IN ANY MANNER DETRIMENTAL TO IT'S INTEREST. THIS PRINT HAS BEEN ISSUED WITH THE UNDERSTANDING THAT IT WILL NOT BE USED FOR MANUFACTURE FOR OTHERS, AND WILL BE RETURNED UPON REQUEST.		ENG. APPROVED	
UNLESS OTHERWISE SPECIFIED: 1) REMOVE ALL BURRS AND SHARP EDGES. 2) DIMENSIONS ARE IN MILLIMETERS. X ±0.1 X.X ±0.1 X.XX ±0.01 X° ±0.5° 3) M PROFILE METRIC THREAD TOLERANCE CLASS 6H/6g PER ISO 965/1.		ESENSSTIAL CHARACTERISTIC: NO		ITEMS INDICATED MAY REQUIRE A SUPPLIER QUALITY PLAN.		MATERIAL REFER NOTE		FINISH ---		TITLE	
										DWG PRODUCT LABEL ENG	
										DRAWING NUMBER D2110215-001	
										REV A	
										SCALE NTS	
										SHEET OF	
										BALLOON KEY:  XX= FIND NUMBER, YY= QUANTITY	