

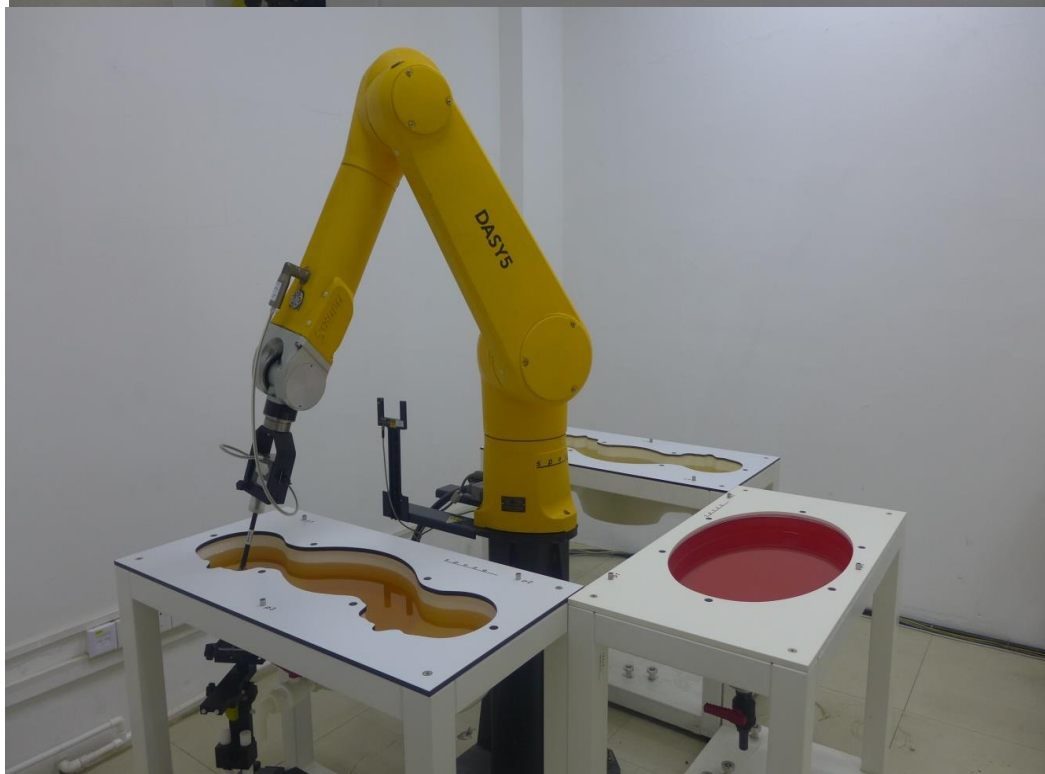


# **Appendix D**

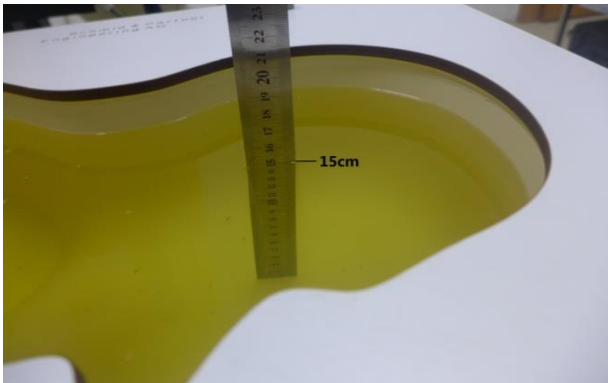
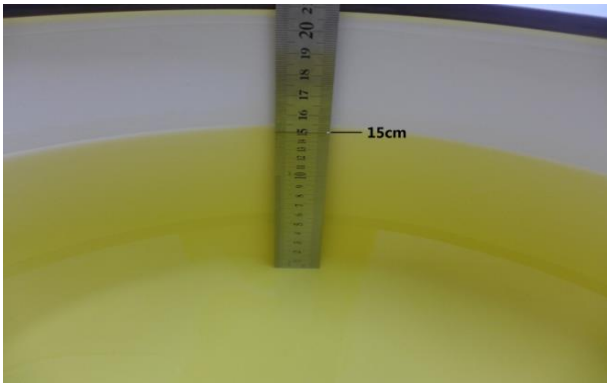
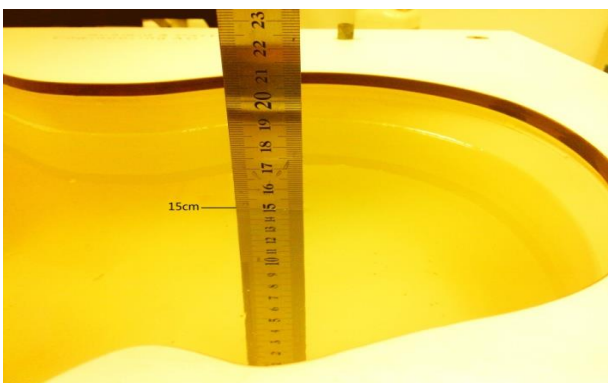
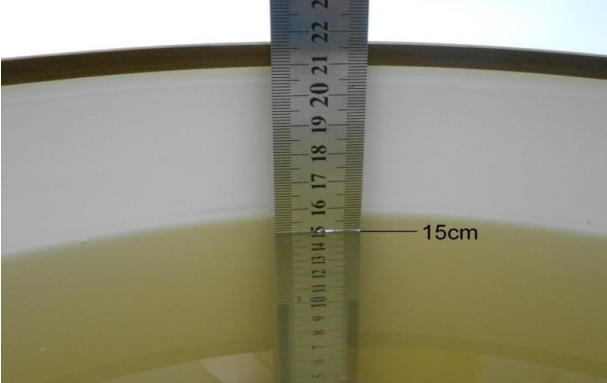
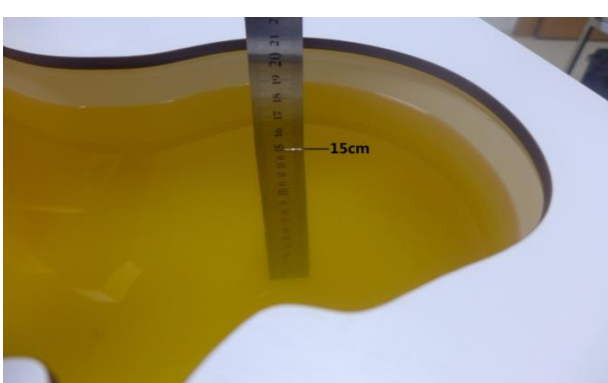
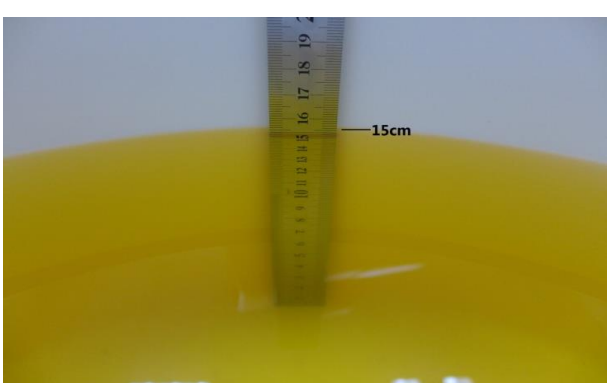
## **Photographs**

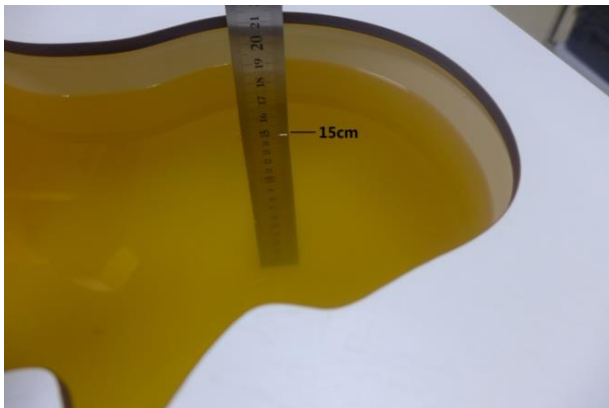
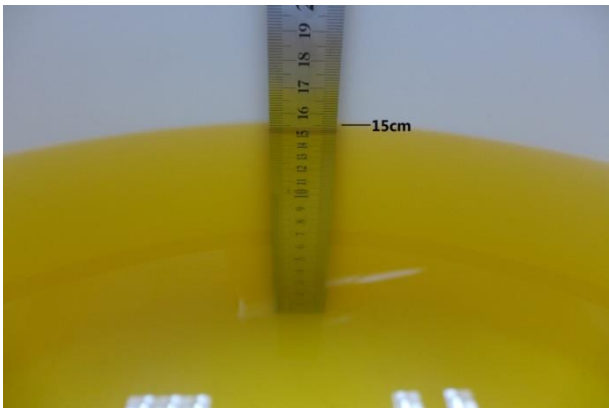
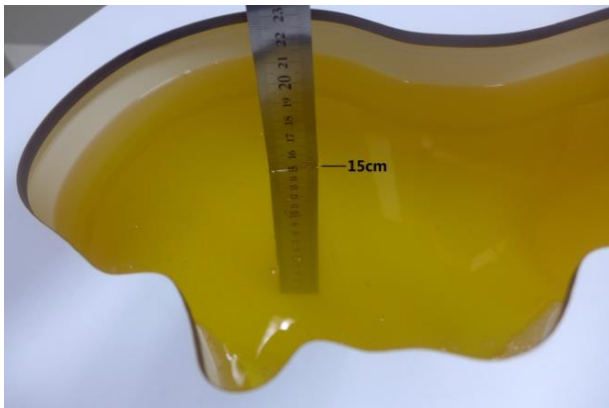
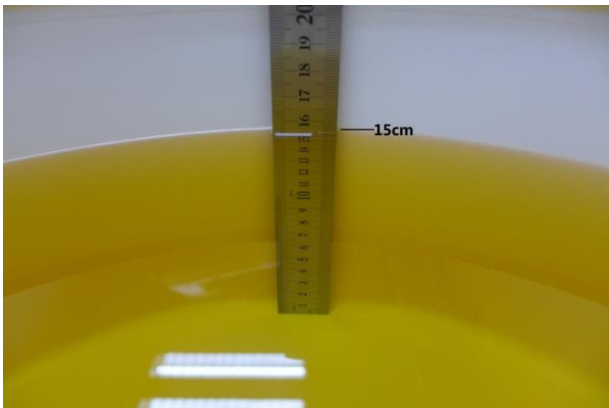
|                                          |
|------------------------------------------|
| 1. SAR measurement System                |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position      |
| 4. EUT Constructional Details            |
| 5. Serial Number of EUT                  |

## 1. SAR measurement System

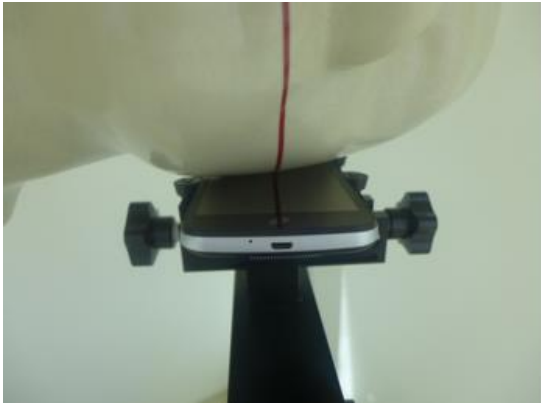
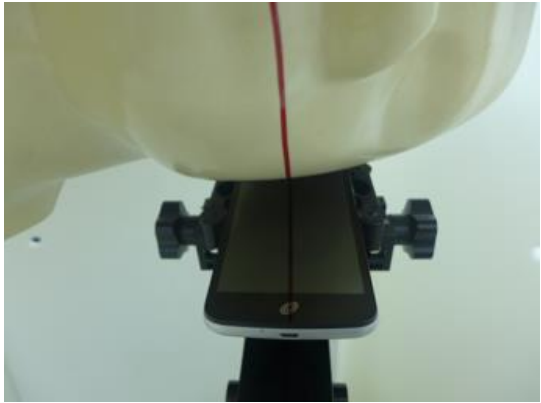
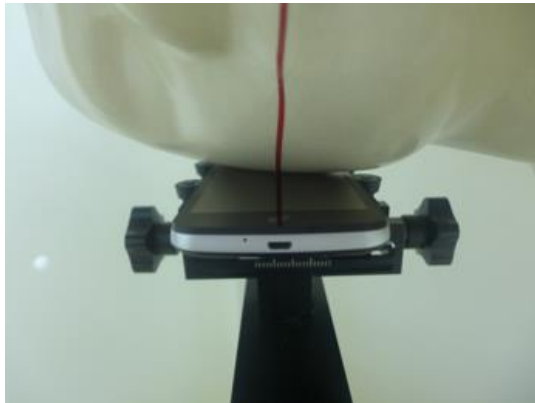
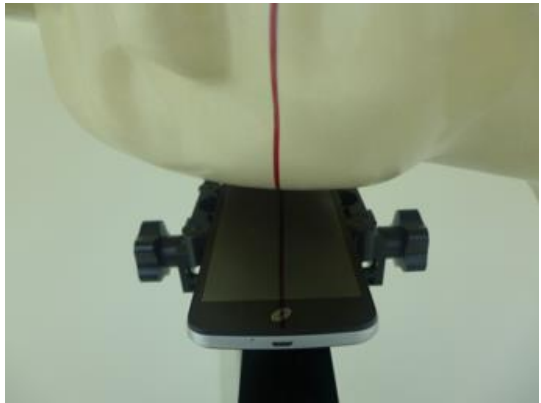


## 2. Photographs of Tissue Simulate Liquid

|                                                                                     |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| <p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>                          | <p><b>Photo 2: Tissue Simulant Liquid for Body 750</b></p>                           |
|    |    |
| <p><b>Photo 3: Tissue Simulant Liquid for Head 835</b></p>                          | <p><b>Photo 4: Tissue Simulant Liquid for Body 835</b></p>                           |
|  |  |
| <p><b>Photo 5: Tissue Simulant Liquid for Head 1750</b></p>                         | <p><b>Photo 6: Tissue Simulant Liquid for Body 1750</b></p>                          |
|  |  |

|                                                                                     |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| <p><b>Photo 7: Tissue Simulant Liquid for Head 1900</b></p>                         | <p><b>Photo 8: Tissue Simulant Liquid for Body 1900</b></p>                          |
|    |    |
| <p><b>Photo 9: Tissue Simulant Liquid for Head 2450</b></p>                         | <p><b>Photo 10: Tissue Simulant Liquid for Body 2450</b></p>                         |
|  |  |

### 3. Photographs of EUT test position

|                                                                                     |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| <p><b>Photo 11: Left cheek</b></p>                                                  | <p><b>Photo 12: Left tilted</b></p>                                                  |
|    |    |
| <p><b>Photo 13: Right cheek</b></p>                                                 | <p><b>Photo 14: Right tilted</b></p>                                                 |
|  |  |
| <p><b>Photo 15: Front side 15mm</b></p>                                             | <p><b>Photo 16: Back side 15mm</b></p>                                               |
|  |  |

|                                                                                     |                                                                                      |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| <p><b>Photo 17: Front side 10mm</b></p>                                             | <p><b>Photo 18: Back side 10mm</b></p>                                               |
|    |    |
| <p><b>Photo 19: Left side 10mm</b></p>                                              | <p><b>Photo 20: Right side 10mm</b></p>                                              |
|  |  |
| <p><b>Photo 21: Top side 10mm</b></p>                                               | <p><b>Photo 22: Bottom side 10mm</b></p>                                             |
|  |  |



#### 4. EUT Constructional Details

| Photo 23: Front View                                                              | Photo 24: Back View                                                                |
|-----------------------------------------------------------------------------------|------------------------------------------------------------------------------------|
|  |  |