NOTE: This record is a scanned copy that captures the original document content and will apply as Medtronic MITG electronic records which are stored in the electronic recordkeeping system. At the time of scanning a verification was completed to the original source hard copy document, to ensure the scanned images are complete and legible.

# Test Report for SAR Evaluation of the McGRATH MAC+ Connected Relay in Accordance with FCC 47 CFR 2.1093 for the US

# 1.0 Device Configuration

## 1.1 Hardware

| McGRATH MAC+ Connected Relay (302-100-000), Test Device ID: M5 | | | |
|---|---|---|---|
| ***Component Name*** | ***Part Number*** | ***Revision*** | ***Comments*** |
| Cosmo, Module, Assembly, PCB, Mainboard | PT00145610 | X12 | ***Customization:***<br>UART-to-USB adapter soldered to UART traces<br><br>***Rationale:***<br>The UART-to-USB adapter allows for wired connection of the test device to a PC for configuration of device software for each test. |
| Cosmo, Battery | PT00145612 | X07 | N/A |

Note: the versions of released device hardware at the time of this reporting were PT00145610 revision B and PT00145612 revision A. The differences between the hardware versions tested and the currently released versions was evaluated by the external test house and the hardware versions were determined to be equivalent. See Section 1 Introduction of the report for more information. The referenced document “Rev B Changes Summary”, which was used to determine equivalency, is included as Attachment A in Agile. The “M5-B” device referenced in the report is a test device provided with the latest versions of hardware (PT00145610 revision B and PT00145612 revision A) which was not used for testing.

## 1.2 Software

Refer to the following for information on device software used for testing:

- Relay Software: RE00569944 revision D (SOFTWARE REFERENCE DRAWING, RF Testing Custom Software Description for McGRATH MAC+ Connected Relay)

## 1.3 Build Components

All components used to build test devices were provided by Mervue from the P3.0 build component stock per Section 3 of RE00520861 revision A.

# 2.0 Document References

## 2.1 Test Plan

RE00568368 revision B (Medtronic | Cosmo | TUV San Diego RF Test Plan) was used to provide guidance for SAR testing. The test plan includes information about relevant test tools.

802 N. Twin Oaks Valley Road, Suite 105 • San Marcos, CA 92069 • U.S.A.
TEL (760) 471-2100 • FAX (760) 471-2121
http://www.rfexposurelab.com

# CERTIFICATE OF COMPLIANCE
# SAR EVALUATION

| | |
|---|---|
| Covidien LLC | Dates of Test: September 29-Ocotober 1, 2025 |
| 15 Hampshire Street | Test Report Number: SAR.20251001 |
| Mansfield, MA 02048 | Revision A |
| | Lab Designation Number: US1195 |

| | |
|---|---|
| FCC ID: | P7G-MR3021 |
| Model(s): | 302-100-000 |
| Marketing Name: | McGRATH™ MAC+ Connected Relay |
| Test Sample: | Engineering Unit Same as Production |
| Serial Number: | M5 |
| Equipment Type: | Wireless Relay Device |
| Classification: | Portable Transmitter Next to Body |
| TX Frequency Range: | 2412 – 2462 MHz |
| Frequency Tolerance: | ± 2.5 ppm |
| Maximum RF Output: | 2450 MHz (b) – 11.0 dBm, 2450 MHz (g) – 10.6 dBm, 2450 MHz (n20) – 10.3 dBm Conducted |
| Signal Modulation: | DSSS, OFDM |
| Antenna Type: | Internal Antenna |
| Application Type: | Certification |
| FCC Rule Parts: | Part 2, 15C |
| KDB Test Methodology: | KDB 447498 D01 v06, KDB 248227 v02r02 |
| Maximum SAR Value: | 1.32 W/kg Reported |
| Separation Distance to Probe: | 0 mm |

This wireless mobile and/or portable device has been shown to be compliant for localized specific absorption rate (SAR) for controlled environment/occupational limits specified in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields, IEEE Std.1528 – 2013 Recommended Practice and had been tested in accordance with the measurement procedures specified in KDB 447498 and KDB 248227 (See test report).

This device is a portable device as defined in FCC 47 CFR 2.1093.

I attest to the accuracy of the data. All measurements were performed by myself or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

RF Exposure Lab, LLC certifies that no party to this application is subject to a denial of Federal benefits that includes FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).

Jay M. Moulton
Vice President

ACCREDITED
Testing Cert. # 2387.01

© 2025 RF Exposure Lab, LLC
*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# Table of Contents

1. Introduction ..... 4
SAR Definition [5] ..... 5
2. SAR Measurement Setup ..... 6
Robotic System ..... 6
System Hardware ..... 6
System Electronics ..... 7
Probe Measurement System ..... 7
3. Probe and Dipole Calibration ..... 14
4. Phantom & Simulating Tissue Specifications ..... 15
Head Simulating Mixture Characterization ..... 15
5. RF Exposure Limits [2] ..... 16
Uncontrolled Environment ..... 16
Controlled Environment ..... 16
6. Measurement Uncertainty ..... 17
7. SAR System Verification ..... 18
Tissue Verification ..... 18
SAR System Verification ..... 18
8. SAR Test Data Summary ..... 19
Procedures Used To Establish Test Signal ..... 19
Device Test Condition ..... 19
9. SAR Test Results ..... 22
10. Test Equipment List ..... 24
11. Conclusion ..... 25
12. References ..... 26
Appendix A – System Validation Plots and Data ..... 27
Appendix B – SAR Test Data Plots ..... 30
Appendix C – SAR Test Setup Photos ..... 32
Appendix D – Probe Calibration Data Sheets ..... 40
Appendix E – Dipole Calibration Data Sheets ..... 51
Appendix F – DAE Calibration Data Sheets ..... 58
Appendix G – Phantom Calibration Data Sheets ..... 64
Appendix H – Validation Summary ..... 66

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

| Comment/Revision | Date |
|---|---|
| Original Release | October 2, 2025 |
| Revision A – Add Version M5-B | October 3, 2025 |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |
| | |

**Note: The latest version supersedes all previous versions listed in the above table. The latest version shall be used.**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 1. Introduction

This measurement report shows compliance of the Covidien LLC Model 302-100-000 FCC ID: P7G-MR3021 with FCC Part 2, 1093, ET Docket 93-62 Rules for mobile and portable devices. The FCC has adopted the guidelines for evaluating the environmental effects of radio frequency radiation to protect the public and workers from the potential hazards of RF emissions due to FCC regulated portable devices. [1]

The test results recorded herein are based on a single type test of Covidien LLC Model 302-100-000 and therefore apply only to the tested sample.

The test procedures, as described in ANSI C95.1 – 1999 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, ANSI C95.3 – 2002 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields, IEEE Std.1528 – 2013 Recommended Practice, KDB 447498 and KDB 248227 were employed.

The following table indicates all the wireless technologies operating in the 302-100-000 Wireless Relay Device. The table also shows the tolerance for the power level for each mode.

| Band | Technology | Tolerance dBm | Lower Tolerance dBm | Upper Tolerance dBm |
|---|---|---|---|---|
| WLAN – 2.4 GHz | 802.11b | N/A | N/A | 11.0 |
| WLAN – 2.4 GHz | 802.11g | N/A | N/A | 10.6 |
| WLAN – 2.4 GHz | 802.11n20 | N/A | N/A | 10.3 |

**Note: The M5-B version is equivalent to the M5 version for SAR testing. This is based on the document Rev B changes Summary provide by the client.**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## SAR Definition [5]

Specific Absorption Rate is defined as the time derivative (rate) of the incremental energy (*dW*) absorbed by (dissipated in) an incremental mass (*dm*) contained in a volume element (*dV*) of a given density ($\rho$).

$$SAR = \frac{d}{dt}\left(\frac{dW}{dm}\right) = \frac{d}{dt}\left(\frac{dW}{\rho dV}\right)$$

SAR is expressed in units of watts per kilogram (W/kg). *SAR* can be related to the electric field at a point by

$$SAR = \frac{\sigma \mid E \mid^2}{\rho}$$

where:

$\sigma$ = conductivity of the tissue (S/m)
$\rho$ = mass density of the tissue (kg/m$^3$)
*E* = rms electric field strength (V/m)

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 2. SAR Measurement Setup

## Robotic System

These measurements are performed using the DASY52 automated dosimetric assessment system. The DASY52 is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland and consists of high precision robotics system (Staubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2.1).

## System Hardware

A cell controller system contains the power supply, robot controller teach pendant (Joystick), and a remote control used to drive the robot motors. The PC consists of the HP Intel Core2 computer with Windows XP system and SAR Measurement Software DASY52, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

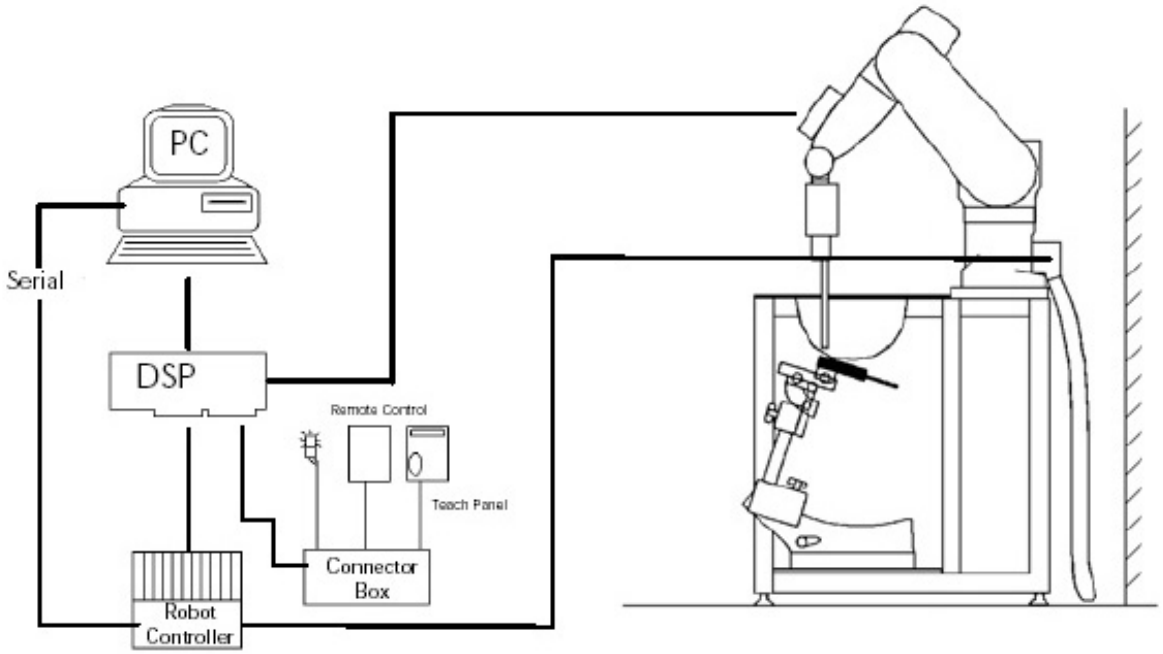


**Figure 2.1 SAR Measurement System Setup**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## System Electronics

The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail below.

## Probe Measurement System

The SAR measurements were conducted with the dosimetric probe EX3DV4, designed in the classical triangular configuration (see Fig. 2.2) and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi fiber line ending at the front of the probe tip. (see Fig. 2.3) It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY52 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.

**DAE System**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## Probe Specifications

**Calibration:** In air from 10 MHz to 6.0 GHz
In brain and muscle simulating tissue at Frequencies of 450 MHz, 835 MHz, 1750 MHz, 1900 MHz, 2450 MHz, 2600 MHz, 3500 MHz, 5200 MHz, 5300 MHz, 5600 MHz, 5800 MHz

**Frequency**: 10 MHz to 6 GHz

**Linearity:** ±0.2dB (30 MHz to 6 GHz)

**Dynamic:** 10 mW/kg to 100 W/kg

**Range:** Linearity: ±0.2dB

**Dimensions:** Overall length: 330 mm

**Tip length:** 20 mm

**Body diameter:** 12 mm

**Tip diameter:** 2.5 mm

**Distance from probe tip to sensor center:** 1 mm

**Application:** SAR Dosimetry Testing
Compliance tests of wireless device




**Figure 2.2 Triangular Probe Configurations**

**Figure 2.3 Probe Thick-Film Technique**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## Probe Calibration Process

### Dosimetric Assessment Procedure

Each probe is calibrated according to a dosimetric assessment procedure described with accuracy better than +/- 10%. The spherical isotropy was evaluated with the procedure described in and found to be better than +/-0.25dB. The sensitivity parameters (Norm X, Norm Y, Norm Z), the diode compression parameter (DCP) and the conversion factor (Conv F) of the probe is tested.

### Free Space Assessment

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/cm$^2$.

### Temperature Assessment

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium, correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor based temperature probe is used in conjunction with the E-field probe

$$SAR = C\frac{\Delta T}{\Delta t}$$

where:

$\Delta t$ = exposure time (30 seconds),

C = heat capacity of tissue (brain or muscle),

$\Delta T$ = temperature increase due to RF exposure.

$$SAR = \frac{|E|^2 \cdot \sigma}{\rho}$$

where:

$\sigma$ = simulated tissue conductivity,

$\rho$ = Tissue density (1.25 g/cm$^3$ for brain tissue)

SAR is proportional to ΔT / Δt , the initial rate of tissue heating, before thermal diffusion takes place.
Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E- field;

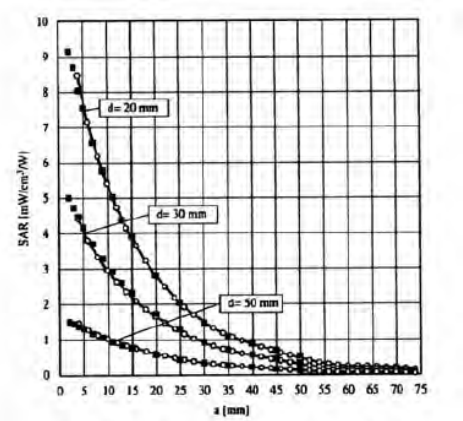


**Figure 2.4 E-Field and Temperature Measurements at 900MHz**

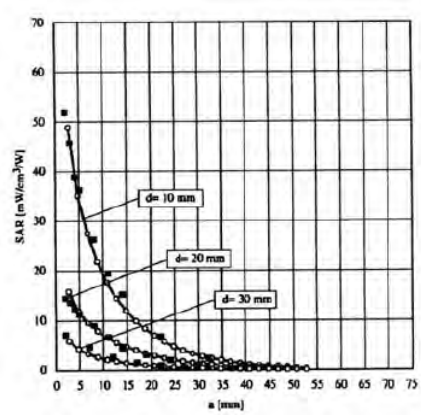


**Figure 2.5 E-Field and Temperature Measurements at 1800MHz**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## Data Extrapolation

The DASY52 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given like below;

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with
$V_i$ = compensated signal of channel i (i=x,y,z)
$U_i$ = input signal of channel i (i=x,y,z)
cf = crest factor of exciting field (DASY parameter)
$dcp_i$ = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:

$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

with
$V_i$ = compensated signal of channel i (i = x,y,z)
$Norm_i$ = sensor sensitivity of channel i (i = x,y,z)
$\mu V/(V/m)^2$ for E-field probes
ConvF = sensitivity of enhancement in solution
$E_i$ = electric field strength of channel i in V/m

The RSS value of the field components gives the total field strength (Hermetian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with
SAR = local specific absorption rate in W/g
$E_{tot}$ = total field strength in V/m
$\sigma$ = conductivity in [mho/m] or [Siemens/m]
$\rho$ = equivalent tissue density in $g/cm^3$

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$

with
$P_{pwe}$ = equivalent power density of a plane wave in $W/cm^2$
$E_{tot}$ = total electric field strength in V/m

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## Scanning procedure

- The DASY installation includes predefined files with recommended procedures for measurements and system check. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The „reference“ and „drift“ measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. +/- 5 %.

- The highest integrated SAR value is the main concern in compliance test applications. These values can mostly be found at the inner surface of the phantom and cannot be measured directly due to the sensor offset in the probe. To extrapolate the surface values, the measurement distances to the surface must be known accurately. A distance error of 0.5mm could produce SAR errors of 6% at 1800 MHz. Using predefined locations for measurements is not accurate enough. Any shift of the phantom (e.g., slight deformations after filling it with liquid) would produce high uncertainties. For an automatic and accurate detection of the phantom surface, the DASY5 system uses the mechanical surface detection. The detection is always at touch, but the probe will move backward from the surface the indicated distance before starting the measurement.

- The „area scan“ measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The scan uses different grid spacings for different frequency measurements. Standard grid spacing for head measurements in frequency ranges ≤ 2GHz is 15 mm in x - and y- dimension. For higher frequencies a finer resolution is needed, thus for the grid spacing is reduced according the following table:

| **Area scan grid spacing for different frequency ranges** | |
|---|---|
| Frequency range | Grid spacing |
| ≤ 2 GHz | ≤ 15 mm |
| 2 – 4 GHz | ≤ 12 mm |
| 4 – 6 GHz | ≤ 10 mm |

Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation. Results of this coarse scan are shown in annex B.

- A „zoom scan” measures the field in a volume around the 2D peak SAR value acquired in the previous „coarse“ scan. It uses a fine meshed grid where the robot moves the probe in steps along all the 3 axis (x,y and z-axis) starting at the bottom of the Phantom. The grid spacing for the cube measurement is varied according to the measured frequency range, the dimensions are given in the following table:

| **Zoom scan grid spacing and volume for different frequency ranges** | | | |
|---|---|---|---|
| Frequency range | Grid spacing for x, y axis | Grid spacing for z axis | Minimum zoom scan volume |
| ≤ 2 GHz | ≤ 8 mm | ≤ 5 mm | ≥ 30 mm |
| 2 – 3 GHz | ≤ 5 mm | ≤ 5 mm | ≥ 28 mm |
| 3 – 4 GHz | ≤ 5 mm | ≤ 4 mm | ≥ 28 mm |
| 4 – 5 GHz | ≤ 4 mm | ≤ 3 mm | ≥ 25 mm |
| 5 – 6 GHz | ≤ 4 mm | ≤ 2 mm | ≥ 22 mm |

DASY is also able to perform repeated zoom scans if more than 1 peak is found during area scan. In this document, the evaluated peak 1g and 10g averaged SAR values are shown in the 2D-graphics in annex B. Test results relevant for the specified standard (see section 3) are shown in table form in section 7.


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## Spatial Peak SAR Evaluation

The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The basis of the evaluation are the SAR values measured at the points of the fine cube grid consisting of all points in the three directions x, y and z. The algorithm that finds the maximal averaged volume is separated into three different stages.

- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 1 to 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.

- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR - values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.

- All neighbouring volumes are evaluated until no neighbouring volume with a higher average value is found.

## Extrapolation

The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the probe tip. The points, calculated from the surface, have a distance of 1 mm from each other.

## Interpolation

The interpolation of the points is done with a 3d-Spline. The 3d-Spline is composed of three one-dimensional splines with the "Not a knot"-condition [W. Gander, Computermathematik, p.141-150] (x, y and z -direction) [Numerical Recipes in C, Second Edition, p.123ff ].

## Volume Averaging

At First the size of the cube is calculated. Then the volume is integrated with the trapezoidal algorithm. 8000 points (20x20x20) are interpolated to calculate the average.

## Advanced Extrapolation

DASY uses the advanced extrapolation option which is able to compensate boundary effects on E-field probes.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

## SAM PHANTOM

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. (see Fig. 2.6)

## Phantom Specification

**Phantom:** Flat Phantom (V5.0)
**Shell Material:** Vivac Composite
**Thickness:** 2.0 ± 0.2 mm

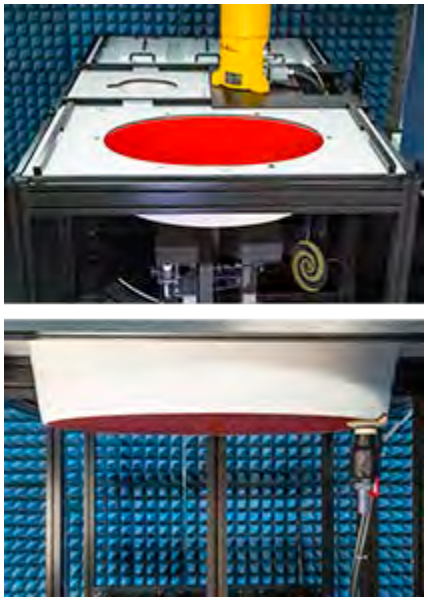

**Figure 2.6 Flat Phantom**

## Device Holder for Transmitters

In combination with the Phantom the Mounting Device (see Fig. 2.7), enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation point is the ear opening. The devices can be easily, accurately, and repeat ably be positioned according to the FCC, CENELEC, IEC and IEEE specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).

**Figure 2.7 Mounting Device**

Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produce infinite number of configurations. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 3. Probe and Dipole Calibration

**See Appendix D and E.**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 4. Phantom & Simulating Tissue Specifications

## Head Simulating Mixture Characterization

The head mixture consist of the material based on the table listed below. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the desired tissue.

**Table 4.1 Typical Composition of Ingredients for Tissue**

| Ingredients | | Simulating Tissue<br>2450 MHz Head |
|---|---|---|
| Mixing Percentage | | |
| Water | | Proprietary Mixture Procured from Speag |
| Sugar | | |
| Salt | | |
| HEC | | |
| Bactericide | | |
| DGBE | | |
| Dielectric Constant | Target | 39.20 |
| Conductivity (S/m) | Target | 1.80 |

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 5. RF Exposure Limits [2]

## Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

## Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

**Table 6.1 Human Exposure Limits**

| | UNCONTROLLED ENVIRONMENT<br>General Population | CONTROLLED ENVIROMENT<br>Professional Population |
|---|---|---|
| SPATIAL PEAK SAR[1]<br>Head | 1.60 W/kg | 8.00 W/kg |
| SPATIAL AVERAGE SAR[2]<br>Whole Body | 0.08 W/kg | 0.40 W/kg |
| SPATIAL PEAK SAR[3]<br>Hands, Feet, Ankles, Wrists | 4.00 W/kg | 20.00 W/kg |

[1] The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
[2] The Spatial Average value of the SAR averaged over the whole body.
[3] The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 6. Measurement Uncertainty

Measurement uncertainty table is not required per KDB 865664 D01 v01 section 2.8.2 page 12. SAR measurement uncertainty analysis is required in the SAR report only when the highest measured SAR in a frequency band is ≥ 1.5 W/kg for 1-g SAR. The equivalent ratio (1.5/1.6) should be applied to extremity and occupational exposure conditions. The highest reported value is less than 1.5 W/kg. Therefore, the measurement uncertainty table SAR testing is not required.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 7. SAR System Verification

## Tissue Verification

**Table 7.1 Measured Tissue Parameters**

| | | 2450 MHz Head | | 2450 MHz Head | |
|---|---|---|---|---|---|
| Date(s) | | Sept. 29, 2025 | | Oct. 1, 2025 | |
| Liquid Temperature (˚C) | 20.0 | Target | Measured | Target | Measured |
| Dielectric Constant: ε | | 39.20 | 38.39 | 39.20 | 38.21 |
| Conductivity: σ | | 1.80 | 1.79 | 1.80 | 1.81 |

See Appendix A for data printout.

## SAR System Verification

Prior to assessment, the system is verified to the ±10% of the specifications at the test frequency by using the system kit. Power is measured at the power listed in the data sheet in appendix A then normalized to 1 watt. (Graphic Plots Attached)

**Table 7.2 System Dipole Validation Target & Measured**

| | Test Frequency | Targeted $SAR_{1g}$ (W/kg) | Measure $SAR_{1g}$ (W/kg) | Tissue Used for Verification | Deviation Target and Fast SAR to SAR (%) | Plot Number |
|---|---|---|---|---|---|---|
| 29-Sep-2025 | 2450 MHz | 53.30 | 52.30 | Head | - 1.88 | 1 |
| 01-Oct-2025 | 2450 MHz | 53.30 | 52.10 | Head | - 2.25 | 2 |

See Appendix A for data plots.

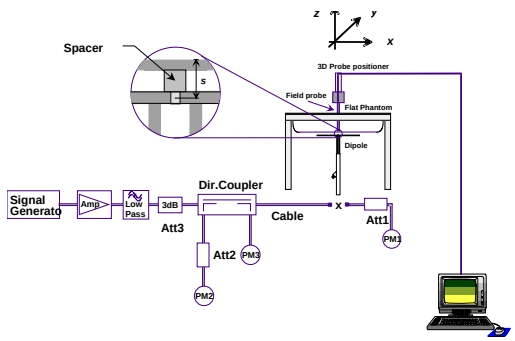


**Figure 7.1 Dipole Validation Test Setup**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 8. SAR Test Data Summary

## See Measurement Result Data Pages

See Appendix B for SAR Test Data Plots.
See Appendix C for SAR Test Setup Photos.

## Procedures Used To Establish Test Signal

The device was either placed into simulated transmit mode using the manufacturer's test codes or the actual transmission is activated through a base station simulator or similar equipment. See data pages for actual procedure used in measurement.

## Device Test Condition

In order to verify that the device was tested at full power, conducted output power measurements were performed before and after each SAR measurement to confirm the output power unless otherwise noted. If a conducted power deviation of more than 5% occurred, the test was repeated. The power drift of each test is measured at the start of the test and again at the end of the test. The drift percentage is calculated by the formula ((end/start)-1)*100 and rounded to three decimal places. The drift percentage is calculated into the resultant SAR value on the data sheet for each test.

The EUT was tested on all sides of the device. All measurements were conducted with the side of the device in direct contact with the phantom.

The data rates used when evaluating the WiFi transmitter were the lowest data rates and widest bandwidth with the highest conduct power limit for each mode. The device was operating at its maximum output power for all measurements.

The antenna was on a minimum of 10 cm of Styrofoam during each test. The following is a pictorial drawing of the locations and separation distances.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Antenna Locations**

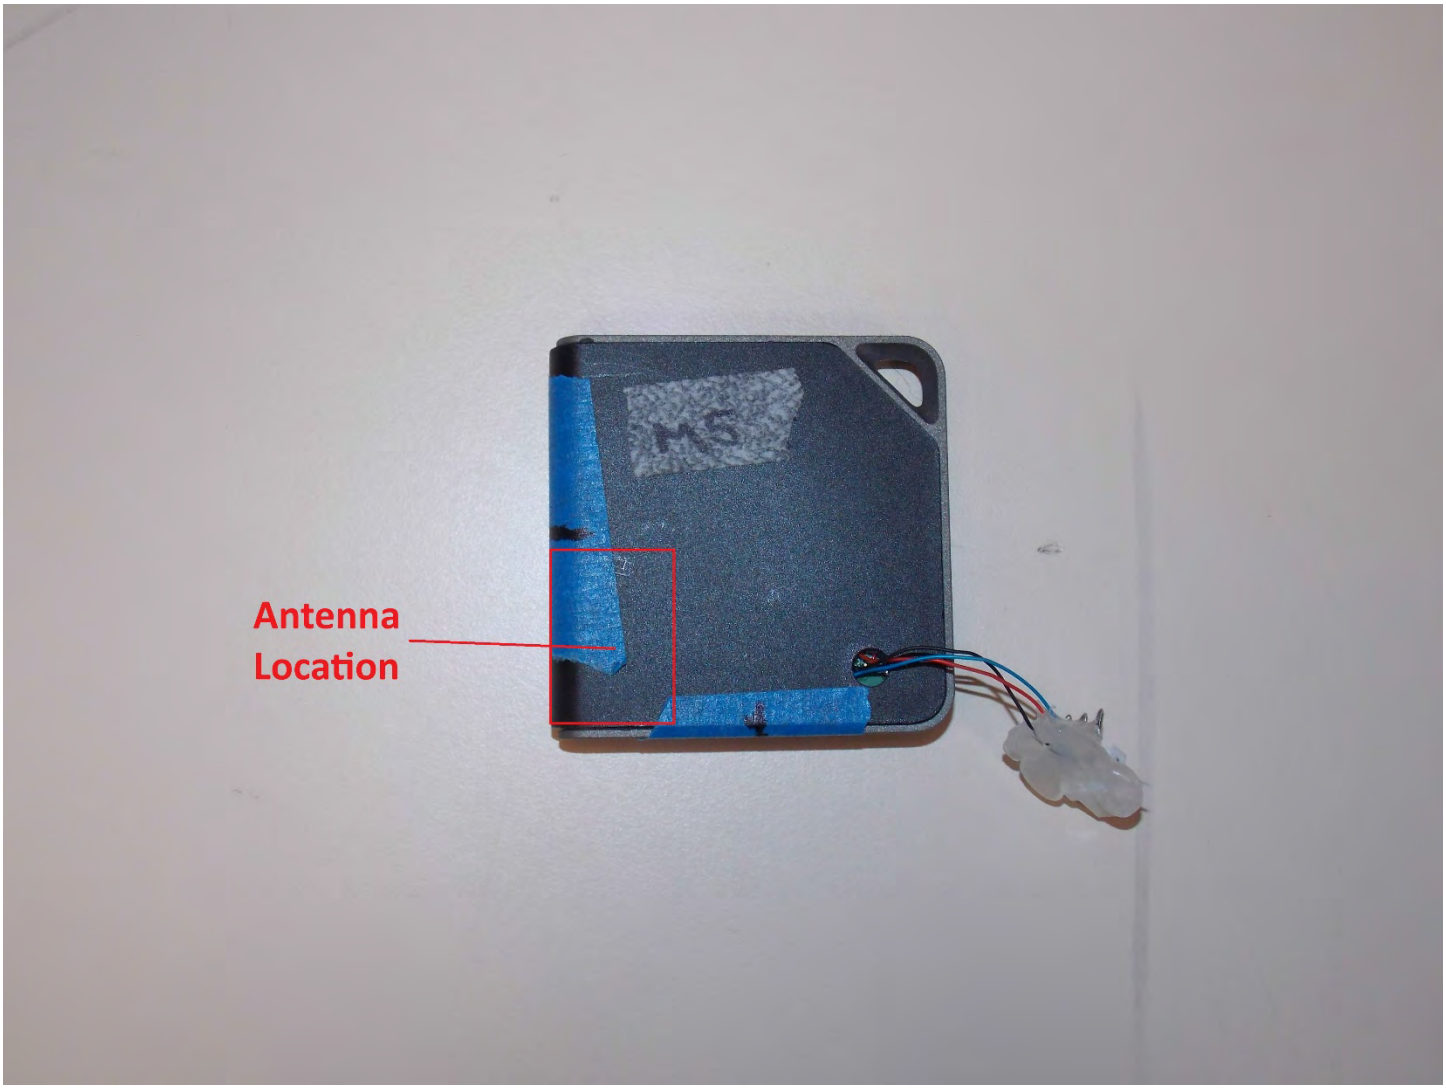



*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

| Band | Mode | Channel | Frequency (MHz) | Avg Power (dBm) | Tune-up Pwr (dBm) |
|---|---|---|---|---|---|
| 2450 MHz | 802.11b | 2 | 2417 | 10.39 | 11.0 |
| | | 6 | 2437 | 10.25 | 11.0 |
| | | 10 | 2457 | 9.96 | 11.0 |
| | 802.11g | 2 | 2417 | Not Required | 10.6 |
| | | 6 | 2437 | | 10.6 |
| | | 10 | 2457 | | 10.6 |
| | 802.11n20 | 2 | 2417 | | 10.3 |
| | | 6 | 2437 | | 10.3 |
| | | 10 | 2457 | | 10.3 |

Note: Channels 1 and 11 had the power reduced; therefore, the testing was conducted on channels 2 and 10.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 9. SAR Test Results

**General Note:**

1. Per KDB 447498 D01v06, the reported SAR is the measured SAR value adjusted for maximum tune-up tolerance.
   a. Tune-up scaling Factor = tune-up limit power (mW) / EUT RF power (mW), where tune-up limit is the maximum rated power among all production units.
   b. For SAR testing of WLAN signal with non-100% duty cycle, the measured SAR is scaled-up by the duty cycle scaling factor which is equal to "1/(duty cycle)"
   c. For WWAN: Reported SAR(W/kg)= Measured SAR(W/kg)*Tune-up Scaling Factor
2. Per KDB 447498 D01v06, for each exposure position, testing of other required channels within the operating mode of a frequency band is not required when the *reported* 1-g or 10-g SAR for the mid-band or highest output power channel is:
   - ≤ 0.8 W/kg or 2.0 W/kg, for 1-g or 10-g respectively, when the transmission band is ≤ 100 MHz
   - ≤ 0.6 W/kg or 1.5 W/kg, for 1-g or 10-g respectively, when the transmission band is between 100 MHz and 200 MHz
   - ≤ 0.4 W/kg or 1.0 W/kg, for 1-g or 10-g respectively, when the transmission band is ≥ 200 MHz
3. Per KDB 865664 D01v01r04, for each frequency band, repeated SAR measurement is required only when the measured SAR is ≥0.8W/kg.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

| Plot No. | Band | Modulation | Test Position | Gap (mm) | Ch. | Freq. (MHz) | Average Power (dBm) | Tune-Up Limit (dBm) | Measured 1g SAR (W/kg) | Reported 1g SAR (W/kg) |
|---|---|---|---|---|---|---|---|---|---|---|
| | 2.45 GHz | CCK | Front | 0mm | 2 | 2417 | 10.39 | 11.00 | 0.939 | 1.08 |
| | 2.45 GHz | CCK | | 0mm | 6 | 2437 | 10.25 | 11.00 | 1.08 | 1.28 |
| | 2.45 GHz | CCK | | 0mm | 10 | 2457 | 9.96 | 11.00 | 0.967 | 1.23 |
| | 2.45 GHz | CCK | Repeat | 0mm | 6 | 2437 | 10.25 | 11.00 | 1.06 | 1.26 |
| | 2.45 GHz | CCK | Back | 0mm | 2 | 2417 | 10.39 | 11.00 | 1.09 | 1.25 |
| 1 | 2.45 GHz | CCK | | 0mm | 6 | 2437 | 10.25 | 11.00 | 1.11 | 1.32 |
| | 2.45 GHz | CCK | | 0mm | 10 | 2457 | 9.96 | 11.00 | 0.975 | 1.24 |
| | 2.45 GHz | CCK | Repeat | 0mm | 6 | 2437 | 10.25 | 11.00 | 1.10 | 1.31 |
| | 2.45 GHz | CCK | Top | 0mm | 6 | 2437 | 10.25 | 11.00 | 0.241 | 0.29 |
| | 2.45 GHz | CCK | Bottom | 0mm | 6 | 2437 | 10.25 | 11.00 | 0.250 | 0.30 |
| | 2.45 GHz | CCK | Right | 0mm | 2 | 2417 | 10.39 | 11.00 | 0.867 | 1.00 |
| | 2.45 GHz | CCK | | 0mm | 6 | 2437 | 10.25 | 11.00 | 0.962 | 1.14 |
| | 2.45 GHz | CCK | | 0mm | 10 | 2457 | 9.96 | 11.00 | 0.813 | 1.03 |
| | 2.45 GHz | CCK | Repeat | 0mm | 6 | 2437 | 10.25 | 11.00 | 0.951 | 1.13 |
| | 2.45 GHz | CCK | Left | 0mm | 6 | 2437 | 10.25 | 11.00 | 0.0976 | 0.12 |

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 10. Test Equipment List

**Table 10.1 Equipment Specifications**

| Type | Calibration Due Date | Calibration Done Date | Serial Number |
|---|---|---|---|
| Staubli Robot TX60L | N/A | N/A | F07/55M6A1/A/01 |
| Measurement Controller CS8c | N/A | N/A | 1012 |
| ELI5 Flat Phantom | N/A | N/A | 1065 |
| Device Holder | N/A | N/A | N/A |
| Data Acquisition Electronics 4 | 01/15/2026 | 01/15/2025 | 1321 |
| SPEAG E-Field Probe EX3DV4 | 01/16/2026 | 01/16/2025 | 7530 |
| Speag Validation Dipole D2450V2 | 05/06/2026 | 05/06/2024 | 829 |
| Agilent N1911A Power Meter | 02/28/2026 | 02/28/2025 | GB45100254 |
| Agilent N1922A Power Sensor | 02/28/2026 | 02/28/2025 | MY45240464 |
| Agilent (HP) 8596E Spectrum Analyzer | 02/28/2026 | 02/28/2025 | 3826A01468 |
| Agilent (HP) 83752A Synthesized Sweeper | 02/28/2026 | 02/28/2025 | 3610A01048 |
| Agilent (HP) 8753C Vector Network Analyzer | 02/28/2026 | 02/28/2025 | 3135A01724 |
| Agilent (HP) 85047A S-Parameter Test Set | 02/28/2026 | 02/28/2025 | 2904A00595 |
| Copper Mountain R140 Vector Reflectometer | 02/28/2026 | 02/28/2025 | 21390004 |
| Agilent 778D Dual Directional Coupler | N/A | N/A | MY48220184 |
| MiniCircuits BW-N20W5+ Fixed 20 dB Attenuator | N/A | N/A | N/A |
| MiniCircuits SPL-10.7+ Low Pass Filter | N/A | N/A | R8979513746 |
| Aprel Dielectric Probe Assembly | N/A | N/A | 0011 |
| Head Equivalent Matter (2450 MHz) | N/A | N/A | N/A |
| UART-USB Connector Cable for Test Setup | N/A | N/A | N/A |

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 11. Conclusion

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The tested device complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body is a very complex phenomena that depends on the mass, shape, and size of the body; the orientation of the body with respect to the field vectors; and, the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# 12. References

[1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radio Frequency Radiation, August 1996

[2] ANSI/IEEE C95.1 – 1992, American National Standard Safety Levels with respect to Human Exposure to Radio Frequency Electromagnetic Fields, 300kHz to 100GHz, New York: IEEE, 1992.

[3] ANSI/IEEE C95.3 – 2002, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, 2002.

[4] IEEE Standard 1528 – 2013, IEEE Recommended Practice for Determining the Peak-Spatial Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communication Devices: Measurement Techniques, June 2013.

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# Appendix A – System Validation Plots and Data

```
************************************************************
Test Result for UIM Dielectric Parameter
Mon 29/Sep/2025
Freq   Frequency(GHz)
FCC_eH Limits for Head Epsilon
FCC_sH Limits for Head Sigma
Test_e Epsilon  of  UIM
Test_s Sigma of UIM
************************************************************
Freq          FCC_eH FCC_sH Test_e Test_s
2.4100        39.26  1.76   38.49  1.74
2.4120        39.258 1.762  38.486 1.742*
2.4200        39.25  1.77   38.47  1.75
2.4300        39.24  1.78   38.45  1.76
2.4370        39.226 1.787  38.443 1.774*
2.4400        39.22  1.79   38.44  1.78
2.4420        39.216 1.792  38.43  1.782*
2.4500        39.20  1.80   38.39  1.79
2.4600        39.19  1.81   38.39  1.80
2.4620        39.186 1.812  38.386 1.802*
2.4700        39.17  1.82   38.37  1.81
2.4720        39.168 1.822  38.366 1.816*
2.4800        39.16  1.83   38.35  1.84

* value interpolated


************************************************************
Test Result for UIM Dielectric Parameter
Wed 01/Oct/2025
Freq   Frequency(GHz)
FCC_eH Limits for Head Epsilon
FCC_sH Limits for Head Sigma
Test_e Epsilon  of  UIM
Test_s Sigma of UIM
************************************************************
Freq          FCC_eH FCC_sH Test_e Test_s
2.4100        39.26  1.76   38.31  1.76
2.4120        39.258 1.762  38.306 1.762*
2.4200        39.25  1.77   38.29  1.77
2.4300        39.24  1.78   38.27  1.78
2.4370        39.226 1.787  38.263 1.794*
2.4400        39.22  1.79   38.26  1.80
2.4420        39.216 1.792  38.25  1.802*
2.4500        39.20  1.80   38.21  1.81
2.4600        39.19  1.81   38.21  1.82
2.4620        39.186 1.812  38.206 1.822*
2.4700        39.17  1.82   38.19  1.83
2.4720        39.168 1.822  38.186 1.836*
2.4800        39.16  1.83   38.17  1.86

* value interpolated
```


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# RF Exposure Lab

## Plot 1

### DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN: 829

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium: HSL2450; Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; $\varepsilon_r$ = 38.39; ρ = 1000 kg/m$^3$
Phantom section: Flat Section

Test Date: Date: 9/29/2025; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 – SN7530; ConvF(7.18, 7.21, 7.46); Calibrated: 1/16/2025;
Sensor-Surface: 2mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1321; Calibrated: 1/15/2025
Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065
Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.14 (7483)

### Procedure Notes:

**Head Verification/2450 MHz/Area Scan (61x101x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm
Maximum value of SAR (interpolated) = 8.42 W/kg

**Head Verification/2450 MHz/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 52.487 V/m; Power Drift = -0.01 dB
Peak SAR (extrapolated) = 10.95 W/kg
$P_{in}$= 100 mW
**SAR(1 g) = 5.23 W/kg; SAR(10 g) = 2.51 W/kg**
Smallest distance from peaks to all points 3 dB below = 9.3 mm
Ratio of SAR at M2 to SAR at M1 = 37.5%
Maximum value of SAR (measured) = 8.94 W/kg

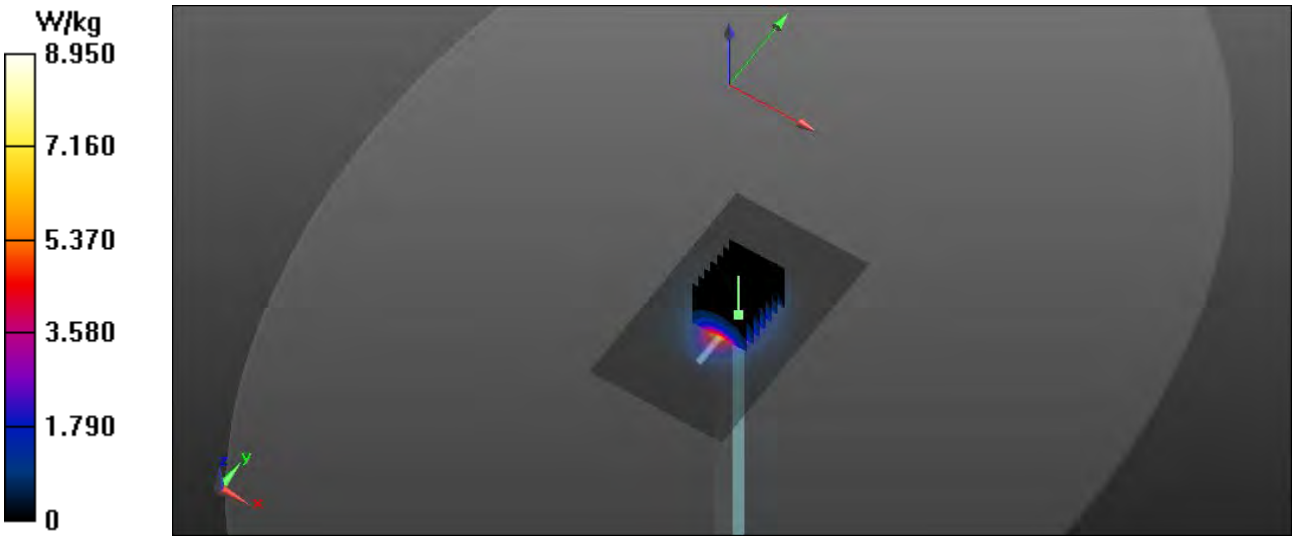



*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# RF Exposure Lab

## Plot 2

### DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: D2450V2 - SN: 829

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium: HSL2450; Medium parameters used: f = 2450 MHz; σ = 1.81 S/m; $\varepsilon_r$ = 38.21; ρ = 1000 kg/m$^3$
Phantom section: Flat Section

Test Date: Date: 10/1/2025; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 – SN7530; ConvF(7.18, 7.21, 7.46); Calibrated: 1/16/2025;
Sensor-Surface: 2mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1321; Calibrated: 1/15/2025
Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065
Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.14 (7483)

### Procedure Notes:

**Head Verification/2450 MHz/Area Scan (61x101x1):** Interpolated grid: dx=1.200 mm, dy=1.200 mm
Maximum value of SAR (interpolated) = 8.67 W/kg

**Head Verification/2450 MHz/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 54.027 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 11.04 W/kg
$P_{in}$= 100 mW
**SAR(1 g) = 5.21 W/kg; SAR(10 g) = 2.49 W/kg**
Smallest distance from peaks to all points 3 dB below = 9.6 mm
Ratio of SAR at M2 to SAR at M1 = 35.9%
Maximum value of SAR (measured) = 8.95 W/kg

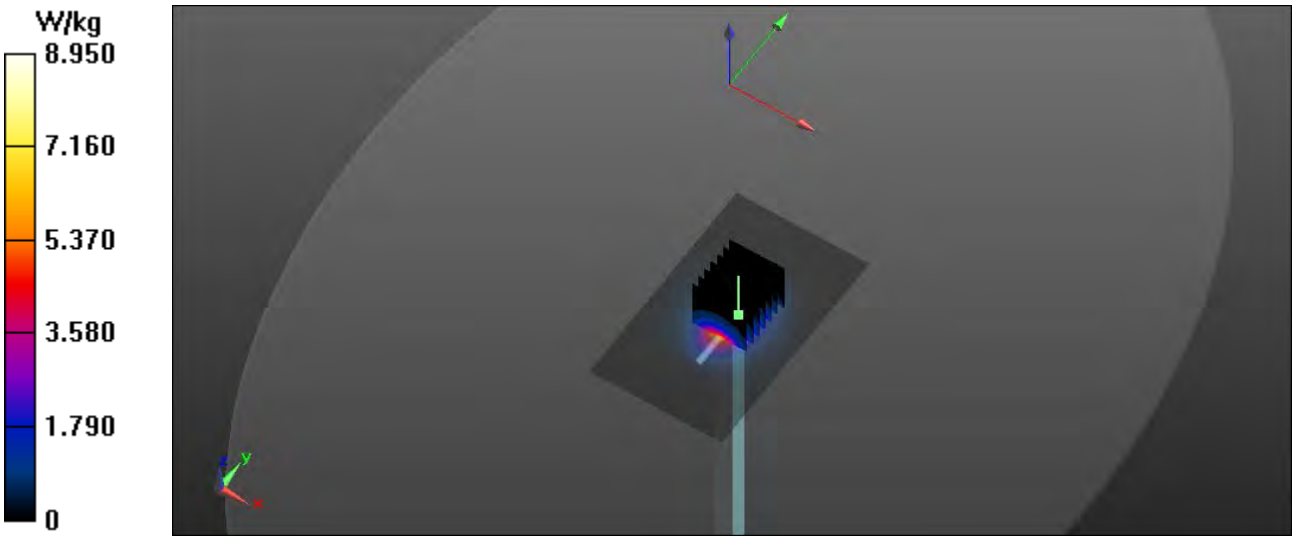


© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# Appendix B – SAR Test Data Plots


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# RF Exposure Lab

## Plot 1

### DUT: Relay; Type: WiFi; Serial: M5

Communication System: WiFi 802.11b (DSSS, 1 Mbps); Frequency: 2437 MHz; Duty Cycle: 1:1
Medium: HSL2450; Medium parameters used (interpolated): f = 2437 MHz; σ = 1.774 S/m; $\varepsilon_r$ = 38.443; ρ = 1000 kg/m$^3$
Phantom section: Flat Section

Test Date: Date: 9/29/2025; Ambient Temp: 23 °C; Tissue Temp: 21 °C

Probe: EX3DV4 - SN7530; ConvF(7.18, 7.21, 7.46); Calibrated: 1/16/2025
Sensor-Surface: 2mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1321; Calibrated: 1/15/2025
Phantom: ELI v4.0; Type: QDOVA001BB; Serial: 1065
Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.14 (7483)

### Procedure Notes:

**2450 MHz/Back Mid 6/Area Scan (9x9x1):** Measurement grid: dx=10mm, dy=10mm

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 1.62 W/kg

**2450 MHz/Back Mid 6/Zoom Scan (9x9x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 12.01 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 2.59 W/kg
**SAR(1 g) = 1.11 W/kg; SAR(10 g) = 0.507 W/kg**
Smallest distance from peaks to all points 3 dB below = 6.1 mm
Ratio of SAR at M2 to SAR at M1 = 48.2%

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 1.91 W/kg

**2450 MHz/Back Mid 6/Zoom Scan (9x9x7)/Cube 1:** Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 12.01 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 2.62 W/kg
**SAR(1 g) = 1.1 W/kg; SAR(10 g) = 0.499 W/kg**
Smallest distance from peaks to all points 3 dB below = 5.8 mm
Ratio of SAR at M2 to SAR at M1 = 45.6%

Info: Interpolated medium parameters used for SAR evaluation.
Maximum value of SAR (measured) = 1.97 W/kg

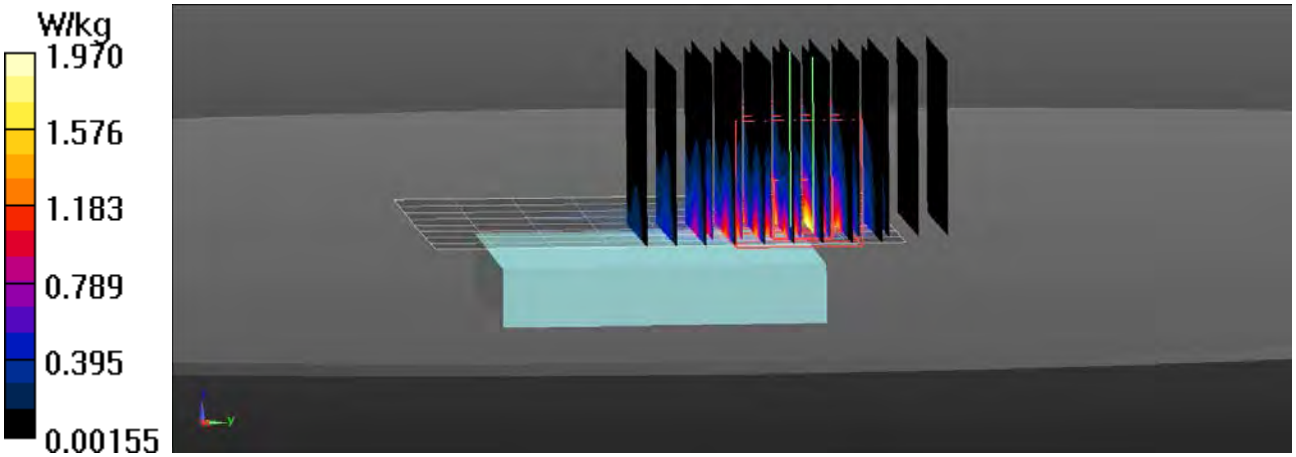


© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# Appendix C – SAR Test Setup Photos

**Test Position Front 0 mm Gap**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Test Position Back 0 mm Gap**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Test Position Top 0 mm Gap**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Test Position Bottom 0 mm Gap**

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Test Position Right 0 mm Gap**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Test Position Left 0 mm Gap**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

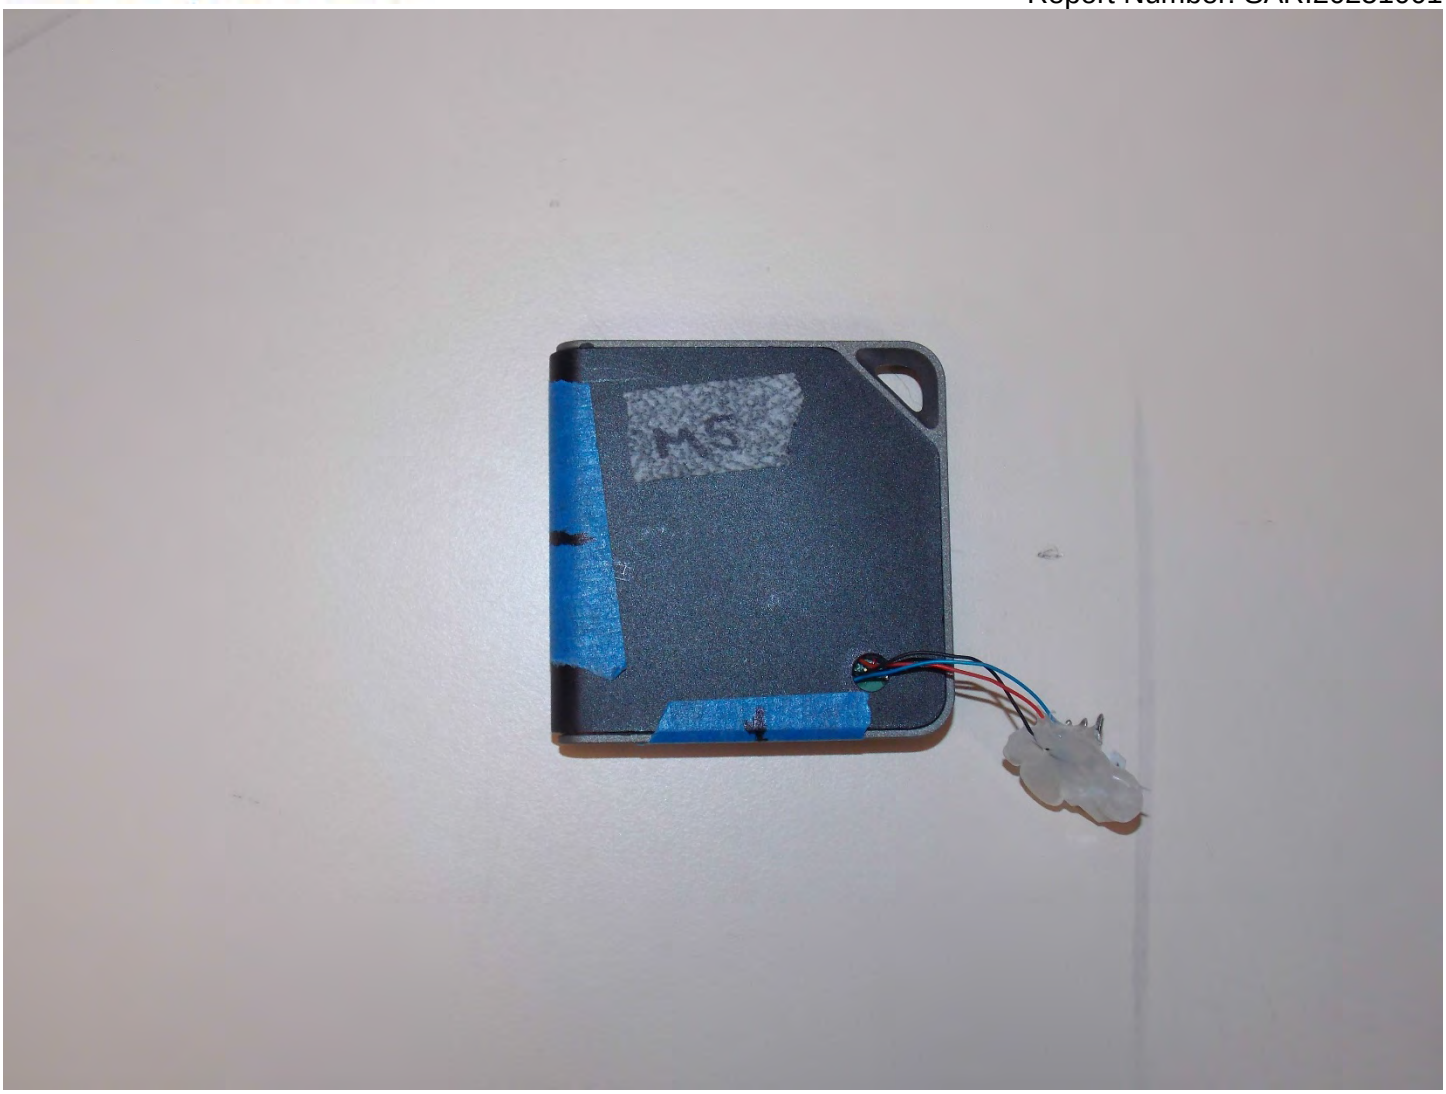


**Front of Device**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Back of Device**


*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

# Appendix D – Probe Calibration Data Sheets

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

**S Schweizerischer Kalibrierdienst**
**C Service suisse d'étalonnage**
**Servizio svizzero di taratura**
**S Swiss Calibration Service**

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

**Client** **RF Exposure Lab**
**San Marcos, USA**

**Certificate No.** **EX-7530_Jan25**

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | EX3DV4 - SN:7530 |
| Calibration procedure(s) | QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6, QA CAL-25.v8<br>Calibration procedure for dosimetric E-field probes |
| Calibration date | January 16, 2025 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID | Calibration Date (Certificate No.) | Sched. Cal. |
|---|---|---|---|
| Power Sensor R&S NRP-33T | SN: 100967 | 28-Mar-24 (No. 217-04038) | Mar-25 |
| Short [S6019i] + Attenuator [S6020i] | SN: L1119 | 26-Mar-24 (No. 217-04048) | Mar-25 |
| OCP DAK-12 | SN: 1016 | 24-Sept-24 (No. OCP-DAK12-1016_Sep24) | Sep-25 |
| OCP DAK-3.5 | SN: 1249 | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25 |
| Reference Probe EX3DV4 | SN: 7349 | 10-Jan-25 (No. EX3-7349_Jan25) | Jan-26 |
| DAE4 | SN: 1301 | 07-Nov-24 (No. DAE4-1301_Nov24) | Nov-25 |

| Secondary Standards | ID | Check Date (in house) | Sched. Check |
|---|---|---|---|
| ACAP 2020 Calibration Box | SN: L1404 | 30-Sept-24 (No. Report_ACAP2020E-Cave_20240930s) | Sep-25 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by | Aidonia Georgiadou | Laboratory Technician | |
| Approved by | Sven Kühn | Technical Manager | |

Issued: January 16, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Glossary

| | |
|---|---|
| TSL | tissue simulating liquid |
| NORMx,y,z | sensitivity in free space |
| ConvF | sensitivity in TSL / NORMx,y,z |
| DCP | diode compression point |
| CF | crest factor (1/duty_cycle) of the RF signal |
| A, B, C, D | modulation dependent linearization parameters |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis |
| Connector Angle | information used in DASY system to align probe sensor X to the robot coordinate system |

## Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices – Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Methods Applied and Interpretation of Parameters:

- *NORMx,y,z*: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the $E^2$-field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)x,y,z = NORMx,y,z * frequency_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- *DCPx,y,z*: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- *PAR*: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- *Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D* are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z * ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ±50 MHz to ±100 MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORMx* (no uncertainty required).

# Parameters of Probe: EX3DV4 - SN:7530

## Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc ($k$ = 2) |
|---|---|---|---|---|
| Norm ($\mu$V/(V/m)$^2$) [A] | 0.42 | 0.53 | 0.43 | ±10.1% |
| DCP (mV) [B] | 98.6 | 99.2 | 100.9 | ±4.7% |

## Calibration Results for Modulation Response

| UID | Communication System Name | | A dB | B dB$\sqrt{\mu V}$ | C | D dB | VR mV | Max dev. | Max Unc[E] $k$ = 2 |
|---|---|---|---|---|---|---|---|---|---|
| 0 | CW | X | 0.00 | 0.00 | 1.00 | 0.00 | 137.5 | ±0.7% | ±4.7% |
| | | Y | 0.00 | 0.00 | 1.00 | | 135.3 | | |
| | | Z | 0.00 | 0.00 | 1.00 | | 140.0 | | |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

[A] The uncertainties of Norm X,Y,Z do not affect the $E^2$-field uncertainty inside TSL (see Pages 5 and 6).
[B] Linearization parameter uncertainty for maximum specified field strength.
[E] Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

# Parameters of Probe: EX3DV4 - SN:7530

## Other Probe Parameters

| | |
|---|---|
| Sensor Arrangement | Triangular |
| Connector Angle | 35.9° |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 9 mm |
| Tip Diameter | 2.5 mm |
| Probe Tip to Sensor X Calibration Point | 1 mm |
| Probe Tip to Sensor Y Calibration Point | 1 mm |
| Probe Tip to Sensor Z Calibration Point | 1 mm |
| Recommended Measurement Distance from Surface | 1.4 mm |

**Note:** Measurement distance from surface can be increased to 3–4 mm for an *Area Scan* job.

# Parameters of Probe: EX3DV4 - SN:7530

## Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz)[C] | Relative Permittivity[F] | Conductivity[F] (S/m) | ConvF X | ConvF Y | ConvF Z | Alpha[G] | Depth[G] (mm) | Unc[H] ($k = 2$) |
|---|---|---|---|---|---|---|---|---|
| 6 | 55.0 | 0.75 | 20.02 | 21.02 | 23.44 | 0.00 | 1.25 | ±13.3% |
| 13 | 55.0 | 0.75 | 18.22 | 19.14 | 21.34 | 0.00 | 1.25 | ±13.3% |
| 30 | 55.0 | 0.75 | 16.88 | 17.73 | 19.77 | 0.00 | 1.25 | ±13.3% |
| 750 | 41.9 | 0.89 | 9.59 | 9.63 | 9.97 | 0.36 | 1.27 | ±11.0% |
| 900 | 41.5 | 0.97 | 8.99 | 9.02 | 9.34 | 0.36 | 1.27 | ±11.0% |
| 1750 | 40.1 | 1.37 | 7.96 | 7.99 | 8.28 | 0.35 | 1.27 | ±11.0% |
| 1900 | 40.0 | 1.40 | 7.83 | 7.86 | 8.14 | 0.34 | 1.27 | ±11.0% |
| 2300 | 39.5 | 1.67 | 7.46 | 7.49 | 7.76 | 0.34 | 1.27 | ±11.0% |
| 2450 | 39.2 | 1.80 | 7.18 | 7.21 | 7.46 | 0.34 | 1.27 | ±11.0% |
| 2600 | 39.0 | 1.96 | 7.06 | 7.09 | 7.34 | 0.34 | 1.27 | ±11.0% |
| 5250 | 35.9 | 4.71 | 5.30 | 5.32 | 5.51 | 0.30 | 1.27 | ±13.1% |
| 5600 | 35.5 | 5.07 | 4.75 | 4.77 | 4.94 | 0.27 | 1.27 | ±13.1% |
| 5750 | 35.4 | 5.22 | 4.80 | 4.82 | 4.99 | 0.26 | 1.27 | ±13.1% |

[C] Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ±50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4–9 MHz, and ConvF assessed at 13 MHz is 9–19 MHz. Above 5 GHz frequency validity can be extended to ±110 MHz.

[F] The probes are calibrated using tissue simulating liquids (TSL) that deviate for $\varepsilon$ and $\sigma$ by less than ±5% from the target values (typically better than ±3%) and are valid for TSL with deviations of up to ±10% if SAR correction is applied.

[G] Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3–6 GHz at any distance larger than half the probe tip diameter from the boundary.

[H] The stated uncertainty is the total calibration uncertainty ($k = 2$) of Norm·ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

# Parameters of Probe: EX3DV4 - SN:7530

## Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz)[C] | Relative Permittivity[F] | Conductivity[F] (S/m) | ConvF X | ConvF Y | ConvF Z | Alpha[G] | Depth[G] (mm) | Unc[H] ($k = 2$) |
|---|---|---|---|---|---|---|---|---|
| 6500 | 34.5 | 6.07 | 5.44 | 5.46 | 5.66 | 0.20 | 1.27 | ±18.6% |

[C] Frequency validity at 6.5 GHz is −600/+700 MHz, and ±700 MHz at or above 7 GHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
[F] The probes are calibrated using tissue simulating liquids (TSL) that deviate for $\varepsilon$ and $\sigma$ by less than ±10% from the target values (typically better than ±6%) and are valid for TSL with deviations of up to ±10%.
[G] Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz; below ±2% for frequencies between 3–6 GHz; and below ±4% for frequencies between 6–10 GHz at any distance larger than half the probe tip diameter from the boundary.
[H] The stated uncertainty is the total calibration uncertainty ($k = 2$) of Norm·ConvF. This is equivalent to the uncertainty component with the symbol CF in Table 9 of IEC/IEEE 62209-1528:2020.

## Frequency Response of E-Field

**(TEM-Cell:ifi110 EXX, Waveguide:R22)**

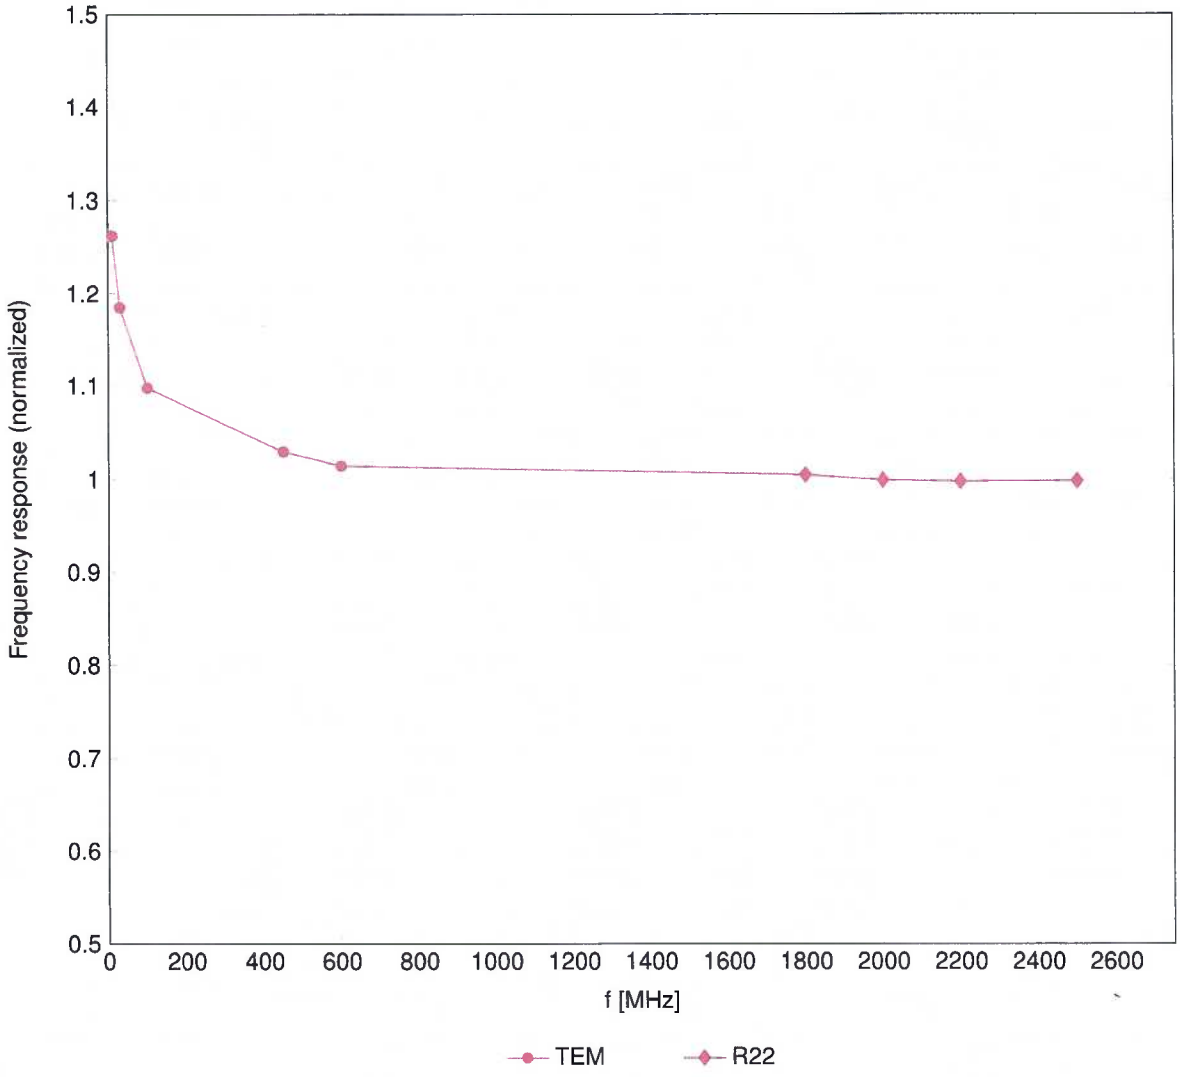


Uncertainty of Frequency Response of E-field: ±6.3% (k=2)

## Receiving Pattern ($\phi$), $\vartheta = 0°$

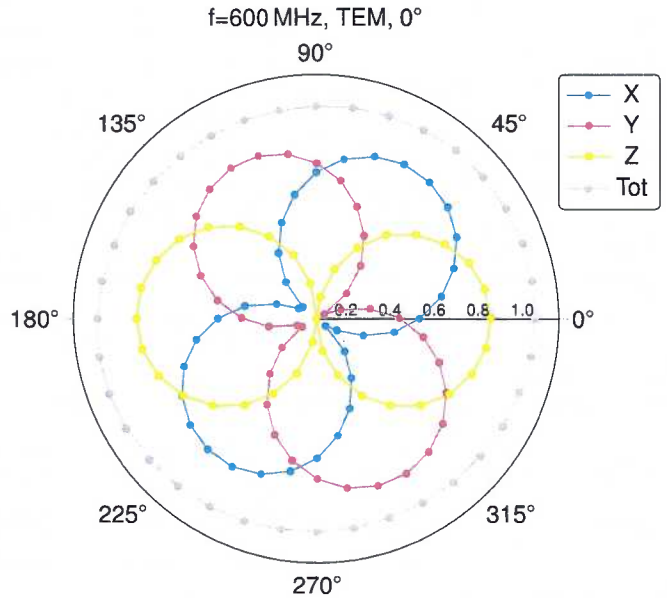


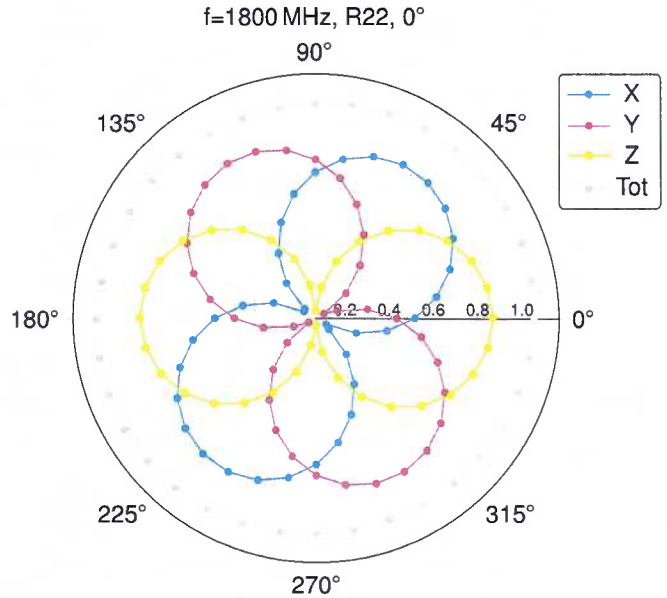


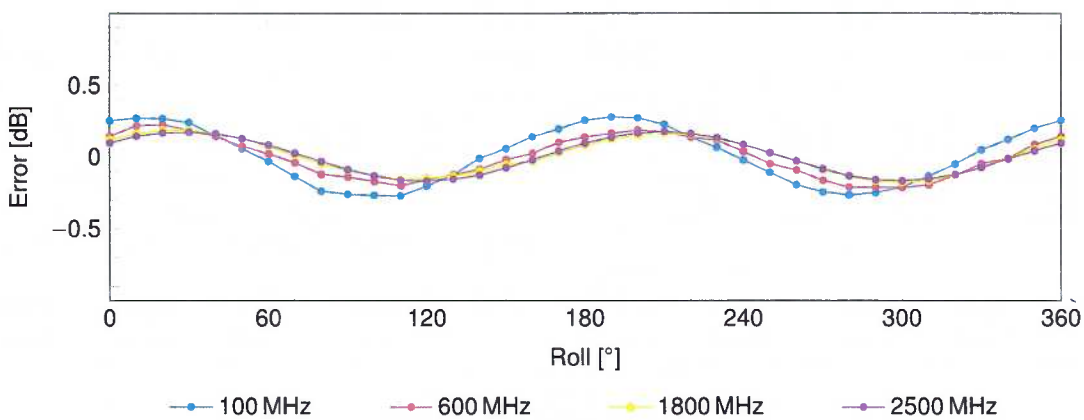


Uncertainty of Axial Isotropy Assessment: ±0.5% (k=2)

## Dynamic Range f($SAR_{head}$)

(TEM cell, $f_{eval}$ = 1900 MHz)

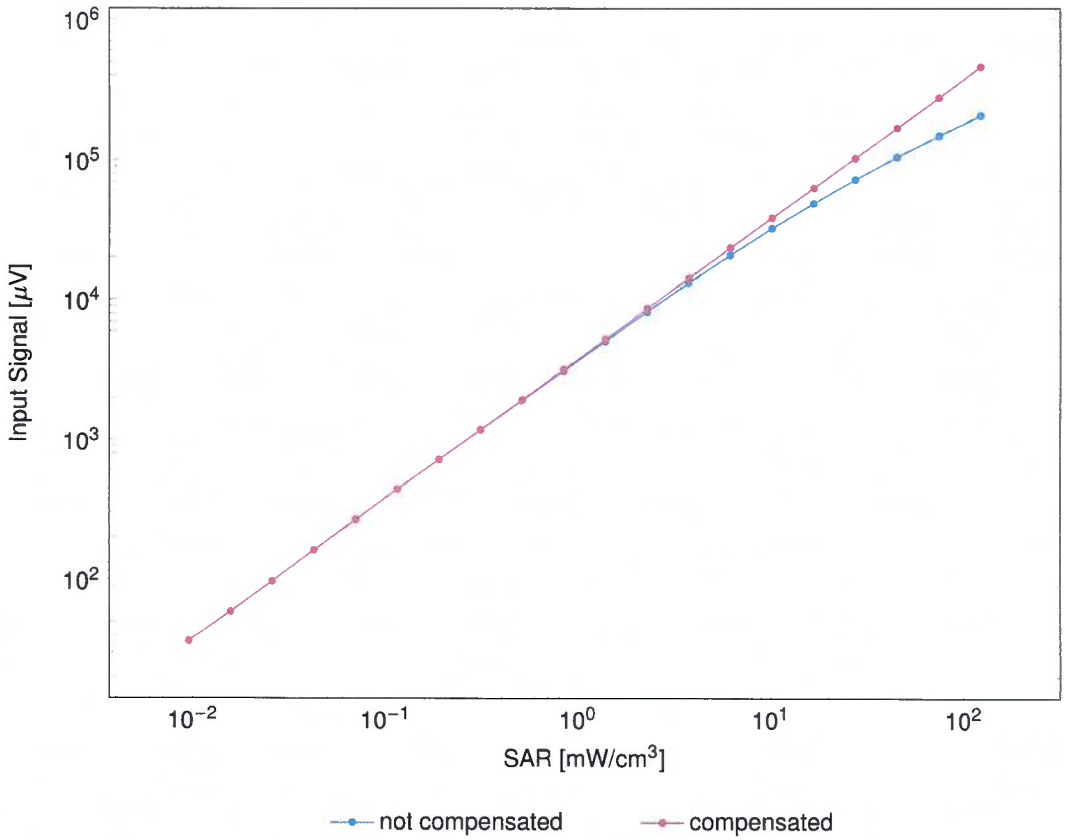


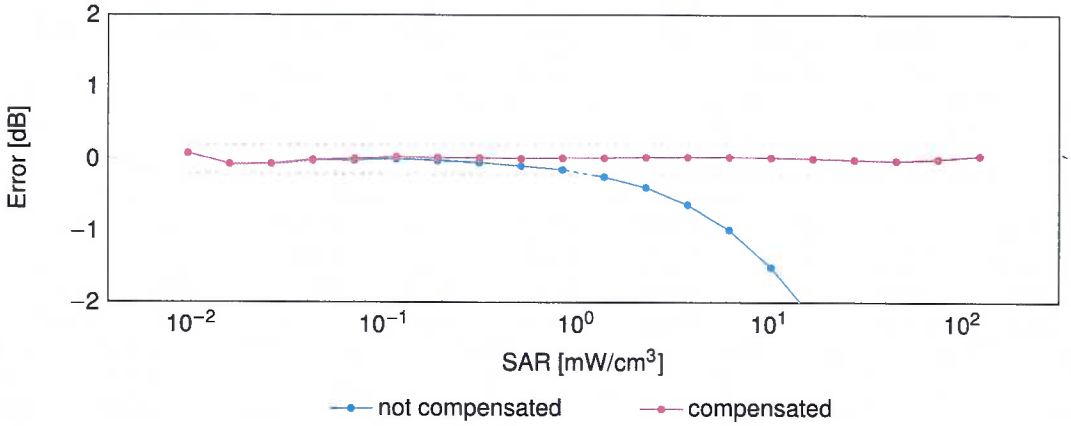


Uncertainty of Linearity Assessment: ±0.6% (k=2)

## Conversion Factor Assessment

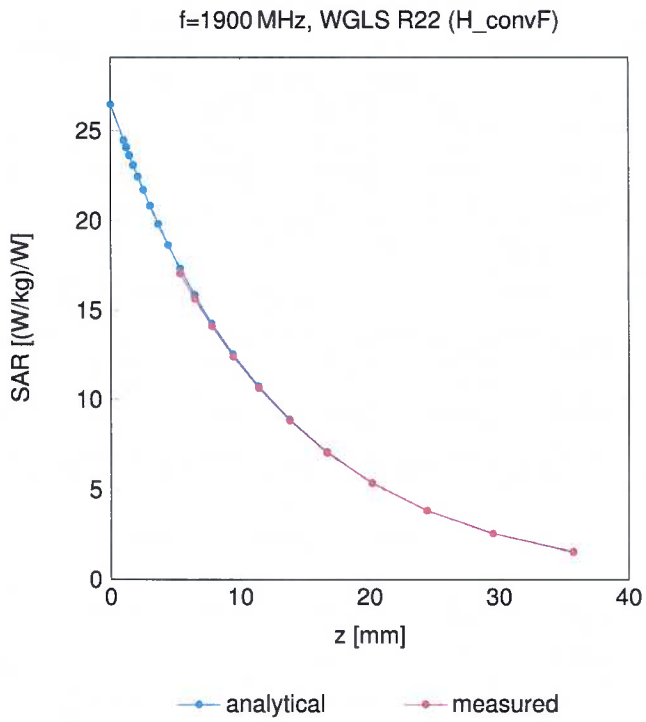


## Deviation from Isotropy in Liquid

**Error $(\phi, \theta)$, f = 900 MHz**

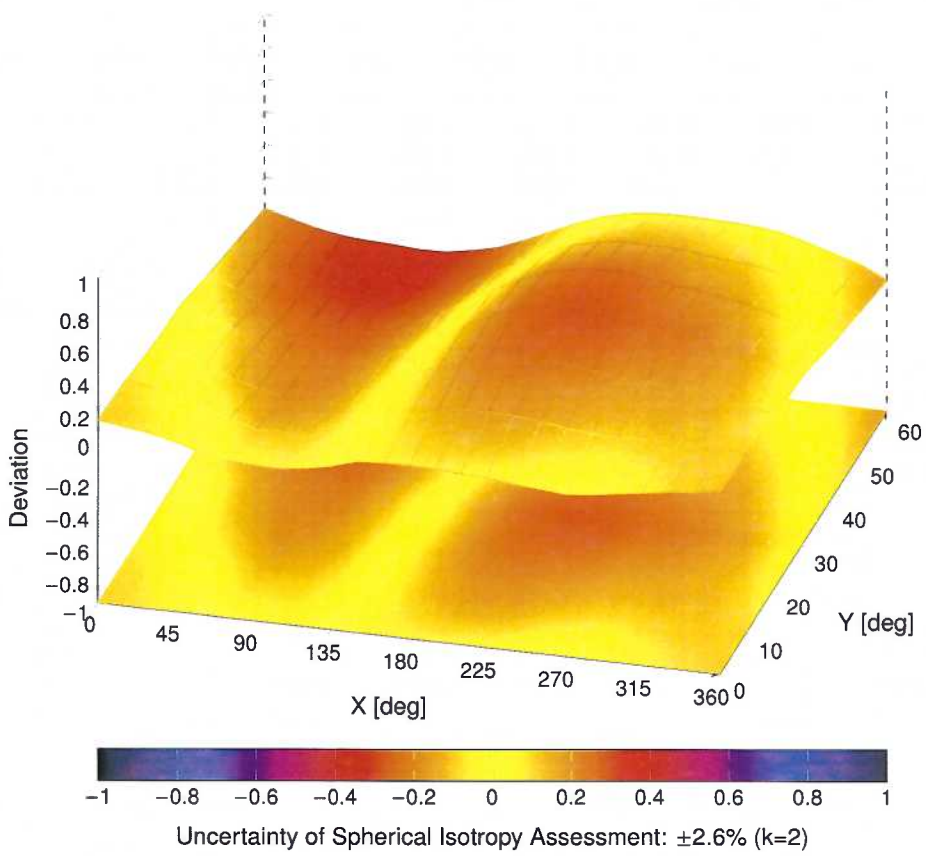


Uncertainty of Spherical Isotropy Assessment: ±2.6% (k=2)

# Appendix E – Dipole Calibration Data Sheets

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
Servizio svizzero di taratura
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

**Client** **RF Exposure Lab**
**San Marcos, USA**

**Certificate No.** **D2450V2-829_May24**

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | D2450V2 - SN:829 |
| Calibration procedure(s) | QA CAL-05.v12<br>Calibration Procedure for SAR Validation Sources between 0.7-3 GHz |
| Calibration date: | May 06, 2024 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|---|---|---|---|
| Power meter NRP2 | SN: 104778 | 26-Mar-24 (No. 217-04036/04037) | Mar-25 |
| Power sensor NRP-Z91 | SN: 103244 | 26-Mar-24 (No. 217-04036) | Mar-25 |
| Power sensor NRP-Z91 | SN: 103245 | 26-Mar-24 (No. 217-04037) | Mar-25 |
| Reference 20 dB Attenuator | SN: BH9394 (20k) | 26-Mar-24 (No. 217-04046) | Mar-25 |
| Type-N mismatch combination | SN: 310982 / 06327 | 26-Mar-24 (No. 217-04047) | Mar-25 |
| Reference Probe EX3DV4 | SN: 7349 | 03-Nov-23 (No. EX3-7349_Nov23) | Nov-24 |
| DAE4 | SN: 601 | 30-Jan-24 (No. DAE4-601_Jan24) | Jan-25 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---|---|---|---|
| Power meter E4419B | SN: GB39512475 | 30-Oct-14 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A | SN: US37292783 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| Power sensor HP 8481A | SN: MY41093315 | 07-Oct-15 (in house check Oct-22) | In house check: Oct-24 |
| RF generator R&S SMT-06 | SN: 100972 | 15-Jun-15 (in house check Oct-22) | In house check: Oct-24 |
| Network Analyzer Agilent E8358A | SN: US41080477 | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by: | Leif Klysner | Laboratory Technician | |
| Approved by: | Sven Kühn | Technical Manager | |

Issued: May 7, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Glossary:

| | |
|---|---|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

## Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation:

c) DASY System Handbook

## Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|---|---|---|
| **DASY Version** | DASY52 | V52.10.4 |
| **Extrapolation** | Advanced Extrapolation | |
| **Phantom** | Modular Flat Phantom | |
| **Distance Dipole Center - TSL** | 10 mm | with Spacer |
| **Zoom Scan Resolution** | dx, dy, dz = 5 mm | |
| **Frequency** | 2450 MHz ± 1 MHz | |

## Head TSL parameters

The following parameters and calculations were applied.

| | **Temperature** | **Permittivity** | **Conductivity** |
|---|---|---|---|
| **Nominal Head TSL parameters** | 22.0 °C | 39.2 | 1.80 mho/m |
| **Measured Head TSL parameters** | (22.0 ± 0.2) °C | 37.9 ± 6 % | 1.88 mho/m ± 6 % |
| **Head TSL temperature change during test** | < 0.5 °C | ---- | ---- |

## SAR result with Head TSL

| **SAR averaged over 1 $cm^3$ (1 g) of Head TSL** | Condition | |
|---|---|---|
| SAR measured | 250 mW input power | 13.7 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | **53.3 W/kg ± 17.0 % (k=2)** |

| **SAR averaged over 10 $cm^3$ (10 g) of Head TSL** | condition | |
|---|---|---|
| SAR measured | 250 mW input power | 6.36 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | **25.0 W/kg ± 16.5 % (k=2)** |

## Appendix (Additional assessments outside the scope of SCS 0108)

## Antenna Parameters with Head TSL

| | |
|---|---|
| Impedance, transformed to feed point | 53.9 Ω + 4.1 jΩ |
| Return Loss | - 25.4 dB |

## General Antenna Parameters and Design

| | |
|---|---|
| Electrical Delay (one direction) | 1.156 ns |

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

| | |
|---|---|
| Manufactured by | SPEAG |

**Extended Calibration**
Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (<-20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB Publication 865664 D01 v01r04.

| D2450V2 SN: 829 - Head | | | | | | |
|---|---|---|---|---|---|---|
| Date of Measurement | Return Loss (dB) | Δ% | Impedance Real (Ω) | ΔΩ | Impedance Imaginary (jΩ) | ΔΩ |
| 5/6/2024 | -25.4 | | 53.9 | | 4.1 | |
| 5/6/2025 | -26.3 | 3.5 | 54.6 | 0.7 | 3.8 | -0.3 |
| | | | | | | |

Date: 06.05.2024

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:829**

Communication System: UID 0 - CW; Frequency: 2450 MHz
Medium parameters used: f = 2450 MHz; $\sigma$ = 1.88 S/m; $\varepsilon_r$ = 37.9; $\rho$ = 1000 kg/m$^3$
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 03.11.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2024
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 116.7 V/m; Power Drift = 0.10 dB
Peak SAR (extrapolated) = 27.4 W/kg
**SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.36 W/kg**
Smallest distance from peaks to all points 3 dB below = 9 mm
Ratio of SAR at M2 to SAR at M1 = 50.6%
Maximum value of SAR (measured) = 21.9 W/kg

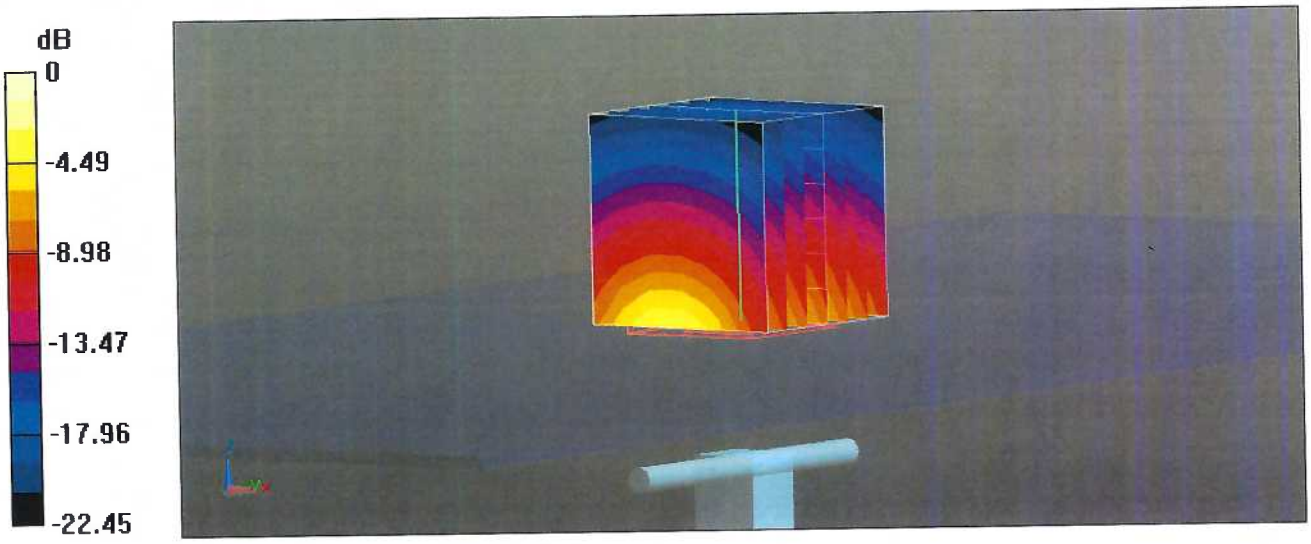


0 dB = 21.9 W/kg = 13.40 dBW/kg

## Impedance Measurement Plot for Head TSL

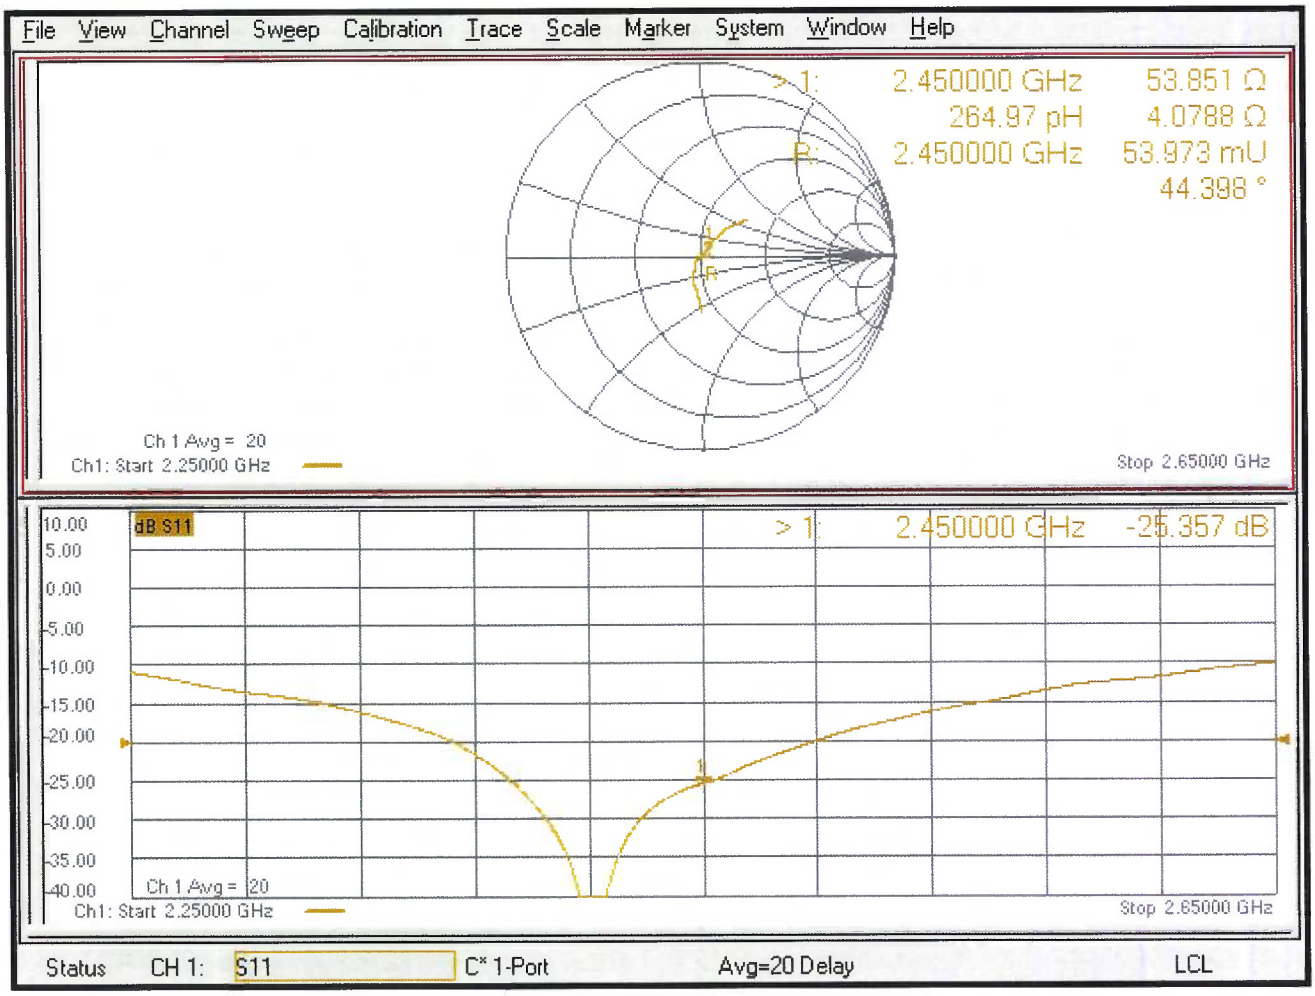

# Appendix F – DAE Calibration Data Sheets

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

**Calibration Laboratory of**
Schmid & Partner
Engineering AG
**Zeughausstrasse 43, 8004 Zurich, Switzerland**

**S** Schweizerischer Kalibrierdienst
**C** Service suisse d'étalonnage
Servizio svizzero di taratura
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

**Client** **RF Exposure Lab**
**San Marcos - USA**

**Certificate No: DAE4-1321_Jan25**

# CALIBRATION CERTIFICATE

| | |
|---|---|
| Object | DAE4 - SD 000 D04 BM - SN: 1321 |
| Calibration procedure(s) | QA CAL-06.v30<br>Calibration procedure for the data acquisition electronics (DAE) |
| Calibration date: | January 15, 2025 |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|---|---|---|---|
| Keithley Multimeter Type 2001 | SN: 0810278 | 27-Aug-24 (No:40547) | Aug-25 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---|---|---|---|
| Auto DAE Calibration Unit | SE UWS 053 AA 1001 | 23-Jan-24 (in house check) | In house check: Jan-25 |
| Calibrator Box V2.1 | SE UMS 006 AA 1002 | 23-Jan-24 (in house check) | In house check: Jan-25 |

| | Name | Function | Signature |
|---|---|---|---|
| Calibrated by: | Adrian Gehring | Laboratory Technician | |
| Approved by: | Sven Kühn | Technical Manager | i.V. |

Issued: January 15, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Glossary

| | |
|---|---|
| DAE | data acquisition electronics |
| Connector angle | information used in DASY system to align probe sensor X to the robot coordinate system. |

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement*: Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

| | | | | |
|---|---|---|---|---|
| High Range: | 1LSB = | 6.1μV , | full range = | -100...+300 mV |
| Low Range: | 1LSB = | 61nV , | full range = | -1.....+3mV |

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X | Y | Z |
|---|---|---|---|
| **High Range** | 405.014 ± 0.02% (k=2) | 404.843 ± 0.02% (k=2) | 405.255 ± 0.02% (k=2) |
| **Low Range** | 3.96697 ± 1.50% (k=2) | 3.99549 ± 1.50% (k=2) | 4.00450 ± 1.50% (k=2) |

## Connector Angle

| | |
|---|---|
| **Connector Angle** to be used in DASY system | 243.0 ° ± 1 ° |

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

| High Range | | Reading (µV) | Difference (µV) | Error (%) |
|---|---|---|---|---|
| Channel X | + Input | 199994.22 | -0.43 | -0.00 |
| Channel X | + Input | 20003.49 | 0.94 | 0.00 |
| Channel X | - Input | -19996.93 | 5.07 | -0.03 |
| Channel Y | + Input | 199992.70 | -1.82 | -0.00 |
| Channel Y | + Input | 20001.78 | -0.69 | -0.00 |
| Channel Y | - Input | -20003.67 | -1.61 | 0.01 |
| Channel Z | + Input | 199991.69 | -2.75 | -0.00 |
| Channel Z | + Input | 20000.76 | -1.84 | -0.01 |
| Channel Z | - Input | -20001.40 | 0.59 | -0.00 |

| Low Range | | Reading (µV) | Difference (µV) | Error (%) |
|---|---|---|---|---|
| Channel X | + Input | 2001.09 | -0.25 | -0.01 |
| Channel X | + Input | 203.11 | 1.43 | 0.71 |
| Channel X | - Input | -197.68 | 0.33 | -0.17 |
| Channel Y | + Input | 2002.02 | 0.58 | 0.03 |
| Channel Y | + Input | 200.50 | -1.28 | -0.64 |
| Channel Y | - Input | -198.75 | -0.71 | 0.36 |
| Channel Z | + Input | 2001.53 | 0.20 | 0.01 |
| Channel Z | + Input | 199.63 | -1.99 | -0.99 |
| Channel Z | - Input | -198.77 | -0.66 | 0.33 |

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Common mode Input Voltage (mV) | High Range Average Reading (µV) | Low Range Average Reading (µV) |
|---|---|---|---|
| Channel X | 200 | 16.74 | 15.11 |
| | - 200 | -14.39 | -16.02 |
| Channel Y | 200 | 1.53 | 1.31 |
| | - 200 | -3.33 | -3.57 |
| Channel Z | 200 | -13.96 | -13.73 |
| | - 200 | 12.34 | 12.23 |

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) |
|---|---|---|---|---|
| Channel X | 200 | - | 0.73 | -4.12 |
| Channel Y | 200 | 8.66 | - | 2.84 |
| Channel Z | 200 | 10.59 | 5.92 | - |

## 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | High Range (LSB) | Low Range (LSB) |
|---|---|---|
| **Channel X** | 15470 | 14859 |
| **Channel Y** | 15581 | 15755 |
| **Channel Z** | 16358 | 16164 |

## 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec
Input 10MΩ

| | Average (μV) | min. Offset (μV) | max. Offset (μV) | Std. Deviation (μV) |
|---|---|---|---|---|
| **Channel X** | 1.26 | 0.17 | 2.34 | 0.48 |
| **Channel Y** | -0.55 | -1.80 | 0.88 | 0.56 |
| **Channel Z** | -0.28 | -1.50 | 1.50 | 0.58 |

## 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

## 7. Input Resistance (Typical values for information)

| | Zeroing (kOhm) | Measuring (MOhm) |
|---|---|---|
| **Channel X** | 200 | 200 |
| **Channel Y** | 200 | 200 |
| **Channel Z** | 200 | 200 |

## 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|---|---|
| **Supply (+ Vcc)** | +7.9 |
| **Supply (- Vcc)** | -7.6 |

## 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|---|---|---|---|
| **Supply (+ Vcc)** | +0.01 | +6 | +14 |
| **Supply (- Vcc)** | –0.01 | -8 | -9 |

# Appendix G – Phantom Calibration Data Sheets

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
info@speag.com, http://www.speag.com

## Certificate of Conformity / First Article Inspection

| | |
|---|---|
| Item | Oval Flat Phantom ELI 4.0 |
| Type No | QD OVA 001 B |
| Series No | 1003 and higher |
| Manufacturer | Untersee Composites<br>Knebelstrasse 8<br>CH-8268 Mannenbach, Switzerland |

**Tests**

Complete tests were made on the prototype units QD OVA 001 AA 1001, QD OVA 001 AB 1002, pre-series units QD OVA 001 BA 1003-1005 as well as on the series units QD OVA 001 BB, 1006 ff.

| Test | Requirement | Details | Units tested |
|---|---|---|---|
| Material thickness | Compliant with the standard requirements | Bottom plate:<br>2.0mm +/- 0.2mm | all |
| Material parameters | Dielectric parameters for required frequencies | < 6 GHz: Rel. permittivity = 4 +/-1, Loss tangent ≤ 0.05 | Material sample |
| Material resistivity | The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions. | DGBE based simulating liquids.<br>Observe Technical Note for material compatibility. | Equivalent phantoms, Material sample |
| Shape | Thickness of bottom material,<br>Internal dimensions,<br>Sagging<br>compatible with standards from minimum frequency | Bottom elliptical 600 x 400 mm<br>Depth 190 mm,<br>Shape is within tolerance for filling height up to 155 mm,<br>Eventual sagging is reduced or eliminated by support via DUT | Prototypes, Sample testing |

**Standards**

[1] CENELEC EN 50361-2001, « Basic standard for the measurement of the Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz – 3 GHz) », July 2001

[2] IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003

[3] IEC 62209 – 1, "Specific Absorption Rate (SAR) in the frequency range of 300 MHz to 3 GHz – Measurement Procedure, Part 1: Hand-held mobile wireless communication devices", February 2005

[4] IEC 62209 – 2, Draft, "Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices – Human models, Instrumentation and Procedures – Part 2: Procedure to determine the Specific Absorption Rate (SAR) in the head and body for 30 MHz to 6 GHz Handheld and Body-Mounted Devices used in close proximity to the Body.", February 2005

[5] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition January 2001

Based on the tests above, we certify that this item is in compliance with the standards [1] to [5] if operated according to the specific requirements and considering the thickness. The dimensions are fully compliant with [4] from 30 MHz to 6 GHz. For the other standards, the minimum lower frequency limit is limited due to the dimensional requirements ([1]: 450 MHz, [2]: 300 MHz, [3]: 800 MHz, [5]: 375 MHz) and possibly further by the dimensions of the DUT.

**Date** 28.4.2008 **Signature / Stamp**

**s p e a g**
Schmid & Partner Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 44 245 9700, Fax +41 44 245 9779
info@speag.com, http://www.speag.com

# Appendix H – Validation Summary

Per FCC KDB 865664 D02 v01r02, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue equivalent media for system validation according to the procedures outlined in FCC KDB 865664 D01 v01r04 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point using the system that normally operates with the probe for routine SAR measurements and according to the required tissue equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

**Table H-1**
**SAR System Validation Summary**

| SAR System # | Freq. (MHz) | Date | Probe S/N | Probe Type | Probe Cal. Point | | Cond. (σ) | Perm. ($\varepsilon_r$) | CW Validation | | | Modulation Validation | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| | | | | | | | | | Sens-itivity | Probe Linearity | Probe Isotropy | Modulation Type | Duty Factor | PAR |
| | | | | | | | | | | | | | | |
| 2 | 2450 | 01/28/2025 | 7530 | EX3DV4 | 2450 | Head | 1.81 | 38.67 | Pass | Pass | Pass | CCK | N/A | Pass |

© 2025 RF Exposure Lab, LLC

*This report shall not be reproduced except in full without the written approval of RF Exposure Lab, LLC.*