

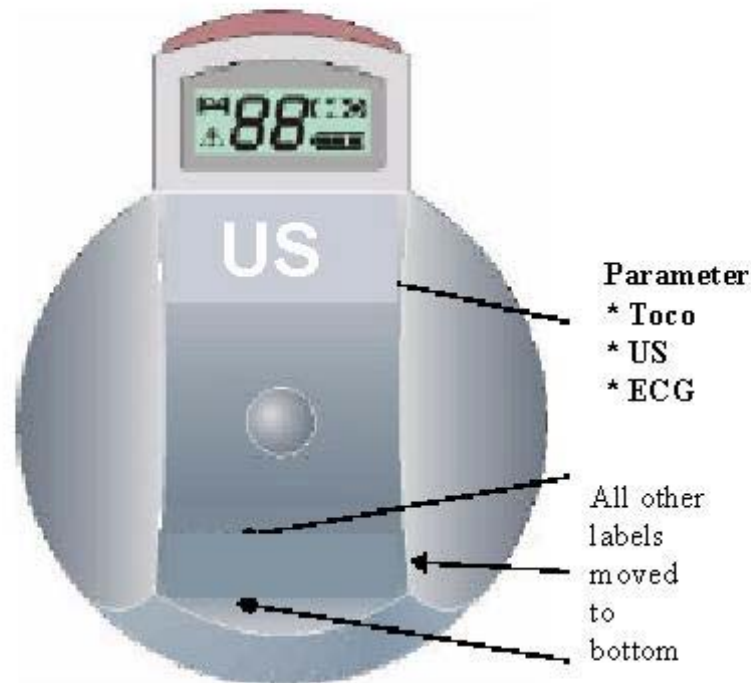


M2720A Cordless Fetal Transducer System Labeling

Transducer top

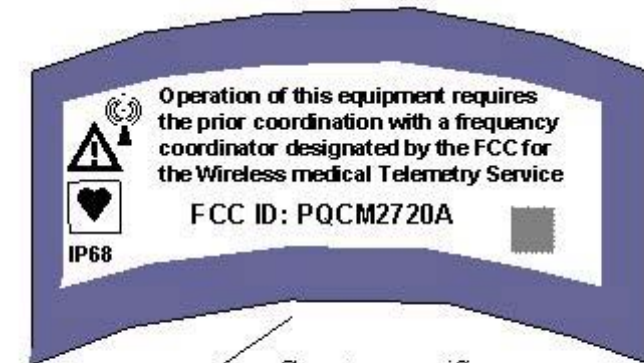

Transducer bottom

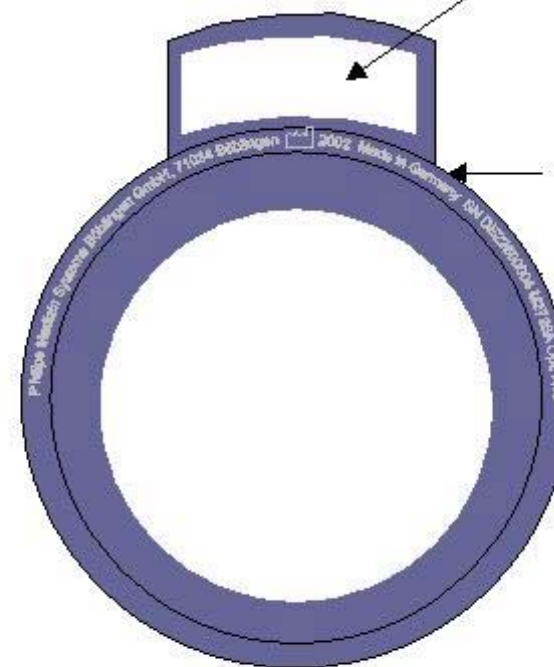

Country specific regulatory labels


Manufacturing address, date, country of origin, serial number, product number (M2725A, M2726A, M2727A) and RF version (Laser printed)

For manufacturing:
2D barcode (3mm*3 mm)

Print 1 slide/page for correct size

Labels and symbols are not scaled!

M2720A Base Station Labeling

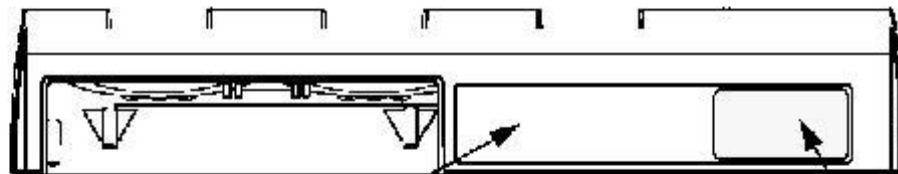


SN label

PTT and Warning label

 Philips Medizin Systeme Boeblingen GmbH 71034 Boeblingen Germany  2002-10 REF M2720A *M2720A* SN DE22400001 *DE22400001* Opt.: A15 Made in Germany	 0388   CAUTION: SHOCK HAZARD. DO NOT REMOVE COVER. SERVICE BY QUALIFIED PERSONNEL ONLY. THIS ISM DEVICE COMPLIES WITH CANADIAN ICES-001. CET APPAREIL ISM EST CONFORME A LA NORME NMB-001 DU CANADA.	M2720A Tested To Comply With FCC Standards FOR HOME OR OFFICE USE IC: 123456789
--	---	---

*Manufacturing date
being updated every month*

*Print 1 slide/page for correct size of rear label
(3 of 9 Barcode and Philips fonts required)*

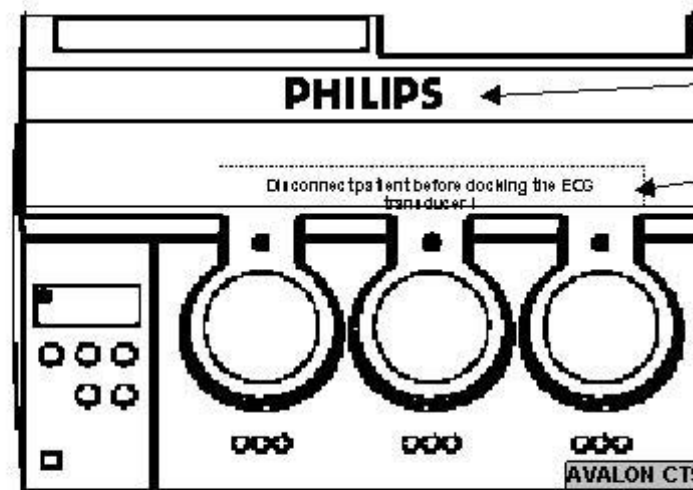

PHILIPS logo
(Tampon print)

ECG warning label

Device name,
*may be located
above display*

Labels and symbols are not scaled!