

# Appendix A

|                            |
|----------------------------|
| System Check 13 MHz Head   |
| System Check 750 MHz Head  |
| System Check 8350 MHz Head |
| System Check 1750 MHz Head |
| System Check 1900 MHz Head |
| System Check 2450 MHz Head |
| System Check 2600 MHz Head |
| System Check 3500 MHz Head |
| System Check 3700 MHz Head |
| System Check 3900 MHz Head |
| System Check 5200 MHz Head |
| System Check 5600 MHz Head |
| System Check 5800 MHz Head |

Summary

|                 |                 |     |             |             |              |               |                |
|-----------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole          | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| CLA-13 – SN1043 | 13.0            | HSL | 20.0        | 27.7        | 28.1         | n/a           | 2.0            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 0                  |      | CW, 0--    | 13.000, 0                       | 18.28             | 0.764                  | 55.9             |

Hardware Setup


|                                    |           |                             |                           |
|------------------------------------|-----------|-----------------------------|---------------------------|
| Phantom                            | TSL       | Probe, Calibration Date     | DAE, Calibration Date     |
| ELI V8.0 (20deg probe tilt) – 2227 | HSL3-6GHz | EX3DV4 – SN7858, 2024-01-09 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | Y           | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-01-02, 12:57 | 2025-01-02, 13:04 |
| psSAR1g [W/Kg]      | 0.050             | 0.049             |
| psSAR10g [W/Kg]     | 0.033             | 0.031             |
| Power Drift [dB]    | 0.01              | 0.04              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

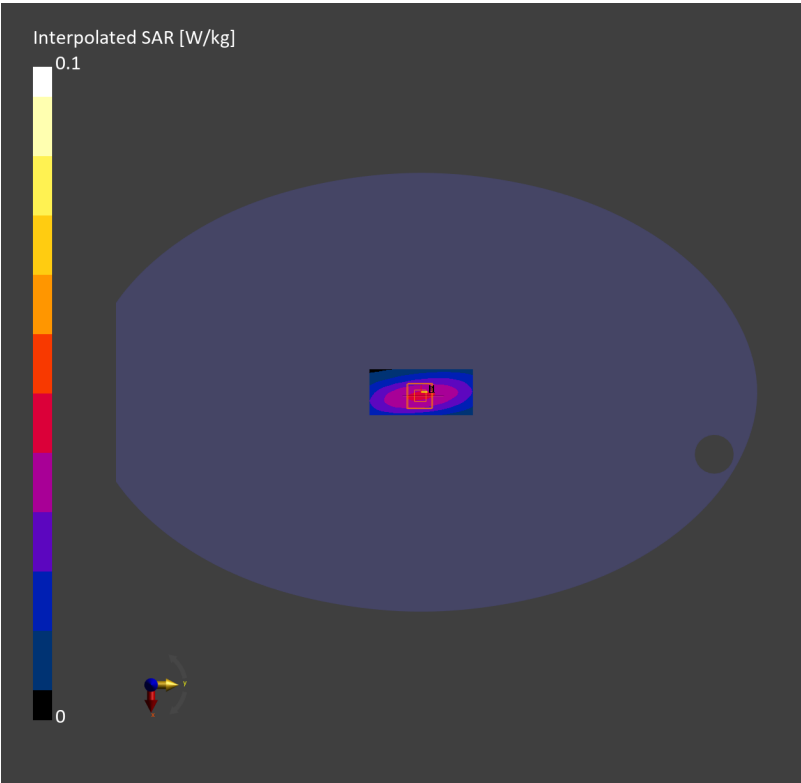

Summary

| Dipole          | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|-----------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D750V3 – SN1231 | 750.0           | HSL | 20.0        | –0.4        | –0.2         | 15.8          | –2.5           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 15                 |      | CW, 0--    | 750.000, 0                      | 9.65              | 0.898                  | 42.0             |

Hardware Setup


| Phantom                                 | TSL    | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|--------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL750 | EX3DV4 – SN7812, 2024–06–25 | DAE4ip Sn1847, 2024–12–31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025–01–22, 17:02 | 2025–01–22, 17:08 |
| psSAR1g [W/Kg]      | 0.854             | 0.867             |
| psSAR10g [W/Kg]     | 0.568             | 0.568             |
| Power Drift [dB]    | –0.00             | –0.01             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

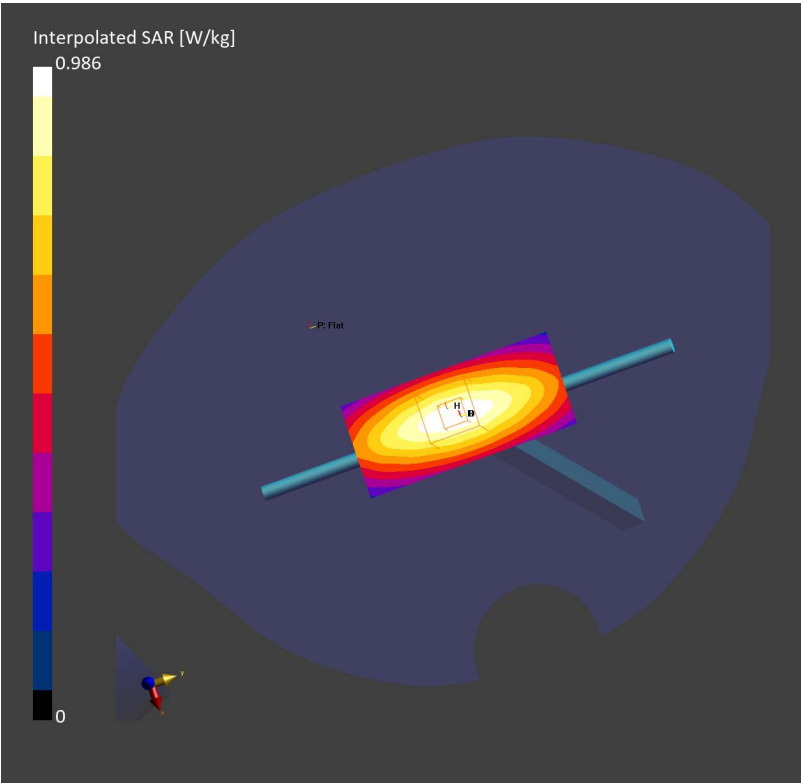

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D835V2 – SN4d302 | 835.0           | HSL | 20.0        | 4.7         | 4.4          | 19.7          | –2.5           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 15                 |      | CW, 0--    | 835.000, 0                      | 9.35              | 0.898                  | 41.2             |

Hardware Setup


| Phantom                                 | TSL    | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|--------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL835 | EX3DV4 – SN7812, 2024–06–25 | DAE4ip Sn1847, 2024–12–31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025–01–22, 08:29 | 2025–01–22, 08:35 |
| psSAR1g [W/Kg]      | 1.00              | 1.02              |
| psSAR10g [W/Kg]     | 0.661             | 0.660             |
| Power Drift [dB]    | –0.01             | –0.01             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

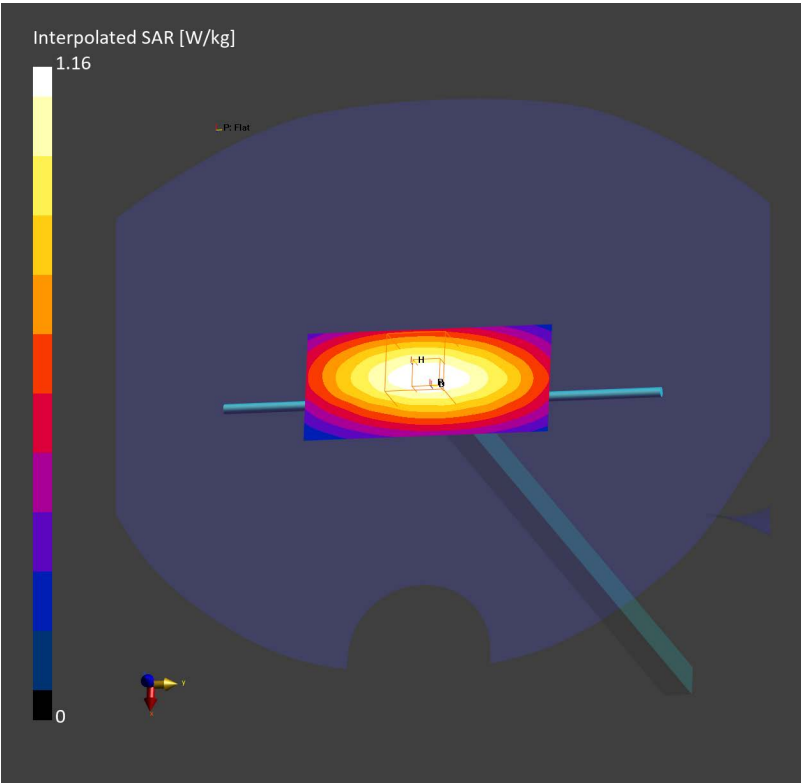

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D835V2 – SN4d302 | 835.0           | HSL | 20.0        | 2.8         | 2.3          | 16.1          | 2.6            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 15                 |      | CW, 0--    | 835.000, 0                      | 9.35              | 0.895                  | 42.0             |

Hardware Setup


| Phantom                                 | TSL    | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|--------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL835 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-25, 10:11 | 2025-01-25, 10:17 |
| psSAR1g [W/Kg]      | 0.976             | 0.989             |
| psSAR10g [W/Kg]     | 0.644             | 0.644             |
| Power Drift [dB]    | -0.01             | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

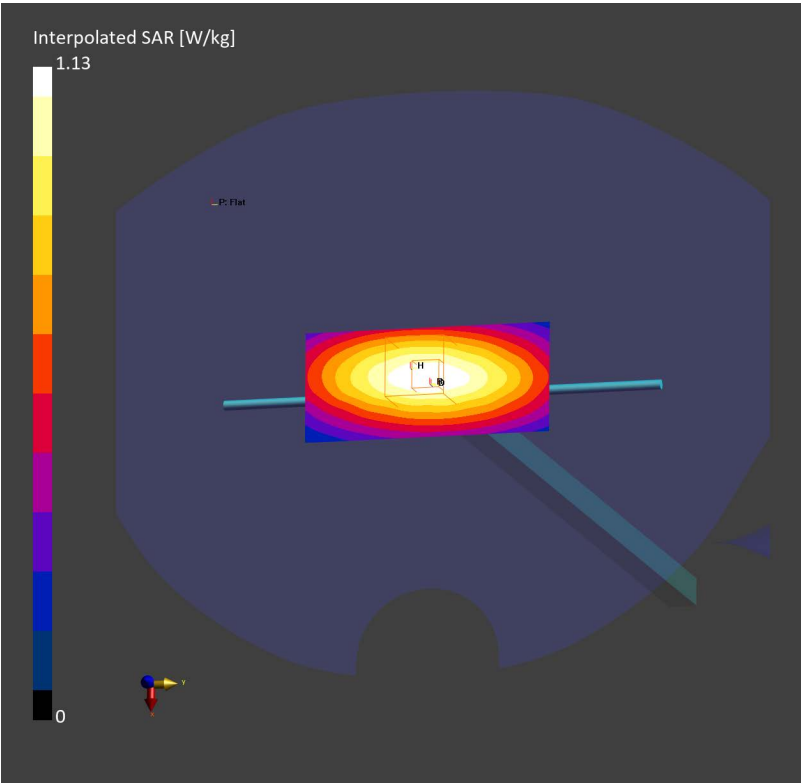

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D835V2 – SN4d302 | 835.0           | HSL | 20.0        | –0.8        | –0.4         | 12.8          | 3.4            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 15                 |      | CW, 0--    | 835.000, 0                      | 9.35              | 0.894                  | 40.8             |

Hardware Setup


| Phantom                                 | TSL    | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|--------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL835 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-05, 17:23 | 2025-02-05, 17:29 |
| psSAR1g [W/Kg]      | 0.939             | 0.961             |
| psSAR10g [W/Kg]     | 0.621             | 0.629             |
| Power Drift [dB]    | 0.00              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

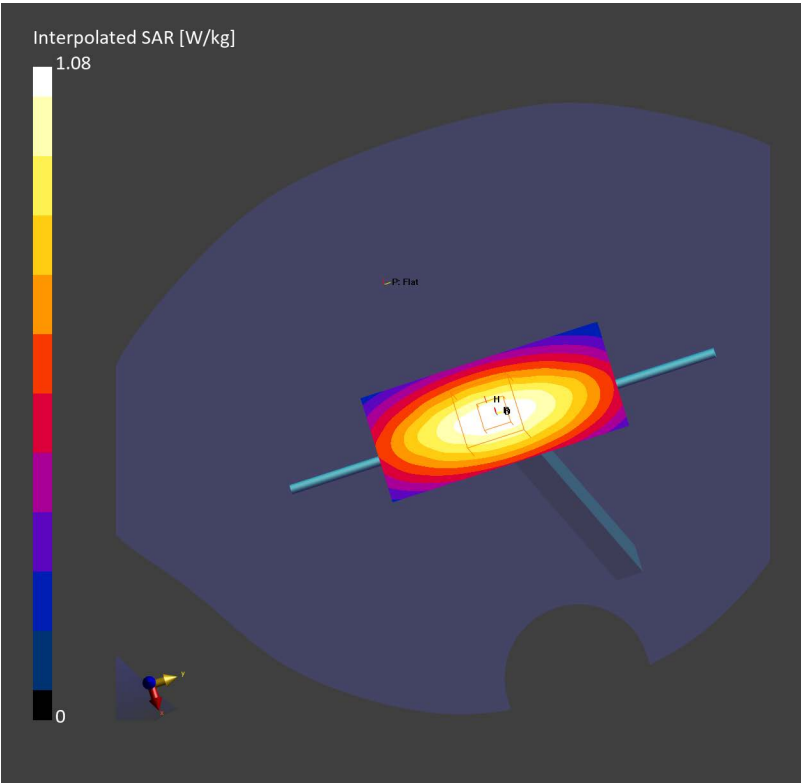

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D1750V2 – SN1115 | 1750.0          | HSL | 20.0        | −0.9        | −0.0         | 6.5           | 2.8            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 1750.000, 0                     | 8.11              | 1.36                   | 39.5             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2168 | HSL1750 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1846, 2024-12-10 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-22, 23:06 | 2025-01-22, 23:13 |
| psSAR1g [W/Kg]      | 3.64              | 3.65              |
| psSAR10g [W/Kg]     | 1.95              | 1.95              |
| Power Drift [dB]    | 0.00              | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

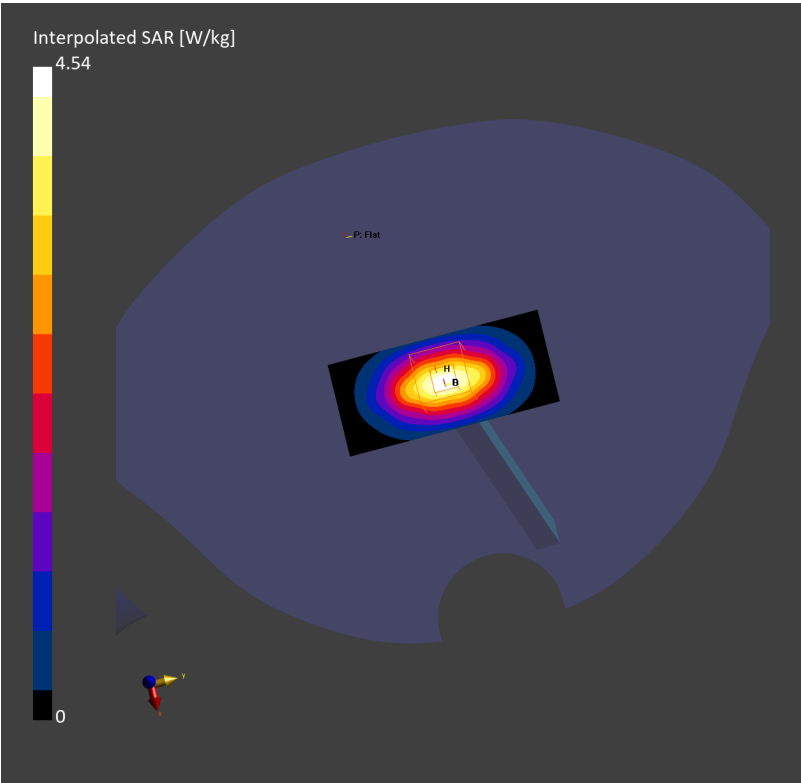

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D1750V2 – SN1115 | 1750.0          | HSL | 20.0        | −2.4        | −1.3         | 4.4           | 3.1            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 1750.000, 0                     | 8.11              | 1.35                   | 39.0             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL1750 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-10, 12:32 | 2025-02-10, 12:38 |
| psSAR1g [W/Kg]      | 3.52              | 3.59              |
| psSAR10g [W/Kg]     | 1.91              | 1.92              |
| Power Drift [dB]    | 0.01              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

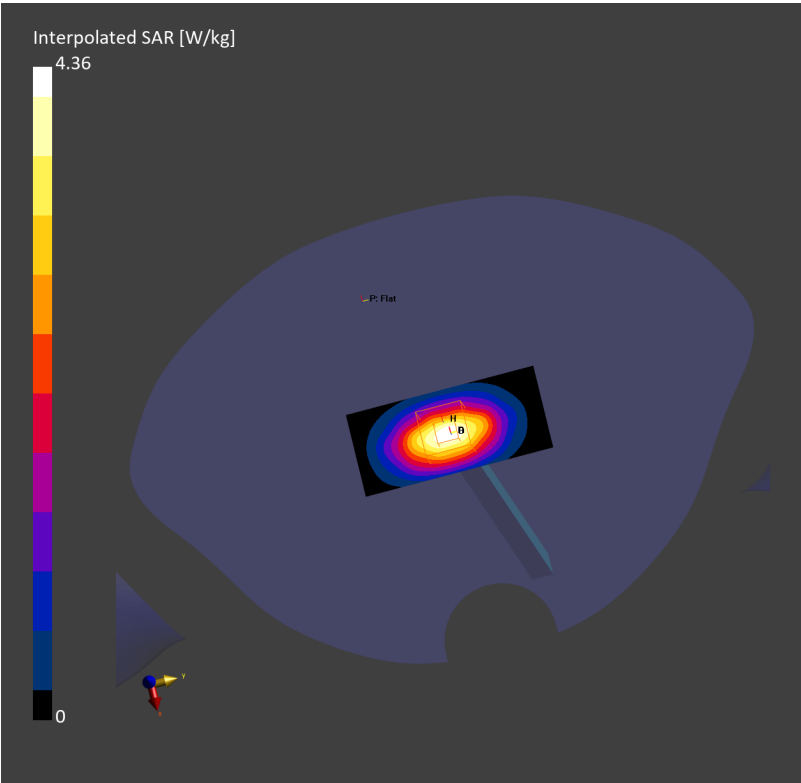

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D1750V2 – SN1115 | 1750.0          | HSL | 20.0        | −4.5        | −4.0         | 1.7           | 2.8            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 1750.000, 0                     | 8.11              | 1.36                   | 40.9             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL1750 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-13, 12:17 | 2025-02-13, 12:24 |
| psSAR1g [W/Kg]      | 3.51              | 3.49              |
| psSAR10g [W/Kg]     | 1.87              | 1.86              |
| Power Drift [dB]    | 0.00              | −0.03             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

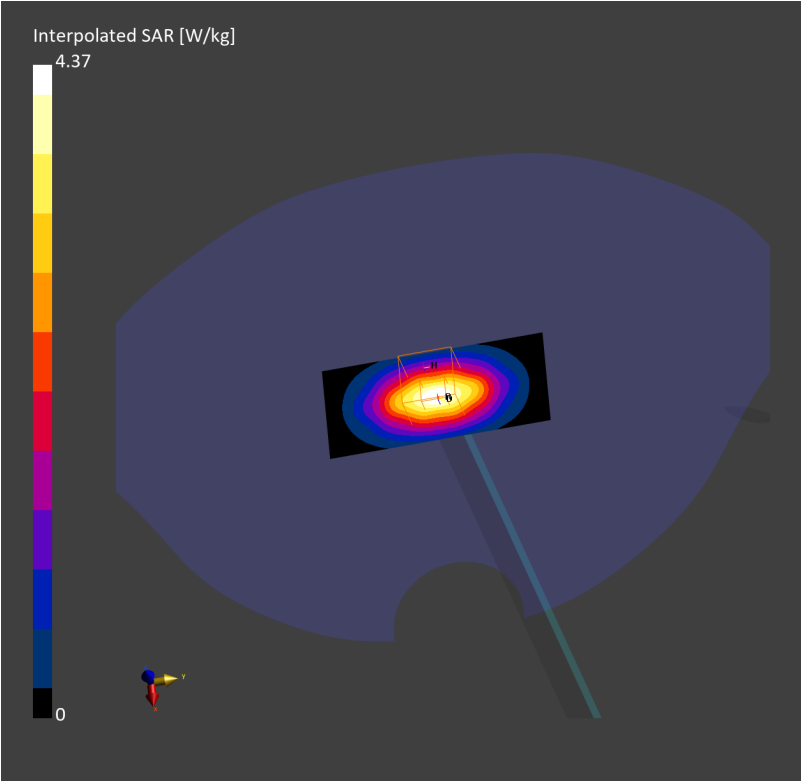

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D1750V2 – SN1115 | 1750.0          | HSL | 20.0        | −0.8        | −0.1         | 8.4           | −3.6           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 1750.000, 0                     | 8.11              | 1.36                   | 39.7             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL1750 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | All points  | All points         |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-04-14, 19:57 | 2025-04-14, 20:07 |
| psSAR1g [W/Kg]      | 3.65              | 3.66              |
| psSAR10g [W/Kg]     | 1.96              | 1.95              |
| Power Drift [dB]    | −0.04             | −0.04             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

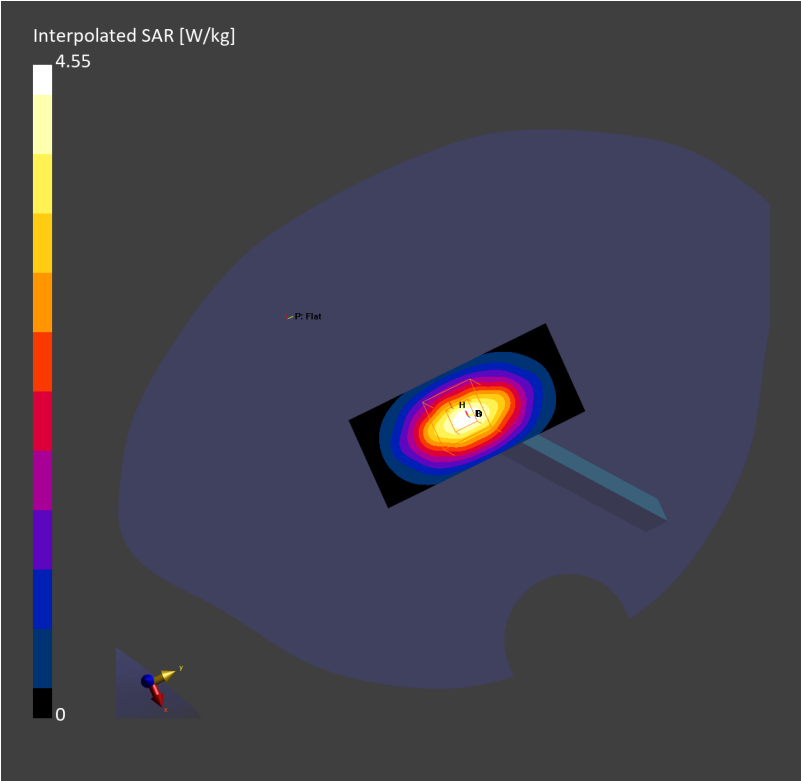

Summary

|                 |                 |     |             |             |              |               |                |
|-----------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole          | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D1900V2 – SN512 | 1900.0          | HSL | 20.0        | 6.3         | 5.7          | 14.9          | 2.7            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 1900.000, 0                     | 7.76              | 1.42                   | 40.3             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2168 | HSL1900 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1846, 2024-12-10 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-01-21, 07:23 | 2025-01-21, 07:30 |
| psSAR1g [W/Kg]      | 4.17              | 4.21              |
| psSAR10g [W/Kg]     | 2.15              | 2.17              |
| Power Drift [dB]    | -0.00             | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

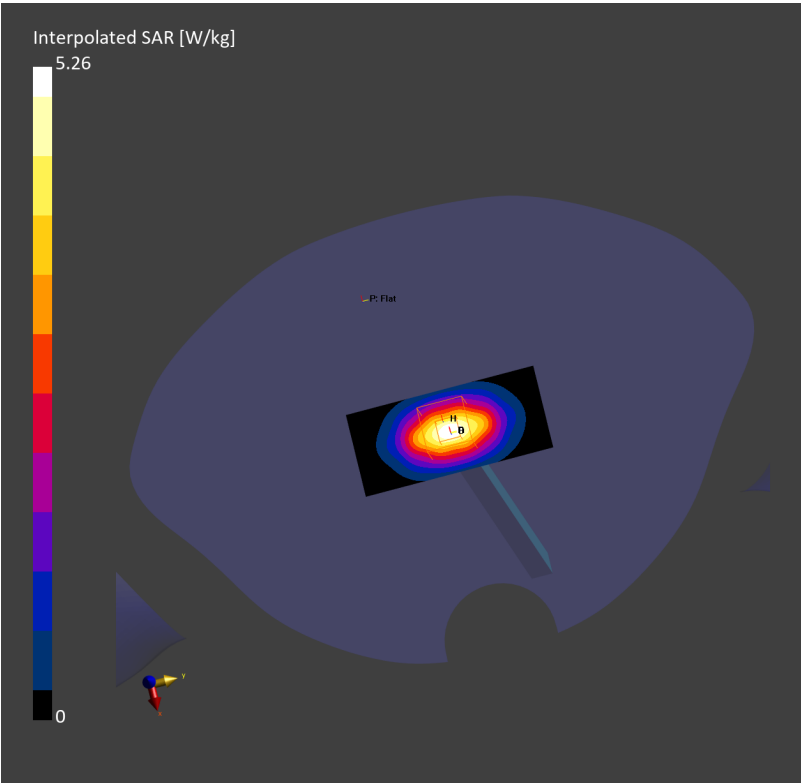

Summary

|                 |                 |     |             |             |              |               |                |
|-----------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole          | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D1900V2 – SN512 | 1900.0          | HSL | 20.0        | 0.3         | 0.2          | 7.4           | 5.2            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 1900.000, 0                     | 7.76              | 1.41                   | 40.2             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL1900 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-02-06, 09:27 | 2025-02-06, 09:33 |
| psSAR1g [W/Kg]      | 3.80              | 3.96              |
| psSAR10g [W/Kg]     | 2.02              | 2.06              |
| Power Drift [dB]    | 0.01              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

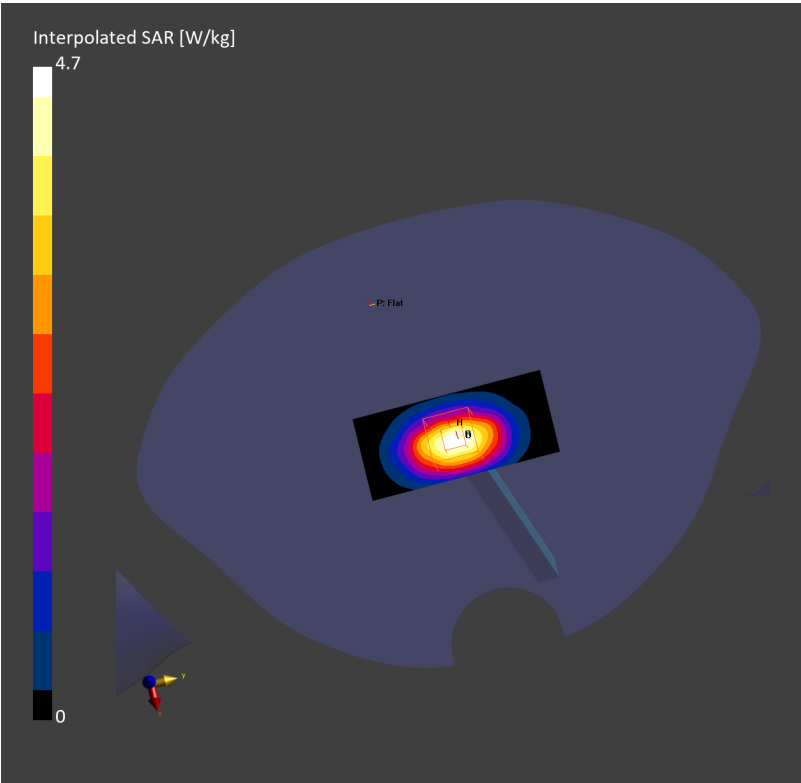

Summary

|                 |                 |     |             |             |              |               |                |
|-----------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole          | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D1900V2 – SN512 | 1900.0          | HSL | 20.0        | 2.7         | 1.9          | 10.2          | 2.7            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 1900.000, 0                     | 7.76              | 1.39                   | 39.3             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL1900 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 90.0 | 32.0 x 32.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 6.0 x 6.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-02-13, 12:49 | 2025-02-13, 12:56 |
| psSAR1g [W/Kg]      | 4.01              | 4.05              |
| psSAR10g [W/Kg]     | 2.07              | 2.09              |
| Power Drift [dB]    | 0.01              | -0.00             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

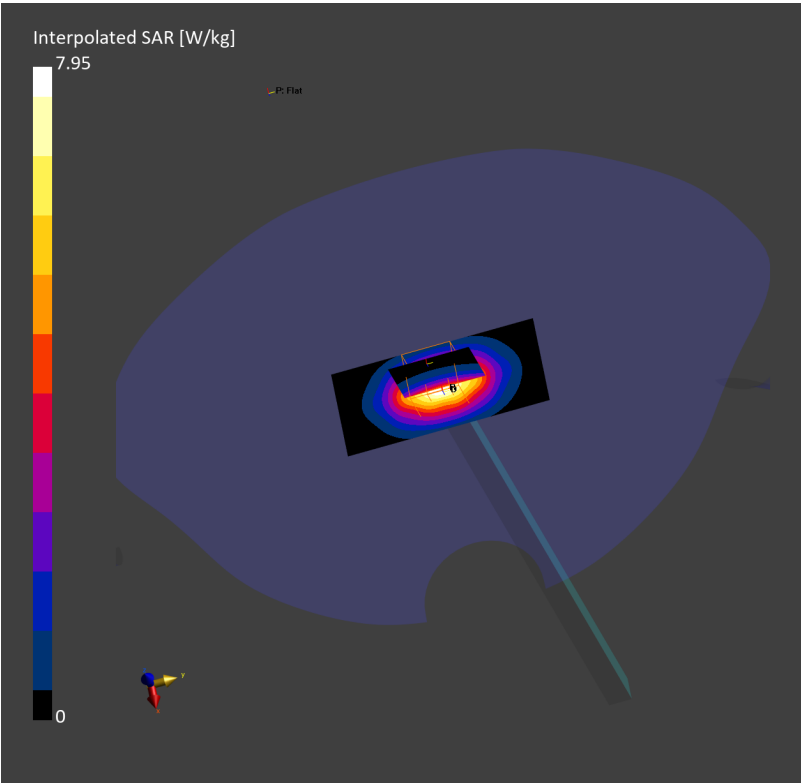

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D2450V2 – SN1099 | 2450.0          | HSL | 20.0        | 5.6         | 5.2          | 10.2          | 1.2            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 2450.000, 0                     | 7.27              | 1.76                   | 39.5             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2168 | HSL2450 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1846, 2024-12-10 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 96.0 | 30.0 x 30.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 12.0 | 5.0 x 5.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | All points  | All points         |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-15, 20:42 | 2025-01-15, 20:52 |
| psSAR1g [W/Kg]      | 5.43              | 5.36              |
| psSAR10g [W/Kg]     | 2.60              | 2.50              |
| Power Drift [dB]    | -0.18             | -0.11             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

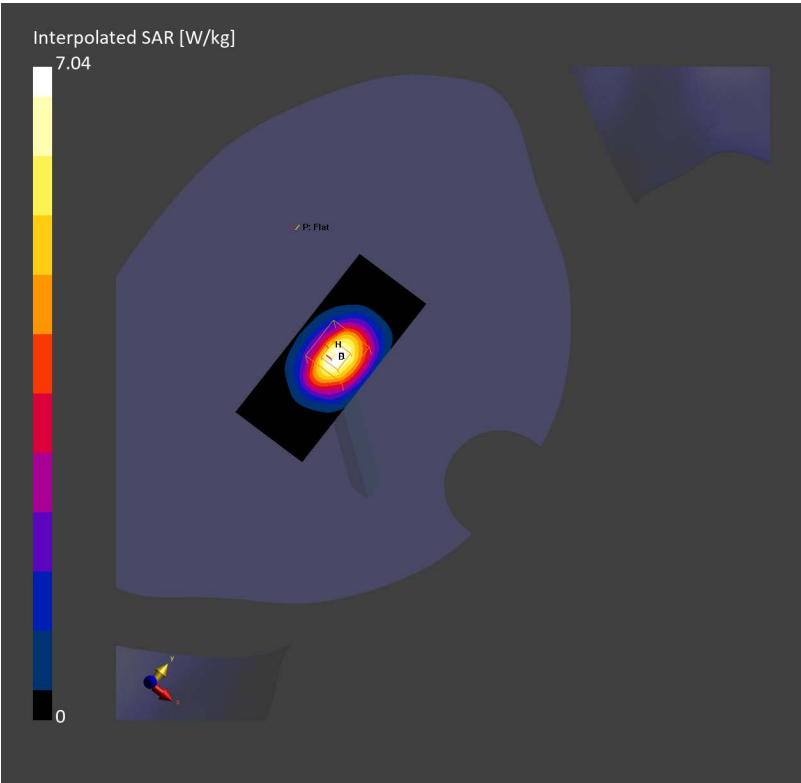

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D2600V2 – SN1094 | 2600.0          | HSL | 20.0        | −0.6        | 0.9          | 0.2           | 2.8            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 2600.000, 0                     | 7.09              | 1.94                   | 38.9             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL2600 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 96.0 | 30.0 x 30.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 12.0 | 5.0 x 5.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-22, 10:12 | 2025-01-22, 10:19 |
| psSAR1g [W/Kg]      | 5.59              | 5.57              |
| psSAR10g [W/Kg]     | 2.50              | 2.52              |
| Power Drift [dB]    | 0.00              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

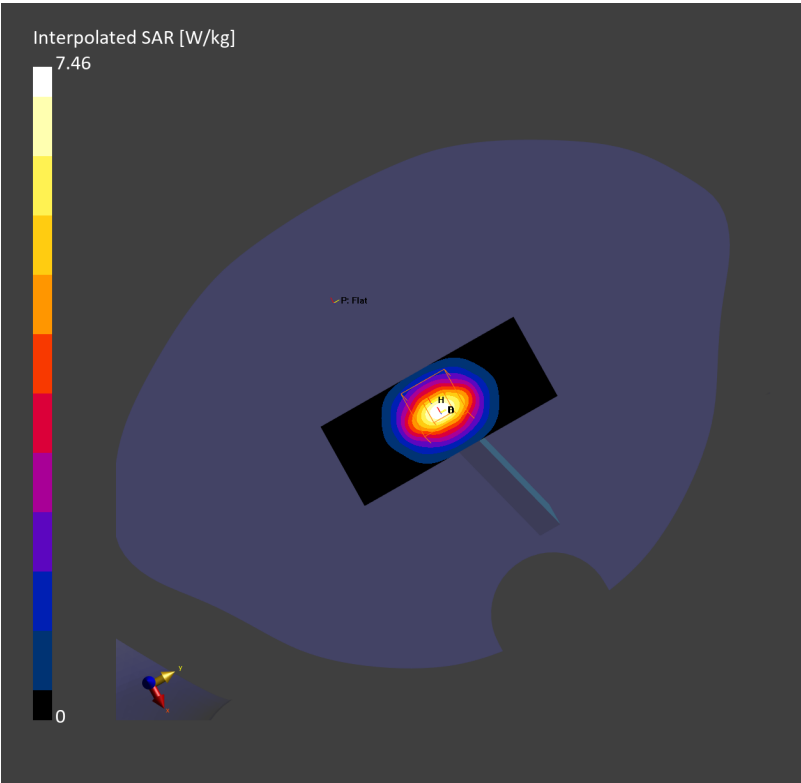

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D2600V2 – SN1094 | 2600.0          | HSL | 20.0        | 0.4         | 1.9          | 1.7           | –3.0           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 2600.000, 0                     | 7.09              | 1.96                   | 39.3             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL2600 | EX3DV4 – SN7812, 2024-06-25 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 96.0 | 30.0 x 30.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 12.0 | 5.0 x 5.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-09, 07:51 | 2025-02-09, 07:57 |
| psSAR1g [W/Kg]      | 5.62              | 5.63              |
| psSAR10g [W/Kg]     | 2.52              | 2.54              |
| Power Drift [dB]    | 0.01              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

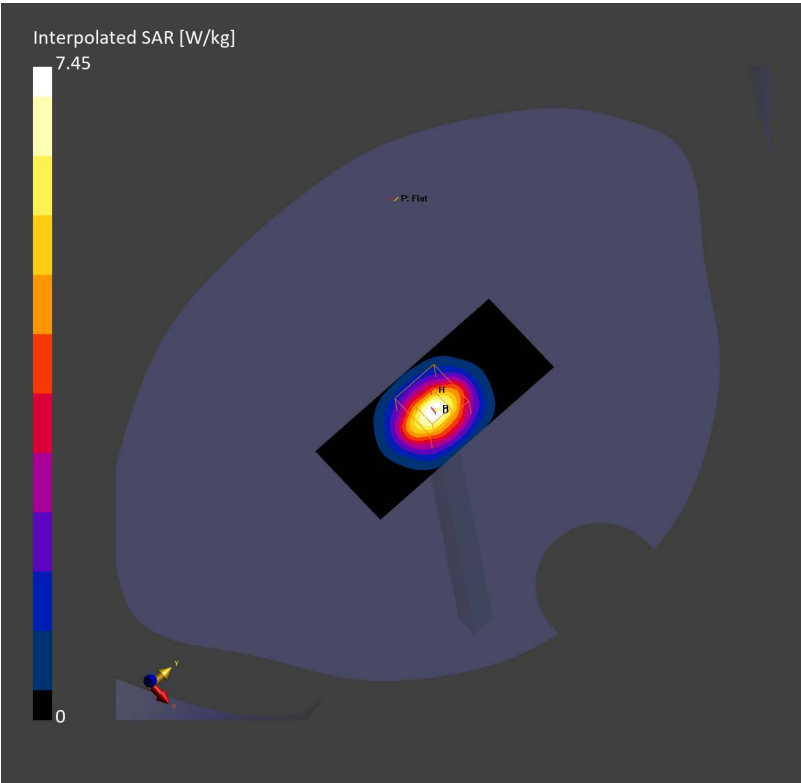

Test Laboratory: TOWE Lab

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D2600V2 – SN1094 | 2600.0          | HSL | 20.0        | 1.0         | 4.6          | –1.8          | –8.3           |

Exposure Conditions

| Phantom Section, TSL         | Test Distance [mm] | Band    | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|------------------------------|--------------------|---------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, Head Simulating Liquid | 10                 | CW, 0-- |            | 2600.000, 0                     | 7.45              | 2.02                   | 39.8             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2168 | HSL2600 | EX3DV4 – SN7758, 2024–09–12 | DAE4ip Sn1846, 2024–12–10 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 96.0 | 30.0 x 30.0 x 30.0 |
| Grid Steps [mm]     | 10.0 x 12.0 | 5.0 x 5.0 x 1.5    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025–03–04, 17:09 | 2025–03–04, 17:16 |
| psSAR1g [W/Kg]      | 5.15              | 5.73              |
| psSAR10g [W/Kg]     | 2.32              | 2.62              |
| Power Drift [dB]    | –0.02             | 0.03              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

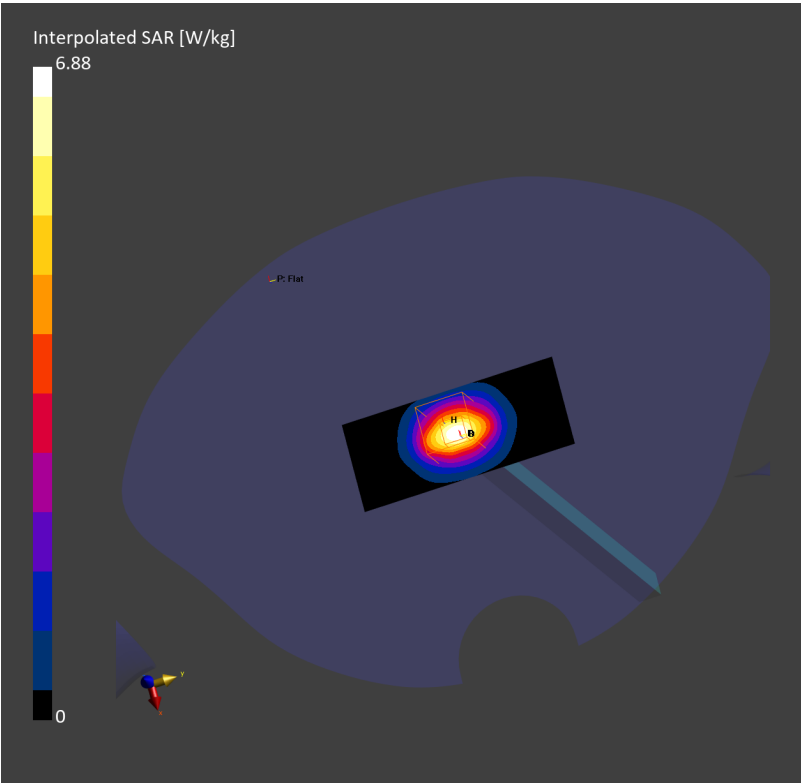

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3500V2 – SN1150 | 3500.0          | HSL | 20.0        | 3.7         | 5.4          | 4.1           | –1.9           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3500.000, 0                     | 6.89              | 2.88                   | 38.1             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3500 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-23, 18:07 | 2025-01-23, 18:12 |
| psSAR1g [W/Kg]      | 6.67              | 6.85              |
| psSAR10g [W/Kg]     | 2.49              | 2.64              |
| Power Drift [dB]    | –0.00             | –0.00             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

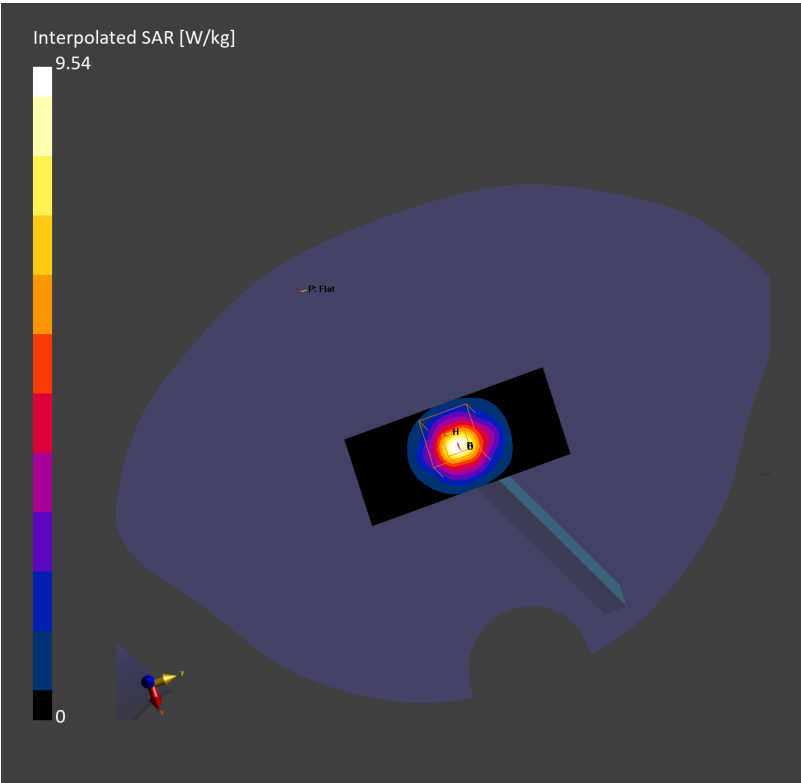

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3500V2 – SN1150 | 3500.0          | HSL | 20.0        | 2.5         | 3.9          | 3.4           | –1.2           |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3500.000, 0                     | 6.89              | 2.90                   | 38.6             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3500 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-08, 08:24 | 2025-02-08, 08:29 |
| psSAR1g [W/Kg]      | 6.60              | 6.77              |
| psSAR10g [W/Kg]     | 2.46              | 2.60              |
| Power Drift [dB]    | –0.00             | –0.02             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

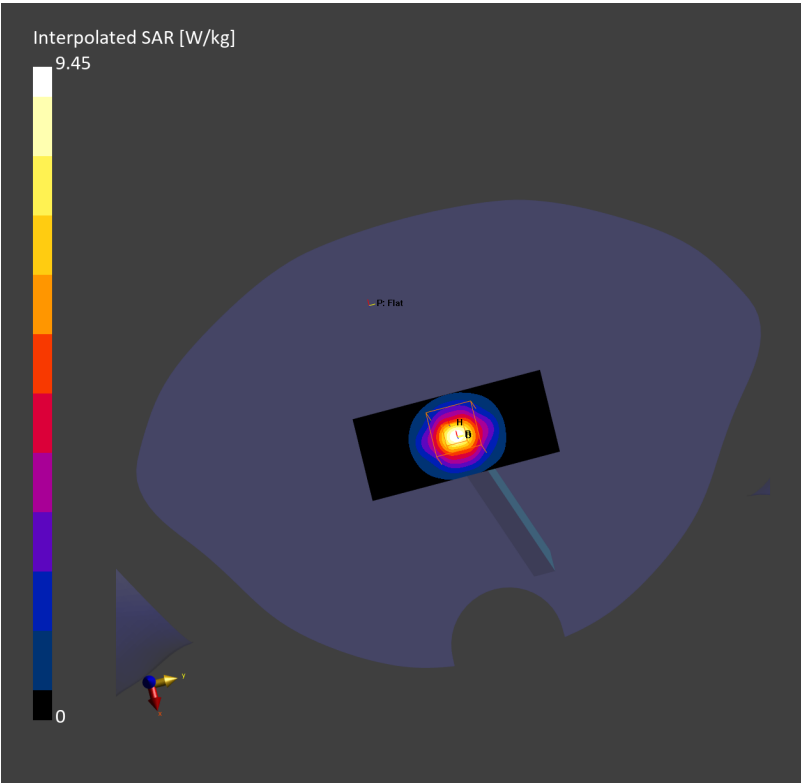

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3500V2 – SN1150 | 3500.0          | HSL | 20.0        | 4.9         | 6.5          | 4.7           | 2.6            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3500.000, 0                     | 6.85              | 2.92                   | 38.6             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3500 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-03-04, 14:51 | 2025-03-04, 14:56 |
| psSAR1g [W/Kg]      | 6.76              | 6.93              |
| psSAR10g [W/Kg]     | 2.51              | 2.66              |
| Power Drift [dB]    | 0.01              | -0.00             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

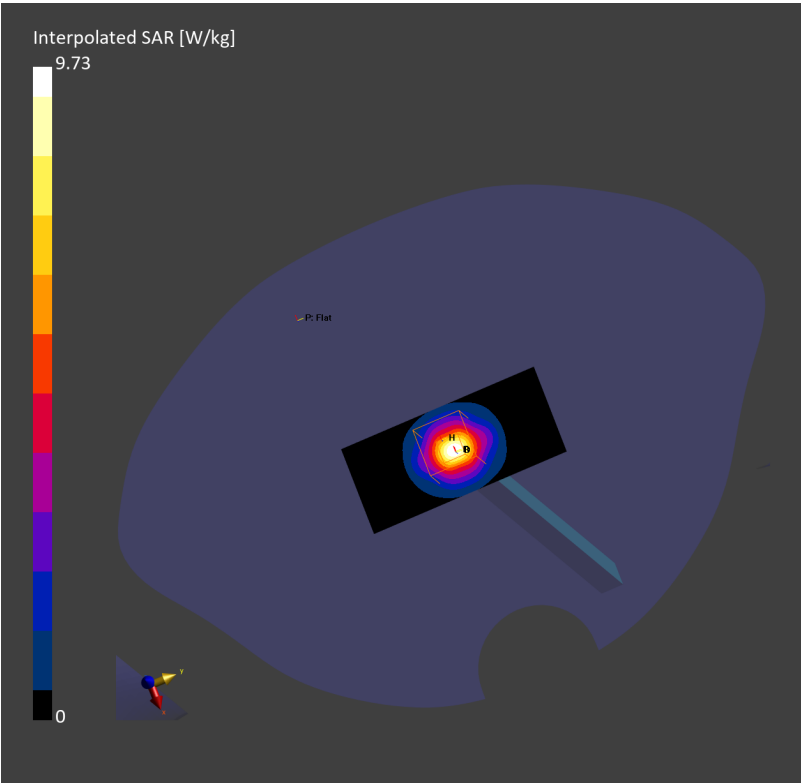

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3700V2 – SN1127 | 3700.0          | HSL | 20.0        | 2.0         | 5.3          | 1.4           | 2.5            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3700.000, 0                     | 6.67              | 3.09                   | 37.8             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3700 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-08, 16:32 | 2025-02-08, 16:37 |
| psSAR1g [W/Kg]      | 6.63              | 6.78              |
| psSAR10g [W/Kg]     | 2.38              | 2.53              |
| Power Drift [dB]    | 0.00              | -0.00             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

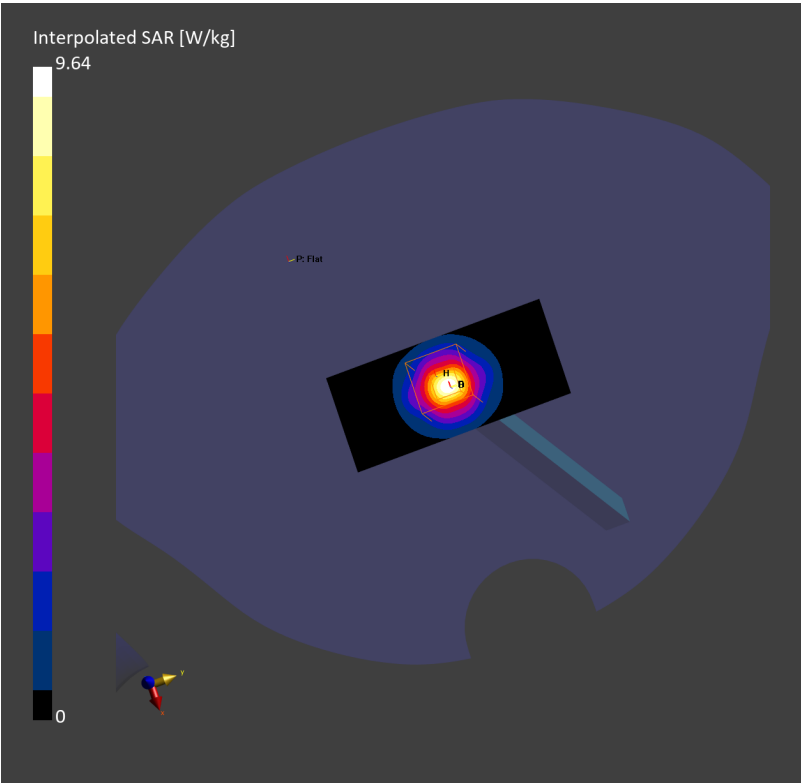

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3700V2 – SN1127 | 3700.0          | HSL | 20.0        | 4.0         | 6.9          | 1.6           | 2.5            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3700.000, 0                     | 6.67              | 3.00                   | 38.7             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3700 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-03-04, 23:30 | 2025-03-04, 23:36 |
| psSAR1g [W/Kg]      | 6.70              | 6.83              |
| psSAR10g [W/Kg]     | 2.41              | 2.56              |
| Power Drift [dB]    | 0.01              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

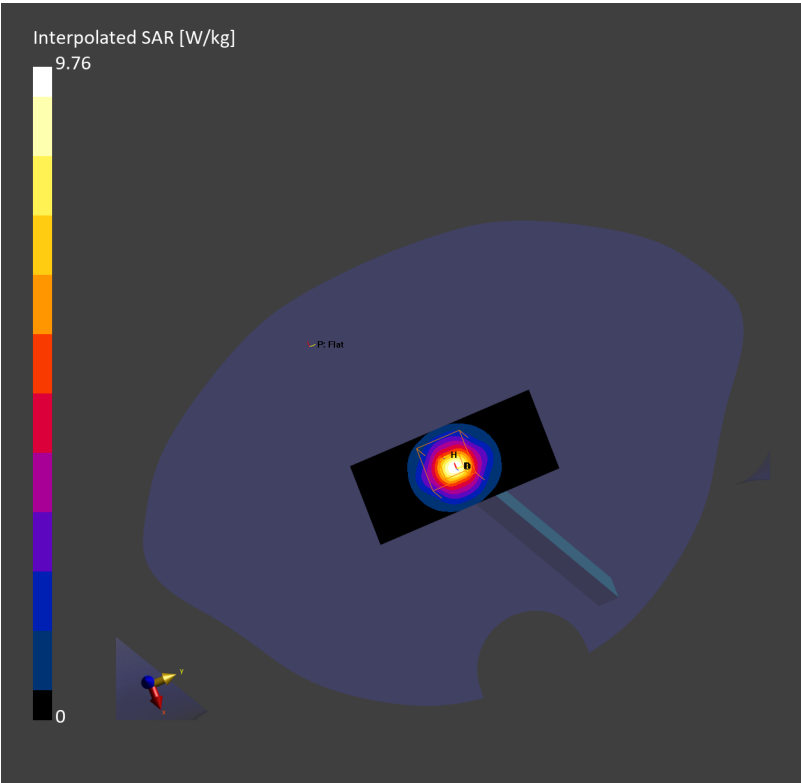

Summary

|                  |                 |     |             |             |              |               |                |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D3900V2 – SN1099 | 3900.0          | HSL | 20.0        | 6.1         | 9.0          | 4.9           | 2.6            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 3900.000, 0                     | 6.58              | 3.29                   | 37.5             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3900 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-01-24, 12:26 | 2025-01-24, 12:32 |
| psSAR1g [W/Kg]      | 7.06              | 7.24              |
| psSAR10g [W/Kg]     | 2.42              | 2.57              |
| Power Drift [dB]    | 0.00              | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

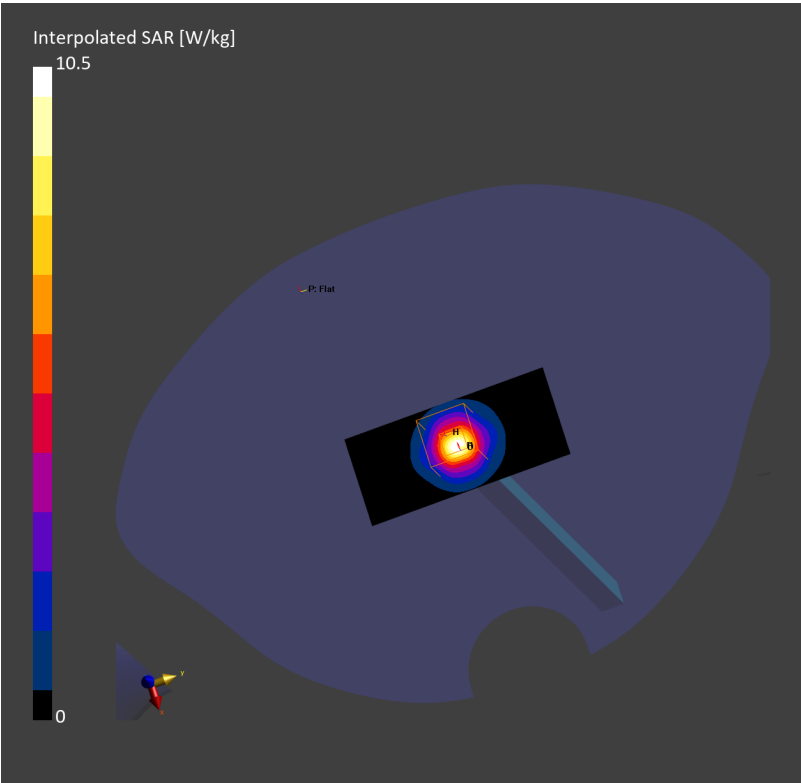

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3900V2 – SN1099 | 3900.0          | HSL | 20.0        | 0.8         | 3.7          | 2.6           | 1.5            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3900.000, 0                     | 6.58              | 3.31                   | 36.9             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3900 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-08, 12:24 | 2025-02-08, 12:29 |
| psSAR1g [W/Kg]      | 6.67              | 6.91              |
| psSAR10g [W/Kg]     | 2.29              | 2.46              |
| Power Drift [dB]    | -0.00             | -0.01             |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

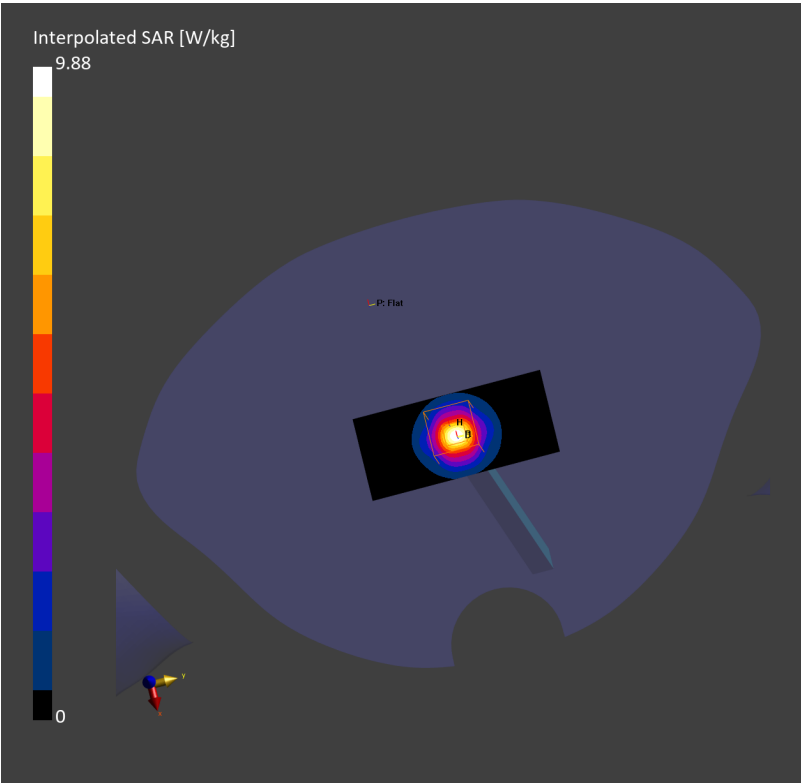

Test Laboratory: TOWE Lab

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D3900V2 – SN1099 | 3900.0          | HSL | 20.0        | 3.5         | 6.5          | 0.5           | 2.6            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 3900.000, 0                     | 6.65              | 3.24                   | 38.0             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL3900 | EX3DV4 – SN3624, 2025-01-15 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 90.0 | 24.0 x 24.0 x 24.0 |
| Grid Steps [mm]     | 10.0 x 15.0 | 5.0 x 5.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.5                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-03-06, 00:25 | 2025-03-06, 00:30 |
| psSAR1g [W/Kg]      | 6.56              | 7.03              |
| psSAR10g [W/Kg]     | 2.24              | 2.50              |
| Power Drift [dB]    | -0.00             | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

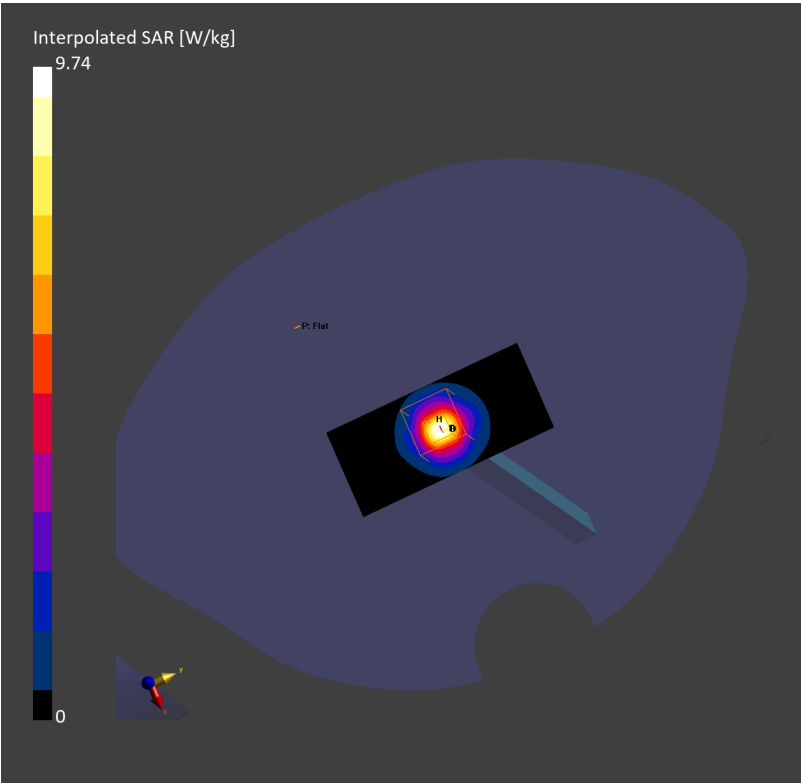

Summary

|                  |                 |     |             |             |              |               |                |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D5GHzV2 – SN1371 | 5200.0          | HSL | 20.0        | –2.9        | 1.0          | –2.7          | 2.3            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 5200.000, 0                     | 5.65              | 4.71                   | 36.2             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024–09–12 | DAE4ip Sn1847, 2024–12–31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025–01–18, 18:31 | 2025–01–18, 18:37 |
| psSAR1g [W/Kg]      | 7.04              | 7.65              |
| psSAR10g [W/Kg]     | 2.07              | 2.26              |
| Power Drift [dB]    | –0.02             | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

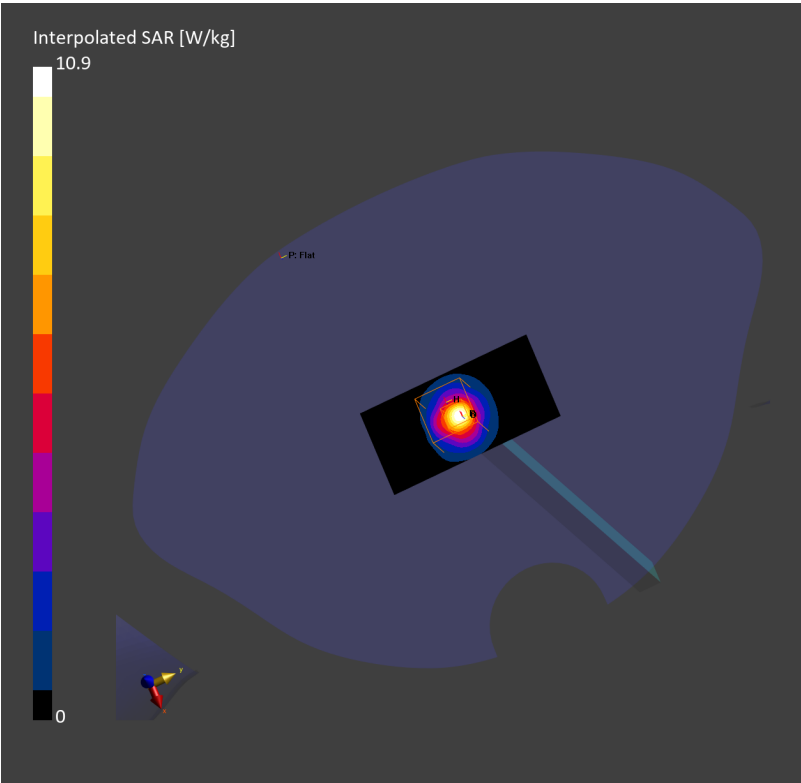

Summary

|                  |                 |     |             |             |              |               |                |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D5GHzV2 – SN1371 | 5200.0          | HSL | 20.0        | 0.8         | 3.1          | –2.5          | 1.3            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 5200.000, 0                     | 5.35              | 4.68                   | 37.0             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024–09–12 | DAE4ip Sn1847, 2024–12–31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025–02–11, 07:21 | 2025–02–11, 07:28 |
| psSAR1g [W/Kg]      | 7.57              | 7.91              |
| psSAR10g [W/Kg]     | 2.16              | 2.29              |
| Power Drift [dB]    | 0.03              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

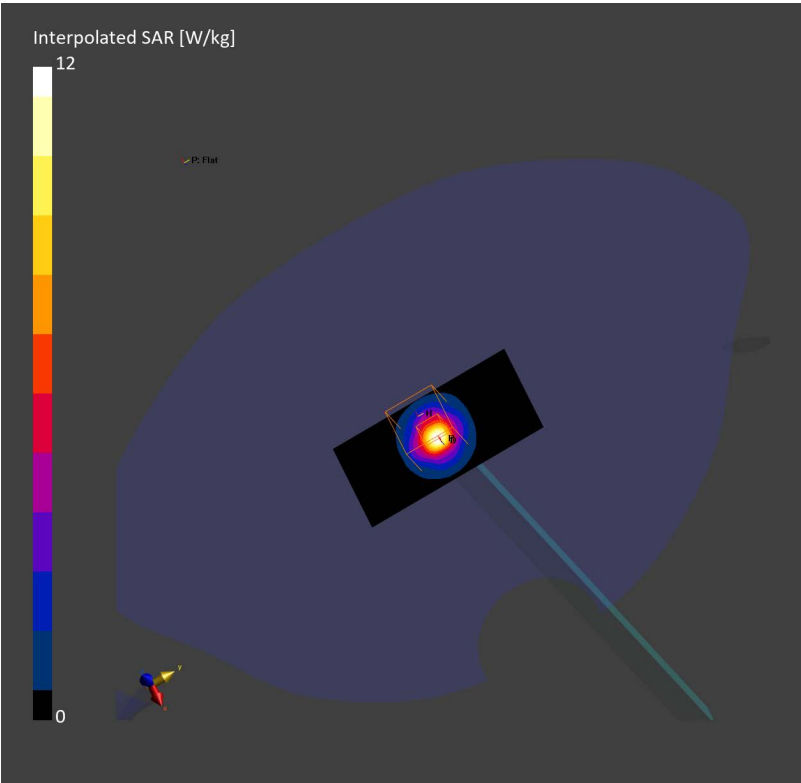

System Performance Check Report

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D5GHzV2 – SN1371 | 5600.0          | HSL | 20.0        | 6.7         | 7.6          | 8.3           | 2.2            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 5600.000, 0                     | 5.06              | 5.18                   | 35.2             |

Hardware Setup


| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024-09-12 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-01-19, 12:06 | 2025-01-19, 12:12 |
| psSAR1g [W/Kg]      | 8.31              | 8.79              |
| psSAR10g [W/Kg]     | 2.35              | 2.51              |
| Power Drift [dB]    | -0.00             | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

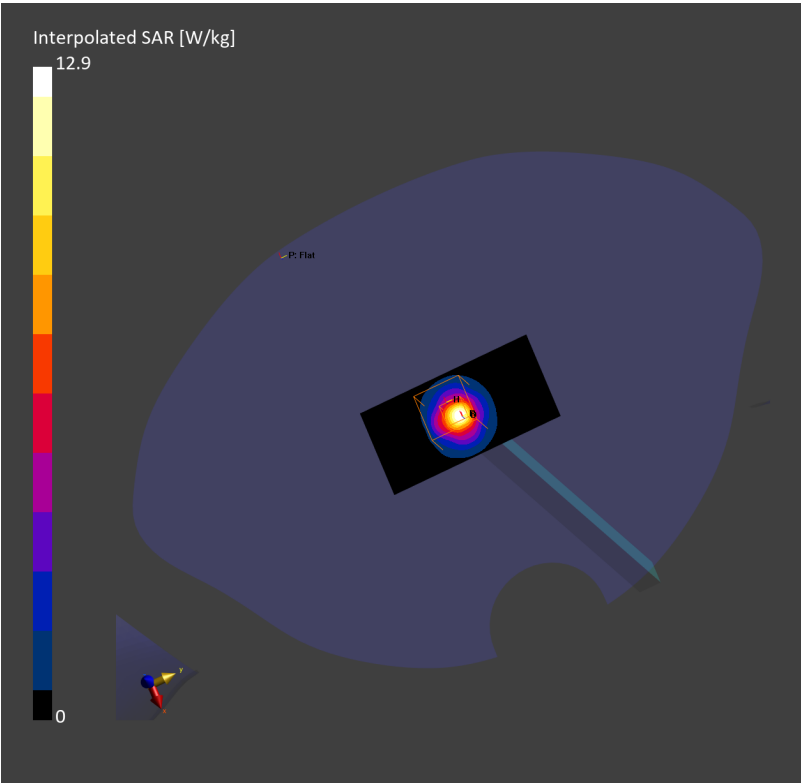

Summary

|                  |                 |     |             |             |              |               |                |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D5GHzV2 – SN1371 | 5600.0          | HSL | 20.0        | 4.4         | 5.2          | 2.9           | 1.3            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 5600.000, 0                     | 4.65              | 5.14                   | 36.0             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024-09-12 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-02-13, 01:45 | 2025-02-13, 01:51 |
| psSAR1g [W/Kg]      | 8.22              | 8.56              |
| psSAR10g [W/Kg]     | 2.30              | 2.44              |
| Power Drift [dB]    | 0.00              | 0.01              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

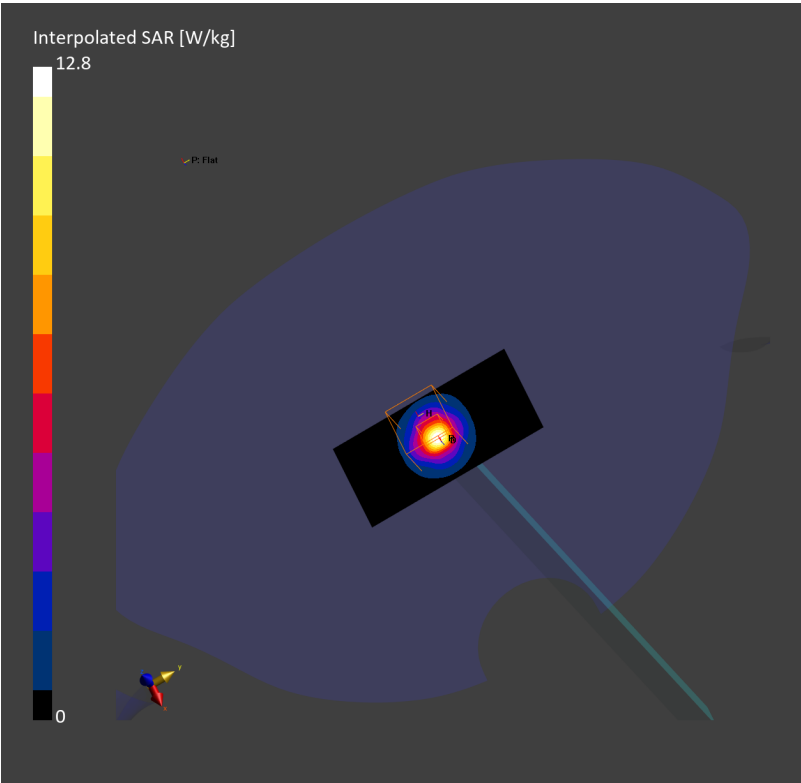

Summary

|                  |                 |     |             |             |              |               |                |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
| D5GHzV2 – SN1371 | 5800.0          | HSL | 20.0        | 3.2         | 5.0          | 4.8           | 2.7            |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat, HSL            | 10                 |      | CW, 0--    | 5800.000, 0                     | 5.03              | 5.45                   | 35.1             |

Hardware Setup


|                                         |         |                             |                           |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024-09-12 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     |             |                    |
|---------------------|-------------|--------------------|
|                     | Area Scan   | Zoom Scan          |
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     |                   |                   |
|---------------------|-------------------|-------------------|
|                     | Area Scan         | Zoom Scan         |
| Date                | 2025-01-19, 08:17 | 2025-01-19, 08:23 |
| psSAR1g [W/Kg]      | 7.73              | 8.23              |
| psSAR10g [W/Kg]     | 2.21              | 2.35              |
| Power Drift [dB]    | 0.00              | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

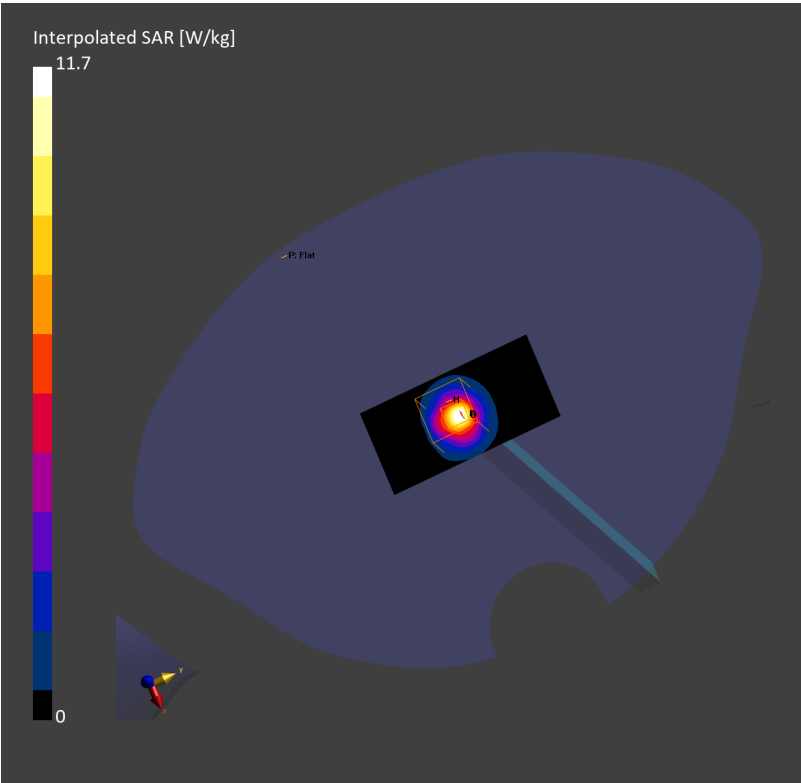

Summary

| Dipole           | Frequency [MHz] | TSL | Power [dBm] | Dev. 1g [%] | Dev. 10g [%] | Dev. Peak [%] | Iso. Error [%] |
|------------------|-----------------|-----|-------------|-------------|--------------|---------------|----------------|
| D5GHzV2 – SN1371 | 5800.0          | HSL | 20.0        | −4.7        | −3.3         | −5.8          | 1.4            |

Exposure Conditions

| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Flat, HSL            | 10                 |      | CW, 0--    | 5800.000, 0                     | 4.81              | 5.41                   | 35.9             |

Hardware Setup

| Phantom                                 | TSL     | Probe, Calibration Date     | DAE, Calibration Date     |
|-----------------------------------------|---------|-----------------------------|---------------------------|
| Twin-SAM V8.0 (30deg probe tilt) – 2173 | HSL5GHz | EX3DV4 – SN7758, 2024-09-12 | DAE4ip Sn1847, 2024-12-31 |

Scans Setup

|                     | Area Scan   | Zoom Scan          |
|---------------------|-------------|--------------------|
| Grid Extents [mm]   | 40.0 x 80.0 | 24.0 x 24.0 x 22.0 |
| Grid Steps [mm]     | 10.0 x 10.0 | 4.0 x 4.0 x 1.4    |
| Sensor Surface [mm] | 3.0         | 1.4                |
| Graded Grid         | N/A         | Yes                |
| Grading Ratio       | N/A         | 1.4                |
| MAIA                | N/A         | N/A                |
| Surface Detection   | VMS + 6p    | VMS + 6p           |
| Scan Method         | Measured    | Measured           |

Measurement Results

|                     | Area Scan         | Zoom Scan         |
|---------------------|-------------------|-------------------|
| Date                | 2025-02-11, 08:19 | 2025-02-11, 08:25 |
| psSAR1g [W/Kg]      | 7.27              | 7.57              |
| psSAR10g [W/Kg]     | 2.03              | 2.15              |
| Power Drift [dB]    | 0.00              | 0.00              |
| Power Scaling       | Disabled          | Disabled          |
| Scaling Factor [dB] |                   |                   |
| TSL Correction      | No correction     | No correction     |

