


Appendix A: Measurement Plots


Symbol Spectrum24 FH:

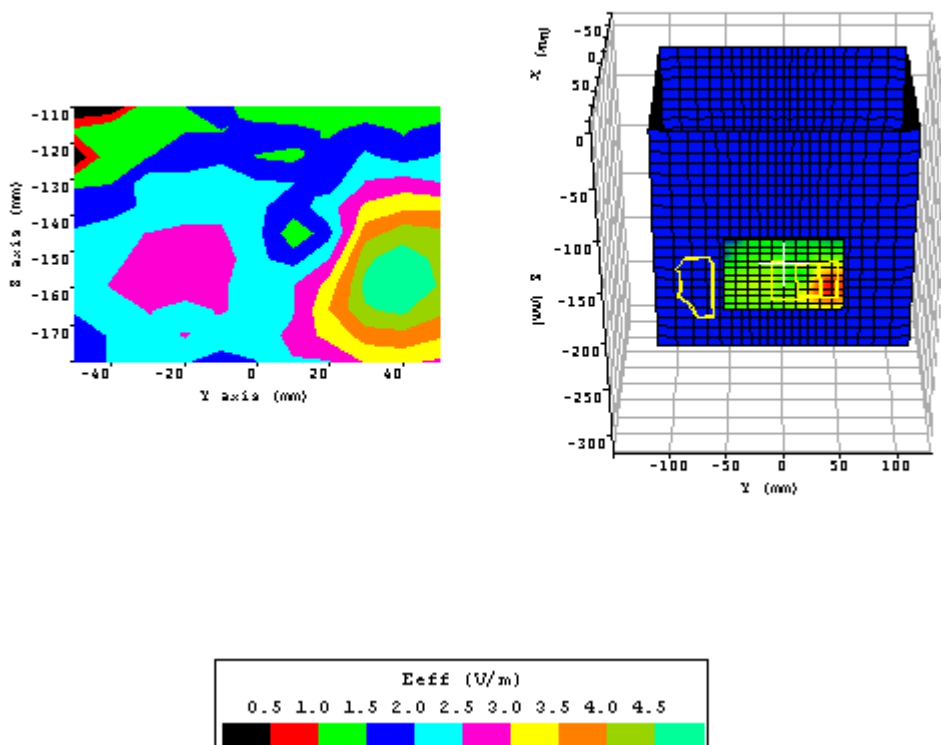

Plot 1.		
Date:	04/14/2003	
Temperature Air / Liquid:	21.0°C / 21.0°C	
Liquid mass density (ρ):	1	
DCP ¹	20	
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386	
Probe S/N:0123 liquid/air conversion Factor	0.816	
Simulated tissue dielectric parameters:	ϵ_r : 51.72	σ : 1.968
Test Position	bystander 1 cm	
Device Frequency	2440 MHz	
Maximum 1 gram SAR:	0.071W/Kg	
Maximum 10 gram SAR:	0.037/Kg	
Power reference start:	0.012W/Kg	
Power reference end	0.012W/Kg	
Power reference change ²	-0.00%	

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

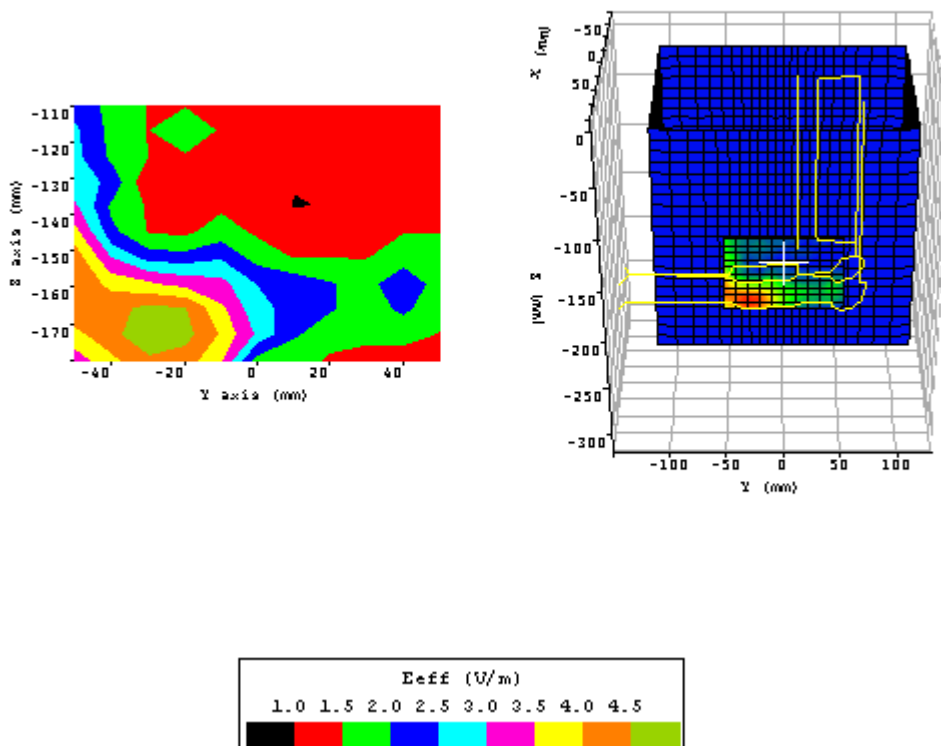

Plot 2.		
Date:	04/14/2003	
Temperature Air / Liquid:	21.0°C / 21.0°C	
Liquid mass density (ρ):	1	
DCP ¹	20	
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386	
Probe S/N:0123 liquid/air conversion Factor	0.816	
Simulated tissue dielectric parameters:	ϵ_r : 51.72	σ : 1.968
Test Position	lap	
Device Frequency	2440 MHz	
Maximum 1 gram SAR:	0.076W/Kg	
Maximum 10 gram SAR:	0.039/Kg	
Power reference start:	0.012W/Kg	
Power reference end	0.012W/Kg	
Power reference change ²	-0.00%	

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

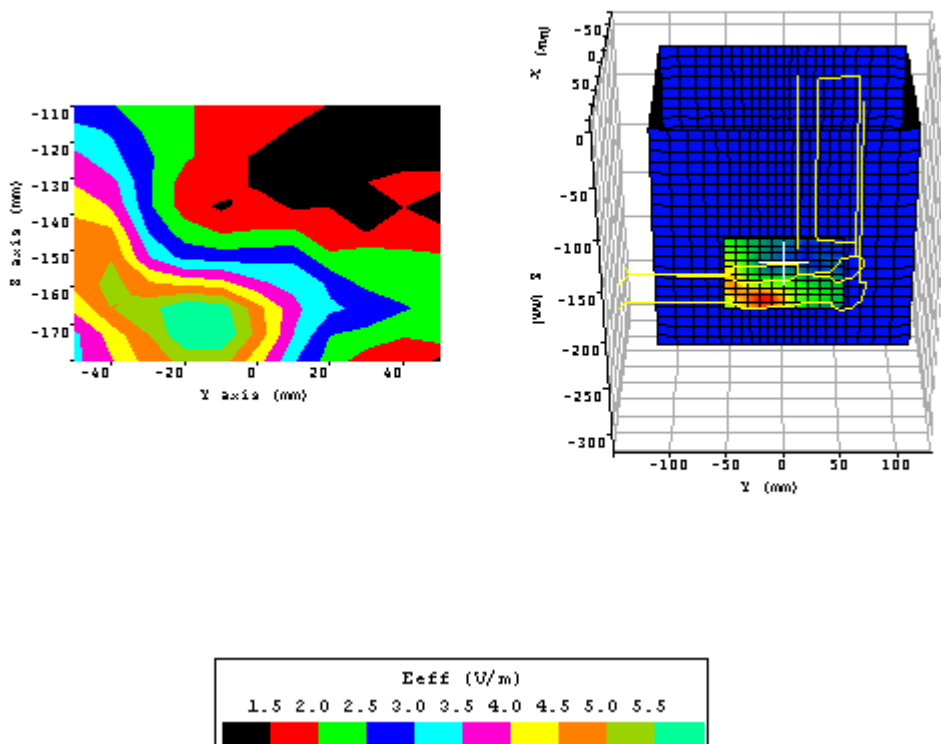

Plot 3.		
Date:	04/14/2003	
Temperature Air / Liquid:	21.0°C / 21.0°C	
Liquid mass density (ρ):	1	
DCP ¹	20	
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386	
Probe S/N:0123 liquid/air conversion Factor	0.816	
Simulated tissue dielectric parameters:	ϵ_r : 51.01	σ : 1.948
Test Position	lap	
Device Frequency	2402 MHz	
Maximum 1 gram SAR:	0.111W/Kg	
Maximum 10 gram SAR:	0.055/Kg	
Power reference start:	0.020W/Kg	
Power reference end	0.020W/Kg	
Power reference change ²	-0.00%	

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

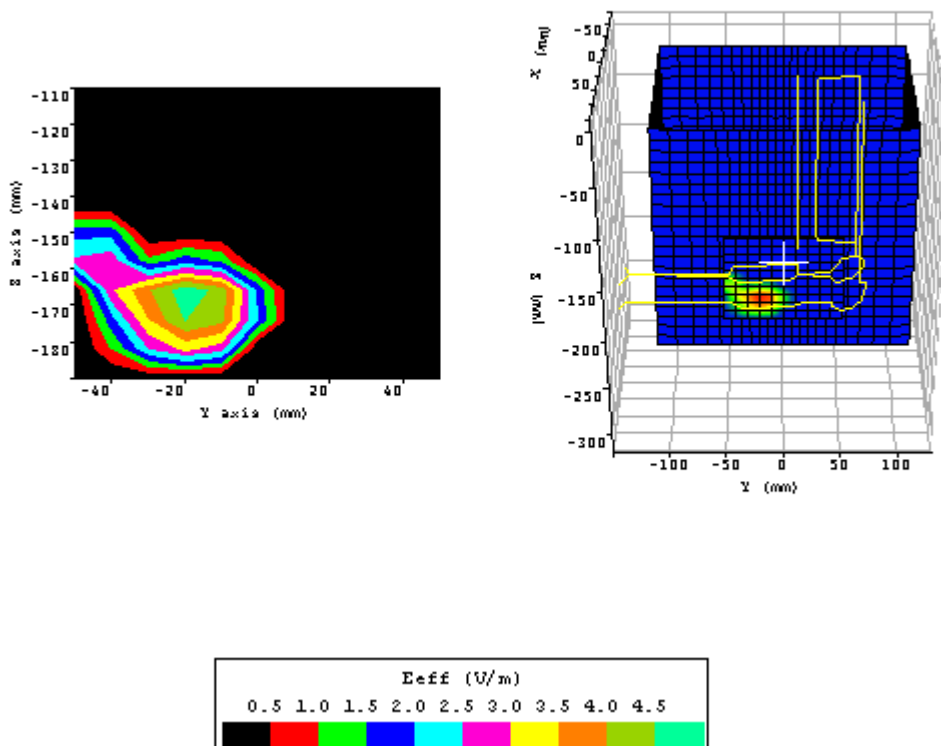

Plot 4.		
Date:	04/14/2003	
Temperature Air / Liquid:	21.0°C / 21.0°C	
Liquid mass density (ρ):	1	
DCP ¹	20	
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386	
Probe S/N:0123 liquid/air conversion Factor	0.816	
Simulated tissue dielectric parameters:	ϵ_r : 51.84	σ : 1.971
Test Position	lap	
Device Frequency	2480 MHz	
Maximum 1 gram SAR:	0.094W/Kg	
Maximum 10 gram SAR:	0.036/Kg	
Power reference start:	0.010W/Kg	
Power reference end	0.010W/Kg	
Power reference change ²	-0.00%	

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.