

ANTENNA TEST REPORT

Test Place

Company Name	UL Japan, Inc. Ise EMC Lab.
Address	4383-326 Asama-cho, Ise-shi, Mie-ken 516-0021 Japan
Telephone Number	+81-596-24-8999

Equipment Under Test (EUT)


Description	Blood Pressure Monitor
Manufacturer	OMRON HEALTHCARE Co. Ltd.
Model Number	HEM-7188T1
Frequency of Operation	2402 MHz to 2480 MHz
Antenna Type	Pattern Antenna

Test Procedure


Test configuration	EUT was placed on a platform of nominal size, 0.5 m by 0.5 m, raised 1.5 m above the conducting ground plane. The measurements were performed for both vertical and horizontal antenna polarization with the Spectrum Analyzer. The setup are shown in Figure 1.
Test procedure	Step 1 The tests have been measured in semi anechoic chamber at the distance of 3 m between the Substitution Antenna and the measuring Antenna, both Antennas were placed for the height 1.5 m. The Substitution Antenna has been connected to the Signal Generator. Step 2 The output power of the Signal Generator was setting value calculated by compensating the finite difference in the Antenna gain of Substitution Antenna. Step 3 The electric field strength at the distance of 3 m is received via the measurement antenna, and the reference value at that time is measured with a spectrum analyzer. Step 4 The measurements were performed for both vertical and horizontal antenna polarization. Step 5 Exchanged the Substitution Antenna to the EUT, the output power of the Signal Generator was setting value calculated by 0 dBm at the input of EUT. Step 6 The EUT was rotated a full revolution and recorded the electric field strength for each degree. Step 7 Calculate and record the difference from the value recorded in Step 6 to the value recorded in Step 3. Step 8 The measurement in steps 5 to 7 repeated with both vertical and horizontal antenna polarization, each position of XY, YZ and ZX-plane of EUT.

Figure 1: Test Setup

Setup for step 1 to 4

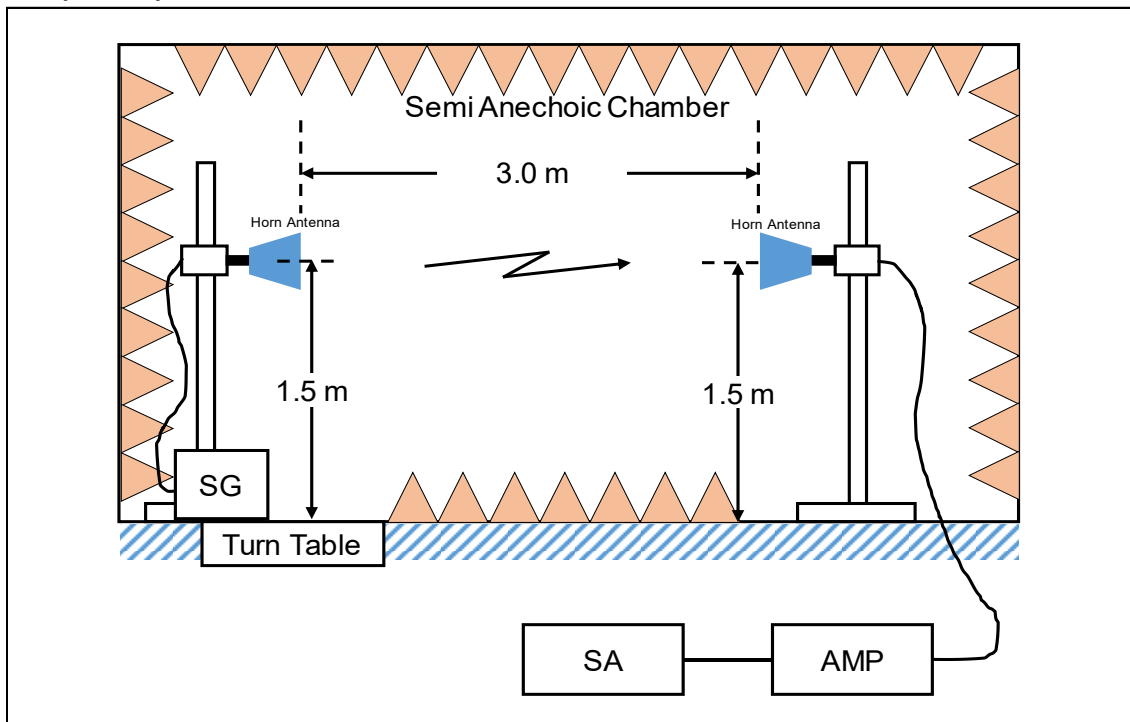

Setup after step 5

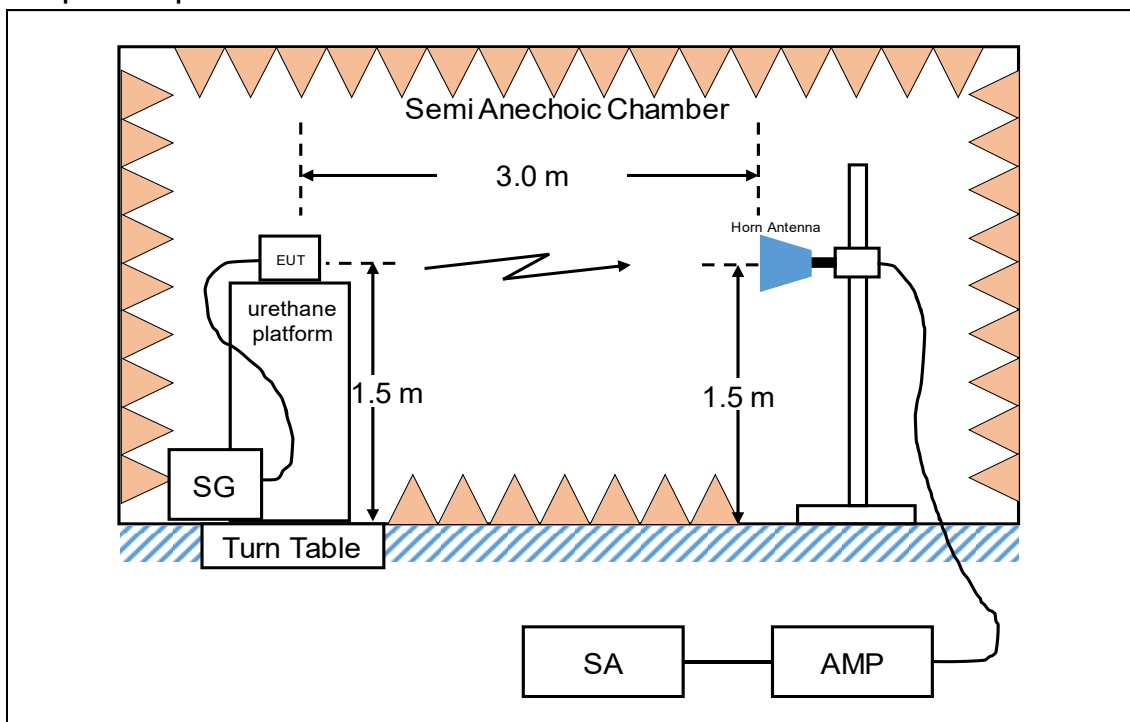

SG: Signal Generator
SA: Spectrum Analyzer
AMP: Pre Amplifier

Test Data

Antenna Pattern and Gain


Test place
Semi Anechoic Chamber
Date
Temperature / Humidity
Engineer

Ise EMC Lab.
No.2
September 27, 2024
22 deg. C / 69 % RH
Takafumi Noguchi


Antenna pattern (Top view)

2402MHz


XY-plane
Gain [dBi]

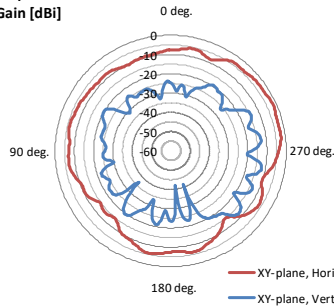

YZ-plane
Gain [dBi]

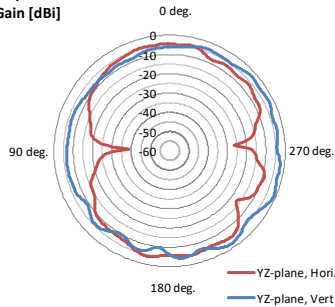


ZX-plane
Gain [dBi]

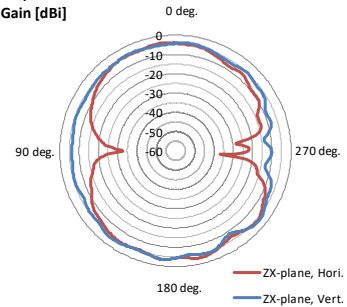


2440MHz


XY-plane
Gain [dBi]

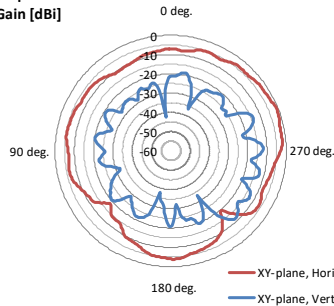

YZ-plane
Gain [dBi]

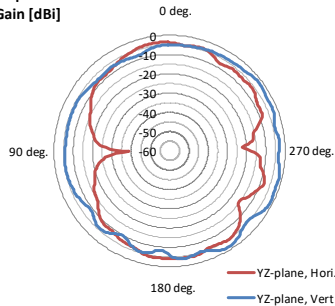


ZX-plane
Gain [dBi]

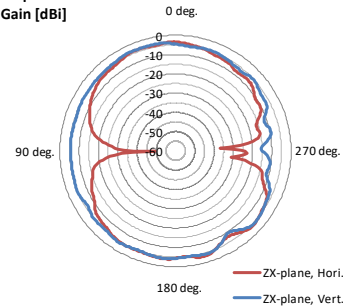


2480MHz


XY-plane
Gain [dBi]

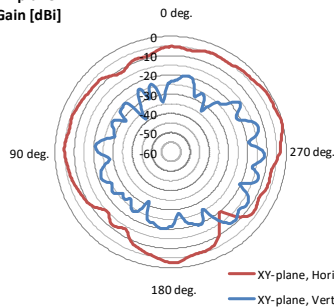

YZ-plane
Gain [dBi]

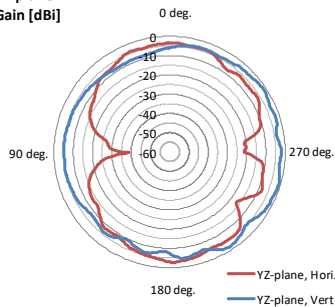

ZX-plane
Gain [dBi]

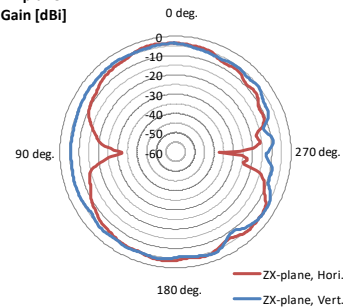

Antenna gain [UNIT: dBi]

Peak

Frequency [MHz]	2402.0	2440.0	2480.0
Peak gain	-1.21	-0.81	-0.43

Hori. : Horizontal
Vert. : Vertical

Average*

Frequency [MHz]		2402.0	2440.0	2480.0
XY-plane	Hori.	-6.62	-6.07	-5.67
	Vert.	-19.59	-19.38	-18.85
	Avg (H/V)	-9.42	-8.89	-8.48
YZ-plane	Hori.	-7.86	-7.48	-7.26
	Vert.	-5.04	-4.49	-4.49
	Avg (H/V)	-6.23	-5.73	-5.66
ZX-plane	Hori.	-6.86	-6.83	-6.73
	Vert.	-5.53	-5.52	-5.45
	Avg (H/V)	-6.14	-6.12	-6.04
Total		-7.02	-6.71	-6.56

*Result of averaging the true value of the value of each degree of angle.

Test Instruments

Test Equipment

Test Item	LIMS ID	Description	Manufacturer	Model	Serial	Last Calibration Date	Cal Int
APG	142004	AC2_Semi Anechoic Chamber(NSA)	TDK	Semi Anechoic Chamber 3m	DA-06902	2023/12/12	24
APG	244707	Thermo-Hygrometer	HIOKI E.E. CORPORATION	LR5001	231202102	2024/01/25	12
APG	142228	Measure, Tape, Steel	KOMELON	KMC-36	-	-	-
APG	141902	Spectrum Analyzer	Keysight Technologies Inc	E4440A	MY46187105	2024/05/30	12
APG	252663	Microwave Cable	Huber+Suhner	SF126E/11PC35/11 PC35/1000MM,5000 MM	616276/126E / 616275/126E	2024/09/10	12
APG	141580	MicroWave System Amplifier	Keysight Technologies Inc	83017A	MY39500779	2024/03/08	12
APG	141512	Horn Antenna 1-18GHz	Schwarzbeck Mess-Elektronik OHG	BBHA9120D	254	2023/10/17	12
APG	141898	Signal Generator	Keysight Technologies Inc	N5182B	MY56200177	2023/11/16	12
APG	197219	Microwave cable	Huber+Suhner	SF126E/11PC35/11 PC35/2000MM	536999/126E	2024/03/19	12
APG	141514	Horn Antenna 1-18GHz	Schwarzbeck Mess-Elektronik OHG	BBHA9120D	01611	2024/06/25	12

***Hyphens for Last Calibration Date and Cal Int (month) are instruments that Calibration is not required (e.g. software), or instruments checked in advance before use.**

The expiration date of the calibration is the end of the expired month.

As for some calibrations performed after the tested dates, those test equipment have been controlled by means of an unbroken chains of calibrations.

All equipment is calibrated with valid calibrations. Each measurement data is traceable to the national or international standards.

Test item: APG: Antenna Pattern and Gain