

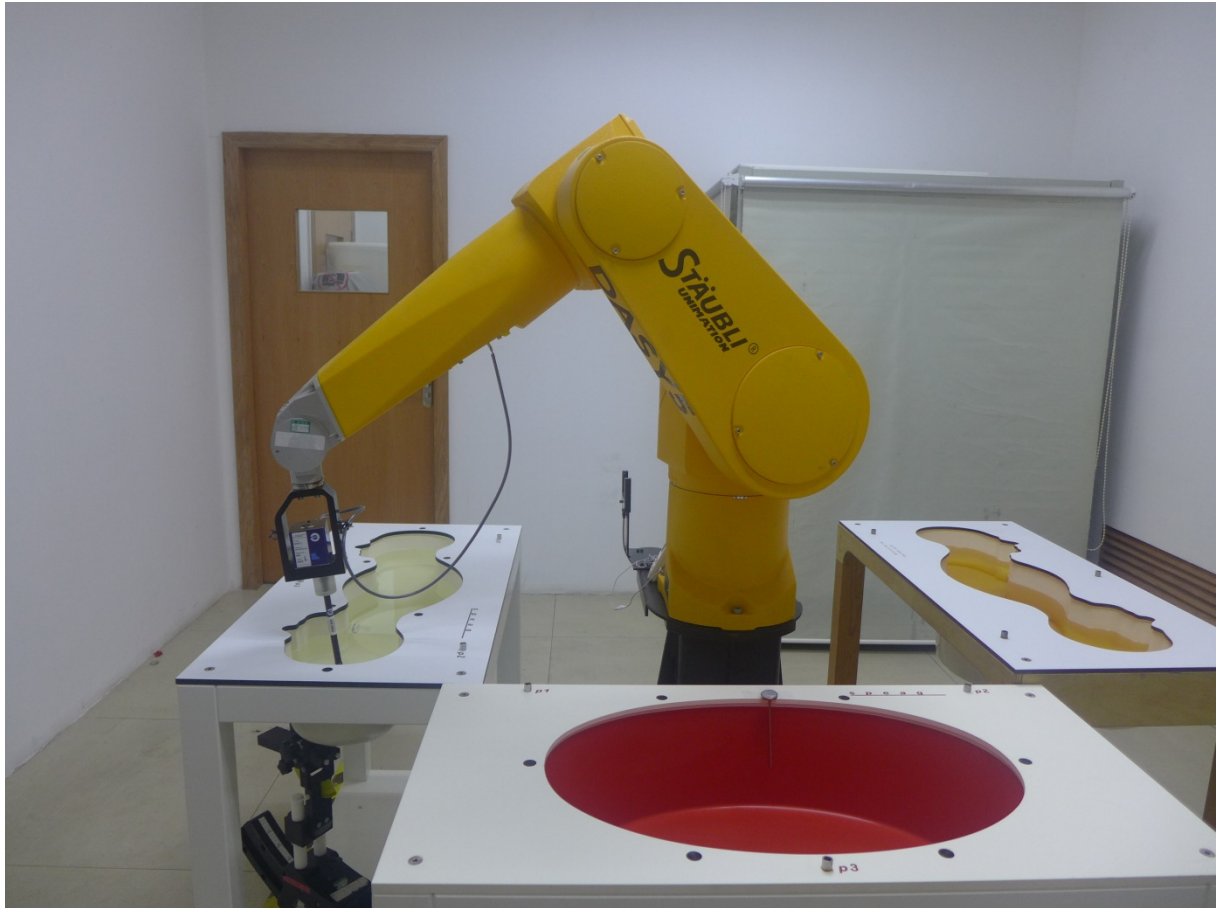


Appendix D

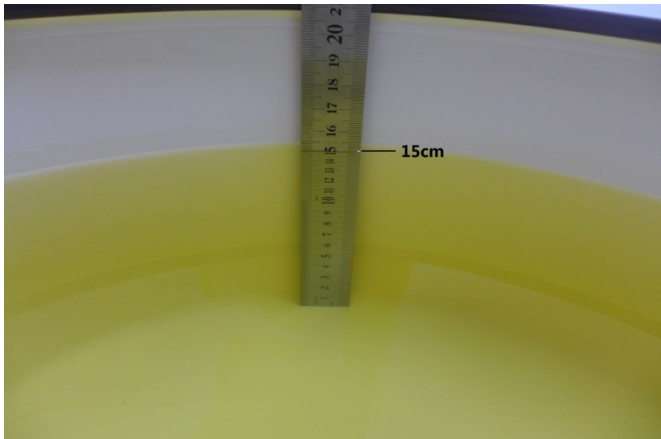
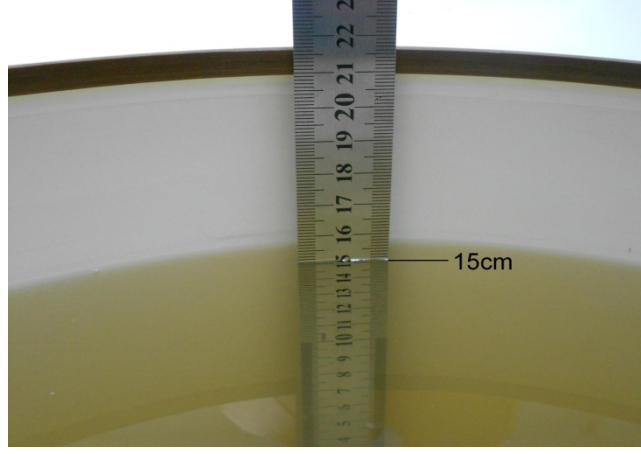
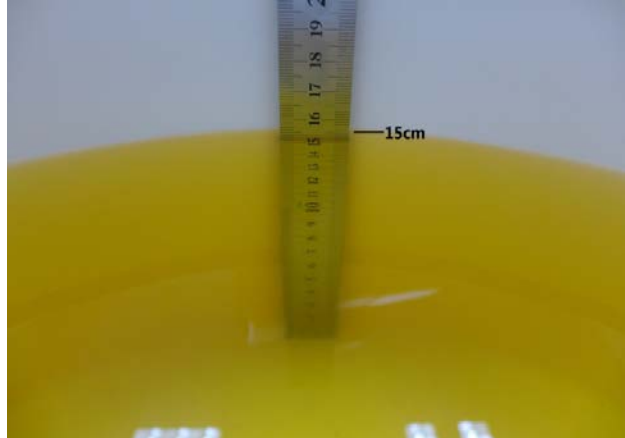
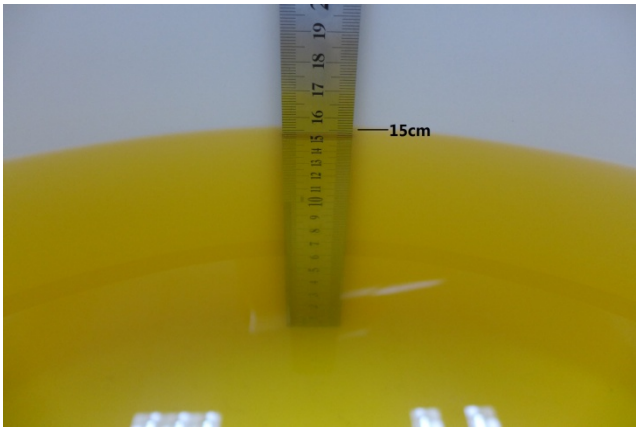
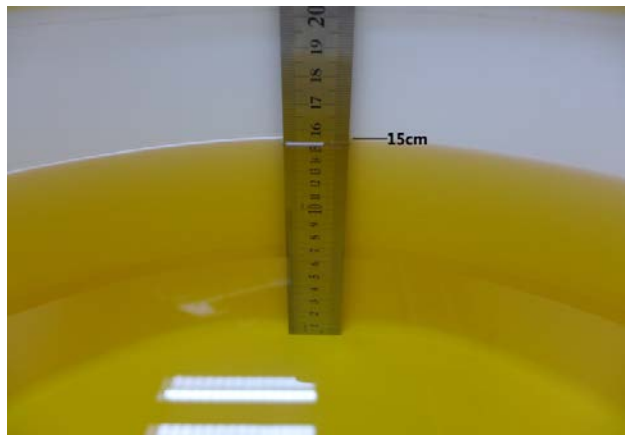
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

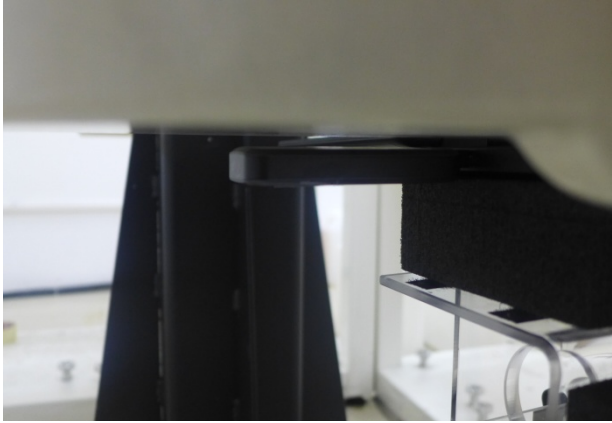
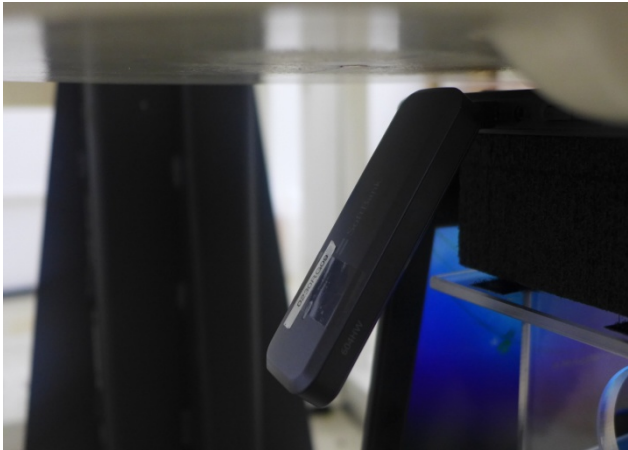
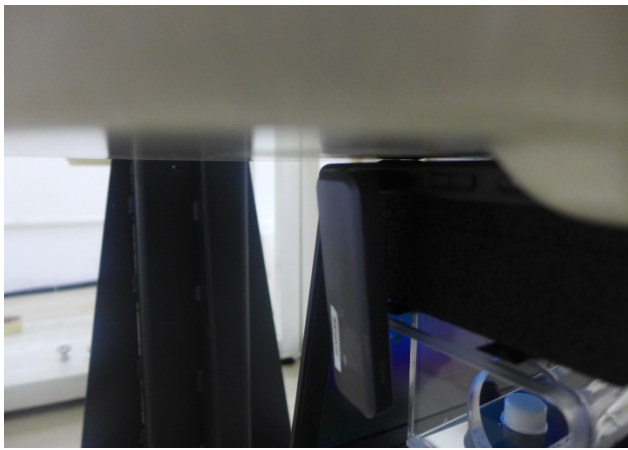
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Body 750	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Body 1750	Photo 4: Tissue Simulant Liquid for Body 1900
	
Photo 5: Tissue Simulant Liquid for Body 2600	N/A
	N/A

3. Photographs of EUT test position

Photo 6: Front side 5mm	Photo 7: Back side 5mm
	
Photo 8: Left side 5mm	Photo 9: Right side 5mm
	
Photo 10: Back side positioned at 45° 5mm	Photo 11: Back side positioned at 90° 5mm
	

4. EUT Constructional Details

Photo 12: Front View	Photo 13: Back View
 A photograph showing the front view of a small, dark-colored USB dongle. The dongle is positioned horizontally next to a metal ruler. The ruler has markings in centimeters (0 to 18) and inches (0 to 6). The dongle is approximately 10 cm long and 1.5 cm wide. The USB connector is visible on the right side.	 A photograph showing the back view of the same USB dongle. The dongle is positioned horizontally next to a metal ruler. The ruler has markings in centimeters (0 to 22) and inches (0 to 6). The dongle is approximately 10 cm long and 1.5 cm wide. The USB connector is visible on the left side. A small red label with white text is visible on the back of the dongle.