

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

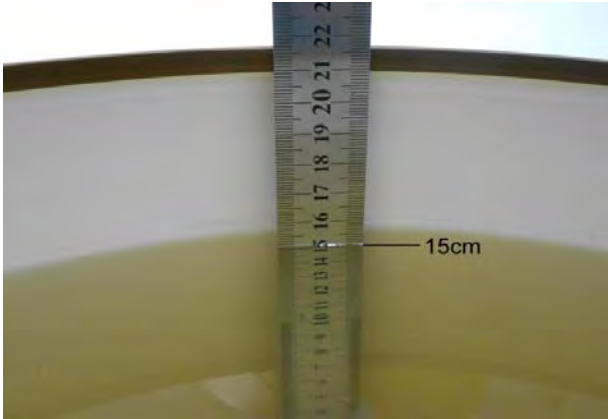
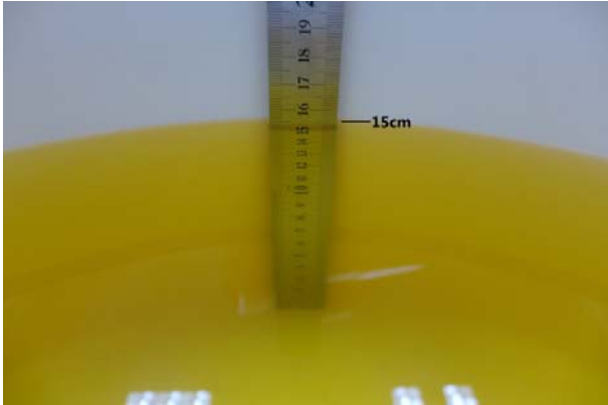
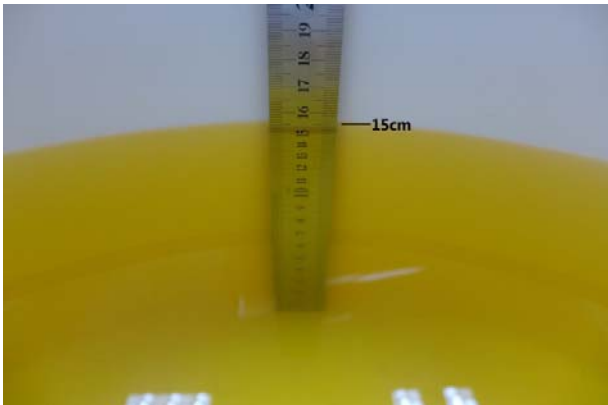
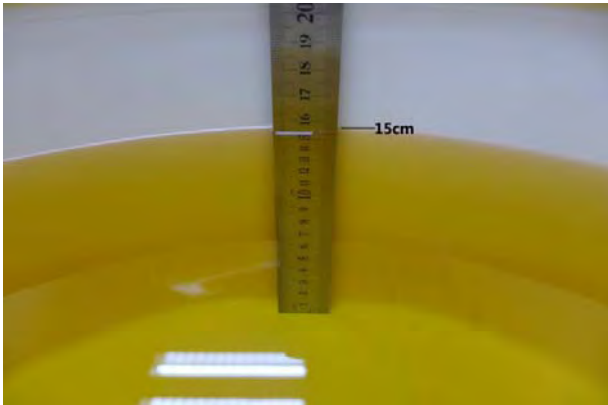
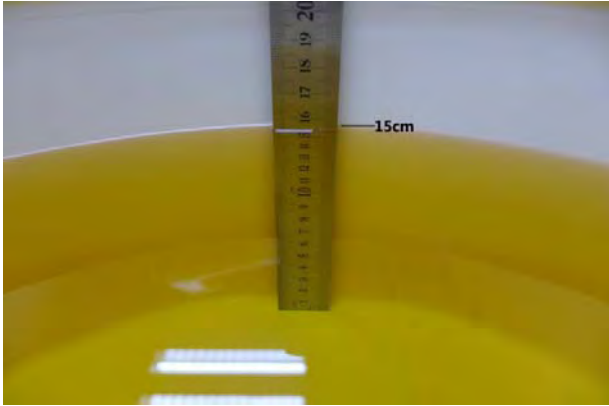
Photo 1: Tissue Simulant Liquid for Body 835	Photo 2: Tissue Simulant Liquid for Body 1750
	
Photo 3: Tissue Simulant Liquid for Body 1900	Photo 4: Tissue Simulant Liquid for Body 2450
	

Photo 5: Tissue Simulant Liquid for Body 2600	N/A
	N/A

3. Photographs of EUT test position

Photo 6: Front side 10mm	Photo 7: Back side 10mm
	
Photo 8: Front side 16mm	Photo 9: Back side 16mm
	
Photo 10: Front side 22mm	Photo 11: Back side 22mm
	

Photo 12: Right side 10mm	Photo 13: Right side 20mm
	
Photo 14: Right side 24mm	Photo 15: Top side 10mm
	
Photo 16: Bottom side 10mm	N/A
	N/A

4. EUT Constructional Details

