

System Check Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260112 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 39.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.16, 7.29, 6.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=24.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 13.9 W/kg; SAR (10g) = 6.54 W/kg;

TSL Correction: Positive only

Pin=24.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = -0.00 dB

SAR (1g) = 14.1 W/kg; SAR (8g) = 7.61 W/kg; SAR (10g) = 6.94 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.1 %

TSL Correction: Positive only

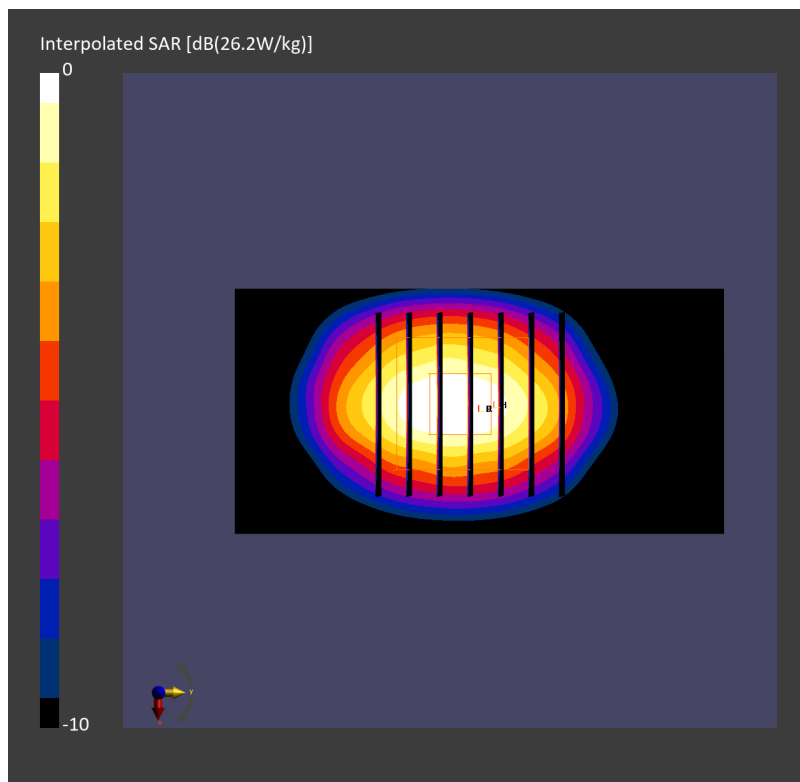

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_600-7200_260114 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.80$ S/m; $\epsilon_r = 40.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(7.16, 7.29, 6.97); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.53 W/kg; SAR (10g) = 1.17 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 31.2 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm


Power Drift = 0.02 dB

SAR (1g) = 2.56 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

TSL Correction: Positive only

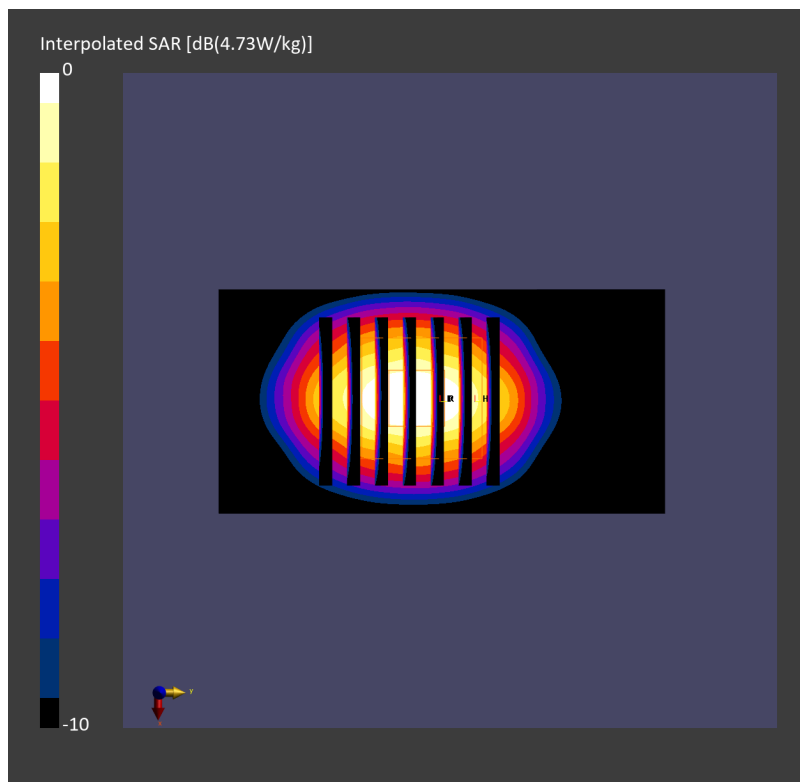

System Check Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260112 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.51$ S/m; $\epsilon_r = 34.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.52, 5.62, 5.37); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.32 W/kg; SAR (10g) = 2.23 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.01 dB

SAR (1g) = 8.27 W/kg; SAR (8g) = 2.83 W/kg; SAR (10g) = 2.44 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.7 %

TSL Correction: Positive only

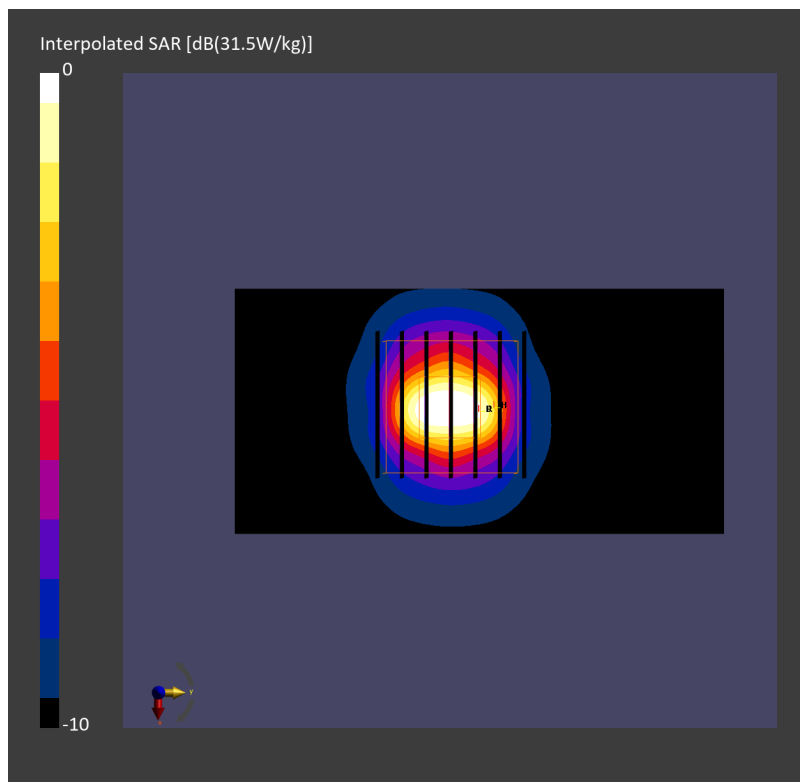

System Check Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_600-7200_260113 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.57$ S/m; $\epsilon_r = 35.5$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.52, 5.62, 5.37); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.33 W/kg; SAR (10g) = 1.01 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.68 W/kg; SAR (8g) = 1.26 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 64.4 %

TSL Correction: Positive only

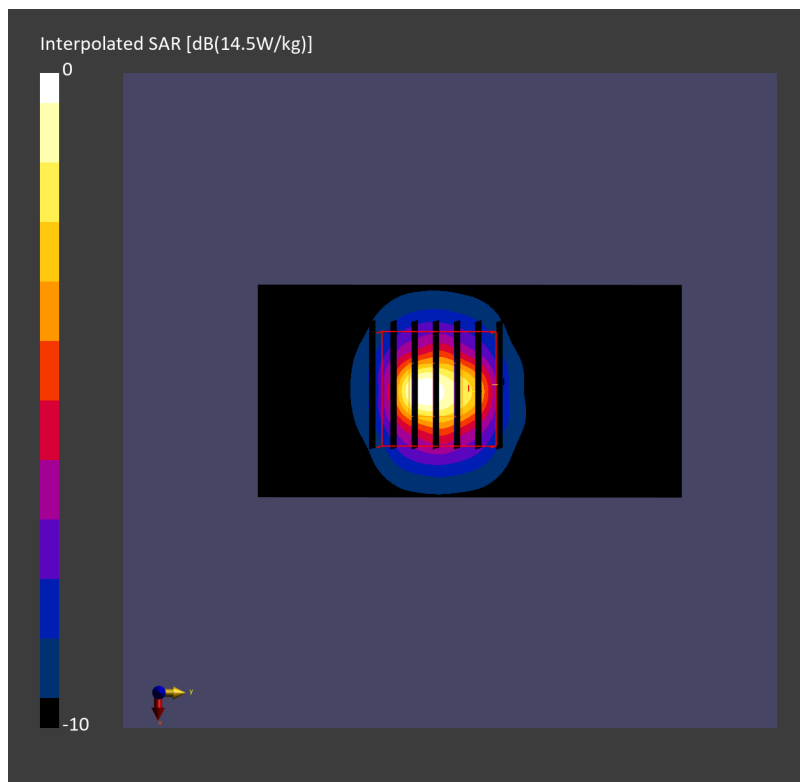

System Check Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260112 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.89$ S/m; $\epsilon_r = 34.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.15, 5.24, 5.01); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.62 W/kg; SAR (10g) = 2.31 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 8.56 W/kg; SAR (8g) = 2.91 W/kg; SAR (10g) = 2.52 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.6 %

TSL Correction: Positive only

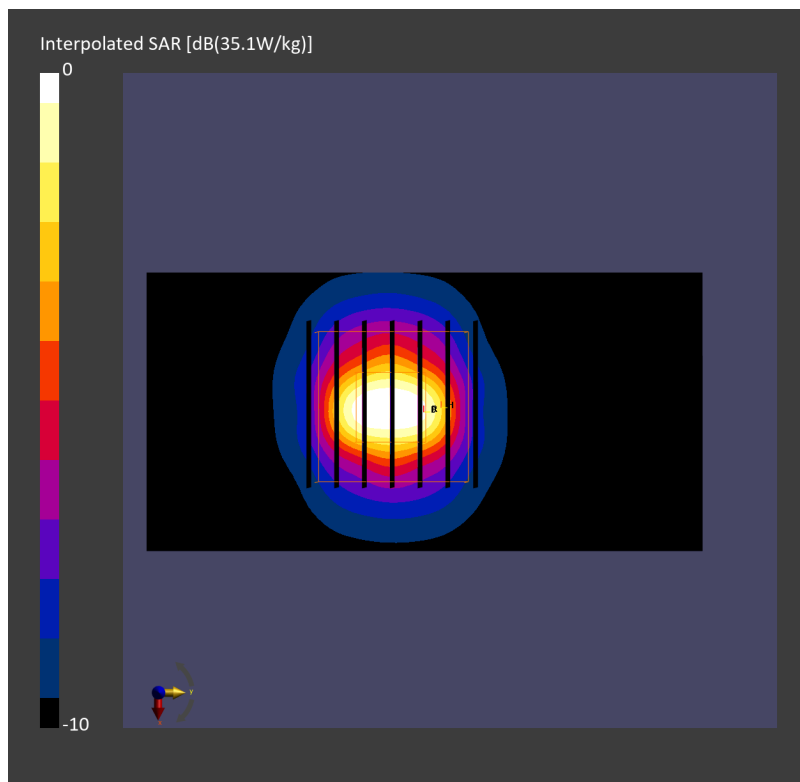

System Check Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_600-7200_260113 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 4.96$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.15, 5.24, 5.01); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.55 W/kg; SAR (10g) = 1.06 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.02 dB

SAR (1g) = 3.96 W/kg; SAR (8g) = 1.34 W/kg; SAR (10g) = 1.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 61.2 %

TSL Correction: Positive only

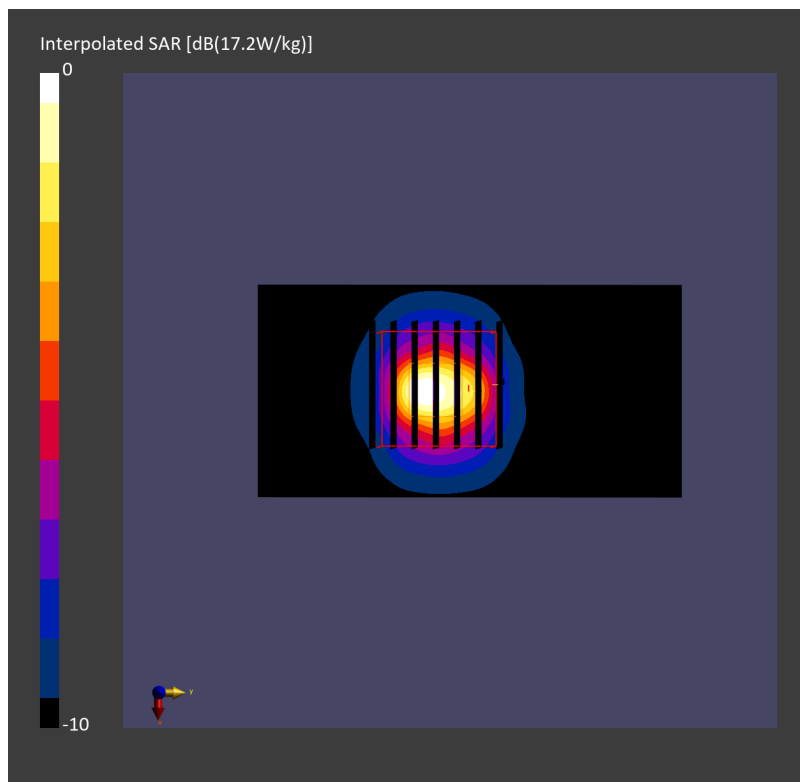

System Check Head_5800MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260112 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.10$ S/m; $\epsilon_r = 33.7$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.03, 5.12, 4.9); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.35 W/kg; SAR (10g) = 2.21 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 8.33 W/kg; SAR (8g) = 2.81 W/kg; SAR (10g) = 2.43 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.2 %

TSL Correction: Positive only

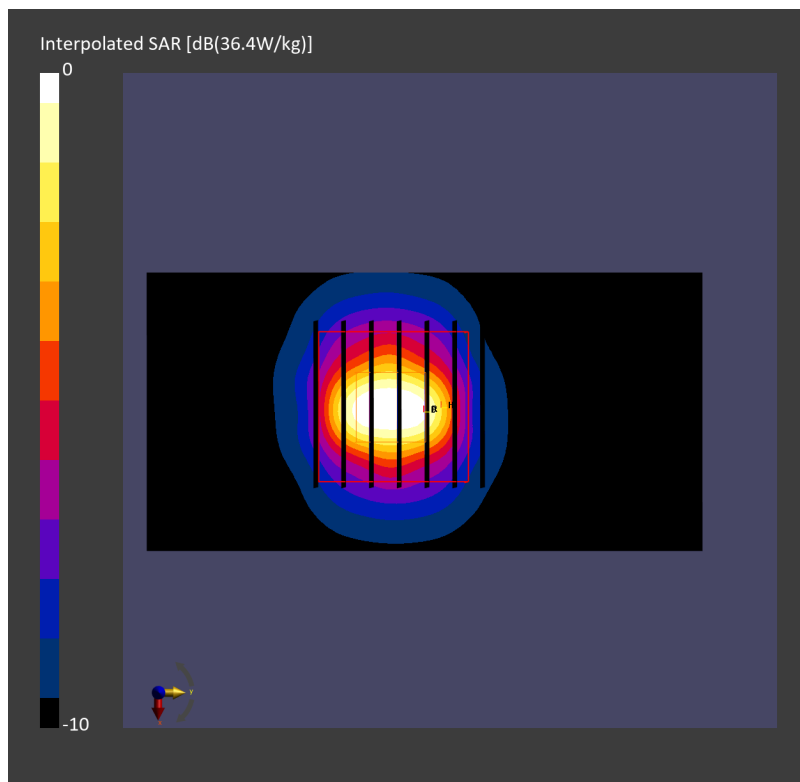

System Check Head_5800MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5800.000 MHz

Medium: HSL_600-7200_260113 Medium parameters used: $f = 5800.000$ MHz; $\sigma = 5.19$ S/m; $\epsilon_r = 34.4$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.03, 5.12, 4.9); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.44 W/kg; SAR (10g) = 1.03 W/kg;

TSL Correction: Positive only

Pin=17.0dBm/Zoom Scan (24.0 mm x 24.0 mm x 22.9 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm


Power Drift = -0.05 dB

SAR (1g) = 3.84 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.12 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 58.7 %

TSL Correction: Positive only

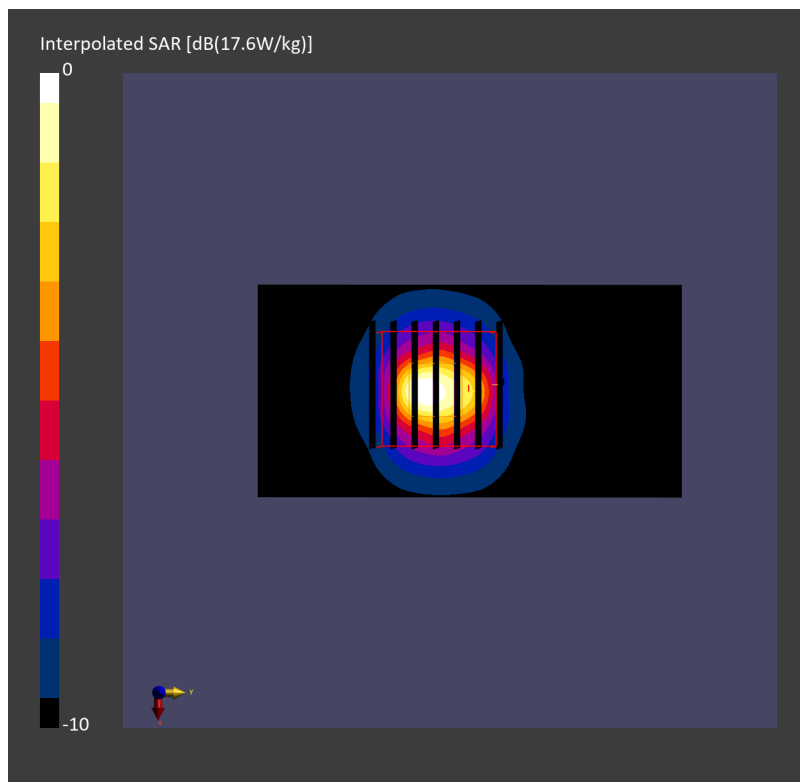

System Check Head_6500MHz

DUT: D6.5GHzV2 - SN1083

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_600-7200_260112 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.86$ S/m; $\epsilon_r = 32.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.51, 5.61, 5.37); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 21.5 W/kg; SAR (10g) = 4.87 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (23.8 mm x 23.8 mm x 22.9 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.08 dB


SAR (1g) = 27.8 W/kg; SAR (8g) = 6.35 W/kg; SAR (10g) = 5.24 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 53.7 %

psAPD (1.0cm², sq) = 278 [W/m²]; psAPD (4.0cm², sq) = 127 [W/m²]

TSL Correction: Positive only

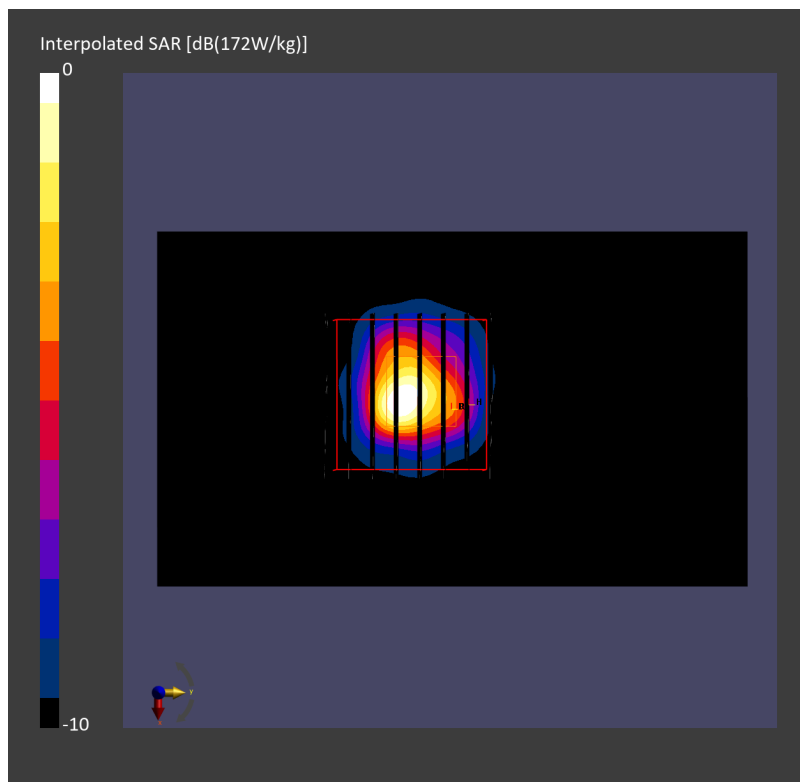

System Check Head_6500MHz

DUT: D6.5GHzV2 - SN1083

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_600-7200_260114 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 5.99$ S/m; $\epsilon_r = 33.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3931; ConvF(5.51, 5.61, 5.37); Calibrated: 2025-10-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2025-11-19
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2204; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 22.0 W/kg; SAR (10g) = 4.75 W/kg;

TSL Correction: Positive only

Pin=20.0dBm/Zoom Scan (23.8 mm x 23.8 mm x 22.9 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = 0.03 dB

SAR (1g) = 27.3 W/kg; SAR (8g) = 6.17 W/kg; SAR (10g) = 5.09 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 52.8 %

psAPD (1.0cm², sq) = 273 [W/m²]; psAPD (4.0cm², sq) = 124 [W/m²]

TSL Correction: Positive only

