

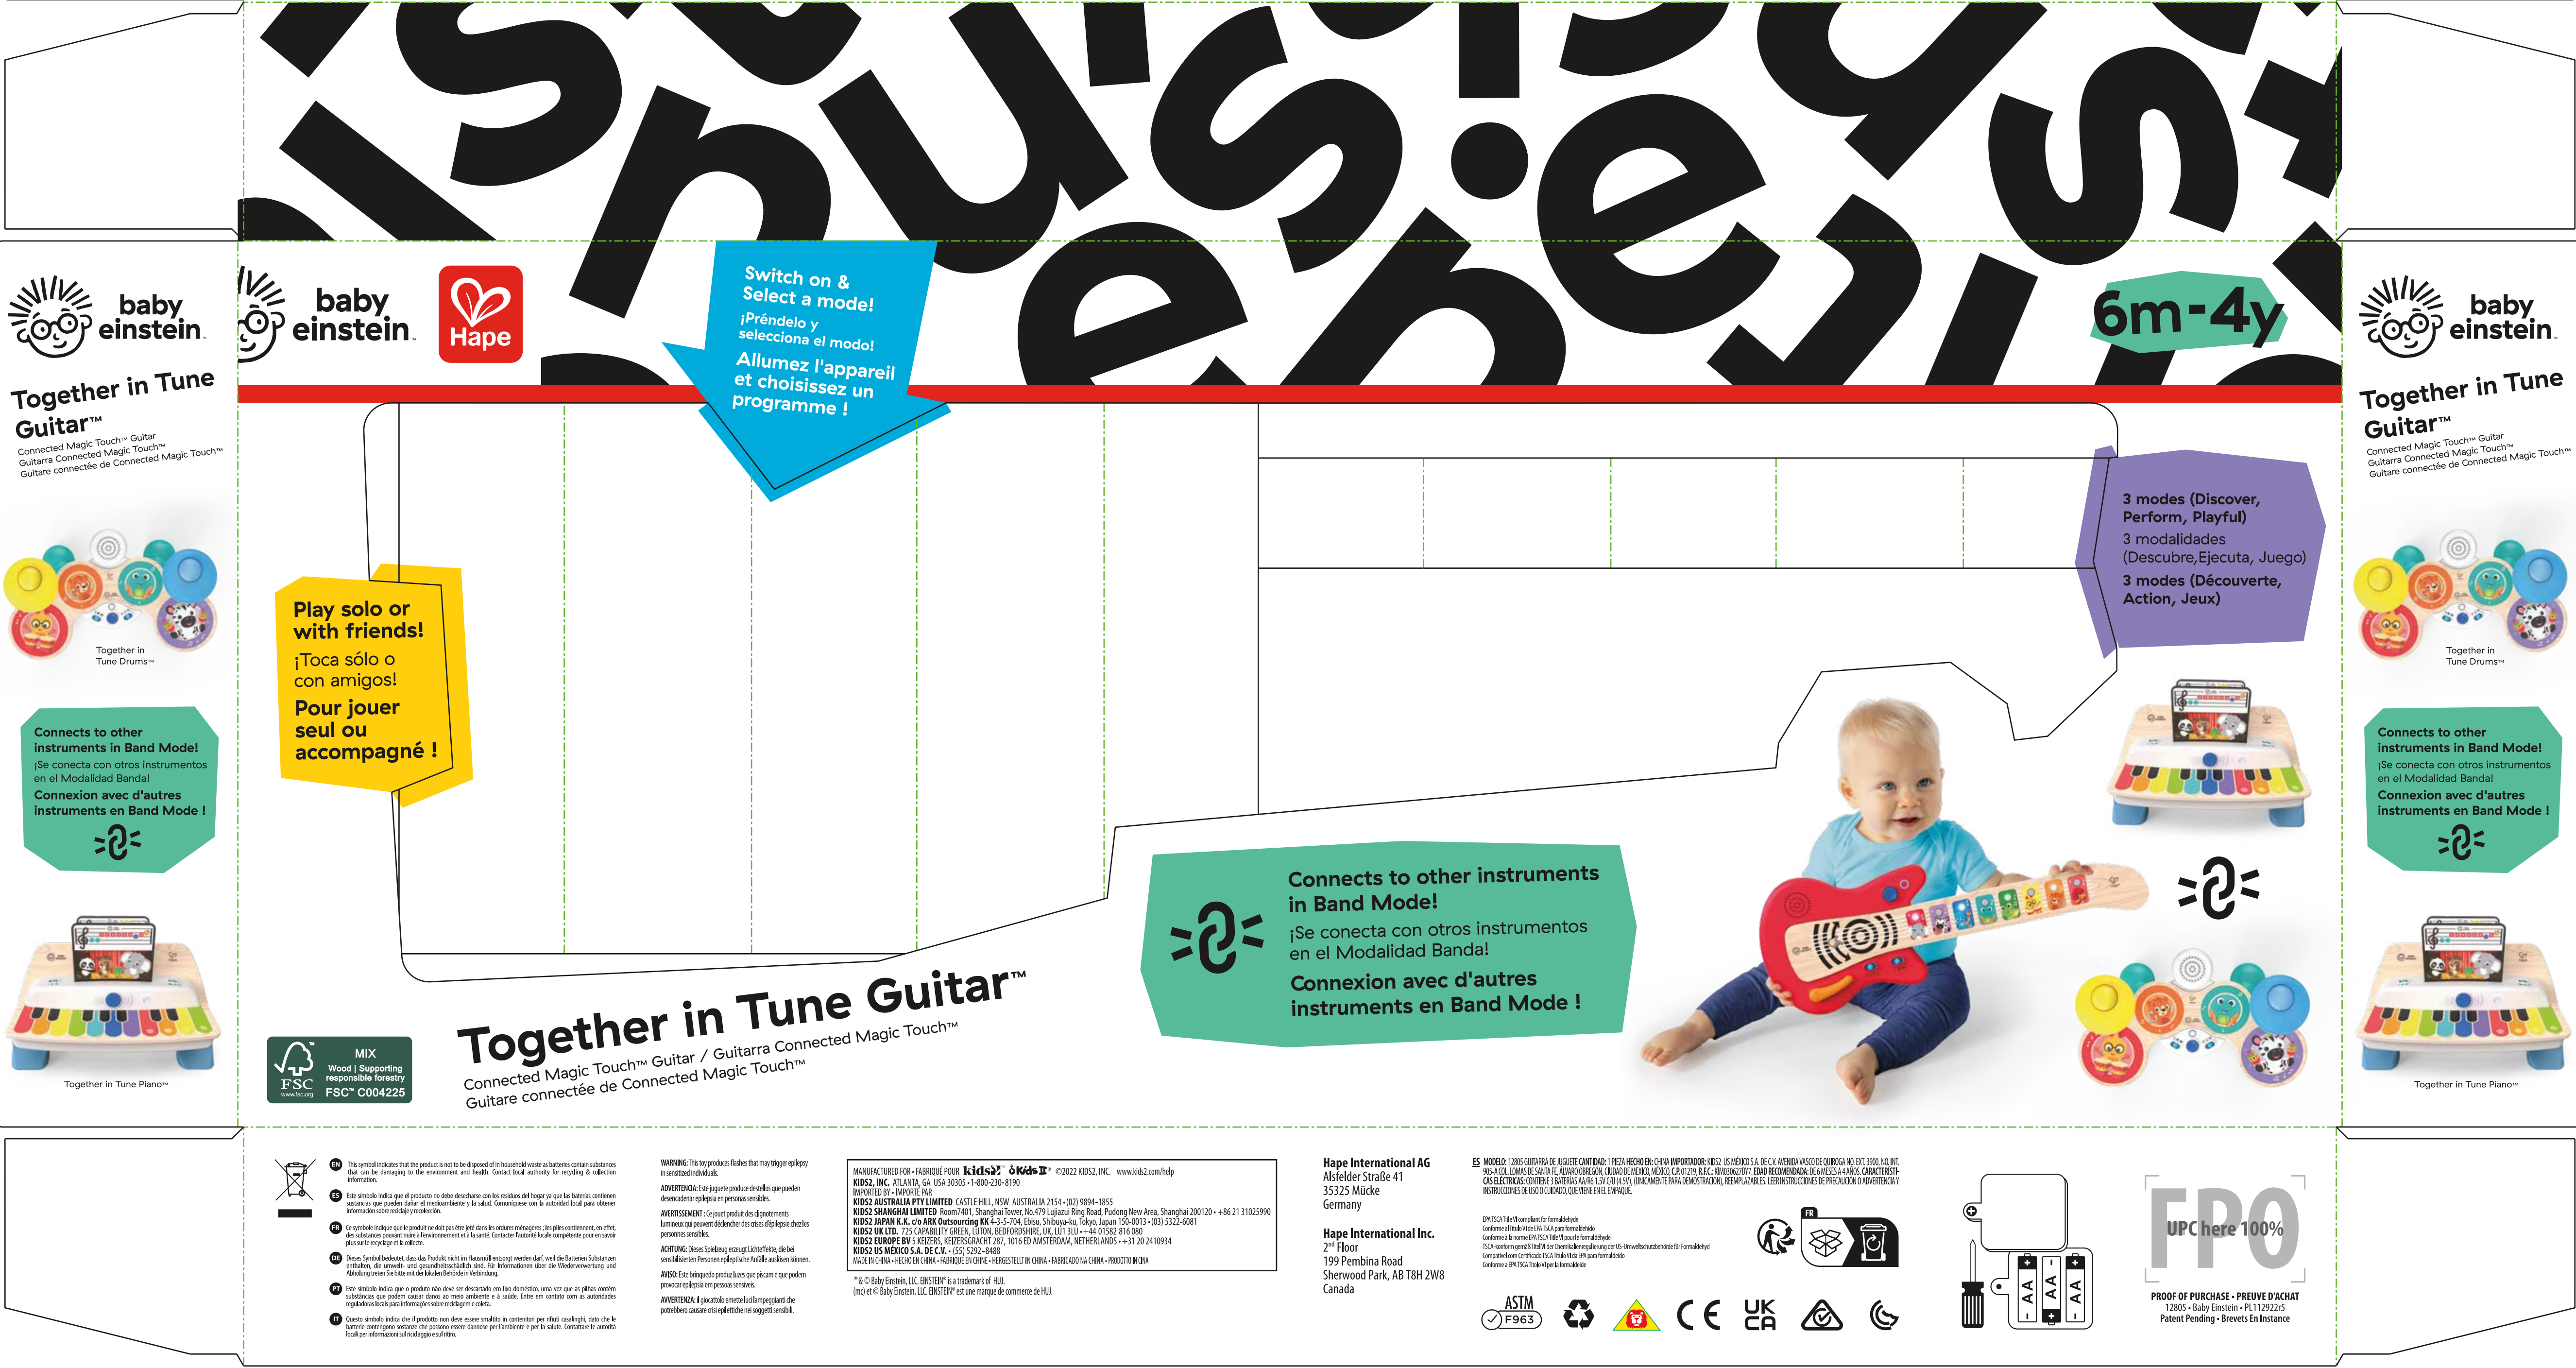
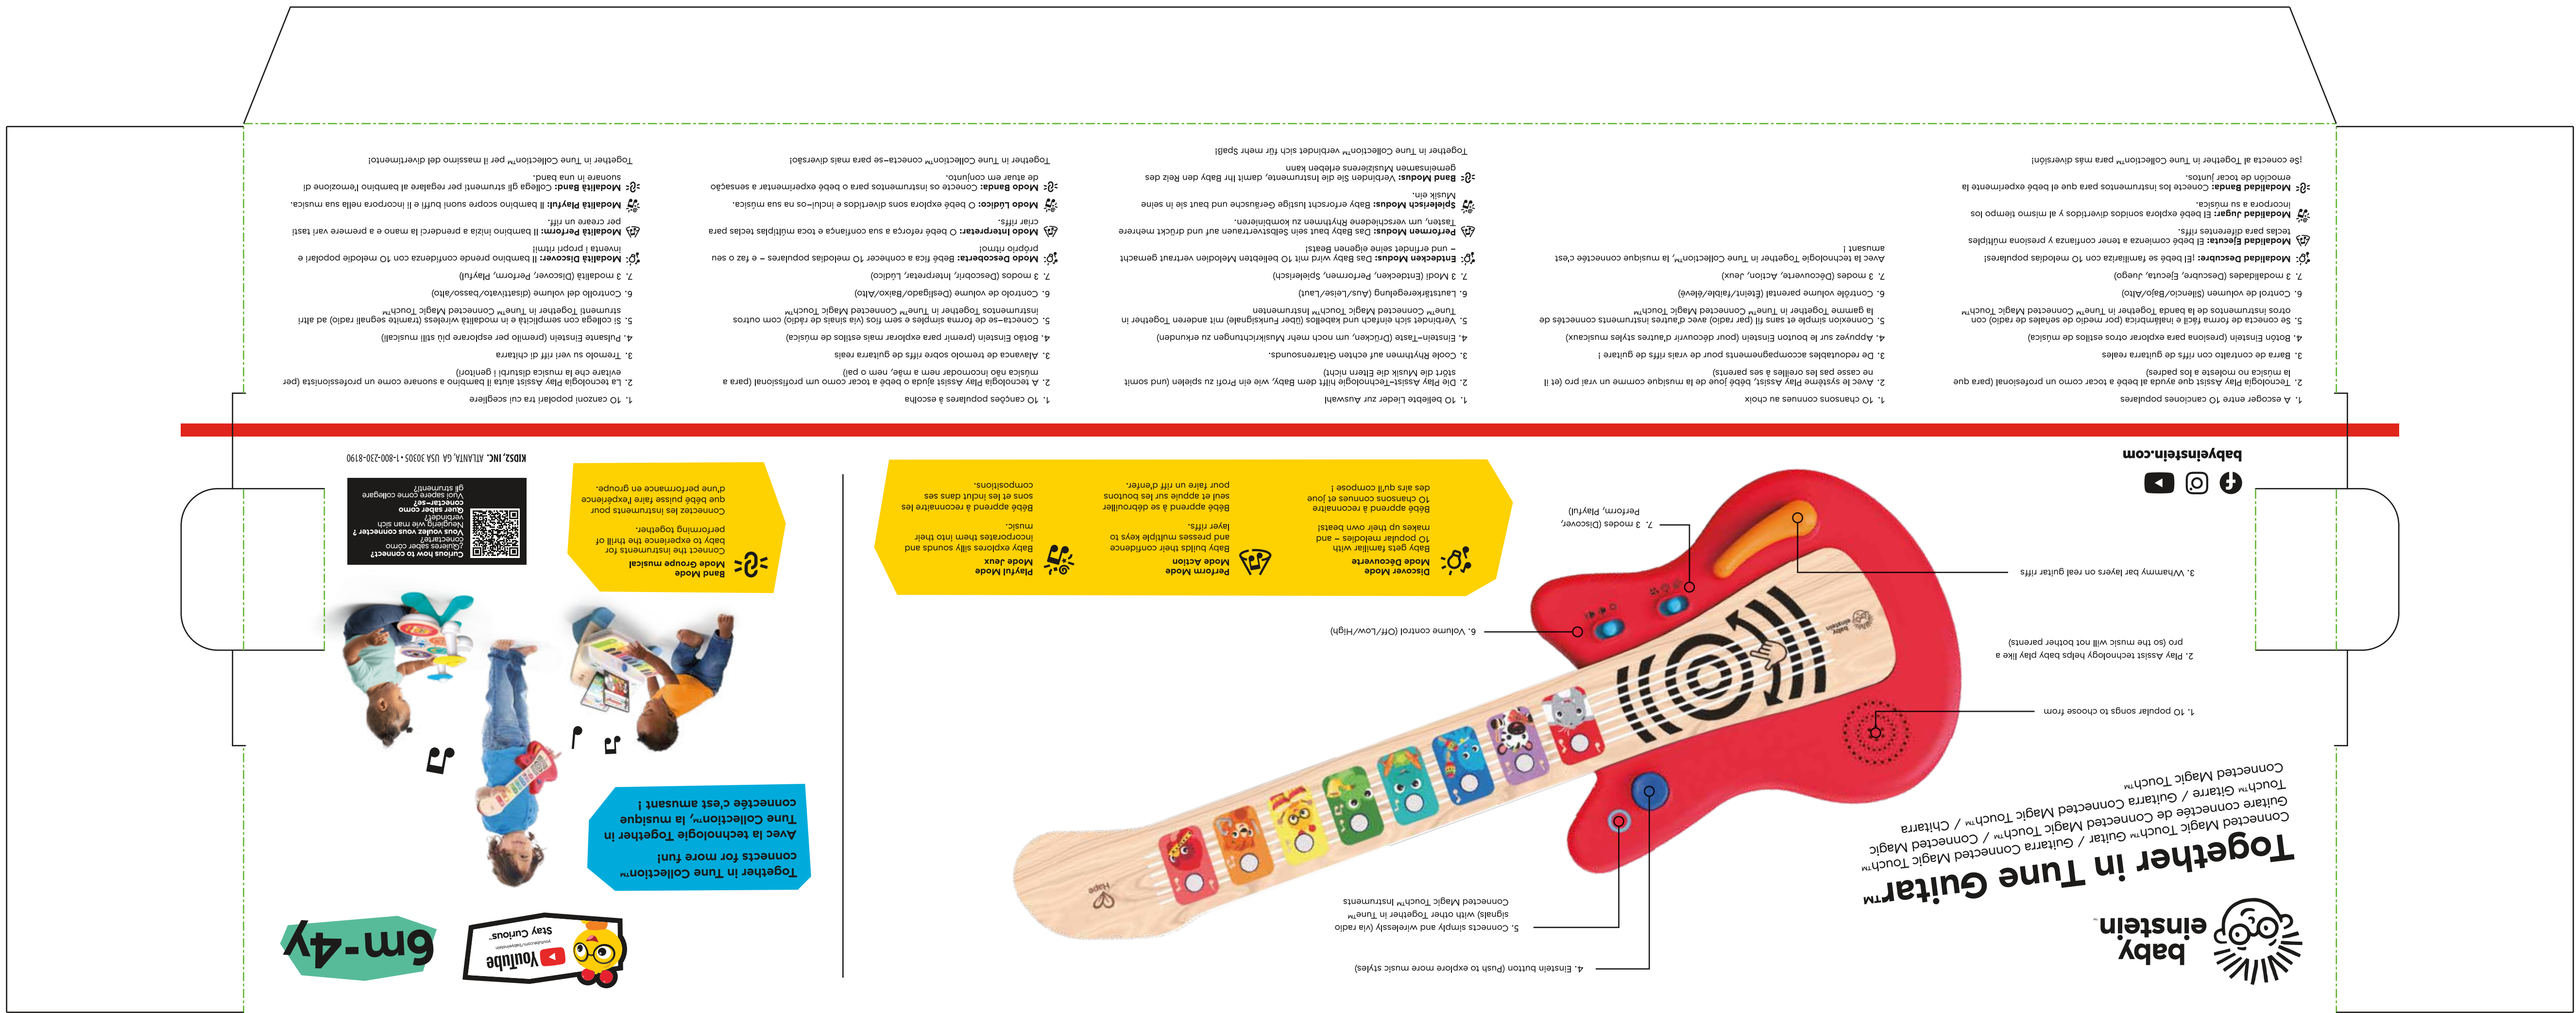


There are two color bars on this proof and in the art file. One to be used with Xerox HP Pro Spectrophotometer. The other can be used with most other spectrophotometers. Printers must report one of the two color bars. All they need to do with (top) edge of the press sheet on sample color and production color. Failure to comply will result in the reworking of film and/or plates at your cost. 数据必须以设计文件包含于两种颜色。一种用于X-11e (设备) 1) Pro 分光光度计。另一种用于其他大部分的光学光度计。在印刷或制造生产时，印刷厂必须选择其中一种颜色并重复添加该颜色直到达到预期的效果。(印12) 2) 另数据上包含更多种颜色输出材料，出版商将提供打印厂参考。

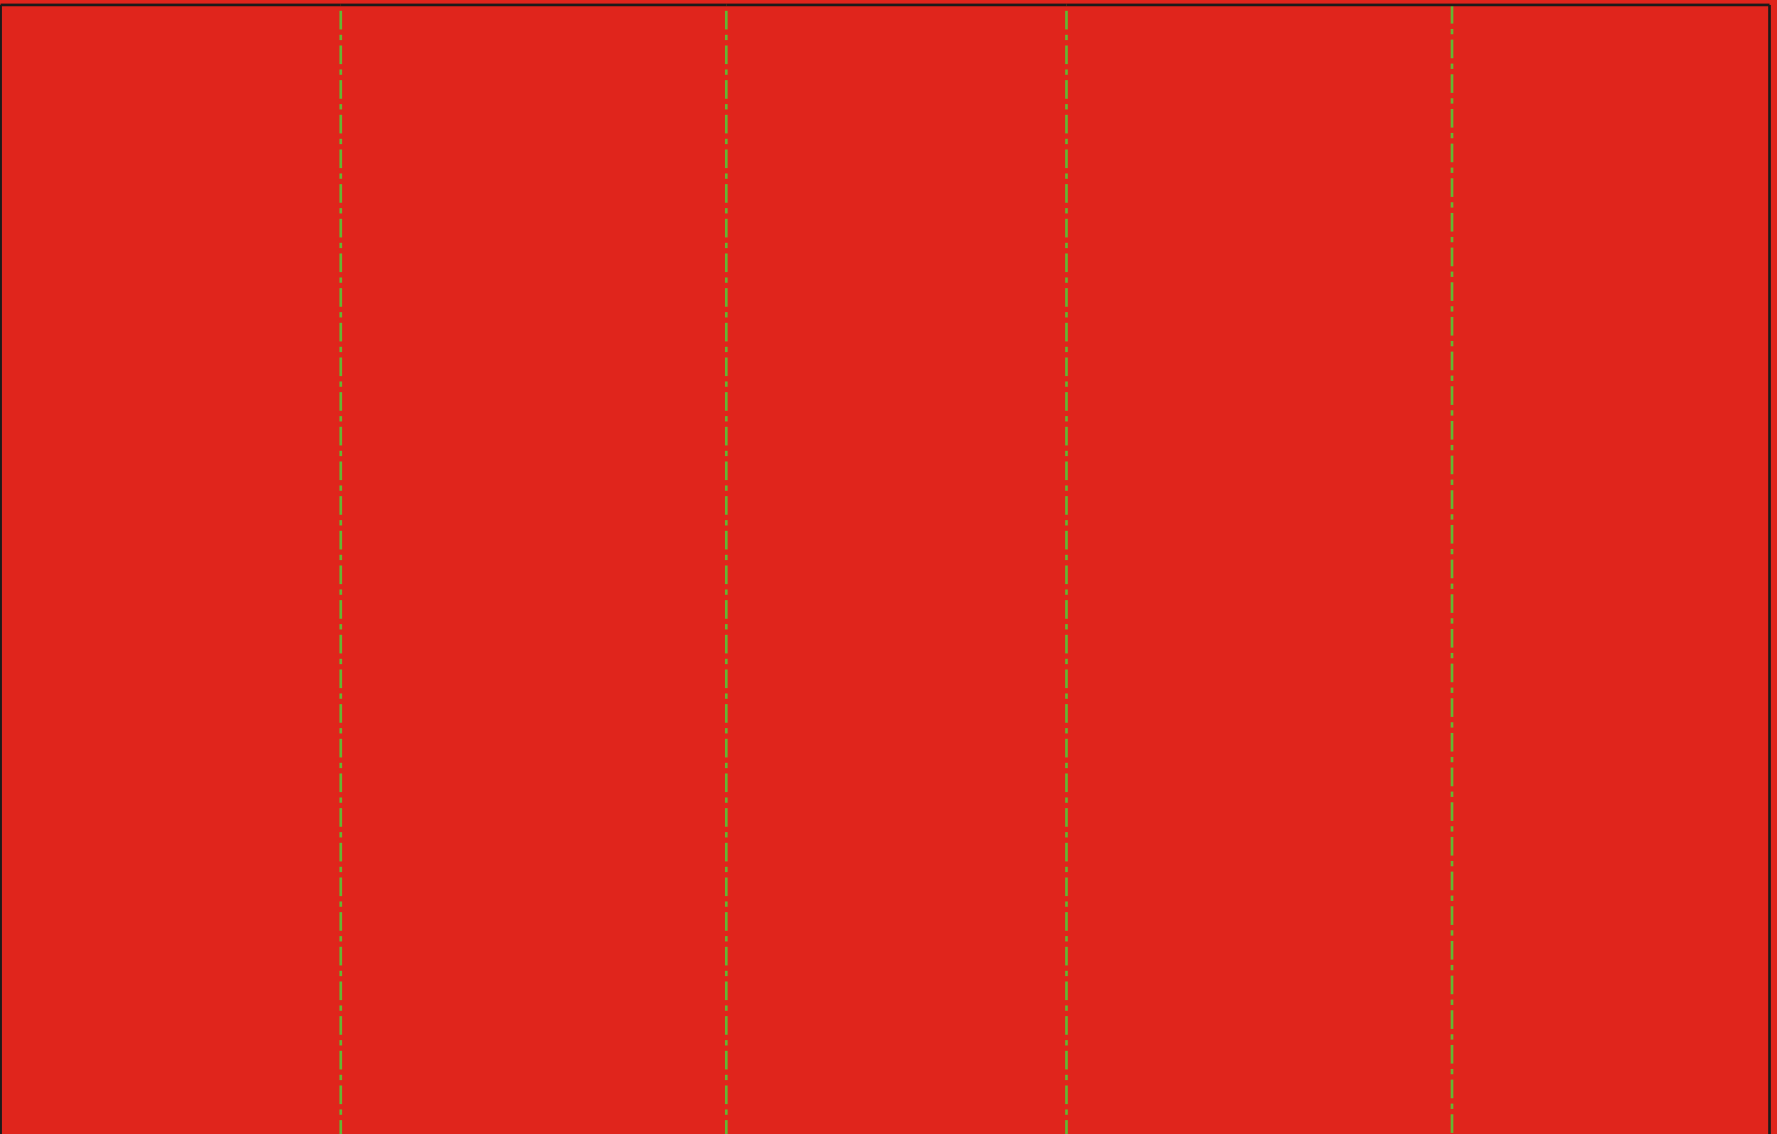

PACKOUT

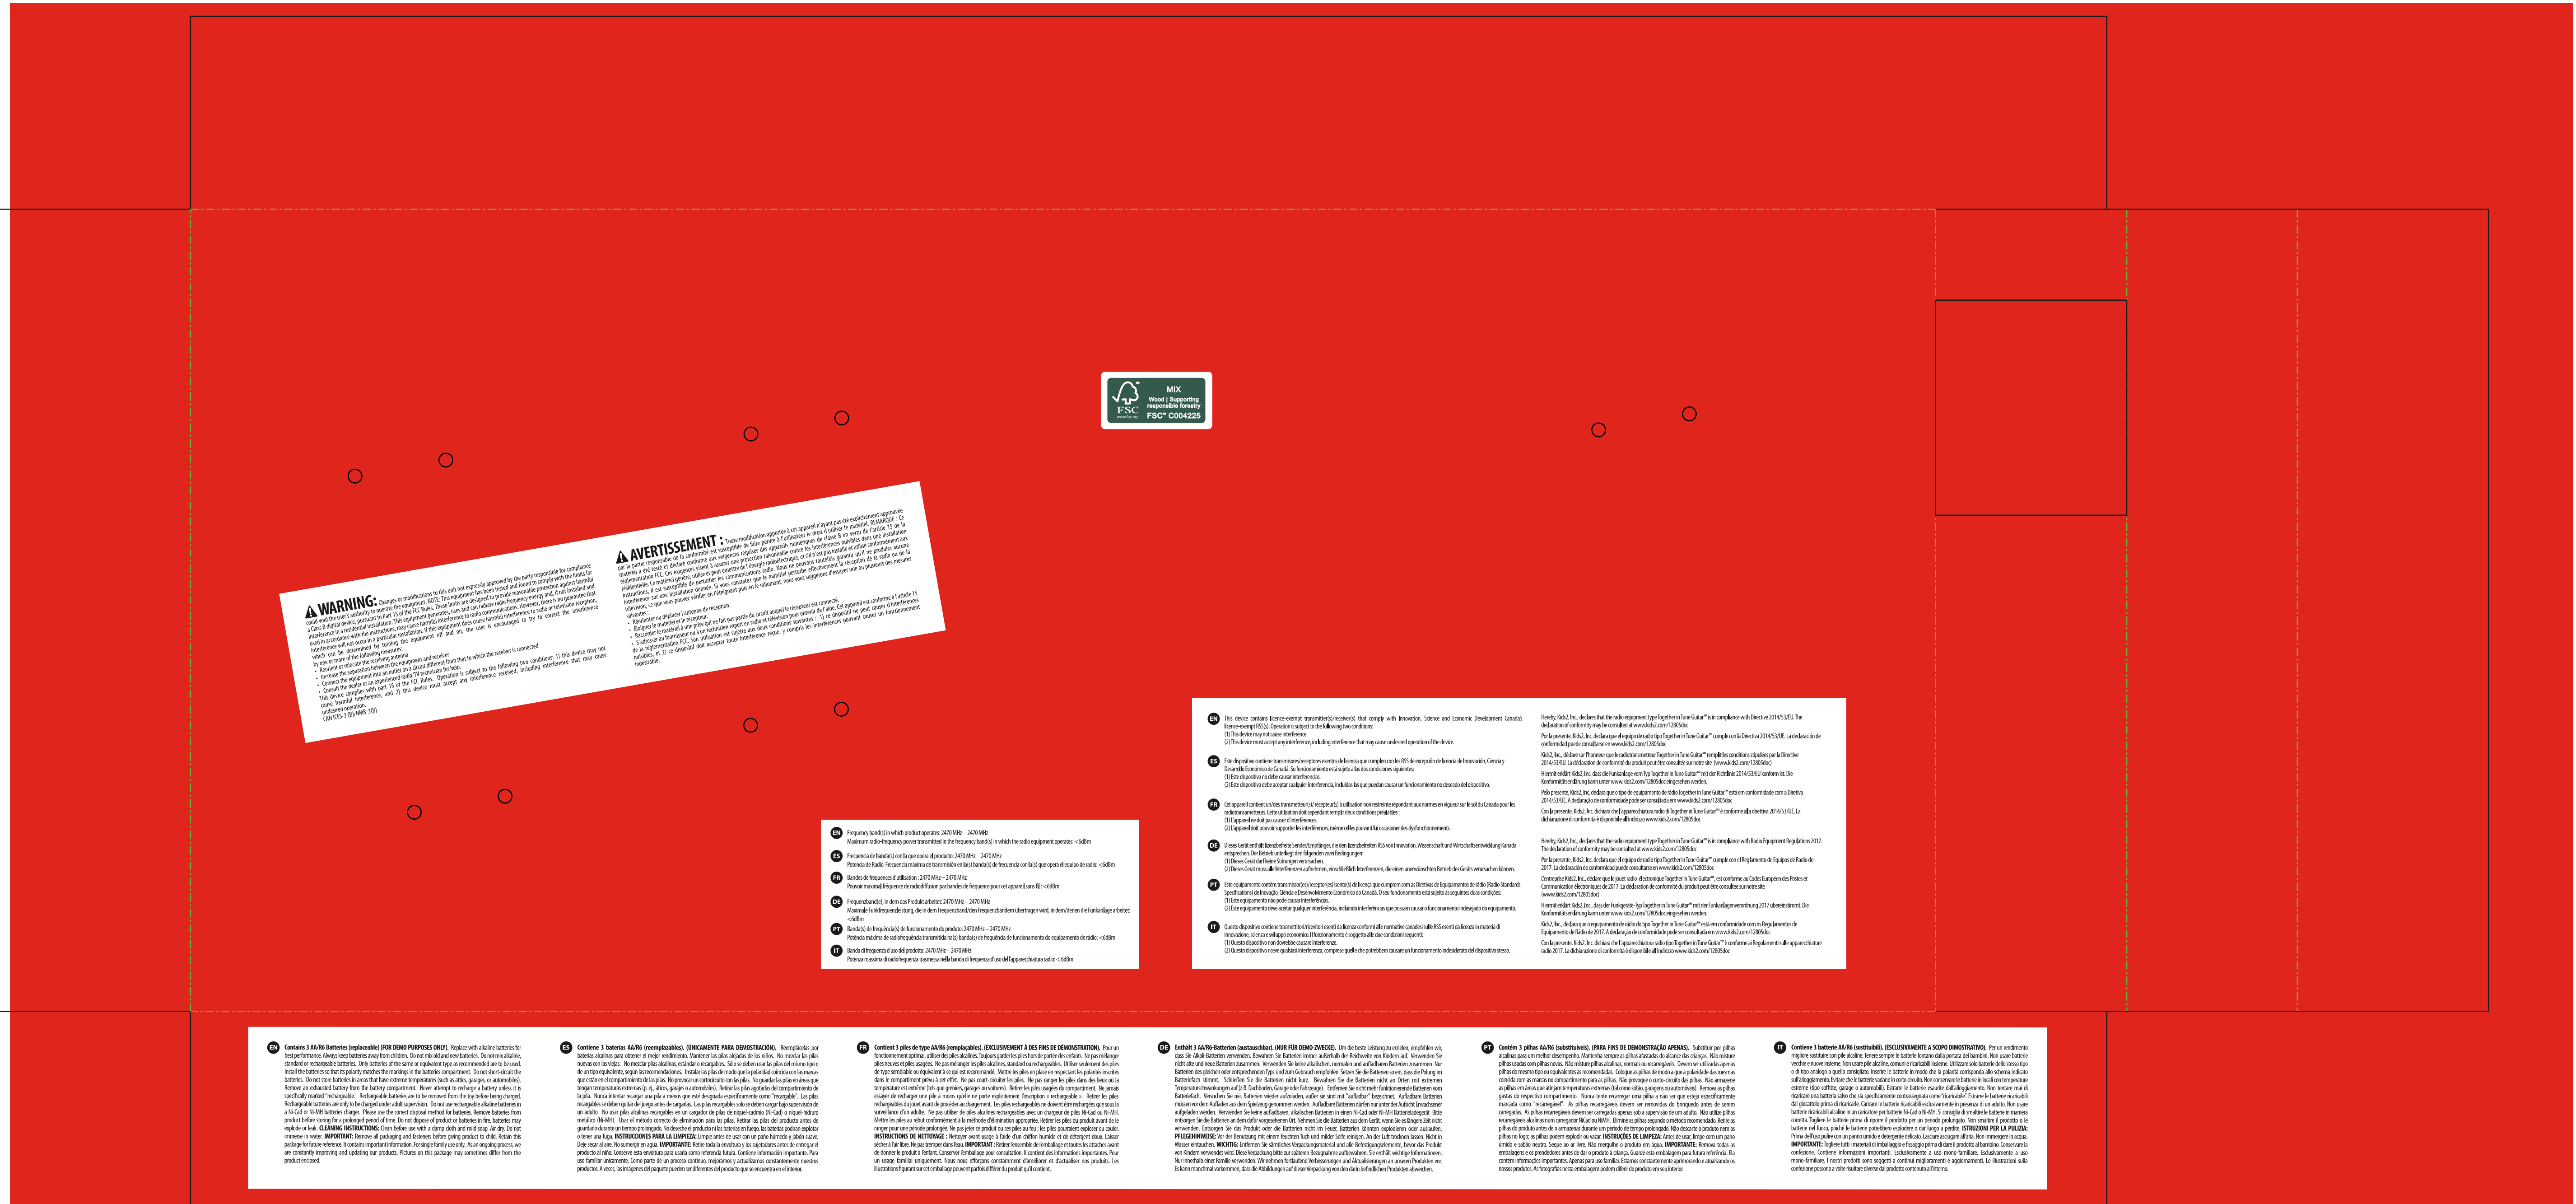

please secure the toy using cable ties

hole locations will be created by manufacturer

