

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 The photograph shows a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically against the container, showing measurements in centimeters. The liquid level is approximately 10 cm high. The container has a blue outer layer and a white inner layer.	NA

3. Photographs of EUT test position

Photo 2: Left Cheek

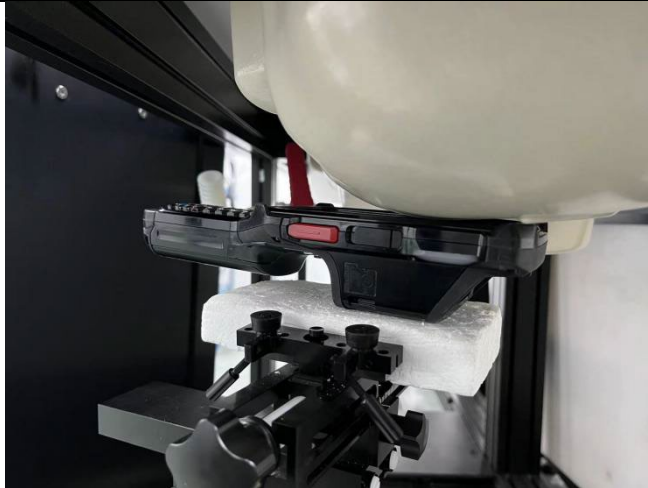


Photo 3: Left Tilted



Photo 4: Right Cheek



Photo 5: Right Tilted



Photo 6: Front Side 15mm




Photo 7: Back Side 15mm






Photo 8: Front Side 10mm



Photo 9: Back Side 10mm



Photo 10: Left Side 10mm



Photo 11: Right Side 10mm



Photo 12: Top Side 10mm



Photo 13: Front Side 0mm



Photo 14: Back Side 0mm



Photo 15: Left Side 0mm



Photo 16: Right Side 0mm



Photo 17: Top Side 0mm



4. EUT Constructional Details

