

# Appendix C

## Calibration certificate

|                                       |
|---------------------------------------|
| 1. Dipole                             |
| CLA13-SN 1032                         |
| D750V3-SN 1214                        |
| D835V2-SN 4d161                       |
| D1750V2-SN1105                        |
| D1950V3-SN 1218                       |
| D2450V2-SN 922                        |
| D2600V2-SN 1158                       |
| D3500V2-SN 1067                       |
| D3700V2-SN 1108                       |
| D3900V2-SN 1083                       |
| D5GHzV2-SN 1174                       |
| D6.5GHzV2-SN 1030                     |
| 5G Verification Source 10 GHZ-SN 2004 |
| 2. DAE                                |
| DAE4ip-SN 1740                        |
| DAE4ip-SN 1826                        |
| 3. Probe                              |
| EX3DV4-SN 3982                        |
| EX3DV4-SN 7735                        |
| EUmmWV4-SN 9718                       |
| 4. Dipole Extend                      |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **SGS-CN (Auden)**

Certificate No: **CLA13-1032\_Feb23**

## CALIBRATION CERTIFICATE

Object **CLA13 - SN: 1032**

Calibration procedure(s) **QA CAL-15.v10**  
**Calibration Procedure for SAR Validation Sources below 700 MHz**

Calibration date: **February 09, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID #               | Cal Date (Certificate No.)      | Scheduled Calibration |
|-----------------------------|--------------------|---------------------------------|-----------------------|
| Power meter NRP             | SN: 104778         | 04-Apr-22 (No. 217-03525/03524) | Apr-23                |
| Power sensor NRP-Z91        | SN: 103244         | 04-Apr-22 (No. 217-03524)       | Apr-23                |
| Power sensor NRP-Z91        | SN: 103245         | 04-Apr-22 (No. 217-03525)       | Apr-23                |
| Reference 20 dB Attenuator  | SN: CC2552 (20x)   | 04-Apr-22 (No. 217-03527)       | Apr-23                |
| Type-N mismatch combination | SN: 310982 / 06327 | 04-Apr-22 (No. 217-03528)       | Apr-23                |
| Reference Probe EX3DV4      | SN: 3877           | 06-Jan-23 (No. EX3-3877_Jan23)  | Jan-24                |
| DAE4                        | SN: 654            | 27-Jan-23 (No. DAE4-654_Jan23)  | Jan-24                |

| Secondary Standards             | ID #             | Check Date (in house)             | Scheduled Check        |
|---------------------------------|------------------|-----------------------------------|------------------------|
| Power meter NRP2                | SN: 107193       | 08-Nov-21 (in house check Dec-22) | In house check: Dec-24 |
| Power sensor NRP-Z91            | SN: 100922       | 15-Dec-09 (in house check Dec-22) | In house check: Dec-24 |
| Power sensor NRP-Z91            | SN: 100418       | 01-Jan-04 (in house check Dec-22) | In house check: Dec-24 |
| RF generator HP 8648C           | SN: US3642U01700 | 04-Aug-99 (in house check Jun-22) | In house check: Jun-24 |
| Network Analyzer Agilent E8358A | SN: US41080477   | 31-Mar-14 (in house check Oct-22) | In house check: Oct-24 |

|                |                                   |                                          |                                                                                                    |
|----------------|-----------------------------------|------------------------------------------|----------------------------------------------------------------------------------------------------|
| Calibrated by: | Name<br><b>Aidonia Georgiadou</b> | Function<br><b>Laboratory Technician</b> | Signature<br> |
| Approved by:   | <b>Sven Kühn</b>                  | <b>Technical Manager</b>                 |               |

Issued: February 10, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- c) DASY System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The source is mounted in a touch configuration below the center marking of the flat phantom.
- *Return Loss:* This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                             |                                  |                                  |
|-----------------------------|----------------------------------|----------------------------------|
| <b>DASY Version</b>         | DASY5                            | V52.10.4                         |
| <b>Extrapolation</b>        | Advanced Extrapolation           |                                  |
| <b>Phantom</b>              | ELI4 Flat Phantom                | Shell thickness: $2 \pm 0.2$ mm  |
| <b>EUT Positioning</b>      | Touch Position                   |                                  |
| <b>Zoom Scan Resolution</b> | $dx, dy = 4.0$ mm, $dz = 1.4$ mm | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>            | $13$ MHz $\pm 1$ MHz             |                                  |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity           |
|------------------------------------------------|---------------------|----------------|------------------------|
| <b>Nominal Head TSL parameters</b>             | $22.0$ °C           | 55.0           | 0.75 mho/m             |
| <b>Measured Head TSL parameters</b>            | $(22.0 \pm 0.2)$ °C | $52.9 \pm 6$ % | $0.72$ mho/m $\pm 6$ % |
| <b>Head TSL temperature change during test</b> | $< 0.5$ °C          | ----           | ----                   |

## SAR result with Head TSL

|                                                                       |                  |                                                              |
|-----------------------------------------------------------------------|------------------|--------------------------------------------------------------|
| <b>SAR averaged over <math>1\text{ cm}^3</math> (1 g) of Head TSL</b> | Condition        |                                                              |
| SAR measured                                                          | 1 W input power  | 0.411 W/kg                                                   |
| SAR for nominal Head TSL parameters                                   | normalized to 1W | <b><math>0.421</math> W/kg <math>\pm 18.4</math> % (k=2)</b> |

|                                                                         |                  |                                                              |
|-------------------------------------------------------------------------|------------------|--------------------------------------------------------------|
| <b>SAR averaged over <math>10\text{ cm}^3</math> (10 g) of Head TSL</b> | condition        |                                                              |
| SAR measured                                                            | 1 W input power  | 0.260 W/kg                                                   |
| SAR for nominal Head TSL parameters                                     | normalized to 1W | <b><math>0.266</math> W/kg <math>\pm 18.0</math> % (k=2)</b> |

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

|                                      |                                   |
|--------------------------------------|-----------------------------------|
| Impedance, transformed to feed point | $51.0 \, \Omega + 6.8 \, j\Omega$ |
| Return Loss                          | - 23.4 dB                         |

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

## DASY5 Validation Report for Head TSL

Date: 09.02.2023

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: CLA13; Type: CLA13; Serial: CLA13 - SN: 1032**

Communication System: UID 0 - CW; Frequency: 13 MHz

Medium parameters used:  $f = 13$  MHz;  $\sigma = 0.72$  S/m;  $\epsilon_r = 52.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(15.33, 15.33, 15.33) @ 13 MHz; Calibrated: 06.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 27.01.2023
- Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2034
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**CLA Calibration for HSL-LF Tissue/CLA-13, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 27.28 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 0.804 W/kg

**SAR(1 g) = 0.411 W/kg; SAR(10 g) = 0.260 W/kg**

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 14 mm)


Ratio of SAR at M2 to SAR at M1 = 79.2%

Maximum value of SAR (measured) = 0.596 W/kg

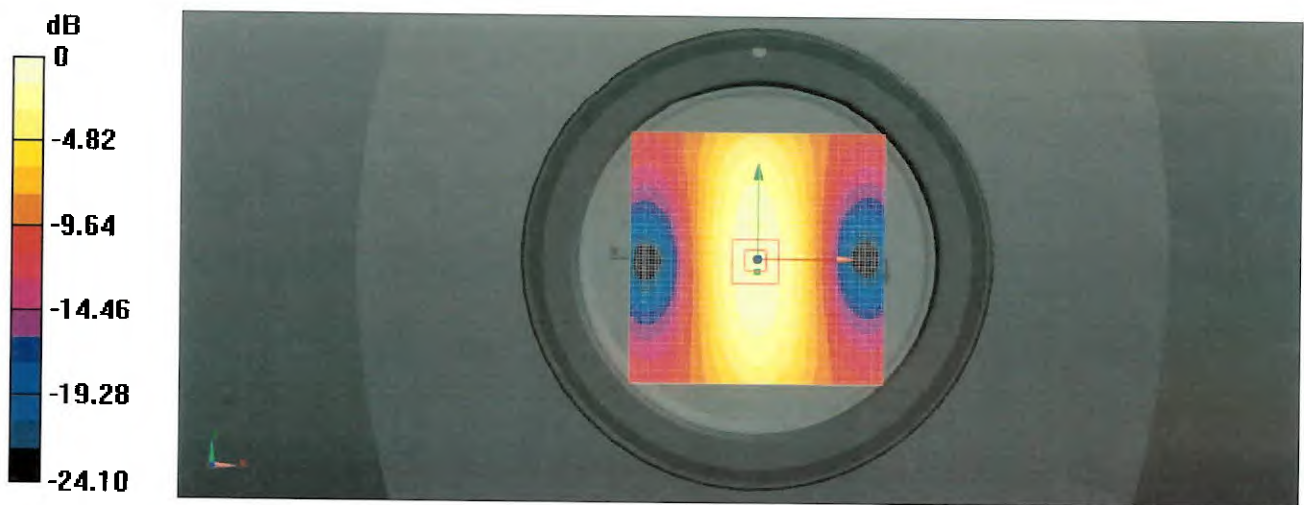

0 dB = 0.596 W/kg = -2.25 dBW/kg

## Impedance Measurement Plot for Head TSL

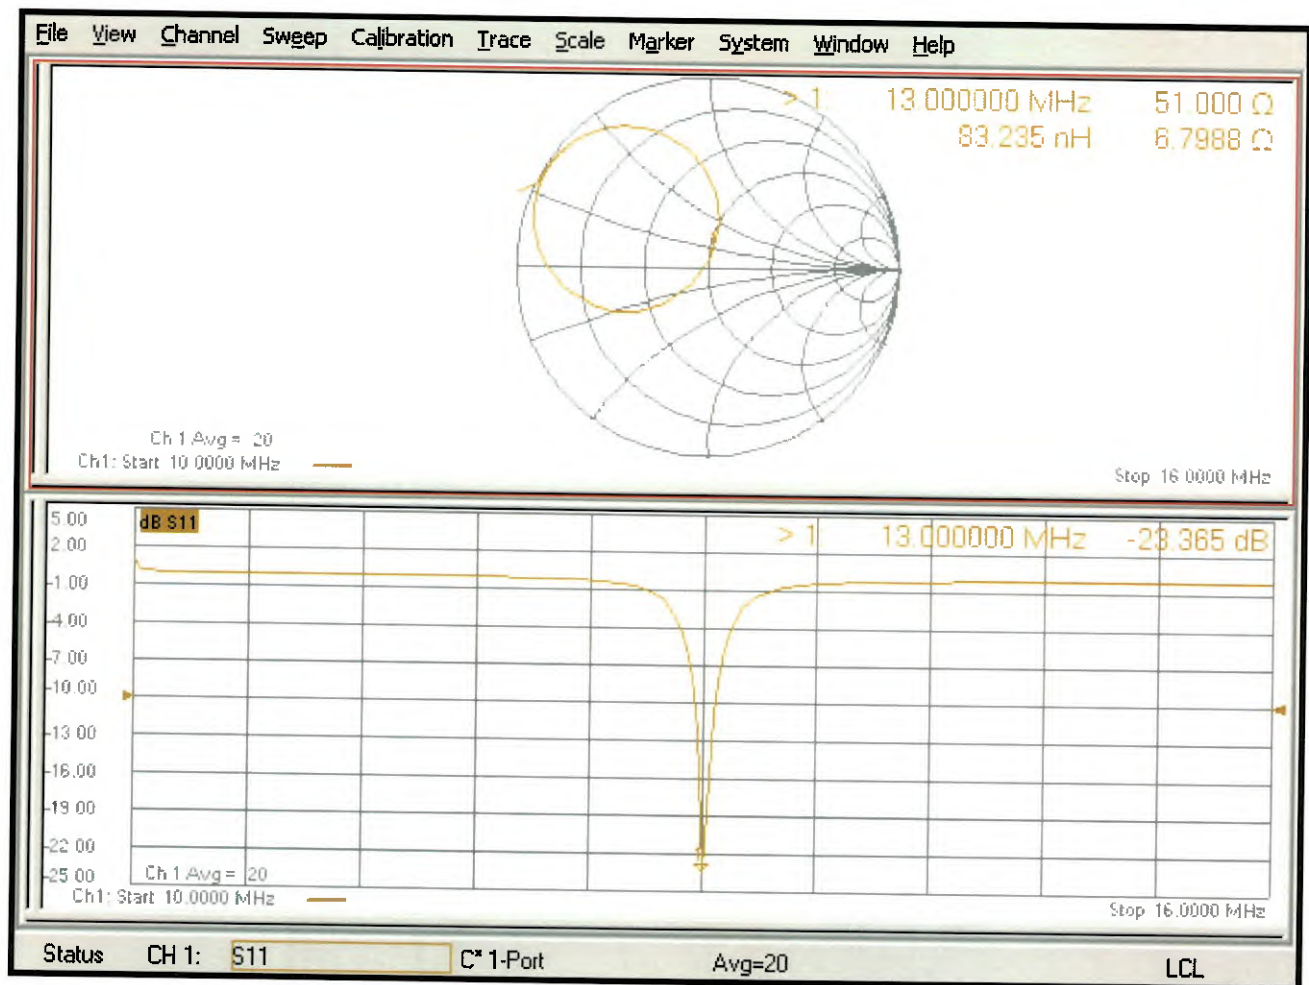

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Client: **SGS**

Certificate No: **25J02Z000195**

## CALIBRATION CERTIFICATE

Object **D750V3 - SN: 1214**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**



Calibration date: **April 1, 2025**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Power sensor NRP6A      | 101369     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Reference Probe EX3DV4  | SN 7307    | 24-May-24(SPEAG, No. EX-7307_May24)       | May-25                |
| DAE4                    | SN 1588    | 13-Sep-24(CTTL-SPEAG, No. 24J02Z000713)   | Sep-25                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 19-Dec-24 (CTTL, No. 24J02X103931)        | Dec-25                |
| NetworkAnalyzer E5071C  | MY46110673 | 18-Dec-24 (CTTL, No. 24J02X103932)        | Dec-25                |
| OCP DAKS                | SN 0015    | 09-Oct-24(SPEAG, No. OCP-DAKS-0015_Oct24) | Oct -25               |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: April 8, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: [cmf@caict.ac.cn](mailto:cmf@caict.ac.cn)

<http://www.caict.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                                     |                          |             |
|-------------------------------------|--------------------------|-------------|
| <b>DASY Version</b>                 | DASY52                   | V52.10.4    |
| <b>Extrapolation</b>                | Advanced Extrapolation   |             |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |             |
| <b>Distance Dipole Center - TSL</b> | 15 mm                    | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |             |
| <b>Frequency</b>                    | 750 MHz $\pm$ 1 MHz      |             |

**Head TSL parameters**

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 41.9           | 0.89 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 42.0 $\pm$ 6 % | 0.91 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —              | —                    |

**SAR result with Head TSL**

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                                |
| SAR measured                                                  | 250 mW input power | 2.17 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>8.54 W/kg <math>\pm</math> 18.8 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.47 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>5.80 W/kg <math>\pm</math> 18.7 % (k=2)</b> |



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 50.7Ω- 3.08jΩ |
| Return Loss                          | - 30.1dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 0.941 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>**DASY5 Validation Report for Head TSL**

Date: 2025-04-01

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1214**

Communication System: UID 0, CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.91$  S/m;  $\epsilon_r = 42.04$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY5 Configuration:**

- Probe: EX3DV4 - SN7307; ConvF(9.25, 9.17, 10.18) @ 750 MHz; Calibrated: 2024-05-28
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1588; Calibrated: 2024-09-13
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 55.64 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 3.07 W/kg

**SAR(1 g) = 2.17 W/kg; SAR(10 g) = 1.47 W/kg**

Smallest distance from peaks to all points 3 dB below = 18 mm

Ratio of SAR at M2 to SAR at M1 = 70.7%

Maximum value of SAR (measured) = 2.80 W/kg

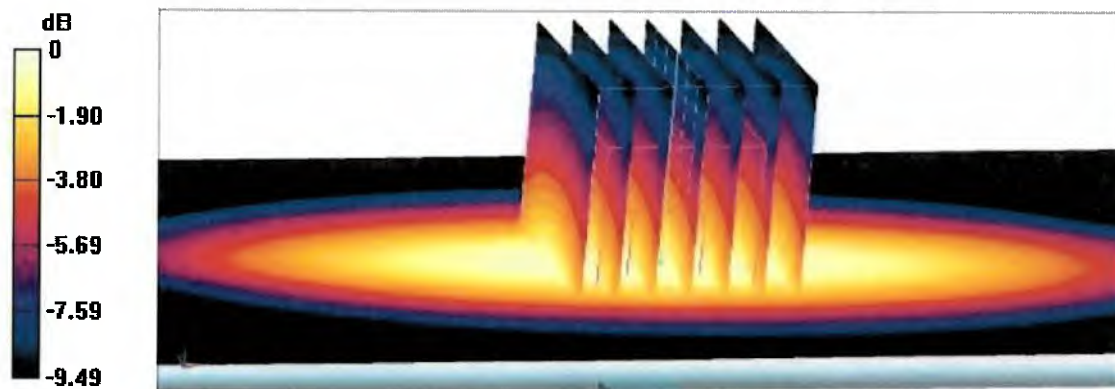


0 dB = 2.80 W/kg = 4.47 dBW/kg



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: [cmf@caict.ac.cn](mailto:cmf@caict.ac.cn) <http://www.caict.ac.cn>

### Impedance Measurement Plot for Head TSL

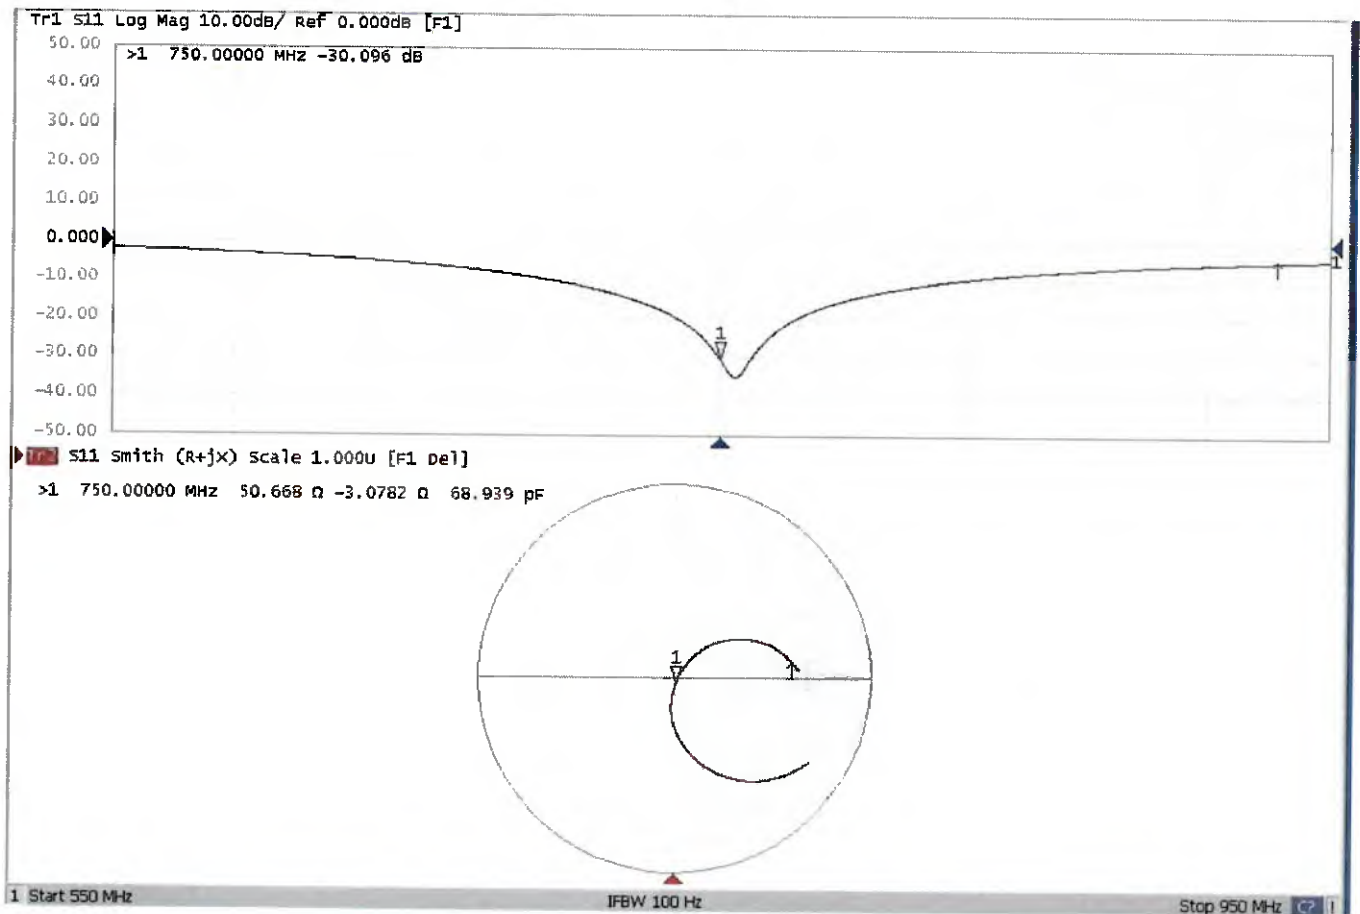

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

Client **SGS**

Certificate No: **J23Z60379**

## CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d161**

Calibration Procedure(s) **FF-Z11-003-01**  
Calibration Procedures for dipole validation kits

Calibration date: **August 25, 2023**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106277     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Power sensor NRP8S      | 104291     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Reference Probe EX3DV4  | SN 3617    | 31-Mar-23(CTTL-SPEAG,No.Z23-60161)        | Mar-24                |
| DAE4                    | SN 1556    | 11-Jan-23(CTTL-SPEAG,No.Z23-60034)        | Jan-24                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 05-Jan-23 (CTTL, No. J23X00107)           | Jan-24                |
| NetworkAnalyzer E5071C  | MY46110673 | 10-Jan-23 (CTTL, No. J23X00104)           | Jan-24                |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: September 1, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |             |
|-------------------------------------|--------------------------|-------------|
| <b>DASY Version</b>                 | DASY52                   | V52.10.4    |
| <b>Extrapolation</b>                | Advanced Extrapolation   |             |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |             |
| <b>Distance Dipole Center - TSL</b> | 15 mm                    | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |             |
| <b>Frequency</b>                    | 835 MHz $\pm$ 1 MHz      |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 41.5           | 0.90 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 42.1 $\pm$ 6 % | 0.90 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | ----           | ----                 |

## SAR result with Head TSL

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| SAR measured                                                  | 250 mW input power | 2.40 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>9.60 W/kg <math>\pm</math> 18.8 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                  | 250 mW input power | 1.54 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>6.16 W/kg <math>\pm</math> 18.7 % (k=2)</b> |

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2117  
 E-mail: emf@caict.ac.cn      http://www.caict.ac.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 50.3Ω- 3.44jΩ |
| Return Loss                          | - 29.3dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.342 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.  
 No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Date: 2023-08-25

**DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d161**

Communication System: UID 0, CW; Frequency: 835 MHz

Medium parameters used:  $f = 835 \text{ MHz}$ ;  $\sigma = 0.904 \text{ S/m}$ ;  $\epsilon_r = 42.11$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(10.1, 10.1, 10.1) @ 835 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$

Reference Value = 57.83 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 3.89 W/kg

**SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.54 W/kg**

Smallest distance from peaks to all points 3 dB below = 17.5 mm

Ratio of SAR at M2 to SAR at M1 = 62.1%

Maximum value of SAR (measured) = 3.34 W/kg

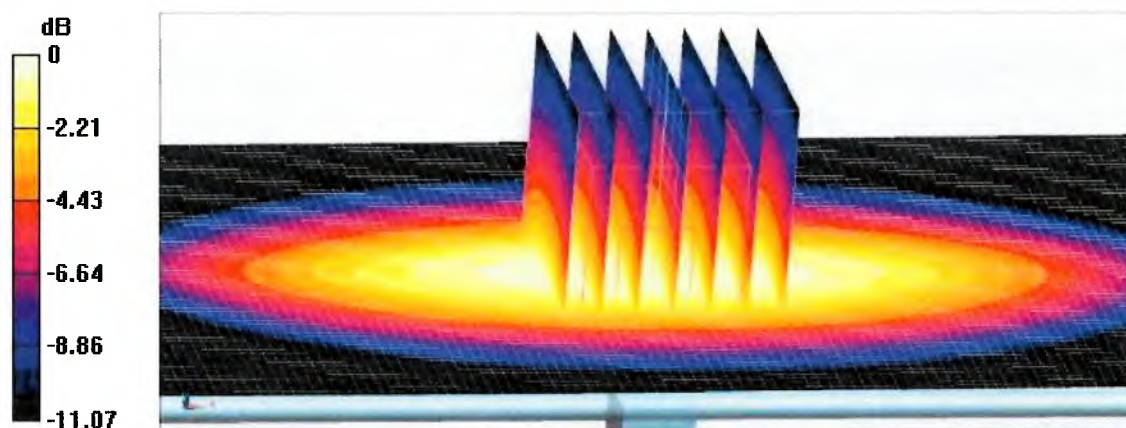

0 dB = 3.34 W/kg = 5.24 dBW/kg




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## Impedance Measurement Plot for Head TSL

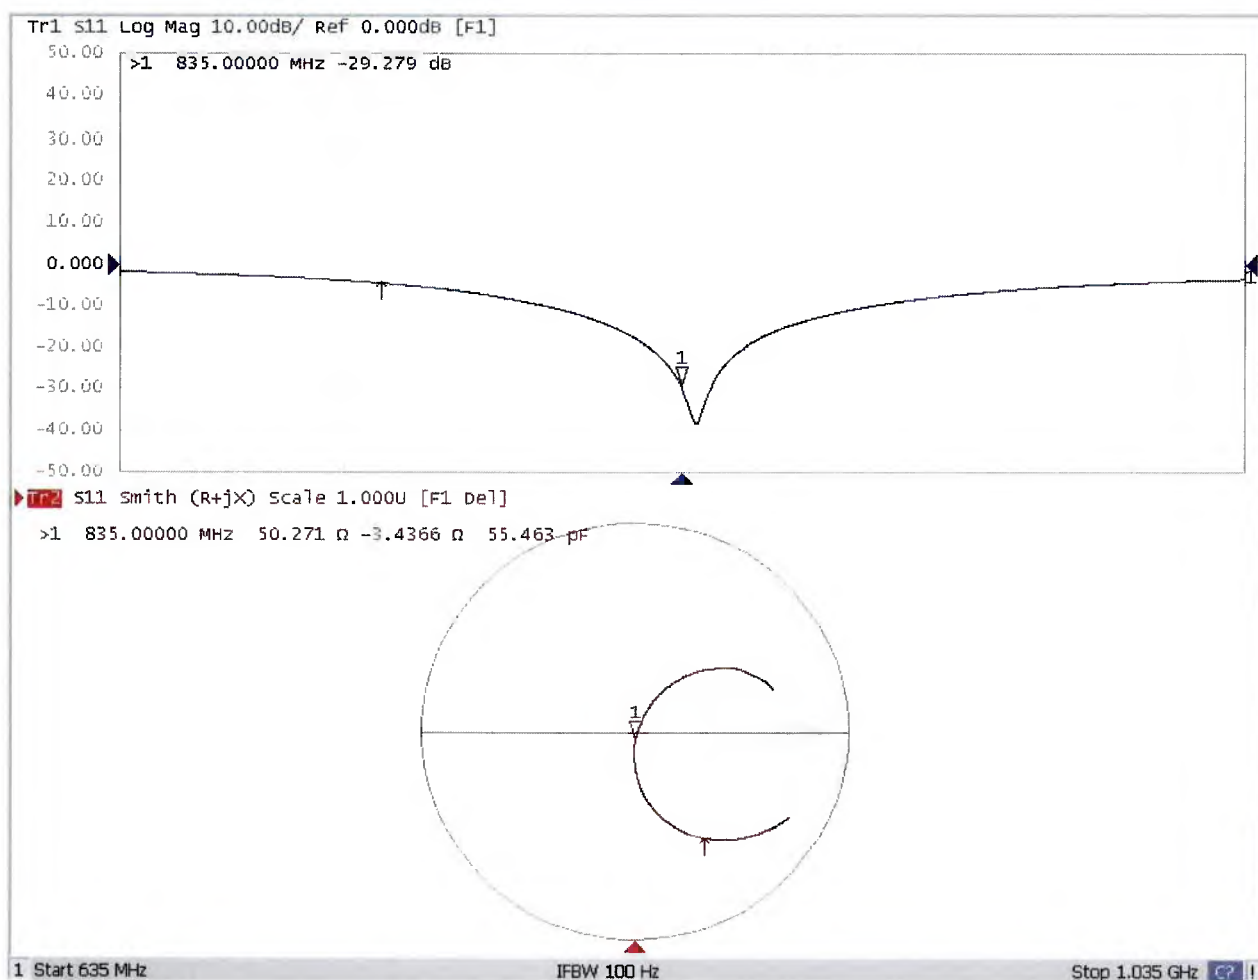

Client **SGS**

Certificate No: **23J02Z80118**

## CALIBRATION CERTIFICATE

Object **D1750V2 - SN: 1105**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**

Calibration date: **November 3, 2023**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.


All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 15-May-23 (CTTL, No.J23X04183)            | May-24                |
| Power sensor NRP6A      | 101369     | 15-May-23 (CTTL, No.J23X04183)            | May-24                |
| Reference Probe EX3DV4  | SN 7464    | 19-Jan-23(CTTL-SPEAG,No.Z22-60565)        | Jan-24                |
| DAE4                    | SN 1556    | 11-Jan-23(CTTL-SPEAG,No.Z23-60034)        | Jan-24                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 05-Jan-23 (CTTL, No. J23X00107)           | Jan-24                |
| Network Analyzer E5071C | MY46110673 | 10-Jan-23 (CTTL, No. J23X00104)           | Jan-24                |

|                | Name        | Function           |
|----------------|-------------|--------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |

Signature



Issued: November 7, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: cmf@caict.ac.cn <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |             |
|-------------------------------------|--------------------------|-------------|
| <b>DASY Version</b>                 | DASY52                   | 52.10.4     |
| <b>Extrapolation</b>                | Advanced Extrapolation   |             |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |             |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |             |
| <b>Frequency</b>                    | 1750 MHz $\pm$ 1 MHz     |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 40.1           | 1.37 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 41.2 $\pm$ 6 % | 1.36 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | ---            | ---                  |

## SAR result with Head TSL

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                              |
|---------------------------------------------------------------|--------------------|------------------------------|
| SAR measured                                                  | 250 mW input power | 8.99 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 36.3 W/kg $\pm$ 18.8 % (k=2) |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                              |
| SAR measured                                                  | 250 mW input power | 4.80 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 19.3 W/kg $\pm$ 18.7 % (k=2) |



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 47.8Ω- 2.61jΩ |
| Return Loss                          | - 29.1dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.125 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DASY5 Validation Report for Head TSL

Date: 2023-11-03

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1105**

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 41.18$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8.54, 8.54, 8.54) @ 1750 MHz; Calibrated: 2023-01-19
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 92.17 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 16.6 W/kg

**SAR(1 g) = 8.99 W/kg; SAR(10 g) = 4.8 W/kg**

Smallest distance from peaks to all points 3 dB below = 9.8 mm

Ratio of SAR at M2 to SAR at M1 = 54.8%


Maximum value of SAR (measured) = 13.8 W/kg

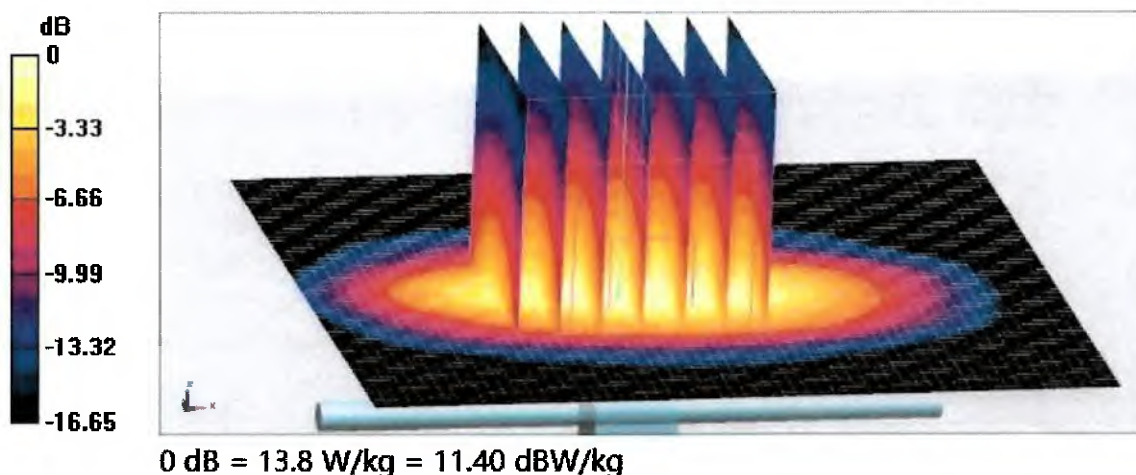



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

### Impedance Measurement Plot for Head TSL

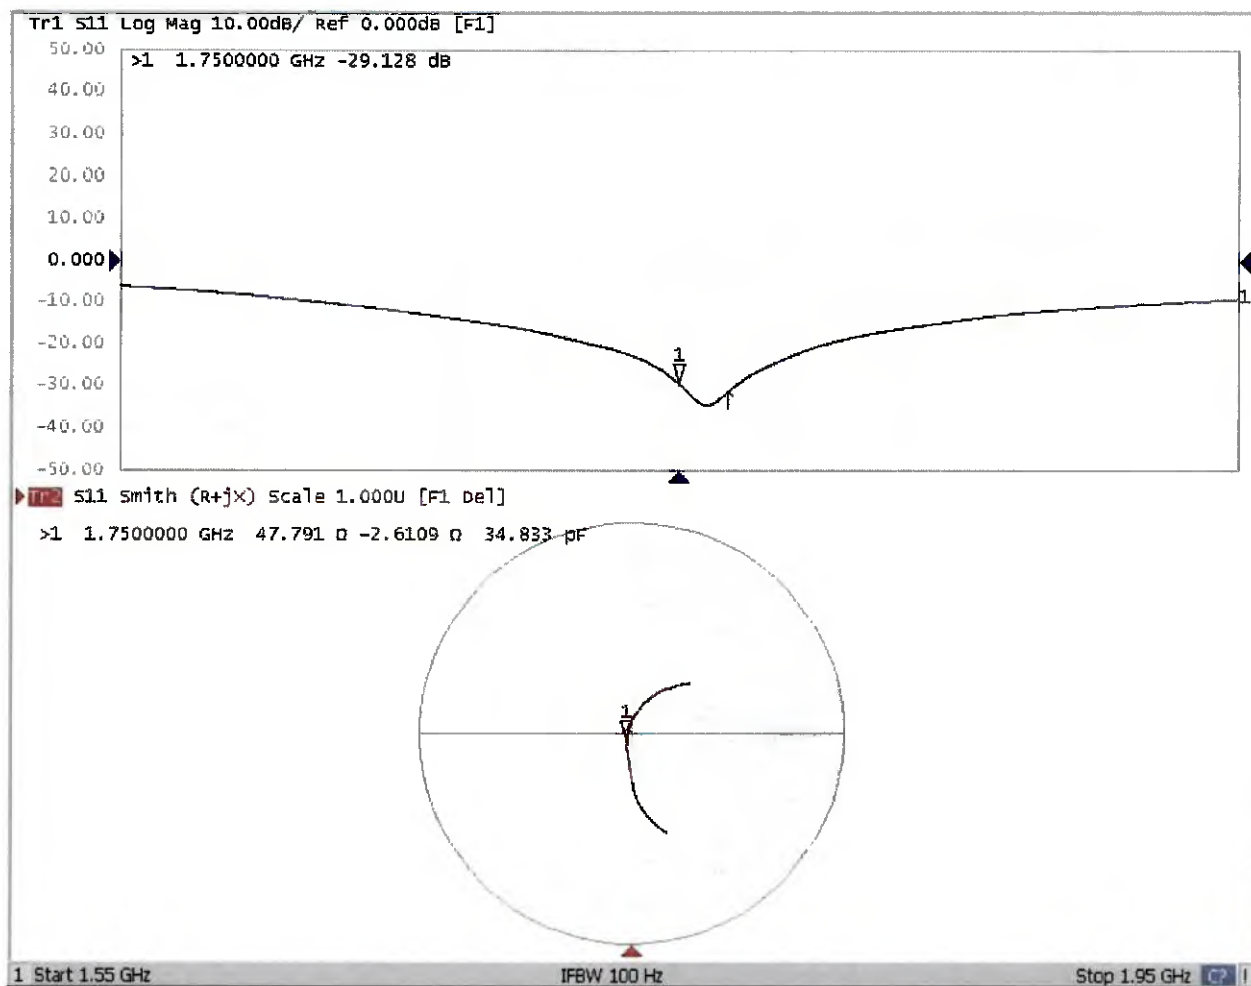

Client **SGS**

Certificate No: **J23Z60228**

## CALIBRATION CERTIFICATE

Object **D1950V3 - SN: 1218**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**



Calibration date: **May 4, 2023**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 10-May-22 (CTTL, No.J22X03103)            | May-23                |
| Power sensor NRP6A      | 101369     | 10-May-22 (CTTL, No.J22X03103)            | May-23                |
| Reference Probe EX3DV4  | SN 7517    | 27-Jan-23(SPEAG,No.EX3-7517_Jan23)        | Jan-24                |
| DAE4                    | SN 1556    | 11-Jan-23(CTTL-SPEAG,No.Z23-60034)        | Jan-24                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49070393 | 17-May-22 (CTTL, No.J22X03157)            | May-23                |
| Network Analyzer E5071C | MY46110673 | 10-Jan-23 (CTTL, No. J23X00104)           | Jan-24                |

|                |             |                    |                                                                                       |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
|                | <b>Name</b> | <b>Function</b>    | <b>Signature</b>                                                                      |
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: May 8, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62302117  
E-mail: cttl@chinattl.com      <http://www.caict.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62302117  
E-mail: cttl@chinattl.com <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |             |
|-------------------------------------|--------------------------|-------------|
| <b>DASY Version</b>                 | DASY52                   | 52.10.4     |
| <b>Extrapolation</b>                | Advanced Extrapolation   |             |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |             |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |             |
| <b>Frequency</b>                    | 1950 MHz $\pm$ 1 MHz     |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 40.0           | 1.40 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 40.6 $\pm$ 6 % | 1.41 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —              | —                    |

## SAR result with Head TSL

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| SAR measured                                                  | 250 mW input power | 10.1 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>40.4 W/kg <math>\pm</math> 18.8 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                  | 250 mW input power | 5.19 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>20.8 W/kg <math>\pm</math> 18.7 % (k=2)</b> |

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62302117  
E-mail: [ctl@chinattl.com](mailto:ctl@chinattl.com) <http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 48.0Ω- 4.71jΩ |
| Return Loss                          | - 25.6dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.106 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62302117  
E-mail: cttl@chinattl.com <http://www.caict.ac.cn>

**DASY5 Validation Report for Head TSL**

Date: 2023-05-04

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 1950 MHz; Type: D1950V3; Serial: D1950V3 - SN: 1218**

Communication System: UID 0, CW; Frequency: 1950 MHz

Medium parameters used:  $f = 1950$  MHz;  $\sigma = 1.409$  S/m;  $\epsilon_r = 40.57$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

**DASY5 Configuration:**

- Probe: EX3DV4 - SN7517; ConvF(8.05, 7.46, 7.73) @ 1950 MHz; Calibrated: 2023-01-27
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 99.61 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 18.7 W/kg

**SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.19 W/kg**

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 54.6%


Maximum value of SAR (measured) = 15.8 W/kg

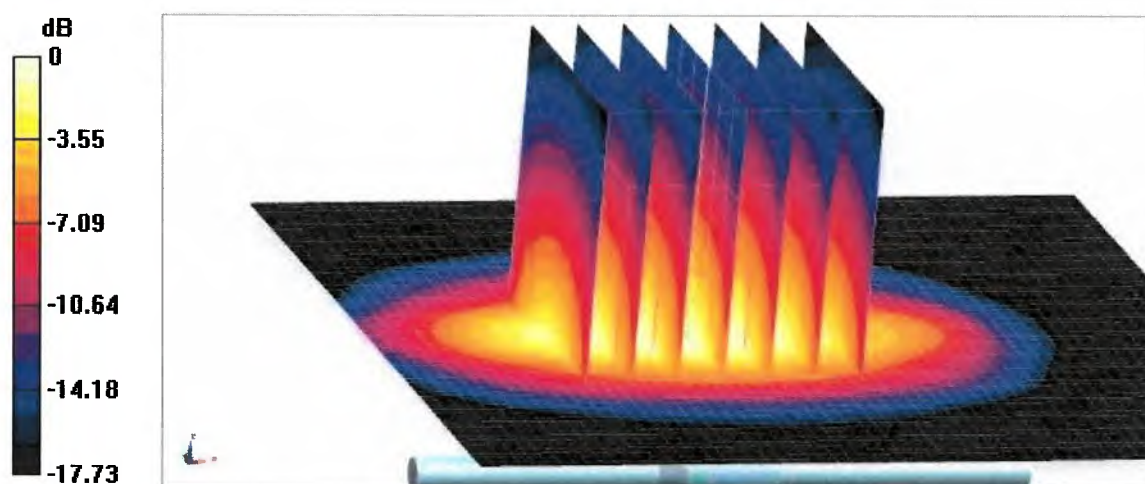

0 dB = 15.8 W/kg = 11.99 dBW/kg

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62302117  
 E-mail: cttl@chinattl.com      <http://www.caict.ac.cn>

## Impedance Measurement Plot for Head TSL

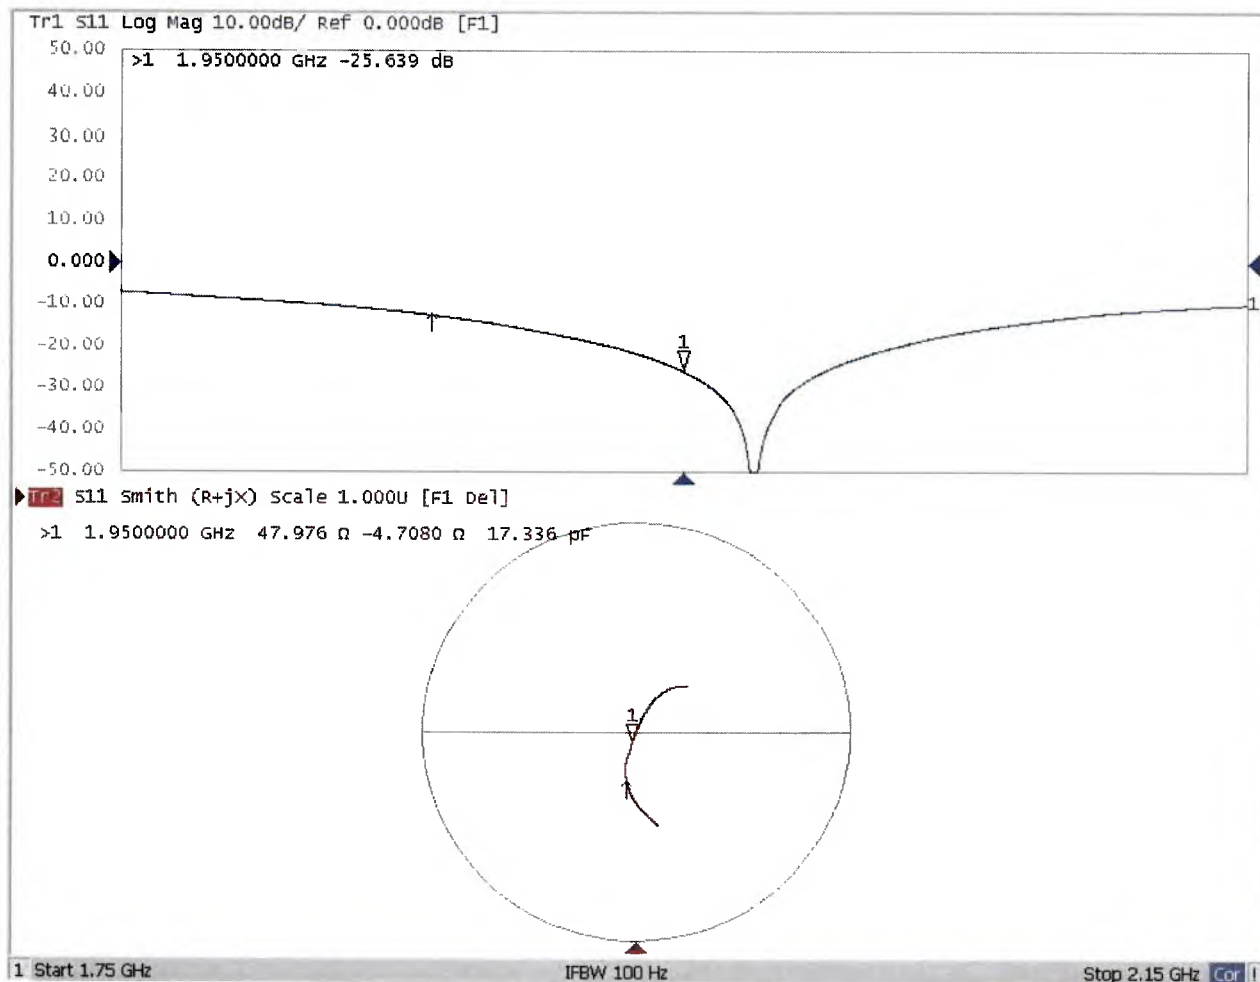

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191  
Tel: +86-10-62304633-2117  
E-mail: cttl@chinattl.com      http://www.caict.ac.cn

Client      **SGS**

Certificate No:      **J23Z60380**

## CALIBRATION CERTIFICATE

Object      D2450V2 - SN: 922

Calibration Procedure(s)      FF-Z11-003-01  
Calibration Procedures for dipole validation kits


Calibration date:      August 28, 2023

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106277     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Power sensor NRP8S      | 104291     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Reference Probe EX3DV4  | SN 3617    | 31-Mar-23(CTTL-SPEAG,No.Z23-60161)        | Mar-24                |
| DAE4                    | SN 1556    | 11-Jan-23(CTTL-SPEAG,No.Z23-60034)        | Jan-24                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 05-Jan-23 (CTTL, No. J23X00107)           | Jan-24                |
| NetworkAnalyzer E5071C  | MY46110673 | 10-Jan-23 (CTTL, No. J23X00104)           | Jan-24                |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: September 1, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: cttl@chinattl.com

http://www.caict.ac.cn

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: cttl@chinattl.com      <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                          |             |
|-------------------------------------|--------------------------|-------------|
| <b>DASY Version</b>                 | DASY52                   | 52.10.4     |
| <b>Extrapolation</b>                | Advanced Extrapolation   |             |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |             |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with Spacer |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |             |
| <b>Frequency</b>                    | 2450 MHz $\pm$ 1 MHz     |             |

## Head TSL parameters

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 39.2           | 1.80 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 39.0 $\pm$ 6 % | 1.84 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | ---            | ---                  |

## SAR result with Head TSL

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| SAR measured                                                  | 250 mW input power | 13.3 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>52.7 W/kg <math>\pm</math> 18.8 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                  | 250 mW input power | 6.19 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>24.6 W/kg <math>\pm</math> 18.7 % (k=2)</b> |



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: cttl@chinattl.com      <http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 53.2Ω+ 5.45jΩ |
| Return Loss                          | - 24.3dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.068 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: cttl@chinattl.com <http://www.caict.ac.cn>

## DASY5 Validation Report for Head TSL

Date: 2023-08-28

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 922**

Communication System: UID 0, CW; Frequency: 2450 MHz

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.835$  S/m;  $\epsilon_r = 39.03$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(7.68, 7.68, 7.68) @ 2450 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.74 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 27.6 W/kg

**SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.19 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 49.1%


Maximum value of SAR (measured) = 22.1 W/kg

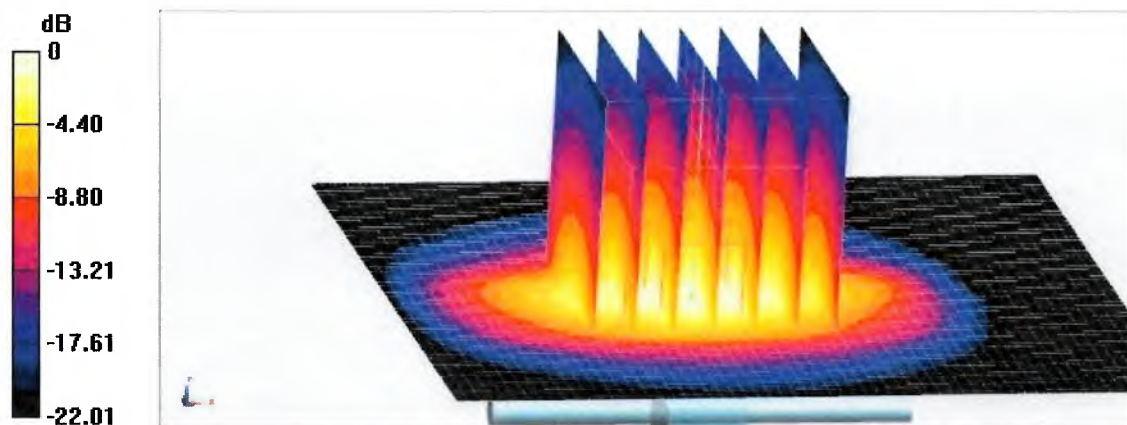

0 dB = 22.1 W/kg = 13.44 dBW/kg

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2117  
 E-mail: cttl@chinattl.com      http://www.caict.ac.cn

## Impedance Measurement Plot for Head TSL

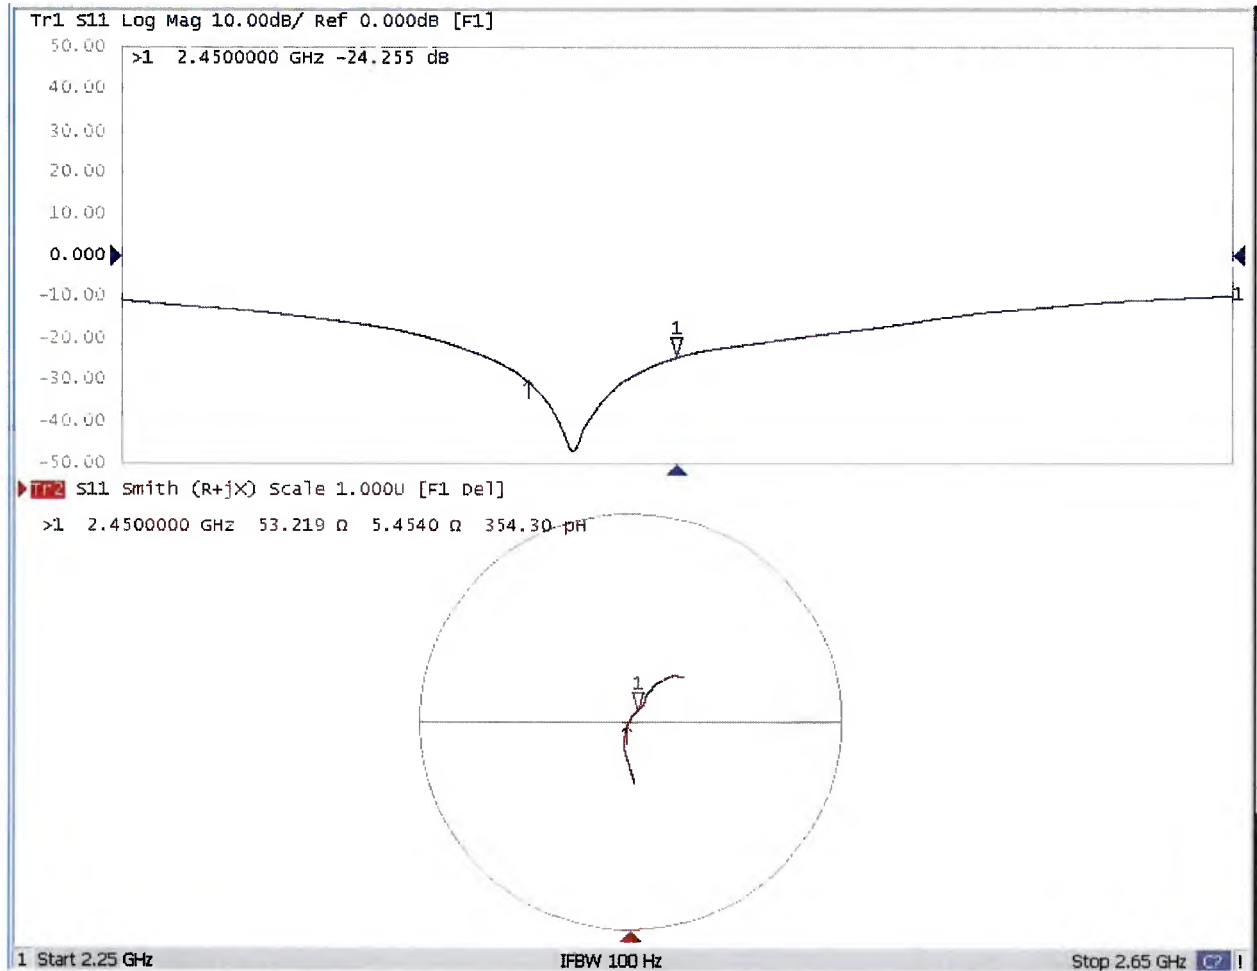

Client: **SGS**

Certificate No: **25J02Z000198**

## CALIBRATION CERTIFICATE

Object **D2600V2 - SN: 1158**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**


Calibration date: **March 31, 2025**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Power sensor NRP6A      | 101369     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Reference Probe EX3DV4  | SN 7307    | 24-May-24(SPEAG, No. EX-7307_May24)       | May-25                |
| DAE4                    | SN 1588    | 13-Sep-24(CTTL-SPEAG, No. 24J02Z000713)   | Sep-25                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 19-Dec-24 (CTTL, No. 24J02X103931)        | Dec-25                |
| NetworkAnalyzer E5071C  | MY46110673 | 18-Dec-24 (CTTL, No. 24J02X103932)        | Dec-25                |
| OCP DAKS                | SN 0015    | 09-Oct-24(SPEAG, No. OCP-DAKS-0015_Oct24) | Oct -25               |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: April 8, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: cmf@caict.ac.cn

<http://www.caict.ac.cn>**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

|                                     |                          |                |
|-------------------------------------|--------------------------|----------------|
| <b>DASY Version</b>                 | <b>DASY52</b>            | <b>52.10.4</b> |
| <b>Extrapolation</b>                | Advanced Extrapolation   |                |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C |                |
| <b>Distance Dipole Center - TSL</b> | 10 mm                    | with Spacer    |
| <b>Zoom Scan Resolution</b>         | dx, dy, dz = 5 mm        |                |
| <b>Frequency</b>                    | 2600 MHz $\pm$ 1 MHz     |                |

**Head TSL parameters**

The following parameters and calculations were applied.

|                                                | <b>Temperature</b>  | <b>Permittivity</b> | <b>Conductivity</b>  |
|------------------------------------------------|---------------------|---------------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 39.0                | 1.96 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 39.2 $\pm$ 6 %      | 1.97 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —                   | —                    |

**SAR result with Head TSL**

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | <b>Condition</b>   |                                                |
| SAR measured                                                  | 250 mW input power | 13.8 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>55.2 W/kg <math>\pm</math> 18.8 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | <b>Condition</b>   |                                                |
| SAR measured                                                  | 250 mW input power | 6.18 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>24.7 W/kg <math>\pm</math> 18.7 % (k=2)</b> |



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 46.9Ω- 5.43jΩ |
| Return Loss                          | - 23.8dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.054 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caict.ac.cn

**DASY5 Validation Report for Head TSL**

Date: 2025-03-31

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1158**

Communication System: UID 0, CW; Frequency: 2600 MHz

Medium parameters used:  $f = 2600$  MHz;  $\sigma = 1.967$  S/m;  $\epsilon_r = 39.15$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.22, 7.19, 7.78) @ 2600 MHz; Calibrated: 2024-05-28
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1588; Calibrated: 2024-09-13
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:  $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm**

Reference Value = 106.2 V/m; Power Drift = 0.00 dB


Peak SAR (extrapolated) = 28.4 W/kg

**SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.18 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.2 mm

Ratio of SAR at M2 to SAR at M1 = 49.5%

Maximum value of SAR (measured) = 22.8 W/kg

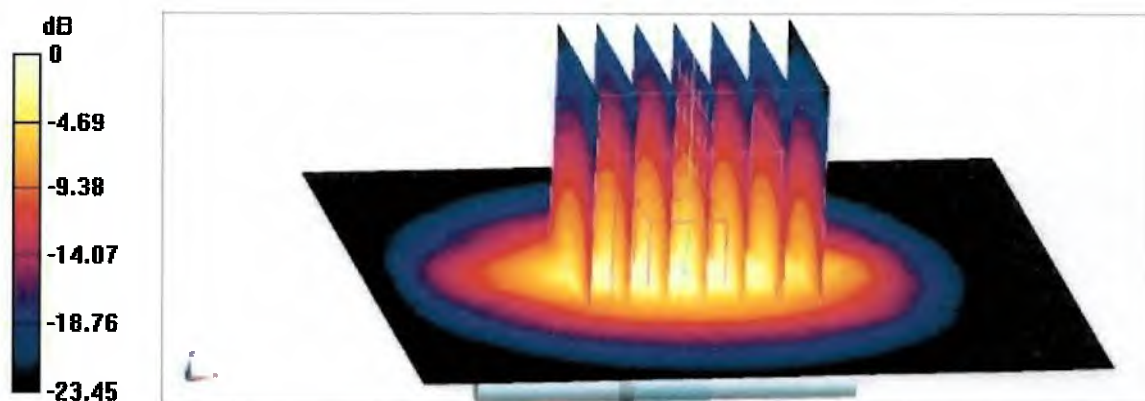

0 dB = 22.8 W/kg = 13.58 dBW/kg




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## Impedance Measurement Plot for Head TSL

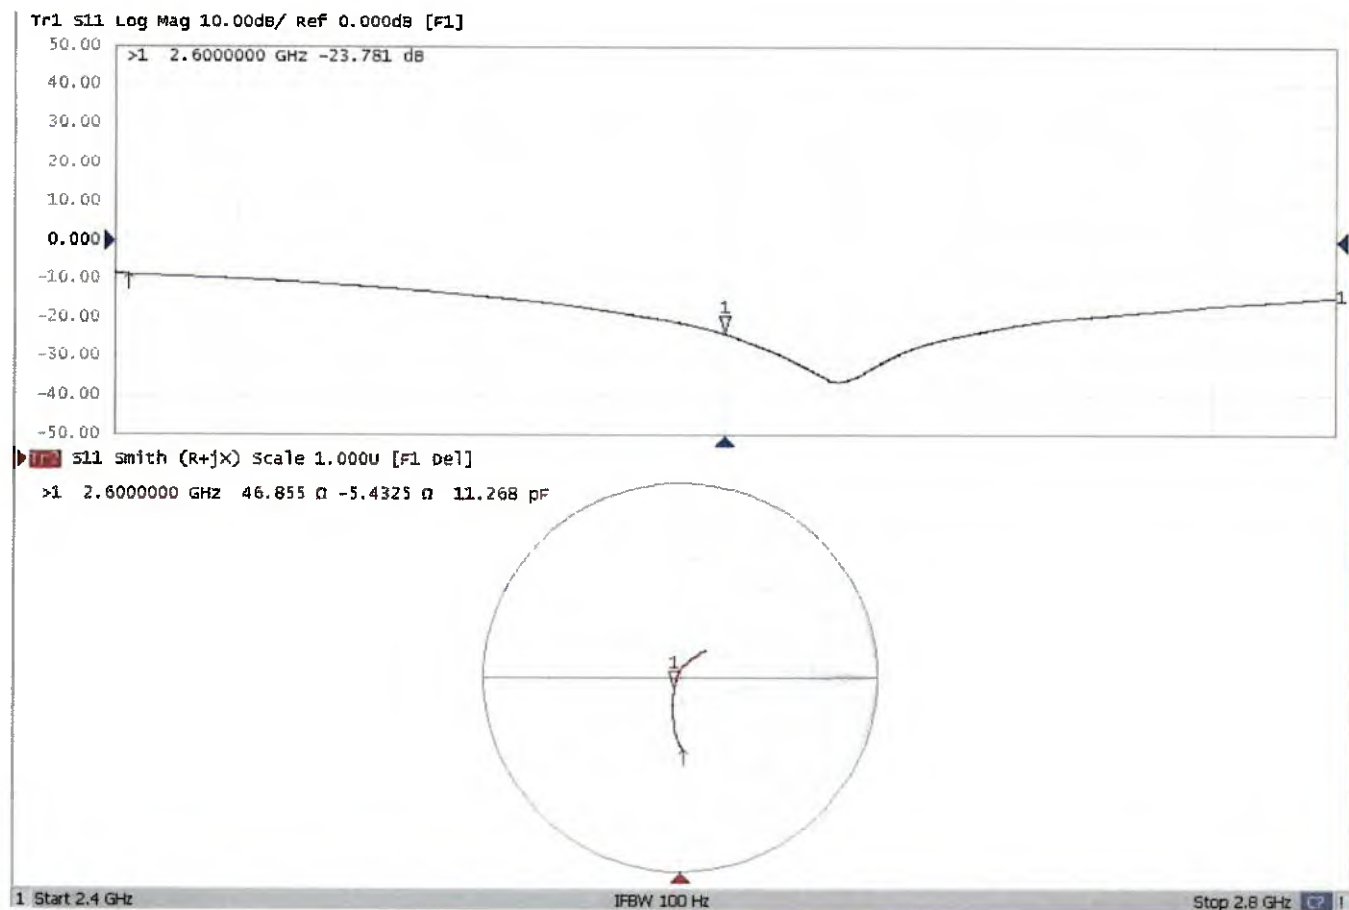



Accredited by the Swiss Accreditation Service (SAS)  
**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 0108**

Client

**Auden**  
Taoyuan City

Certificate No.

**D3500V2-1067\_Jan25**

## CALIBRATION CERTIFICATE

Object

**D3500V2 - SN: 1067**

Calibration procedure(s)

**QA CAL-22.v7**  
**Calibration Procedure for SAR Validation Sources between 3 - 10 GHz**

Calibration date

**January 16, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 22-Jul-24 (No. 4030A315008547)         | Jul-25        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 25-Jan-24 (No. 4030-315007551)         | Jan-25        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               |                  |                       |
|---------------|------------------|-----------------------|
|               | Name             | Function              |
| Calibrated by | Krešimir Franjić | Laboratory Technician |
| Approved by   | Sven Kühn        | Technical Manager     |

Signature

Issued: January 16, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

## Calibration Laboratory of

Schmid & Partner  
Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                          |                                     |
|-------------------------------------|------------------------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR                         | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation                   |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom                     |                                     |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                    | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 5mm, dz = 1.4mm                 | Graded Ratio = 1.5 mm (Z direction) |
| <b>Frequency</b>                    | 3400MHz $\pm$ 1MHz<br>3500MHz $\pm$ 1MHz |                                     |

## Head TSL parameters at 3400 MHz

The following parameters and calculations were applied.

|                                                | Temperature        | Permittivity  | Conductivity        |
|------------------------------------------------|--------------------|---------------|---------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C            | 38.0          | 2.81 mho/m          |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2)°C | 38.1 $\pm$ 6% | 2.85 mho/m $\pm$ 6% |
| <b>Head TSL temperature change during test</b> | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 3400 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                               |
|-------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                         | 20 dBm input power | 6.86 W/kg                     |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | 68.6 W/kg $\pm$ 19.9% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                               |
|---------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                           | 20 dBm input power | 2.61 W/kg                     |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 26.1 W/kg $\pm$ 19.5% (k = 2) |

**Head TSL parameters at 3500 MHz**

The following parameters and calculations were applied.

|                                         | Temperature   | Permittivity | Conductivity   |
|-----------------------------------------|---------------|--------------|----------------|
| Nominal Head TSL parameters             | 22.0 °C       | 37.9         | 2.91 mho/m     |
| Measured Head TSL parameters            | (22.0 ±0.2)°C | 37.9 ±6%     | 2.93 mho/m ±6% |
| Head TSL temperature change during test | < 0.5 °C      |              |                |

**SAR result with Head TSL at 3500 MHz**

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                          |
|-------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                   | 20 dBm input power | 6.45 W/kg                |
| SAR for nominal Head TSL parameters                   | normalized to 1W   | 64.5 W/kg ±19.9% (k = 2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | Condition          |                          |
|---------------------------------------------------------|--------------------|--------------------------|
| SAR for nominal Head TSL parameters                     | 20 dBm input power | 2.45 W/kg                |
| SAR for nominal Head TSL parameters                     | normalized to 1W   | 24.5 W/kg ±19.5% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 3400 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 44.0 $\Omega$ – 5.6 j $\Omega$ |
| Return Loss | -21.2 dB                       |

**Antenna Parameters with Head TSL at 3500 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 51.8 $\Omega$ – 3.1 j $\Omega$ |
| Return Loss | -29.2 dB                       |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.137 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

|                  |                 |     |             |
|------------------|-----------------|-----|-------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
| D3500V2 - SN1067 | 3400            | HSL | 20          |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat                 | 10                 |      | CW, 0--    | 3400, 0                         | 6.55              | 2.85                   | 38.1             |

Hardware Setup

|                 |                    |                             |                           |
|-----------------|--------------------|-----------------------------|---------------------------|
| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
| MFP V8.0 Center | HSL, 2025-01-16    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     |                 |
|---------------------|-----------------|
|                     | Zoom Scan       |
| Grid Extents [mm]   | 28 x 28 x 28    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |

Measurement Results

|                     |                     |
|---------------------|---------------------|
|                     | Zoom Scan           |
| Date                | 2025-01-16          |
| psSAR1g [W/Kg]      | 6.86                |
| psSAR10g [W/Kg]     | 2.61                |
| Power Drift [dB]    | -0.04               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |



0 dB = 17.7 W/Kg

System Performance Check Report

Summary

|                  |                 |     |             |
|------------------|-----------------|-----|-------------|
| Dipole           | Frequency [MHz] | TSL | Power [dBm] |
| D3500V2 - SN1067 | 3500            | HSL | 20          |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat                 | 10                 |      | CW, 0--    | 3500, 0                         | 6.63              | 2.93                   | 37.9             |

Hardware Setup

|                 |                    |                             |                           |
|-----------------|--------------------|-----------------------------|---------------------------|
| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
| MFP V8.0 Center | HSL, 2025-01-16    | EX3DV4 - SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup

|                     |                 |
|---------------------|-----------------|
|                     | Zoom Scan       |
| Grid Extents [mm]   | 28 x 28 x 28    |
| Grid Steps [mm]     | 5.0 x 5.0 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.5             |
| MAIA                | N/A             |
| Surface Detection   | VMS + 6p        |
| Scan Method         | Measured        |


Measurement Results

|                     |                     |
|---------------------|---------------------|
|                     | Zoom Scan           |
| Date                | 2025-01-16          |
| psSAR1g [W/Kg]      | 6.45                |
| psSAR10g [W/Kg]     | 2.45                |
| Power Drift [dB]    | 0.00                |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |



0 dB = 16.8 W/Kg

## Impedance Measurement Plot for Head TSL

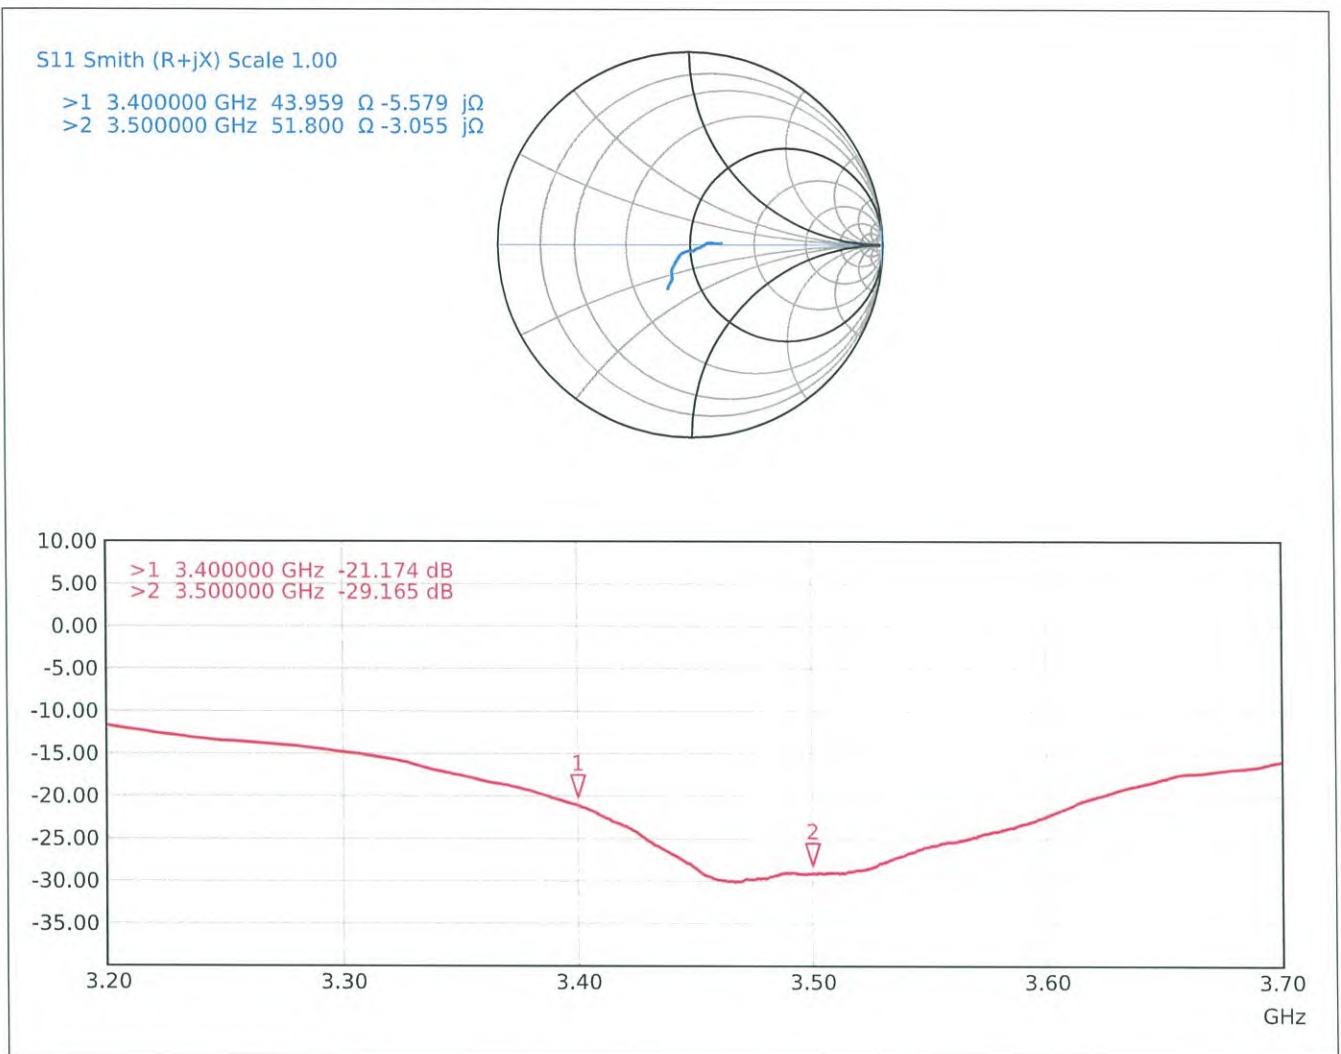

Client **SGS**

Certificate No: **25J02Z000200**

## CALIBRATION CERTIFICATE

Object **D3700V2 - SN: 1108**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**


Calibration date: **April 1, 2025**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Power sensor NRP6A      | 101369     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Reference Probe EX3DV4  | SN 7307    | 24-May-24(SPEAG, No. EX-7307_May24)       | May-25                |
| DAE4                    | SN 1588    | 13-Sep-24(CTTL-SPEAG, No. 24J02Z000713)   | Sep-25                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 19-Dec-24 (CTTL, No. 24J02X103931)        | Dec-25                |
| NetworkAnalyzer E5071C  | MY46110673 | 18-Dec-24 (CTTL, No. 24J02X103932)        | Dec-25                |
| OCP DAKS                | SN 0015    | 09-Oct-24(SPEAG, No. OCP-DAKS-0015_Oct24) | Oct -25               |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: April 8, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a k**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2117  
 E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                            |                                  |
|-------------------------------------|----------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY52                     | 52.10.4                          |
| <b>Extrapolation</b>                | Advanced Extrapolation     |                                  |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C   |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                      | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4 mm, dz = 1.4 mm | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 3700 MHz $\pm$ 1 MHz       |                                  |

## Head TSL parameters at 3700 MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.7           | 3.12 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 38.0 $\pm$ 6 % | 3.07 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —              | —                    |

## SAR result with Head TSL at 3700 MHz

|                                                               |                    |                              |
|---------------------------------------------------------------|--------------------|------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                              |
| SAR measured                                                  | 100 mW input power | 6.53 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 65.6 W/kg $\pm$ 24.4 % (k=2) |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                              |
| SAR measured                                                  | 100 mW input power | 2.40 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 24.1 W/kg $\pm$ 24.2 % (k=2) |



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 3700 MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 44.3Ω+ 3.82jΩ |
| Return Loss                          | - 22.8dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.039 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## DASY5 Validation Report for Head TSL

Date: 2025-04-01

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 3700 MHz; Type: D3700V2; Serial: D3700V2 - SN: 1108**

Communication System: UID 0, CW; Frequency: 3700 MHz;

Medium parameters used:  $f = 3700$  MHz;  $\sigma = 3.067$  S/m;  $\epsilon_r = 37.96$ ;  $\rho = 1000$  kg/m<sup>3</sup>


Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(6.21, 6.24, 6.72) @ 3700 MHz;  
Calibrated: 2024-05-28
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1588; Calibrated: 2024-09-13
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial:  
1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration /Pin=100mW, d=10mm, f=3700 MHz/Zoom Scan,**  
**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
Reference Value = 65.57 V/m; Power Drift = -0.06 dB  
Peak SAR (extrapolated) = 17.2 W/kg  
**SAR(1 g) = 6.53 W/kg; SAR(10 g) = 2.4 W/kg**  
Smallest distance from peaks to all points 3 dB below = 7.9 mm  
Ratio of SAR at M2 to SAR at M1 = 76%  
Maximum value of SAR (measured) = 12.2 W/kg

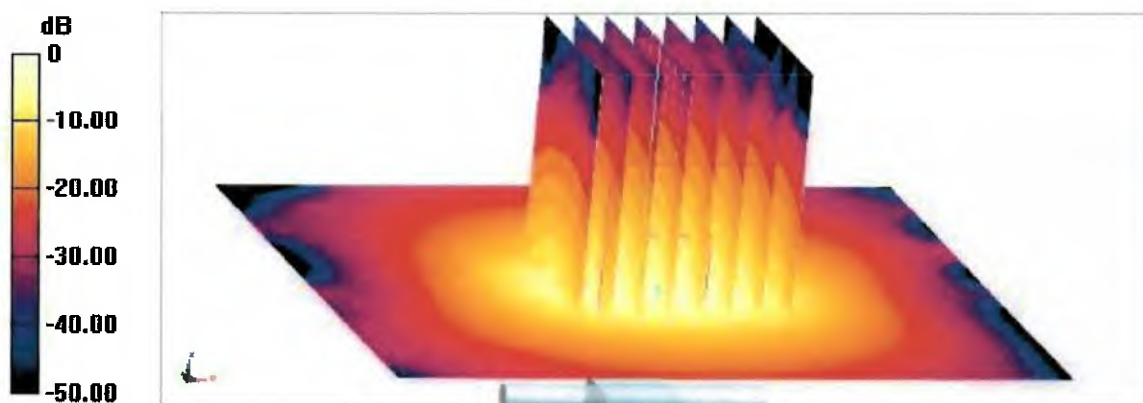


0 dB = 12.2 W/kg = 10.86 dBW/kg



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Impedance Measurement Plot for Head TSL

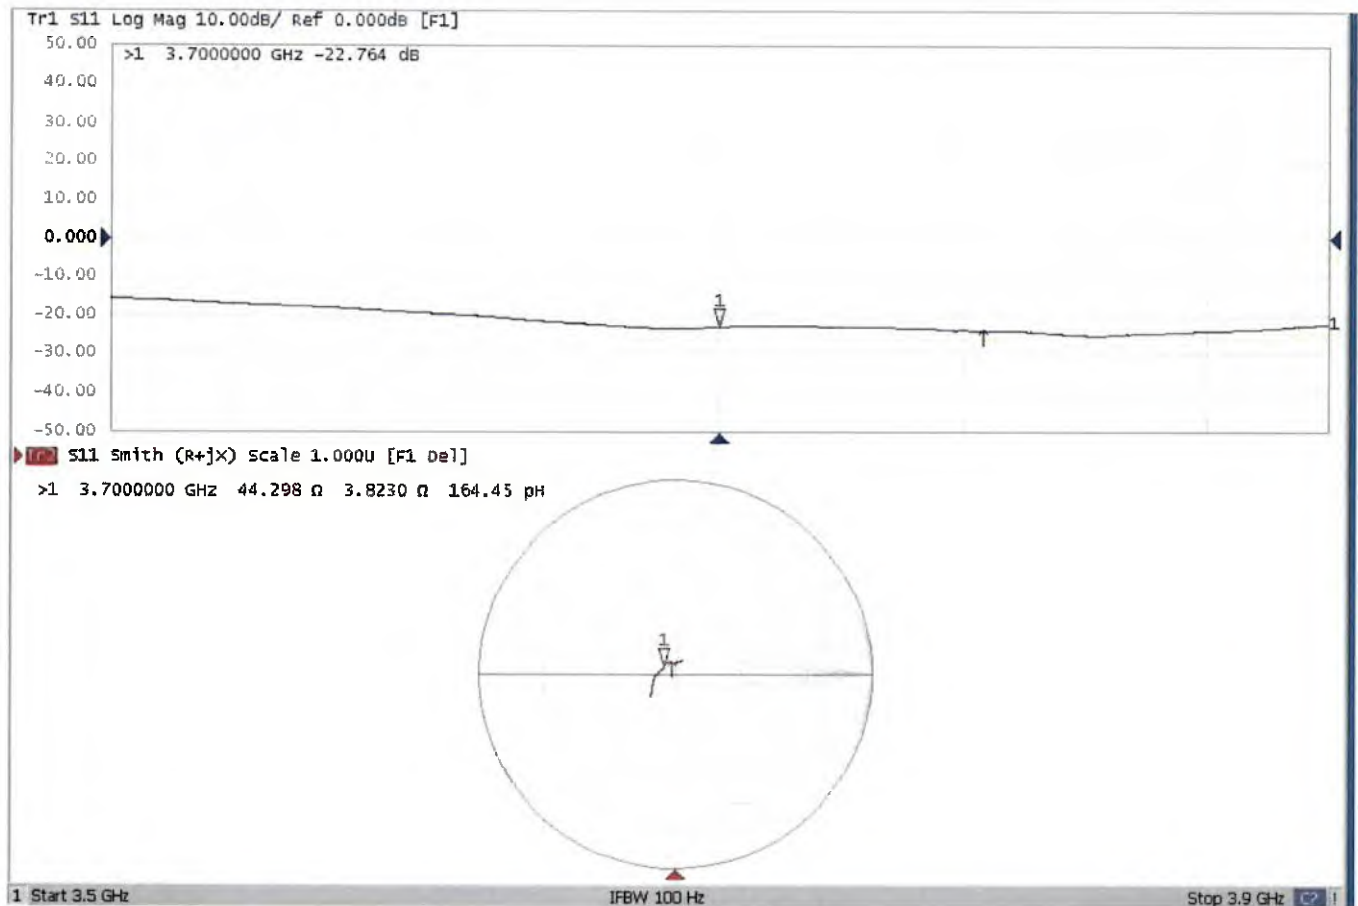

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn      <http://www.caict.ac.cn>

Client      **SGS**

Certificate No:      **25J02Z000201**

## CALIBRATION CERTIFICATE

Object      **D3900V2 - SN: 1083**

Calibration Procedure(s)      **FF-Z11-003-01**  
Calibration Procedures for dipole validation kits


Calibration date:      **March 31, 2025**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106276     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Power sensor NRP6A      | 101369     | 17-May-24 (CTTL, No. J24X04107)           | May-25                |
| Reference Probe EX3DV4  | SN 7307    | 24-May-24(SPEAG, No. EX-7307_May24)       | May-25                |
| DAE4                    | SN 1588    | 13-Sep-24(CTTL-SPEAG, No. 24J02Z000713)   | Sep-25                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 19-Dec-24 (CTTL, No. 24J02X103931)        | Dec-25                |
| NetworkAnalyzer E5071C  | MY46110673 | 18-Dec-24 (CTTL, No. 24J02X103932)        | Dec-25                |
| OCP DAKS                | SN 0015    | 09-Oct-24(SPEAG, No. OCP-DAKS-0015_Oct24) | Oct -25               |

|                | Name        | Function           | Signature                                                                             |
|----------------|-------------|--------------------|---------------------------------------------------------------------------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |  |
| Reviewed by:   | Lin Jun     | SAR Test Engineer  |  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |  |

Issued: April 8, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a k**  
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                              |                                  |
|-------------------------------------|----------------------------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY52                                       | 52.10.4                          |
| <b>Extrapolation</b>                | Advanced Extrapolation                       |                                  |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C                     |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                        | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4 mm, dz = 1.4 mm                   | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 3900 MHz $\pm$ 1 MHz<br>4100 MHz $\pm$ 1 MHz |                                  |

## Head TSL parameters at 3900MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.5           | 3.32 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 37.5 $\pm$ 6 % | 3.36 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —              | —                    |

## SAR result with Head TSL at 3900MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                              |
|---------------------------------------------------------------|--------------------|------------------------------|
| SAR measured                                                  | 100 mW input power | 6.77 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 67.6 W/kg $\pm$ 24.4 % (k=2) |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                              |
| SAR measured                                                  | 100 mW input power | 2.35 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 23.5 W/kg $\pm$ 24.2 % (k=2) |

## Head TSL parameters at 4100MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 37.2           | 3.53 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 37.0 $\pm$ 6 % | 3.55 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | —              | —                    |

## SAR result with Head TSL at 4100MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                              |
|---------------------------------------------------------------|--------------------|------------------------------|
| SAR measured                                                  | 100 mW input power | 6.80 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 67.9 W/kg $\pm$ 24.4 % (k=2) |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                              |
| SAR measured                                                  | 100 mW input power | 2.34 W/kg                    |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 23.4 W/kg $\pm$ 24.2 % (k=2) |



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: cmf@caict.ac.cn <http://www.caict.ac.cn>

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 3900MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 44.0Ω- 4.62jΩ |
| Return Loss                          | - 21.9dB      |

### Antenna Parameters with Head TSL at 4100MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 55.9Ω+ 1.21jΩ |
| Return Loss                          | - 24.9dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.008 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caict.ac.cn>

## **DASY5 Validation Report for Head TSL**

Date: 2025-03-31

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 3900 MHz; Type: D3900V2; Serial: D3900V2 - SN: 1083**

Communication System: UID 0, CW; Frequency: 3900 MHz; Frequency: 4100 MHz;

Medium parameters used:  $f = 3900$  MHz;  $\sigma = 3.362$  S/m;  $\epsilon_r = 37.48$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 4100$  MHz;  $\sigma = 3.551$  S/m;  $\epsilon_r = 36.96$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(6.49, 6.55, 7.02) @ 3900 MHz; ConvF(6.31, 6.38, 6.85) @ 4100 MHz; Calibrated: 2024-05-28
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1588; Calibrated: 2024-09-13
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration /Pin=100mW, d=10mm, f=3900 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**

Reference Value = 55.97 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 19.0 W/kg

**SAR (1 g) = 6.77 W/kg; SAR (10 g) = 2.35 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 74.8%

Maximum value of SAR (measured) = 13.0 W/kg

**Dipole Calibration /Pin=100mW, d=10mm, f=4100 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm**

Reference Value = 54.81 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 20.2 W/kg

**SAR (1 g) = 6.8 W/kg; SAR (10 g) = 2.34 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 72.8%

Maximum value of SAR (measured) = 13.4 W/kg




Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: [cmf@caict.ac.cn](mailto:cmf@caict.ac.cn)

<http://www.caict.ac.cn>

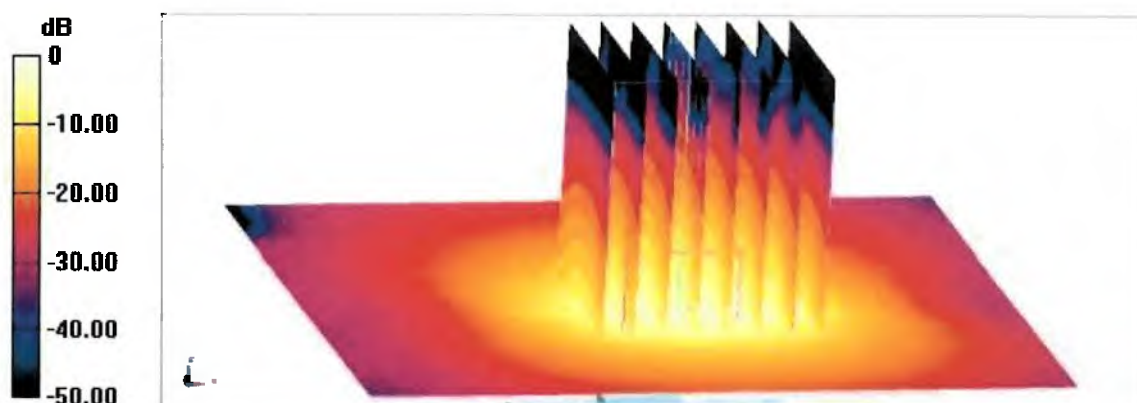


0 dB = 13.4 W/kg = 11.27 dBW/kg



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

## Impedance Measurement Plot for Head TSL

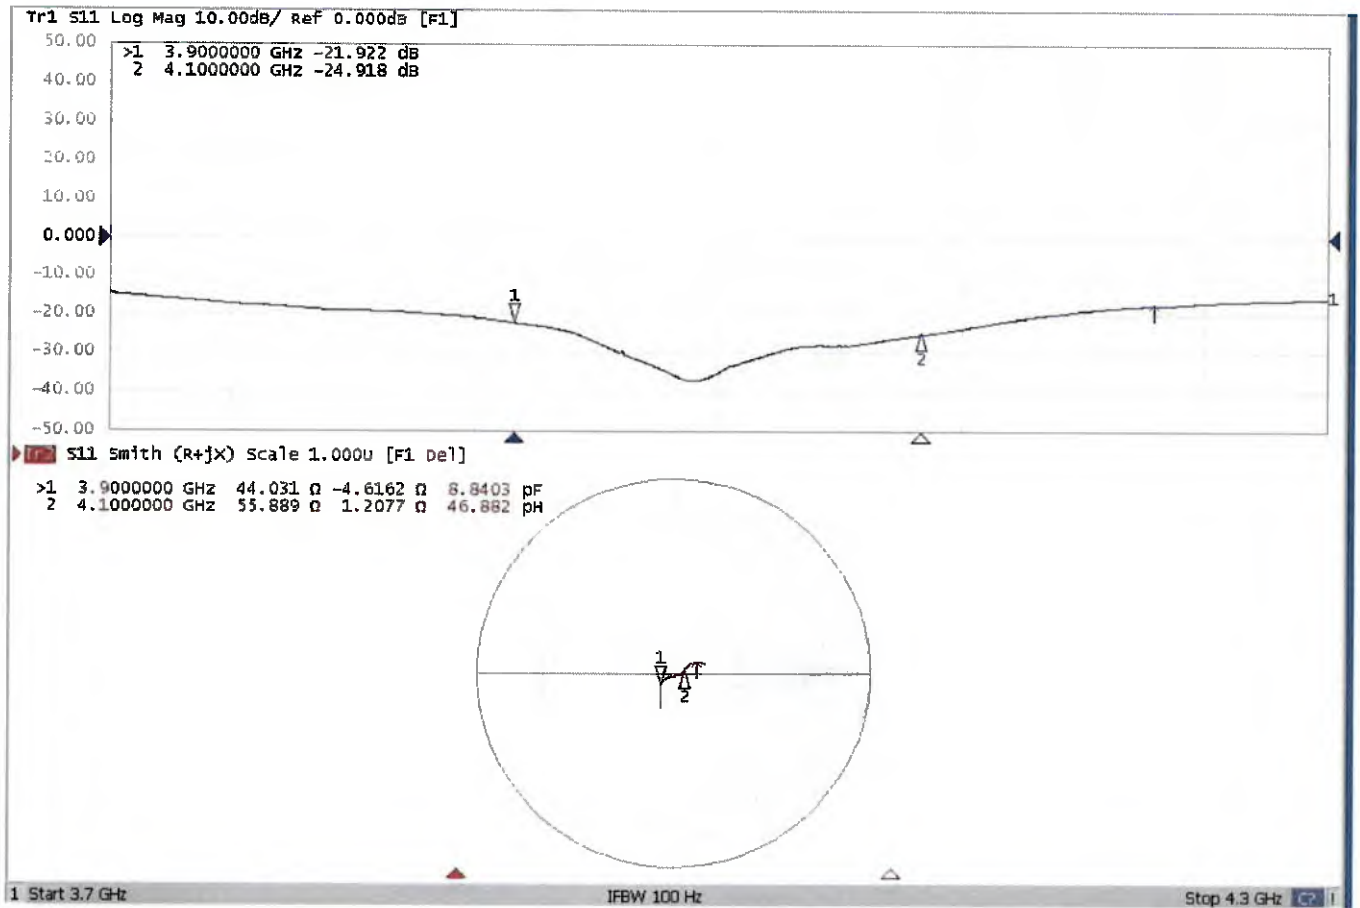

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn      http://www.caic.ac.cn

Client **SGS**

Certificate No: **J23Z60381**

## CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1174**

Calibration Procedure(s) **FF-Z11-003-01**  
**Calibration Procedures for dipole validation kits**

Calibration date: **August 23, 2023**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.


All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards       | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|-------------------------------------------|-----------------------|
| Power Meter NRP2        | 106277     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Power sensor NRP8S      | 104291     | 22-Sep-22 (CTTL, No.J22X09561)            | Sep-23                |
| Reference Probe EX3DV4  | SN 3617    | 31-Mar-23(CTTL-SPEAG,No.Z23-60161)        | Mar-24                |
| DAE4                    | SN 1556    | 11-Jan-23(CTTL-SPEAG,No.Z23-60034)        | Jan-24                |
| Secondary Standards     | ID #       | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
| Signal Generator E4438C | MY49071430 | 05-Jan-23 (CTTL, No. J23X00107)           | Jan-24                |
| NetworkAnalyzer E5071C  | MY46110673 | 10-Jan-23 (CTTL, No. J23X00104)           | Jan-24                |

|                | Name        | Function           |
|----------------|-------------|--------------------|
| Calibrated by: | Zhao Jing   | SAR Test Engineer  |
| Reviewed by:   | Lin Hao     | SAR Test Engineer  |
| Approved by:   | Qi Dianyuan | SAR Project Leader |

Signature



Issued: August 30, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caic.ac.cn>

### Glossary:

|       |                                            |
|-------|--------------------------------------------|
| TSL   | tissue simulating liquid                   |
| ConvF | sensitivity in TSL / NORM <sub>x,y,z</sub> |
| N/A   | not applicable or not measured             |

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

- c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- **Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- **Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- **Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- **Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- **SAR measured:** SAR measured at the stated antenna input power.
- **SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- **SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn      <http://www.caic.ac.cn>

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                                                                      |                                  |
|-------------------------------------|----------------------------------------------------------------------|----------------------------------|
| <b>DASY Version</b>                 | DASY52                                                               | 52.10.4                          |
| <b>Extrapolation</b>                | Advanced Extrapolation                                               |                                  |
| <b>Phantom</b>                      | Triple Flat Phantom 5.1C                                             |                                  |
| <b>Distance Dipole Center - TSL</b> | 10 mm                                                                | with Spacer                      |
| <b>Zoom Scan Resolution</b>         | dx, dy = 4 mm, dz = 1.4 mm                                           | Graded Ratio = 1.4 (Z direction) |
| <b>Frequency</b>                    | 5250 MHz $\pm$ 1 MHz<br>5600 MHz $\pm$ 1 MHz<br>5750 MHz $\pm$ 1 MHz |                                  |

## Head TSL parameters at 5250MHz

The following parameters and calculations were applied.

|                                                | Temperature         | Permittivity   | Conductivity         |
|------------------------------------------------|---------------------|----------------|----------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C             | 35.9           | 4.71 mho/m           |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2) °C | 35.2 $\pm$ 6 % | 4.63 mho/m $\pm$ 6 % |
| <b>Head TSL temperature change during test</b> | <1.0 °C             | ---            | ---                  |

## SAR result with Head TSL at 5250MHz

|                                                               |                    |                                                |
|---------------------------------------------------------------|--------------------|------------------------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                                |
| SAR measured                                                  | 100 mW input power | 7.76 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>77.2 W/kg <math>\pm</math> 24.4 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                                |
| SAR measured                                                  | 100 mW input power | 2.20 W/kg                                      |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>21.9 W/kg <math>\pm</math> 24.2 % (k=2)</b> |



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caic.ac.cn

### Head TSL parameters at 5600MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.5         | 5.07 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.6 ± 6 %   | 5.00 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C         | ---          | ---              |

### SAR result with Head TSL at 5600MHz

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                 |
| SAR measured                                                  | 100 mW input power | 8.16 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>81.1 W/kg ± 24.4 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.30 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>22.8 W/kg ± 24.2 % (k=2)</b> |

### Head TSL parameters at 5750MHz

The following parameters and calculations were applied.

|                                         | Temperature     | Permittivity | Conductivity     |
|-----------------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters             | 22.0 °C         | 35.4         | 5.22 mho/m       |
| Measured Head TSL parameters            | (22.0 ± 0.2) °C | 34.4 ± 6 %   | 5.16 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C         | ---          | ---              |

### SAR result with Head TSL at 5750MHz

|                                                               |                    |                                 |
|---------------------------------------------------------------|--------------------|---------------------------------|
| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>   | Condition          |                                 |
| SAR measured                                                  | 100 mW input power | 7.83 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>77.8 W/kg ± 24.4 % (k=2)</b> |
| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                                 |
| SAR measured                                                  | 100 mW input power | 2.19 W/kg                       |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | <b>21.7 W/kg ± 24.2 % (k=2)</b> |

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

http://www.caic.ac.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 5250MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 47.3Ω- 7.19jΩ |
| Return Loss                          | - 22.1dB      |

### Antenna Parameters with Head TSL at 5600MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 53.9Ω- 2.14jΩ |
| Return Loss                          | - 27.4dB      |

### Antenna Parameters with Head TSL at 5750MHz

|                                      |               |
|--------------------------------------|---------------|
| Impedance, transformed to feed point | 53.2Ω- 5.17jΩ |
| Return Loss                          | - 24.6dB      |

### General Antenna Parameters and Design

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.111 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

### Additional EUT Data

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|



In Collaboration with

**s p e a g**  
**CALIBRATION LABORATORY**



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caic.ac.cn>

## **DASY5 Validation Report for Head TSL**

Date: 2023-08-23

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1174**

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz,  
Frequency: 5750 MHz

Medium parameters used:  $f = 5250$  MHz;  $\sigma = 4.627$  S/m;  $\epsilon_r = 35.17$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5600$  MHz;  $\sigma = 5$  S/m;  $\epsilon_r = 34.58$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Medium parameters used:  $f = 5750$  MHz;  $\sigma = 5.162$  S/m;  $\epsilon_r = 34.36$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

### **DASY5 Configuration:**

- Probe: EX3DV4 - SN3617; ConvF(5.5, 5.5, 5.5) @ 5250 MHz; ConvF(5.01, 5.01, 5.01) @ 5600 MHz; ConvF(5.15, 5.15, 5.15) @ 5750 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

### **Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,**

**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.33 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 30.9 W/kg

**SAR(1 g) = 7.76 W/kg; SAR(10 g) = 2.2 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.5%

Maximum value of SAR (measured) = 18.1 W/kg

### **Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,**

**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 62.15 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 35.2 W/kg

**SAR(1 g) = 8.16 W/kg; SAR(10 g) = 2.3 W/kg**

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.9%

Maximum value of SAR (measured) = 19.6 W/kg


Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2117

E-mail: emf@caict.ac.cn

<http://www.caic.ac.cn>

**Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan,**  
**dist=1.4mm (8x8x7)/Cube 0:** Measurement grid: dx=4mm, dy=4mm, dz=1.4mm  
 Reference Value = 59.71 V/m; Power Drift = -0.04 dB  
 Peak SAR (extrapolated) = 35.1 W/kg  
**SAR(1 g) = 7.83 W/kg; SAR(10 g) = 2.19 W/kg**  
 Smallest distance from peaks to all points 3 dB below = 7.4 mm  
 Ratio of SAR at M2 to SAR at M1 = 61.7%  
 Maximum value of SAR (measured) = 19.6 W/kg

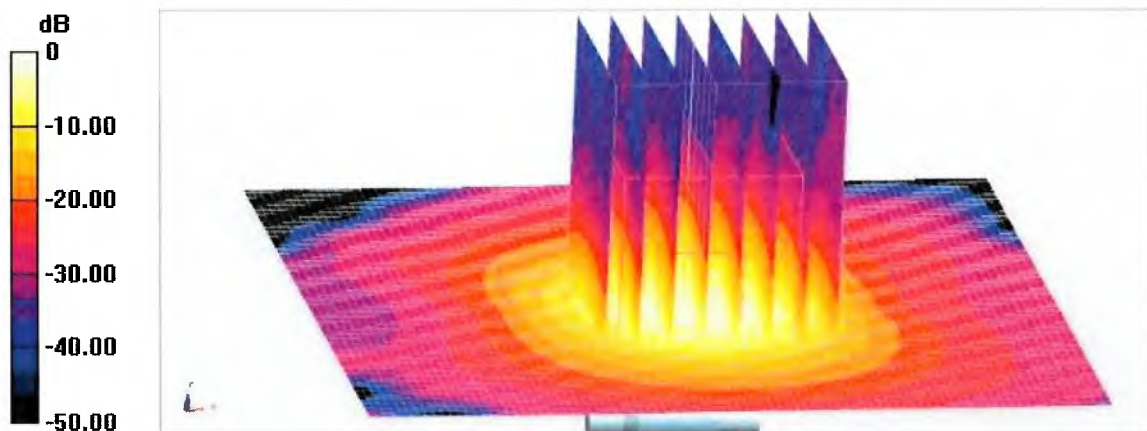


0 dB = 19.6 W/kg = 12.92 dBW/kg



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2117  
E-mail: emf@caict.ac.cn <http://www.caic.ac.cn>

## Impedance Measurement Plot for Head TSL

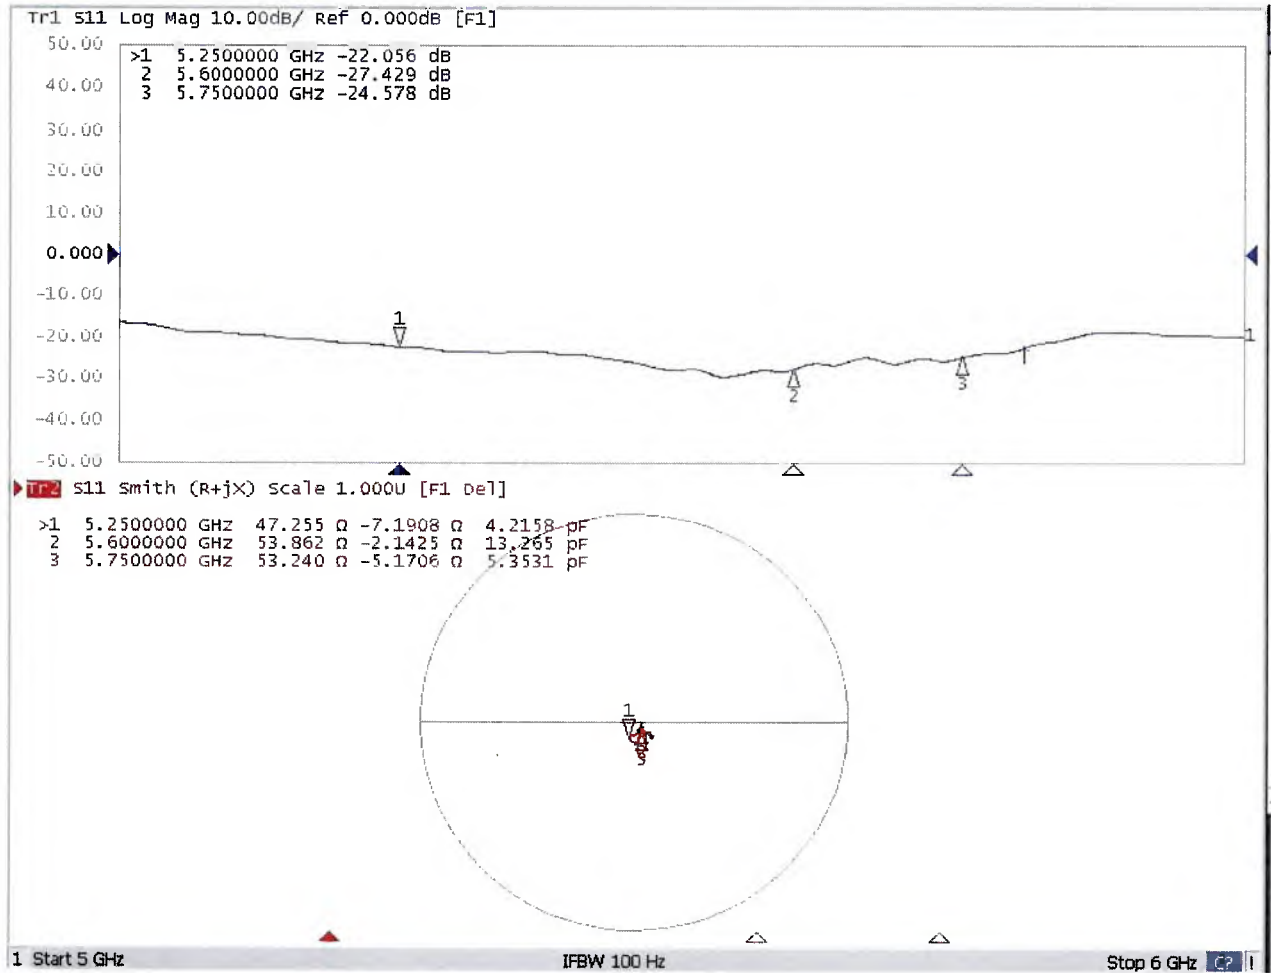



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

|        |                             |                 |                             |
|--------|-----------------------------|-----------------|-----------------------------|
| Client | <b>SGS</b><br><b>Suzhou</b> | Certificate No. | <b>D6.5GHzV2-1030_Feb25</b> |
|--------|-----------------------------|-----------------|-----------------------------|

## CALIBRATION CERTIFICATE

Object **D6.5GHzV2 - SN: 1030**

Calibration procedure(s) **QA CAL-22.v7**  
**Calibration Procedure for SAR Validation Sources between 3 - 10 GHz**

Calibration date **February 13, 2025**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                          | ID         | Cal Date (Certificate No.)             | Scheduled Cal |
|--------------------------------------------|------------|----------------------------------------|---------------|
| Power Sensor R&S NRP-33T                   | SN: 100967 | 28-Mar-24 (No. 217-04038)              | Mar-25        |
| Power Sensor R&S NRP18A                    | SN: 101859 | 06-Feb-25 (No. 4030A315009541)         | Feb-26        |
| Spectrum Analyzer R&S FSV40                | SN: 101832 | 29-Jan-25 (No. 4030A315009658)         | Jan-26        |
| Mismatch; Short [S4188] Attenuator [S4423] | SN: 1152   | 28-Mar-24 (No. 217-04050)              | Mar-25        |
| OCP DAK-12                                 | SN: 1016   | 24-Sept-24 (No. OCP-DAK12-1016_Sep24)  | Sep-25        |
| OCP DAK-3.5                                | SN: 1249   | 23-Sept-24 (No. OCP-DAK3.5-1249_Sep24) | Sep-25        |
| Reference Probe EX3DV4                     | SN: 7349   | 10-Jan-25 (No. EX3-7349_Jan25)         | Jan-26        |
| DAE4ip                                     | SN: 1836   | 28-Oct-24 (No. DAE4ip-1836_Oct24)      | Oct-25        |

| Secondary Standards          | ID         | Check Date (in house)                      | Scheduled Check |
|------------------------------|------------|--------------------------------------------|-----------------|
| ACAD Source Box              | SN: 1000   | 28-May-24 (No. 675-ACAD_Source_Box-240528) | May-25          |
| Signal Generator R&S SMB100A | SN: 182081 | 28-May-24 (No. 675-CAL16-S4588-240528)     | May-25          |
| Mismatch; SMA                | SN: 1102   | 22-May-24 (No. 675-Mismatch_SMA-240522)    | May-25          |

|               | Name              | Function                     | Signature |
|---------------|-------------------|------------------------------|-----------|
| Calibrated by | <b>Paulo Pina</b> | <b>Laboratory Technician</b> |           |
| Approved by   | <b>Sven Kühn</b>  | <b>Technical Manager</b>     |           |

Issued: February 13, 2025

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

**The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates**

**Accreditation No.: SCS 0108**

## Glossary

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

## Calibration is Performed According to the Following Standards

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation

- DASY System Handbook

## Methods Applied and Interpretation of Parameters

- *Measurement Conditions*: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL*: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss*: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay*: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured*: SAR measured at the stated antenna input power.
- *SAR normalized*: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters*: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                                     |                            |                                     |
|-------------------------------------|----------------------------|-------------------------------------|
| <b>DASY Version</b>                 | DASY8 Module SAR           | 16.4.0                              |
| <b>Extrapolation</b>                | Advanced Extrapolation     |                                     |
| <b>Phantom</b>                      | Modular Flat Phantom       |                                     |
| <b>Distance Dipole Center - TSL</b> | 5 mm                       | with spacer                         |
| <b>Zoom Scan Resolution</b>         | dx, dy = 3.4mm, dz = 1.4mm | Graded Ratio = 1.4 mm (Z direction) |
| <b>Frequency</b>                    | 6500MHz $\pm$ 1MHz         |                                     |

## Head TSL parameters at 6500 MHz

The following parameters and calculations were applied.

|                                                | Temperature        | Permittivity  | Conductivity        |
|------------------------------------------------|--------------------|---------------|---------------------|
| <b>Nominal Head TSL parameters</b>             | 22.0 °C            | 34.5          | 6.07 mho/m          |
| <b>Measured Head TSL parameters</b>            | (22.0 $\pm$ 0.2)°C | 34.4 $\pm$ 6% | 6.17 mho/m $\pm$ 6% |
| <b>Head TSL temperature change during test</b> | < 0.5 °C           |               |                     |

## SAR result with Head TSL at 6500 MHz

| <b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b> | Condition          |                              |
|-------------------------------------------------------------|--------------------|------------------------------|
| SAR for nominal Head TSL parameters                         | 20 dBm input power | 29.7 W/kg                    |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | 297 W/kg $\pm$ 24.7% (k = 2) |

| <b>SAR averaged over 8 cm<sup>3</sup> (8 g) of Head TSL</b> | Condition          |                               |
|-------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                         | 20 dBm input power | 6.62 W/kg                     |
| SAR for nominal Head TSL parameters                         | normalized to 1W   | 66.2 W/kg $\pm$ 24.4% (k = 2) |

| <b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b> | Condition          |                               |
|---------------------------------------------------------------|--------------------|-------------------------------|
| SAR for nominal Head TSL parameters                           | 20 dBm input power | 5.43 W/kg                     |
| SAR for nominal Head TSL parameters                           | normalized to 1W   | 54.3 W/kg $\pm$ 24.4% (k = 2) |

**Appendix (Additional assessments outside the scope of SCS 0108)****Antenna Parameters with Head TSL at 6500 MHz**

|             |                                |
|-------------|--------------------------------|
| Impedance   | 52.1 $\Omega$ – 4.6 j $\Omega$ |
| Return Loss | -26.1 dB                       |

**APD (Absorbed Power Density)**

| APD averaged over 1 cm <sup>3</sup> | Condition          |                               |
|-------------------------------------|--------------------|-------------------------------|
| APD measured                        | 20 dBm input power | 297 W/kg                      |
| APD measured                        | normalized to 1W   | 2970 W/kg $\pm$ 29.2% (k = 2) |

| APD averaged over 4 cm <sup>3</sup> | Condition          |                               |
|-------------------------------------|--------------------|-------------------------------|
| APD measured                        | 20 dBm input power | 132 W/kg                      |
| APD measured                        | normalized to 1W   | 1320 W/kg $\pm$ 28.9% (k = 2) |

\*The reported APD values have been derived using the psSAR1g and psSAR8g.

**General Antenna Parameters and Design**

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |       |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

System Performance Check Report

Summary

|                    |                 |     |             |
|--------------------|-----------------|-----|-------------|
| Dipole             | Frequency [MHz] | TSL | Power [dBm] |
| D6.5GHzV2 ~ SN1030 | 6500            | HSL | 20          |

Exposure Conditions

|                      |                    |      |            |                                 |                   |                        |                  |
|----------------------|--------------------|------|------------|---------------------------------|-------------------|------------------------|------------------|
| Phantom Section, TSL | Test Distance [mm] | Band | Group, UID | Frequency [MHz], Channel Number | Conversion Factor | TSL Conductivity [S/m] | TSL Permittivity |
| Flat                 | 5                  |      | CW, 0--    | 6500, 0                         | 5.49              | 6.17                   | 34.4             |

Hardware Setup


|                 |                    |                             |                           |
|-----------------|--------------------|-----------------------------|---------------------------|
| Phantom         | TSL, Measured Date | Probe, Calibration Date     | DAE, Calibration Date     |
| MFP V8.0 Center | HSL, 2025-02-13    | EX3DV4 ~ SN7349, 2025-01-10 | DAE4ip Sn1836, 2024-10-28 |

Scans Setup


|                     |                 |
|---------------------|-----------------|
|                     | Zoom Scan       |
| Grid Extents [mm]   | 22 x 22 x 22    |
| Grid Steps [mm]     | 3.4 x 3.4 x 1.4 |
| Sensor Surface [mm] | 1.4             |
| Graded Grid         | Yes             |
| Grading Ratio       | 1.4             |
| MAIA                | N/A             |
| Surface Detection   | All points      |
| Scan Method         | Measured        |

Measurement Results

|                     |                     |
|---------------------|---------------------|
|                     | Zoom Scan           |
| Date                | 2025-02-13          |
| psSAR1g [W/Kg]      | 29.7                |
| psSAR10g [W/Kg]     | 5.43                |
| Power Drift [dB]    | -0.08               |
| Power Scaling       | Disabled            |
| Scaling Factor [dB] |                     |
| TSL Correction      | Positive / Negative |

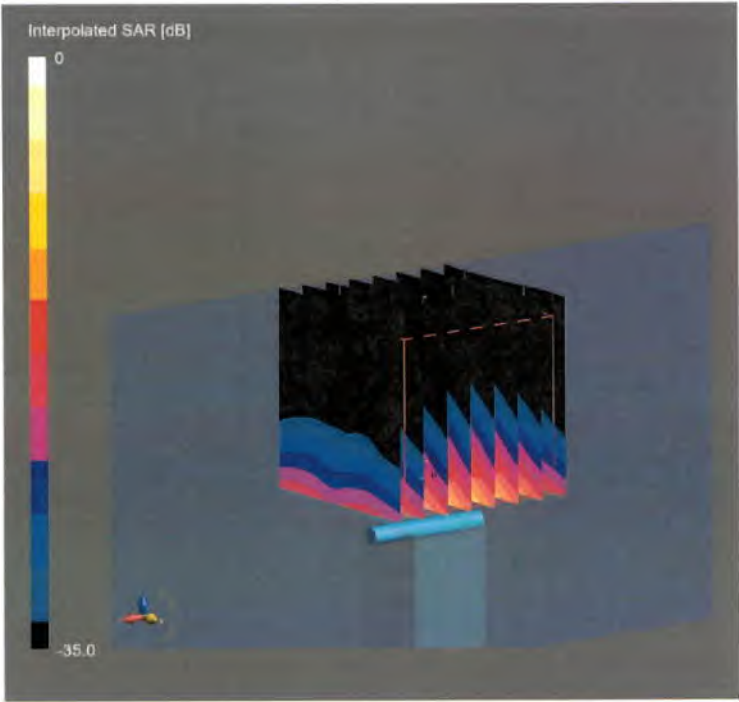

0 dB = 189 W/Kg

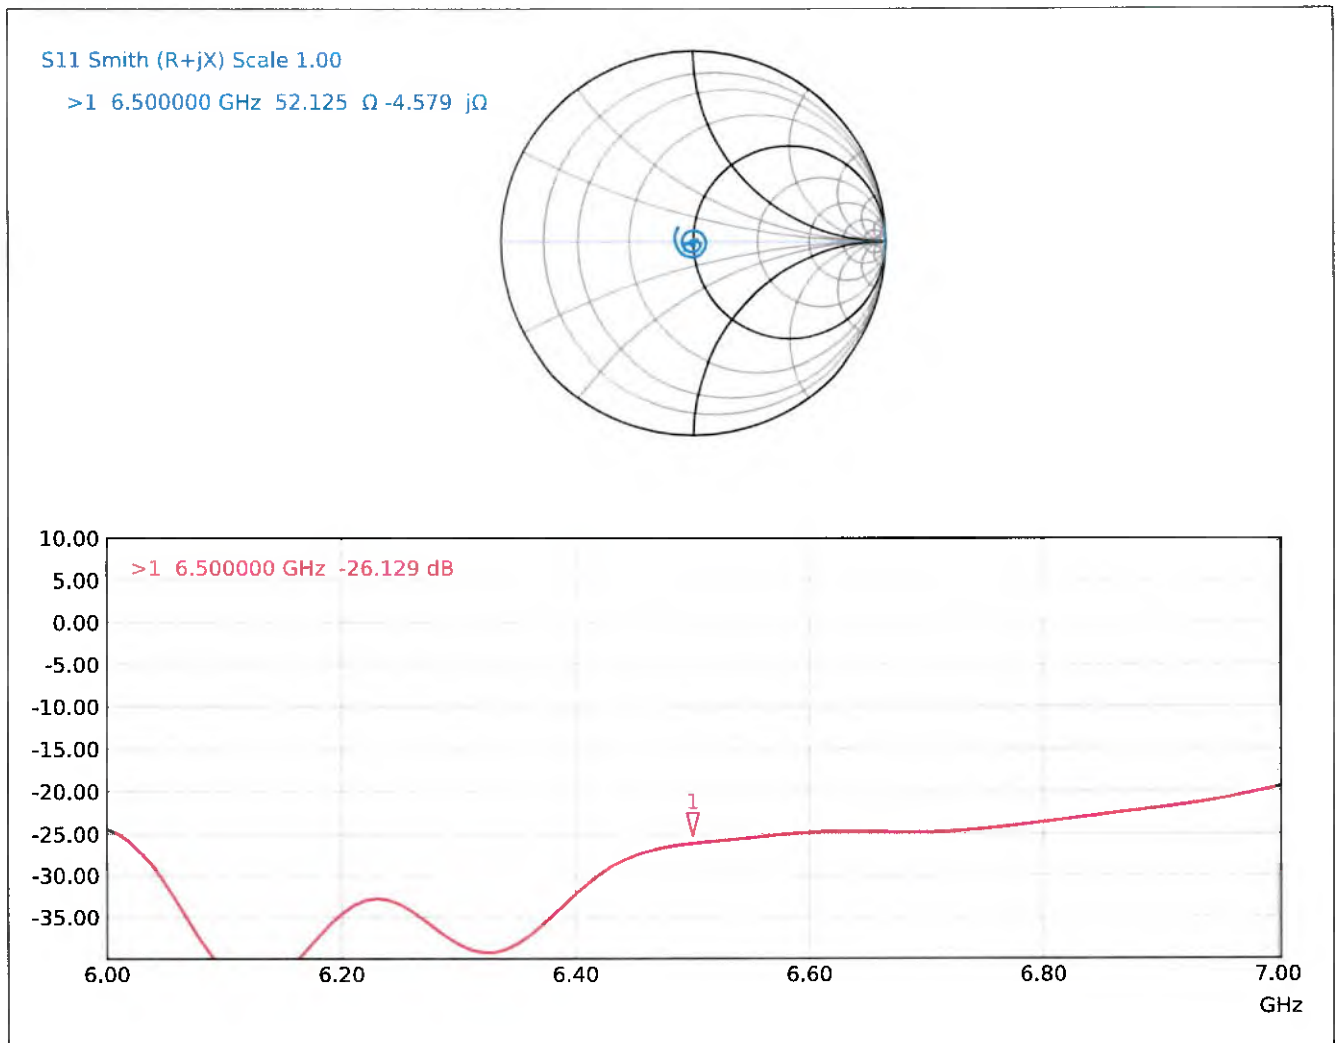**Impedance Measurement Plot for Head TSL**



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **SGS**  
**Shenzhen**

Certificate No. **5G-Veri10-2004\_Aug24**

## CALIBRATION CERTIFICATE

Object **5G Verification Source 10 GHz - SN: 2004**

Calibration procedure(s) **QA CAL-45.v5**  
**Calibration procedure for sources in air above 6 GHz**

Calibration date: **August 20, 2024**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                 | ID #           | Cal Date (Certificate No.)        | Scheduled Calibration  |
|-----------------------------------|----------------|-----------------------------------|------------------------|
| Reference Probe EUmmWV3<br>DAE4ip | SN: 9374       | 04-Dec-23 (No. EUmm-9374_Dec23)   | Dec-24                 |
|                                   | SN: 1602       | 08-Nov-23 (No. DAE4ip-1602_Nov23) | Nov-24                 |
| Secondary Standards               | ID #           | Check Date (in house)             | Scheduled Check        |
| RF generator R&S SMF100A          | SN: 100184     | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24 |
| Power sensor R&S NRP18S-10        | SN: 101258     | 29-Nov-23 (in house check Nov-23) | In house check: Nov-24 |
| Network Analyzer Keysight E5063A  | SN: MY54504221 | 31-Oct-19 (in house check Oct-22) | In house check: Oct-25 |

|                |                        |                                   |
|----------------|------------------------|-----------------------------------|
| Calibrated by: | Name<br>Joanna Lleshaj | Function<br>Laboratory Technician |
| Approved by:   | Sven Kühn              | Technical Manager                 |

Signature

Issued: August 23, 2024

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



## Glossary

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

CW Continuous wave

## Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45, Calibration procedure for sources in air above 6 GHz.
- IEC/IEEE 63195-1, "Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (frequency range of 6 GHz to 300 GHz)", May 2022

## Methods Applied and Interpretation of Parameters

- *Coordinate System:* z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- *Measurement Conditions:* (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. The forward power is measured prior and after the measurement with a power sensor. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by far-field measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- *Horn Positioning:* The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- *E- field distribution:* E field is measured in two x-y-plane (10mm, 10mm +  $\lambda/4$ ) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm<sup>2</sup> and 4cm<sup>2</sup>) power density values at 10mm in front of the horn.
- *Field polarization:* Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

## Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m<sup>2</sup>) averaged over the surface area of 1 cm<sup>2</sup> and 4cm<sup>2</sup> at the nominal operational frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.