


Otto Bock®

QUALITY FOR LIFE

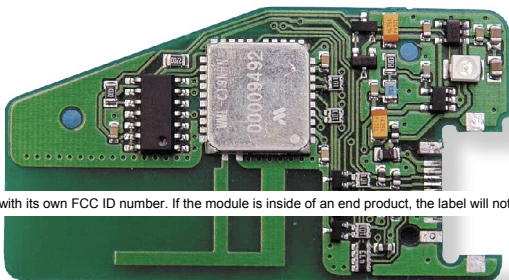

The EUT is labeled with its own FCC ID number. If the module is inside of an end product, the label will not be visible.


CE FC




BionicLinkModule



①

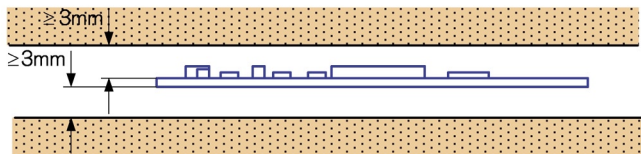

The EUT is labeled with its own FCC ID number. If the module is inside of an end product, the label will not be visible.

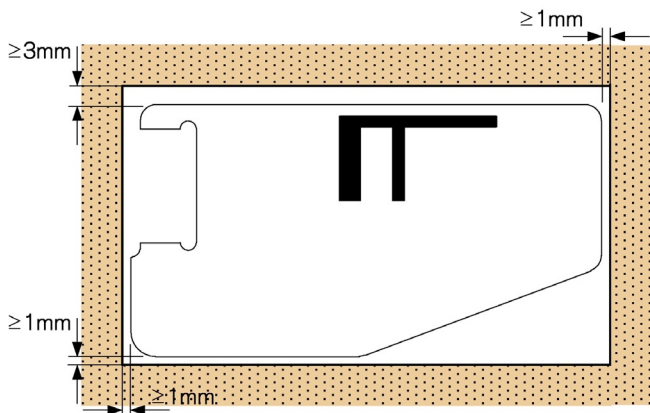

③

Attention: To be installed by trained staff only.

1 Intended Use

The *BionicLinkModule* is used for a cordless configuration and diagnosis of other Otto Bock products. Its main purpose is the replacement of the currently used serial cables. It has a three wire serial interface.

2 Description and Function

It uses *Bluetooth®* technology, because this technology allows an easy connection to a PC, a PDA or to a similar device. These devices either must have the *Bluetooth®* functionality incorporated or use an external *Bluetooth®* interface such as a USB dongle or a Compact Flash- or PC-Card.

The *BionicLinkModule* is conceived as a modular device, which can be permanently built into other products of Otto Bock.

Special Features of the *BionicLinkModule* are:

- The module is very flat.
- Onboard PCB antenna, to achieve a higher antenna efficiency compared to the wide spread ceramic antennas. The goal is to maximize the connection range without increasing the output power of the RF components. This avoids unnecessary spurious emissions and minimizes the power drain out of the battery of the prosthetic device.
- One single LED indicator shows the user if the module is powered (LED is on) and if data is transmitted (LED flashing).

3 Technical Data

Temperature Range: 0° - 60°C

Supply Voltage Range: 3.5 – 4.7V

Bluetooth Class II

4 Mounting Restrictions:

- The module has to be mounted in a way to insure that the human tissue is held at a minimum distance as shown in figure (2) and (3).
- The module has to be placed isolated from metal surfaces at a minimum distance of 1mm, as shown in figure (1).
- It is forbidden to make any modifications, especially of the antenna.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

Modifications not expressly approved by Otto Bock could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment.

This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications.

Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

This product has a modular FCC approval according to FCC public notice DA 00-1407 (released: June 26th, 2000)

The EUT is labeled with its own FCC ID number. If the module is inside of an end product, the label will not be visible. In this case the end product will be labeled exterior with the following information:

"This device contains FCC ID: SJ3MUG6081"

End users may not be provided with the module installation instructions.

OEM integrators and end-users must be provided with transmitter operating conditions for satisfying RF exposure compliance. For portable applications OEM integrators need no SAR evaluation. The max source-based time-averaged output of 0.5 mW is below the low threshold of 24mW for $d < 1.5$ cm.

Use only the supplied or approved antenna. Unauthorized antennas, modifications or attachments could damage the terminal and may contravene local RF emission regulations or invalidate type approval.



Industry
Canada



Otto Bock Healthcare Products GmbH

Kaiserstraße 39 · 1070 Wien · Austria

Tel. (+43-1) 526 95 48 · Telefax (+43-1) 526 79 85

vertrieb.austria@ottobock.com · www.ottobock.at

Otto Bock has been certified by the German Society for the Certification of Quality Assurance Systems (DQS) in accordance with DIN EN ISO 9001, Reg. No. 779 (Management System).