


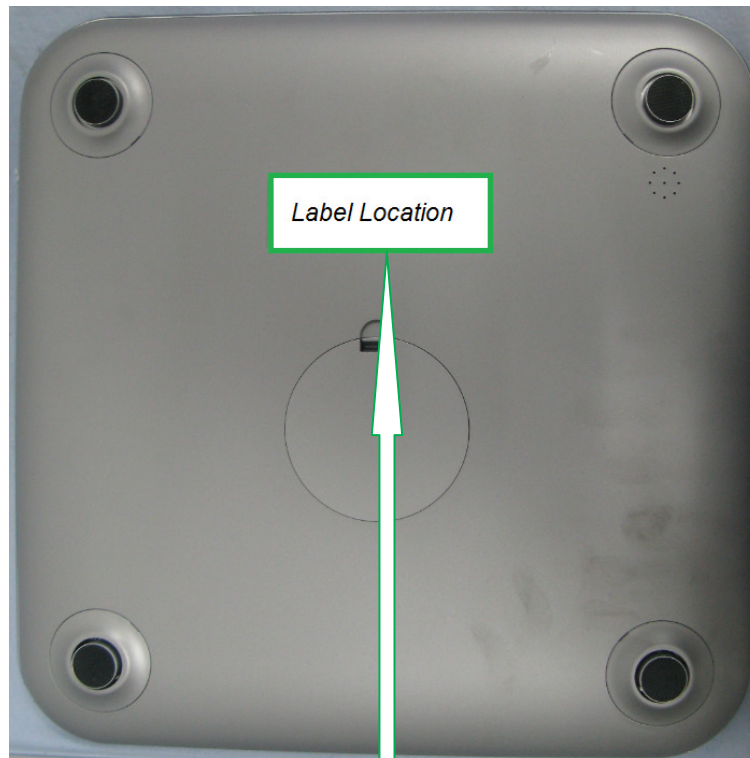

Label Location

## iHealth Wireless Scale Lite

Model/Modèle/Modello/Modelo/Modell/Modelo/Type/Μοντέλο: HS4S

Batteries/Piles/Batterie/Pilas/Batterien/Pilhas/Batterijen/μπαταρίες: 4×1.5V  size AAA

Manufactured for/Fabriqu   pour/Prodotto per/Fabricado por/Manufactured for/Fabricada para/Geproduceerd voor/  
Κατασκευ  ζεται για την:

iHealth Lab Inc. Mountain View, CA 94043 USA. [www.ihealthlabs.com](http://www.ihealthlabs.com) +1-855-816-7705

Made in China/Fabriqu   en Chine/Prodotto in Cina/Fabricado en China/Made in China/Fabricada na China/Made in  
China/Κατασκευ  ζεται στην Κ  να

THIS DEVICE COMPLIES WITH PART 15 OF THE FCC RULES. Operation is subject to the following two conditions:

1) This device may not cause harmful interference, and

2) this device must accept any interference received, including interference that may cause undesired operation.

FCC ID: SLRHS4S CAN ICES-3(B)/NMB-3(B)

IC: 10913A-HS4S SN

