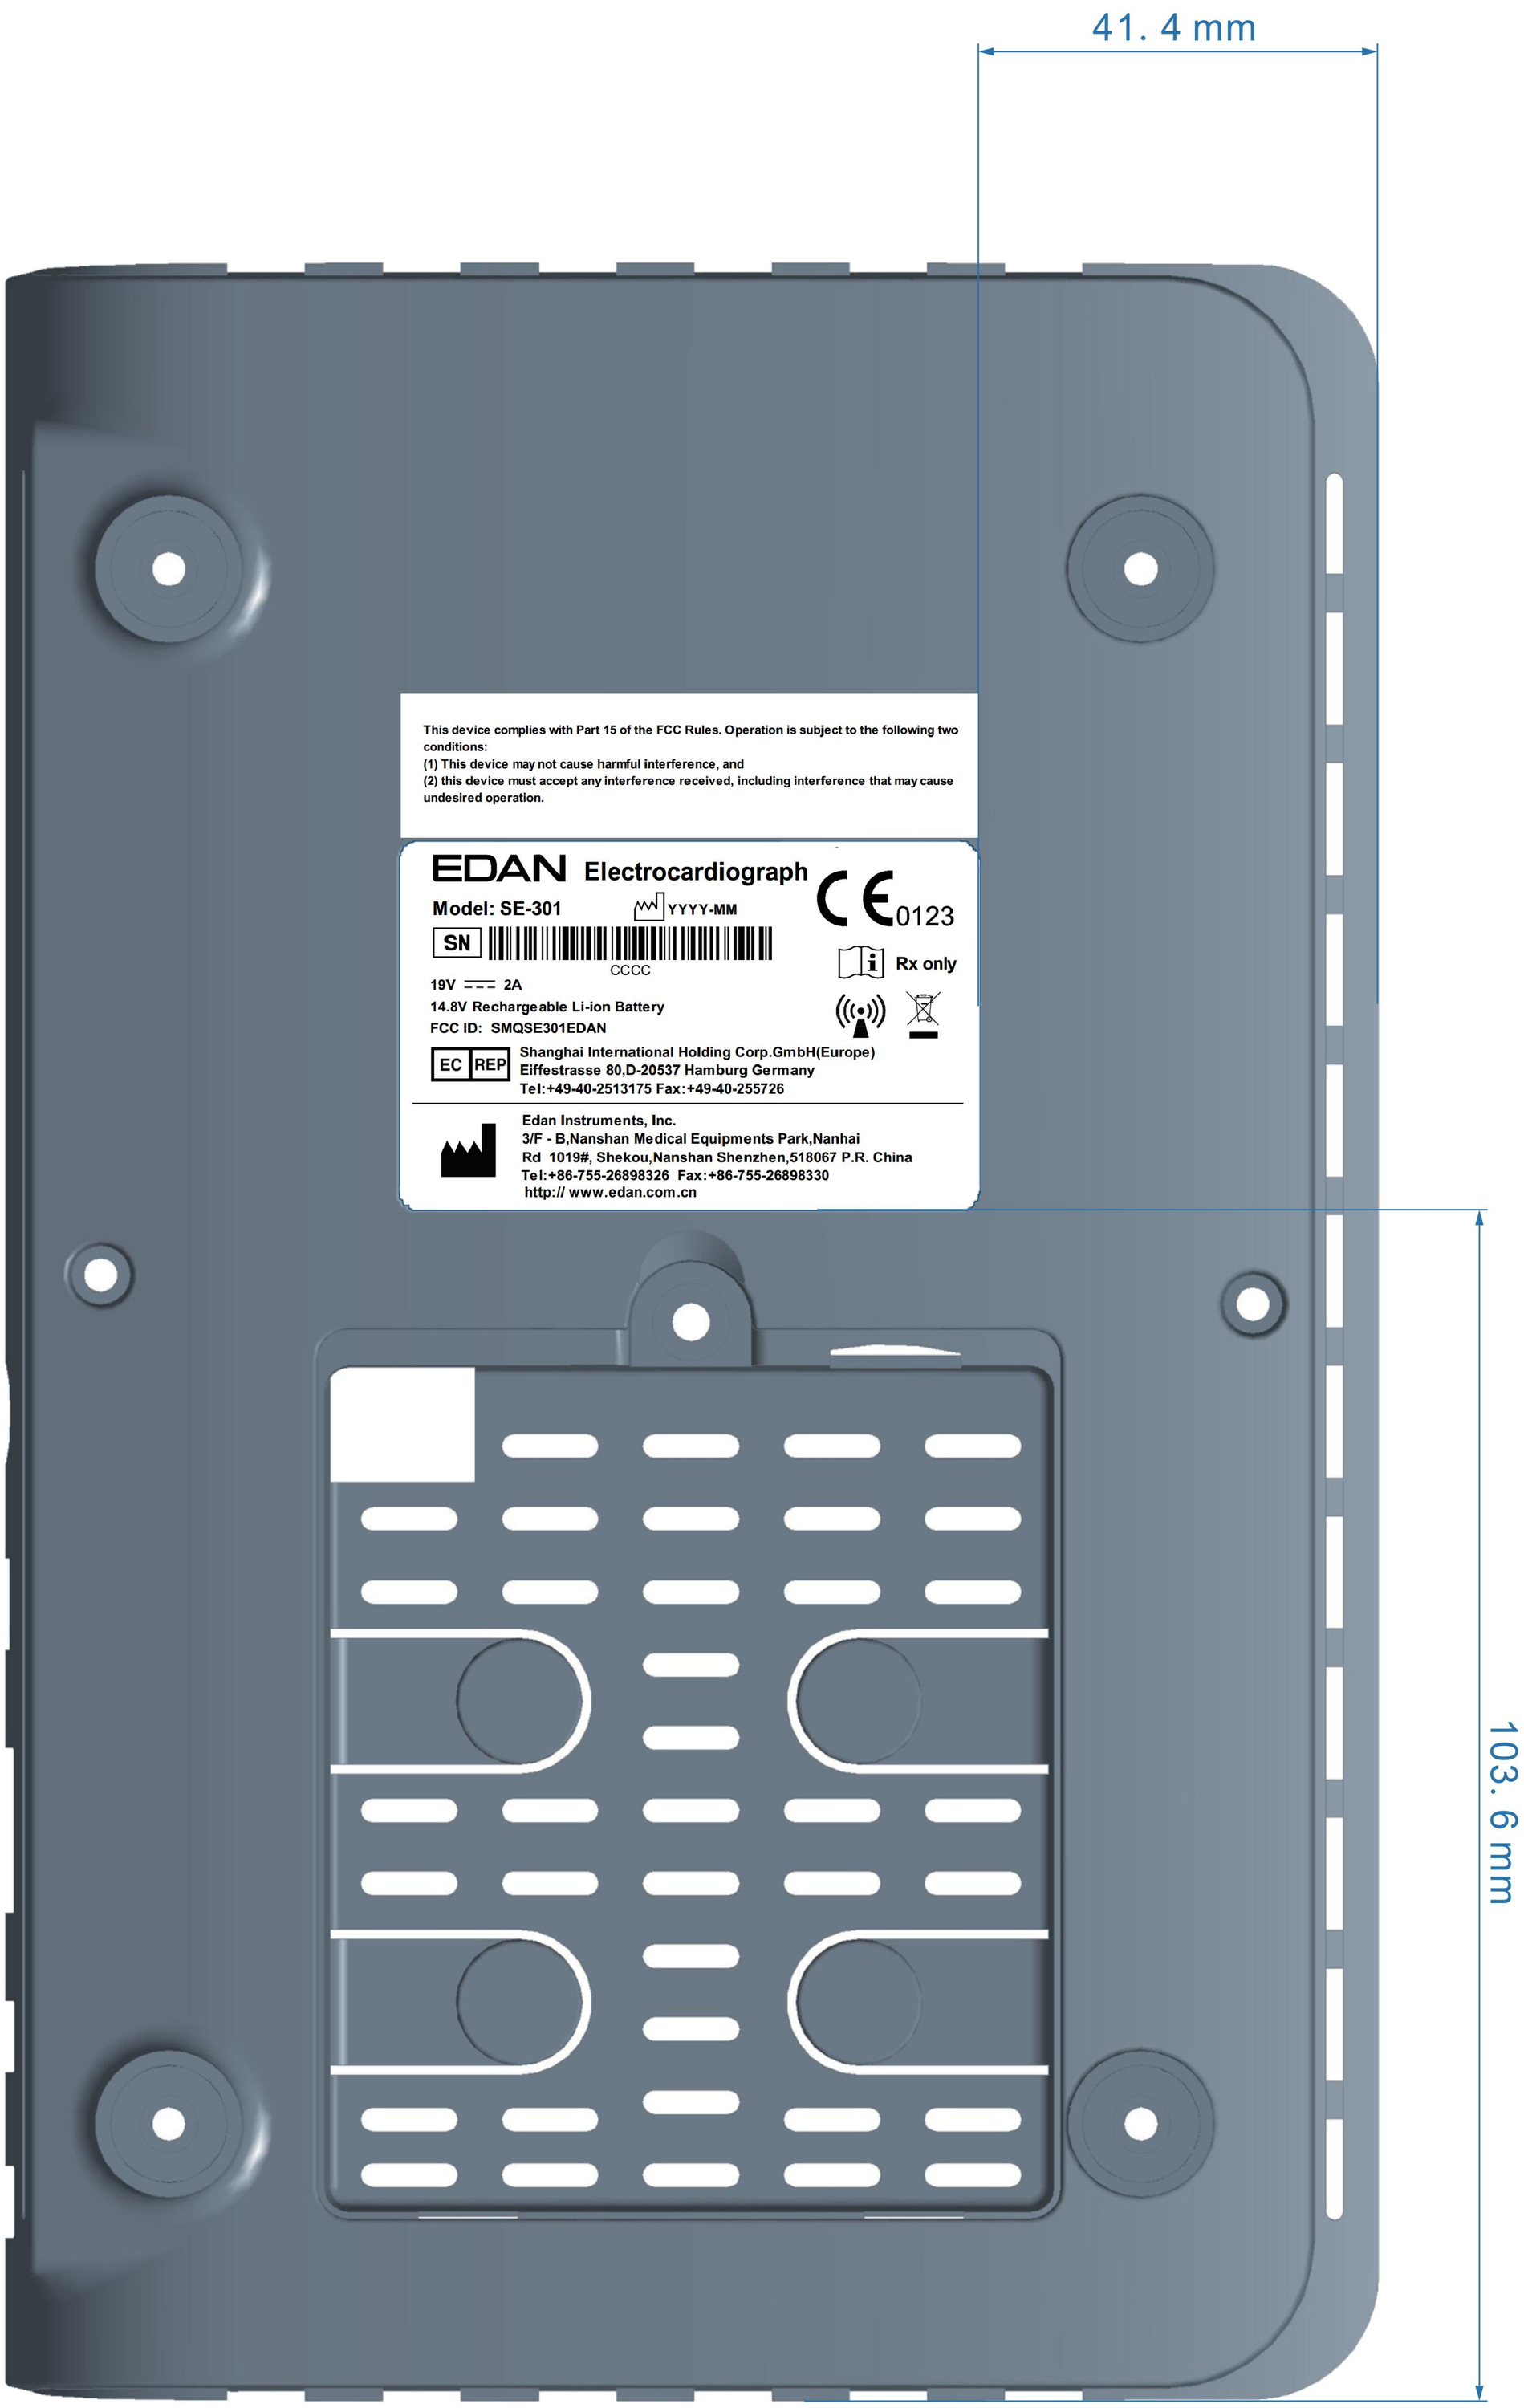
41. 4 mm
103. 6 mm
This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) this device must accept any interference received, including interference that may cause undesired operation.
EDAN Electrocardiograph
Model: SE-301
YYYY-MM
SN
CCCC
0123
Rx only
19V 2A
14.8V Rechargeable Li-ion Battery
FCC ID: SMQSE301EDAN
EC REP
Shanghai International Holding Corp.GmbH(Europe)
Eiffestrasse 80,D-20537 Hamburg Germany
Tel:+49-40-2513175 Fax:+49-40-255726
Edan Instruments, Inc.
3/F - B,Nanshan Medical Equipments Park,Nanhai
Rd 1019#, Shekou,Nanshan Shenzhen,518067 P.R. China
Tel:+86-755-26898326 Fax:+86-755-26898330
http:// www.edan.com.cn