

Appendix A

System Check 835 MHz Head
System Check 2450 MHz Head
System Check 5200 MHz Head
System Check 5300 MHz Head
System Check 5600 MHz Head
System Check 5800 MHz Head

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D835V2 – SN4d302	835.0	HSL	20.0	–3.7	–1.2	9.2	–4.1

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	15	CW, 0––	835.000, 0		9.37	0.906	41.9

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin–SAM V8.0 (30deg probe tilt) – 2168	HSL835	EX3DV4 – SN7858, 2026–02–20	DAE4ip Sn1846, 2026–01–07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026–04–28, 08:40	2026–04–28, 08:47
psSAR1g [W/Kg]	0.915	0.937
psSAR10g [W/Kg]	0.603	0.627
Power Drift [dB]	–0.00	–0.02
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

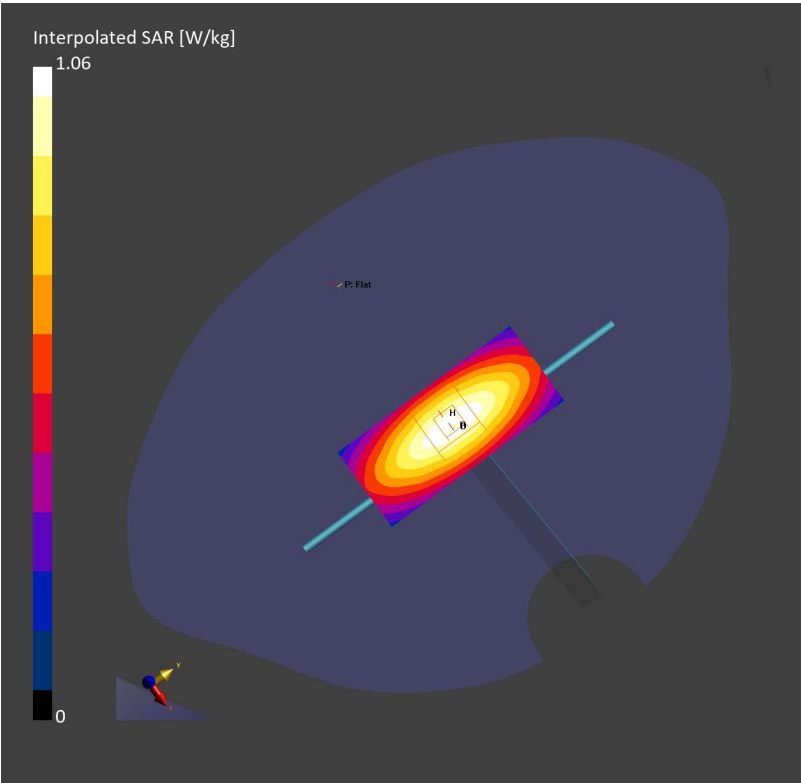

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D2450V2 – SN1099	2450.0	HSL	20.0	–1.9	1.1	–4.7	–6.4

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	10	CW, 0--		2450.000, 0	7.24	1.83	39.3

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) – 2173	HSL2450	EX3DV4 – SN7812, 2026–01–19	DAE4 Sn799, 2026–02–26

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 96.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 12.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026–03–12, 08:56	2026–03–12, 09:03
psSAR1g [W/Kg]	4.96	5.01
psSAR10g [W/Kg]	2.28	2.42
Power Drift [dB]	0.06	0.08
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

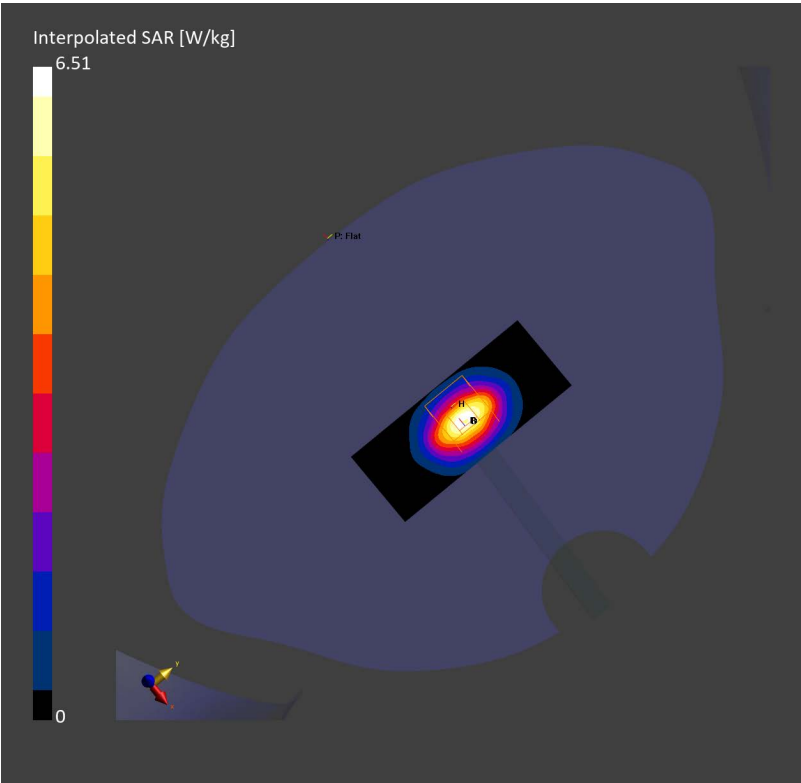

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D5GHzV2 – SN1371	5200.0	HSL	20.0	–0.3	4.3	–13.8	–3.5

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	10	CW, 0––		5200.000, 0	5.05	4.65	36.4

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin–SAM V8.0 (30deg probe tilt) – 2173	HSL5GHz	EX3DV4 – SN7812, 2026–01–19	DAE4 Sn799, 2026–02–26

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 24.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026–03–13, 07:18	2026–03–13, 07:25
psSAR1g [W/Kg]	7.34	7.85
psSAR10g [W/Kg]	2.14	2.33
Power Drift [dB]	–0.00	0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

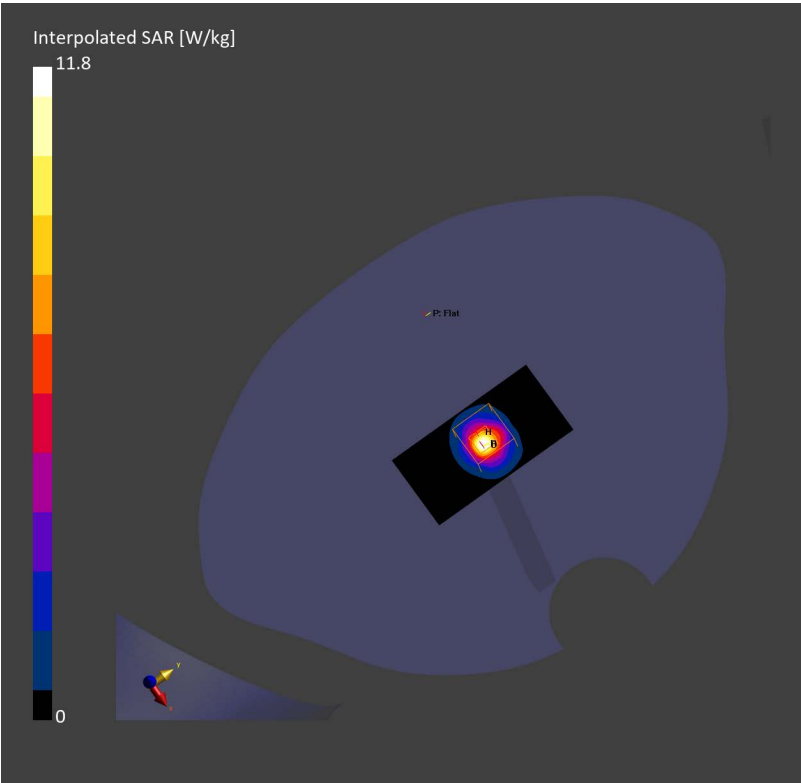

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D5GHzV2 – SN1371	5300.0	HSL	20.0	3.0	6.3	–8.7	3.4

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	10	CW, 0--		5300.000, 0	5.05	4.76	36.4

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) – 2173	HSL5GHz	EX3DV4 – SN7812, 2026-01-19	DAE4 Sn799, 2026-02-26

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 24.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026-03-13, 07:33	2026-03-13, 07:39
psSAR1g [W/Kg]	7.75	8.31
psSAR10g [W/Kg]	2.24	2.45
Power Drift [dB]	–0.00	0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

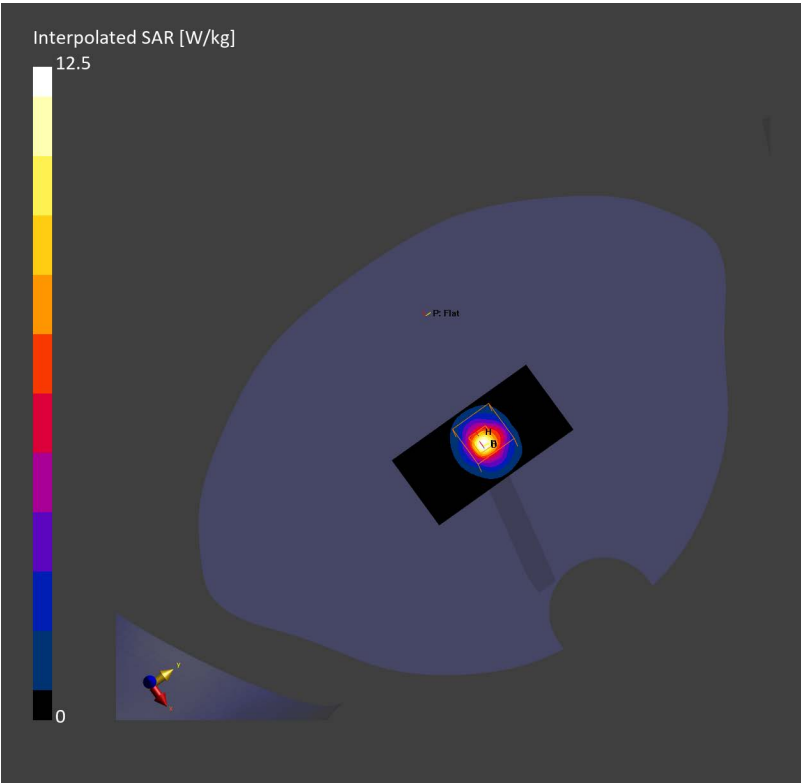

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D5GHzV2 – SN1371	5600.0	HSL	20.0	2.7	5.9	–6.4	3.2

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	10	CW, 0--	5600.000, 0		4.46	5.11	35.4

Hardware Setup


Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) – 2173	HSL5GHz	EX3DV4 – SN7812, 2026-01-19	DAE4 Sn799, 2026-02-26

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 24.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026-03-13, 07:44	2026-03-13, 07:52
psSAR1g [W/Kg]	8.23	8.45
psSAR10g [W/Kg]	2.36	2.47
Power Drift [dB]	–0.00	–0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

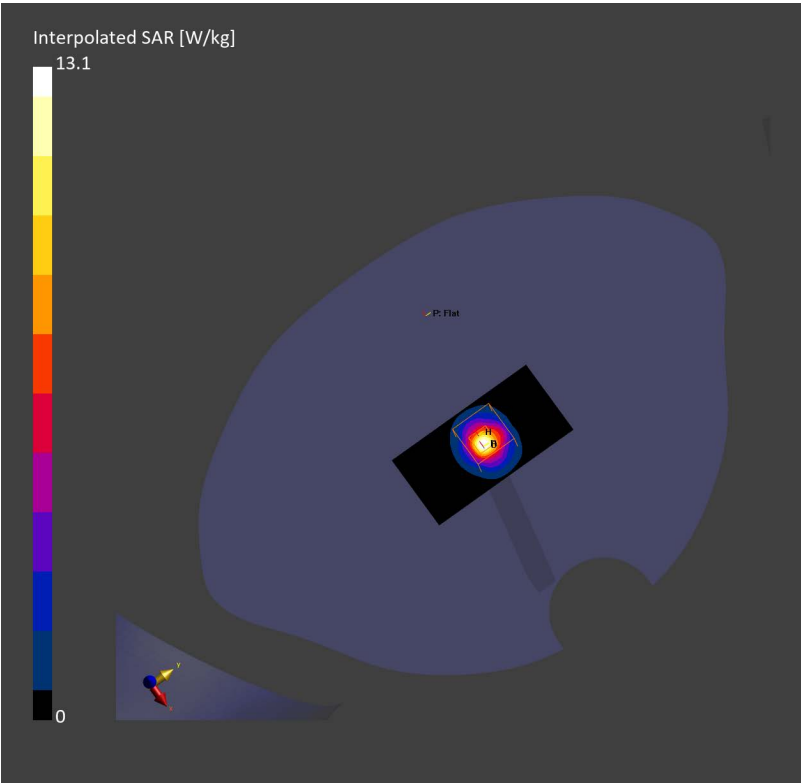

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]	Dev. 1g [%]	Dev. 10g [%]	Dev. Peak [%]	Iso. Error [%]
D5GHzV2 – SN1371	5800.0	HSL	20.0	−4.3	−0.9	−13.4	3.4

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, Head Simulating Liquid	10	CW, 0--	5800.000, 0		4.52	5.38	35.3

Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) – 2173	HSL5GHz	EX3DV4 – SN7812, 2026-01-19	DAE4 Sn799, 2026-02-26

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	24.0 x 24.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2026-03-13, 07:58	2026-03-13, 08:05
psSAR1g [W/Kg]	7.32	7.63
psSAR10g [W/Kg]	2.10	2.22
Power Drift [dB]	−0.01	0.02
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	No correction	No correction

