



In Collaboration with
s p e a g
CALIBRATION LABORATORY



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: cmf@caict.ac.cn <http://www.caict.ac.cn>

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 1900 MHz

Impedance, transformed to feed point	$52.7\Omega + 4.83j\Omega$
Return Loss	- 25.4dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.106 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn http://www.caict.ac.cn

**DASY6 Validation Report for Head TSL**

Date: 2026-02-04

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D1900V2 – SN 5d231	1900	HSL	24

Exposure Conditions


Phantom	Position, Test	Band Group,	Frequency	Conversion	TSL Cond.	TSL
Section, TSL	Distance [mm]	UID	[MHz]	Factor	[S/m]	Permittivity
Flat	10	CW,	1900	8.58	1.42	40.7

Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	1900Head	EX3DV4 - SN7600, 2026-01-19	DAE4 Sn1588, 2025-08-29

Scan Setup**Measurement Results**

	Zoom Scan		Zoom Scan
Grid Extents [mm]	30.0×30.0×30.0	psSAR1g [W/kg]	10.0
Grid Steps [mm]	6.0×6.0×1.5	psSAR10g [W/kg]	5.19
Sensor Surface [mm]	1.4	Power Drift [dB]	-0.00
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.5	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	80.2
Scan Method	Measured	Dist 3dB Peak [mm]	9.6

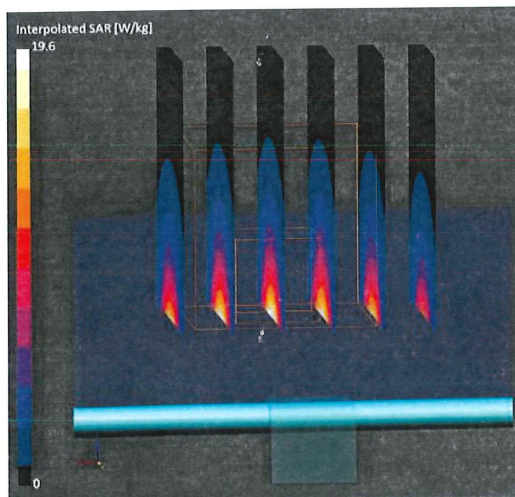


Certificate No: 26J02Z000087

Page 5 of 6



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62304633-2711
 E-mail: emf@caict.ac.cn http://www.caict.ac.cn

Impedance Measurement Plot for Head TSL

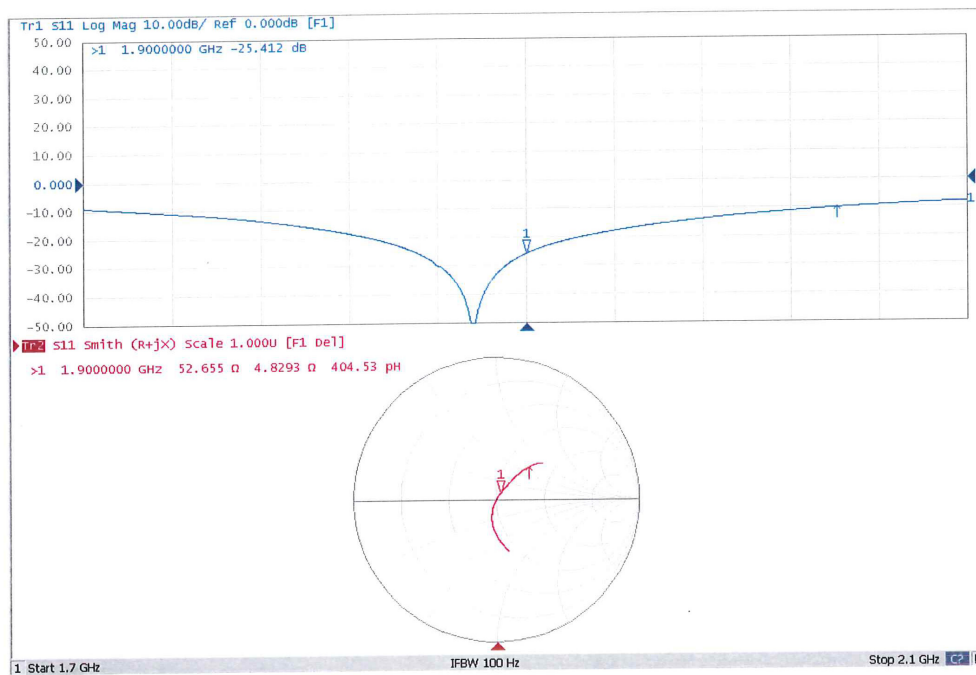

***** END OF REPORT *****