

APPENDIX

11. Photographs of Test Setup

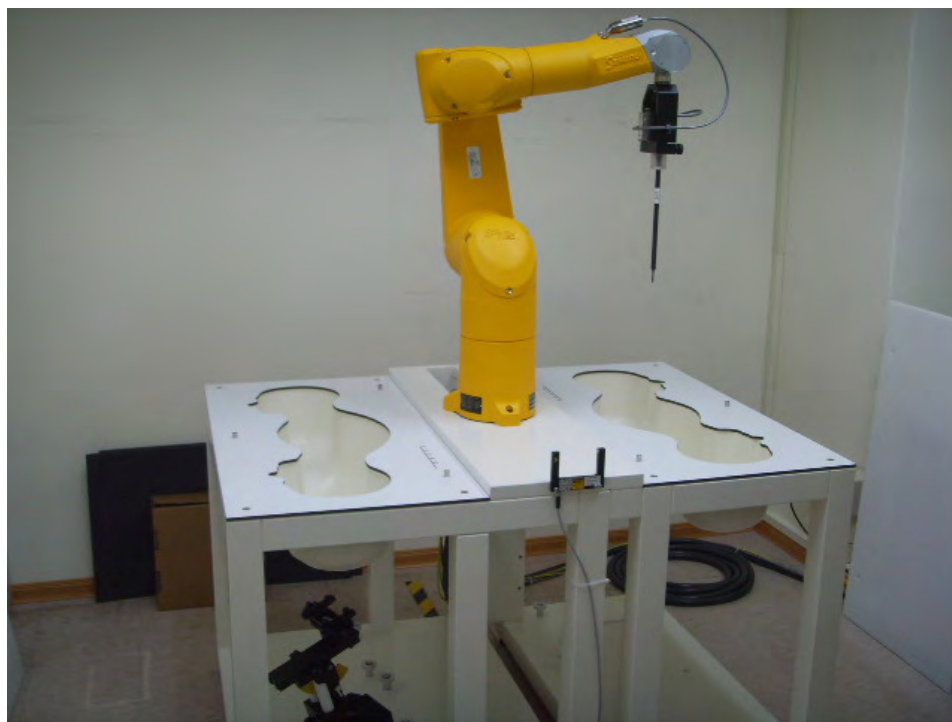


Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth

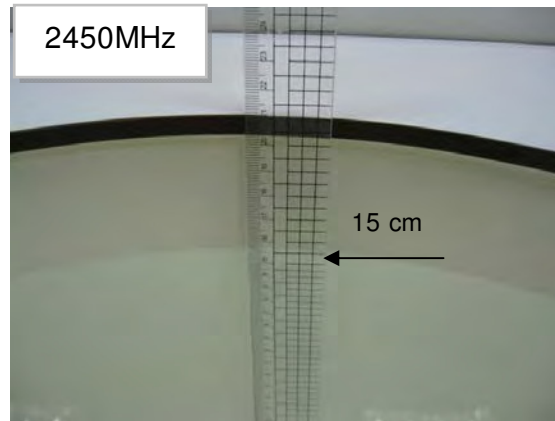


Fig.2

Body - distance between flat phantom and EUT is 0 mm

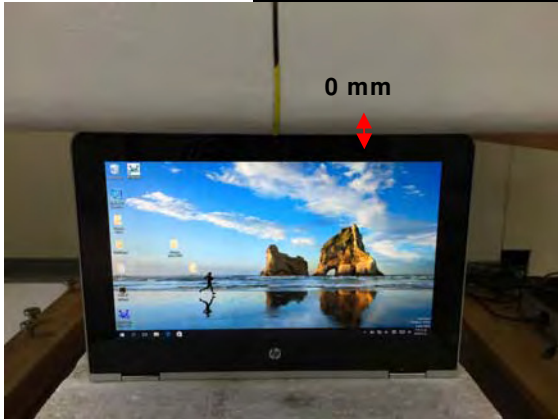


Fig.3 EUT Top side to flat phantom

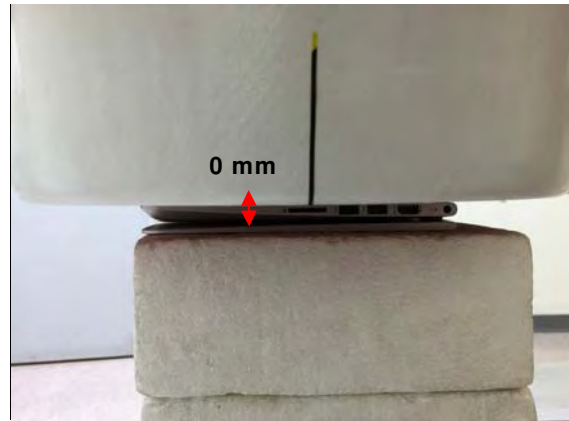


Fig.4 EUT Back side to flat phantom

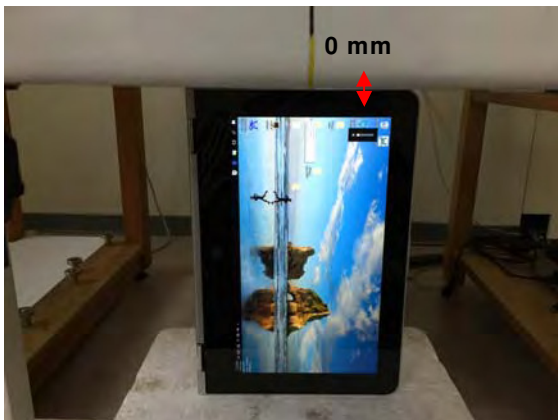


Fig.5 EUT Left side to flat phantom

12. Photographs of the EUT



Fig.6 Front view of EUT



Fig.7 Back view of EUT



Fig.8 Tablet mode of EUT(Front view)

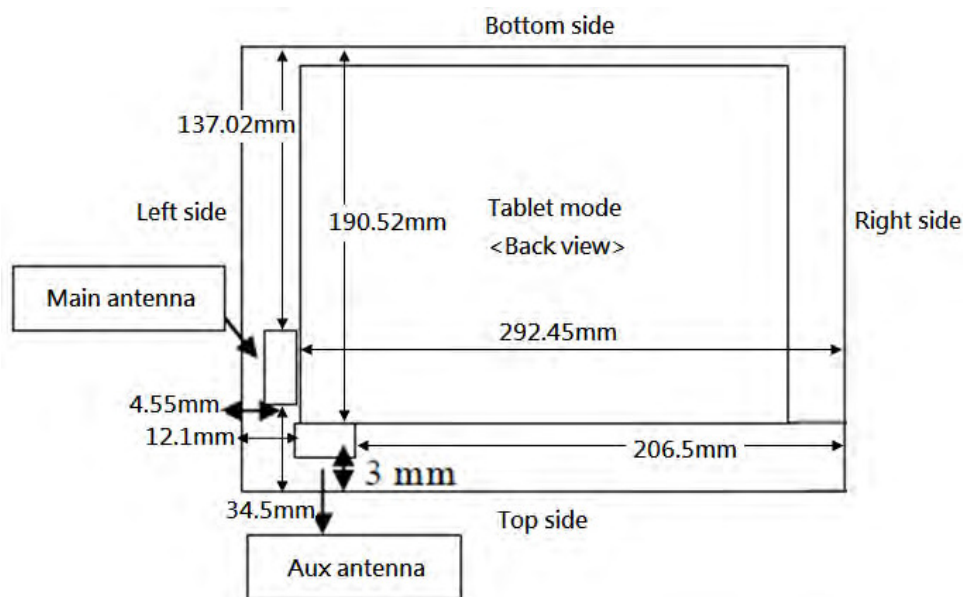


Fig.9 Antenna position of EUT (Back view of tablet mode)

- End of Report -