

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid (Head & Body)

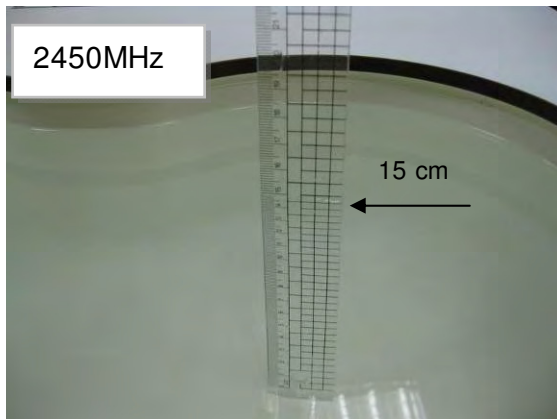


Fig.2.1

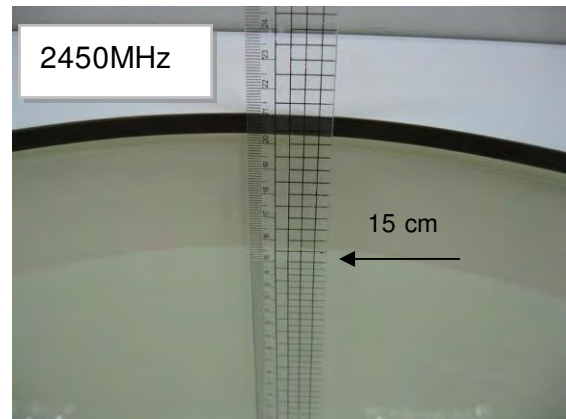


Fig.2.2

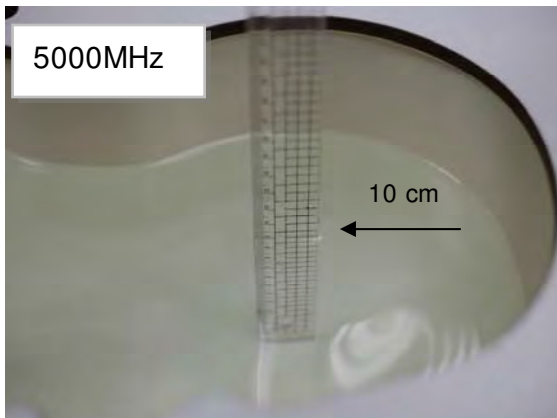


Fig.2.3

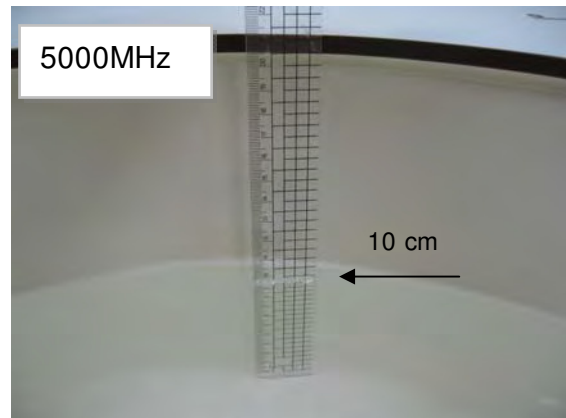


Fig.2.4

Head Mode

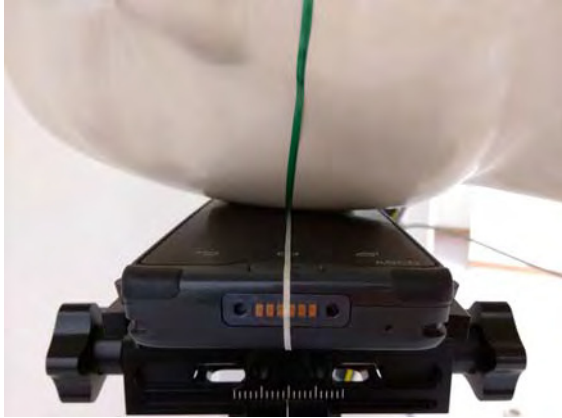


Fig.3 Right Head Section / Cheek-Touch Position

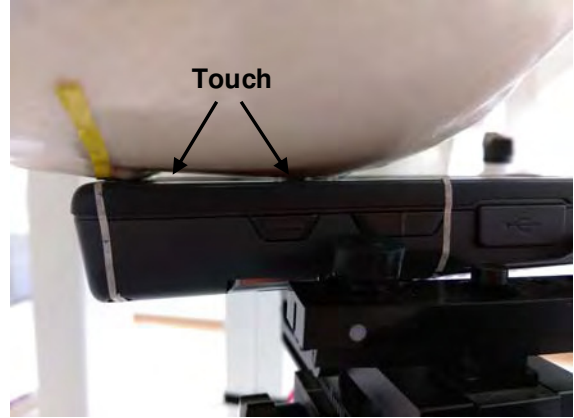


Fig.4 Right Head Section / Ear-Tilt Position(15°)


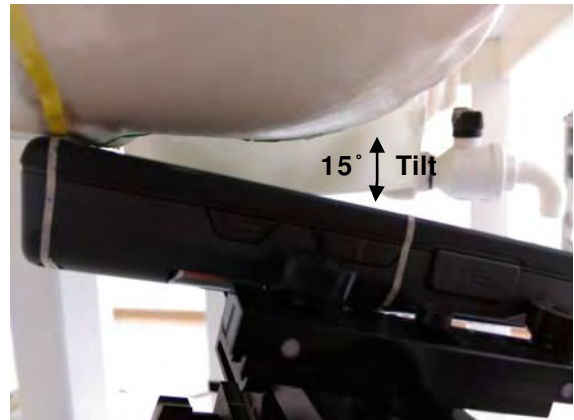


Fig.5 Left Head Section / Cheek-Touch Position

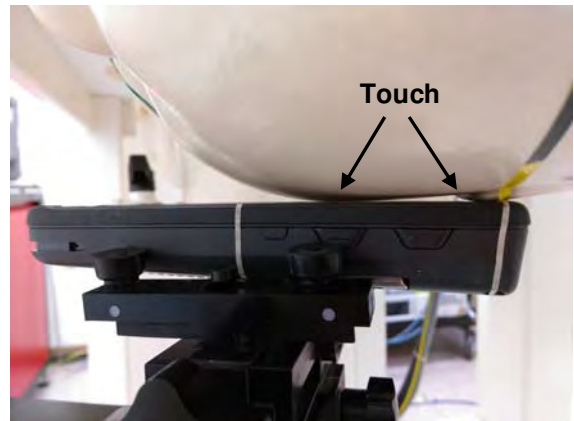

Head Mode



Fig.6 Left Head Section / Ear-Tilt Position(15°)

Body-worn - distance between flat phantom and mobile phone is 15 mm



Fig.7 EUT Front side to flat phantom



Fig.8 EUT Back to flat phantom

Hand - distance between flat phantom and mobile phone is 0 mm



Fig.9 EUT Back side to flat phantom

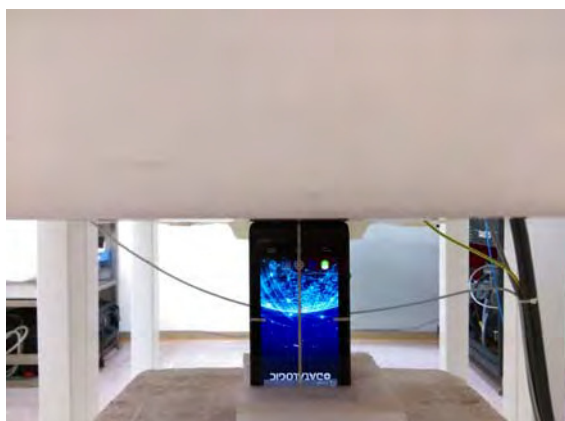
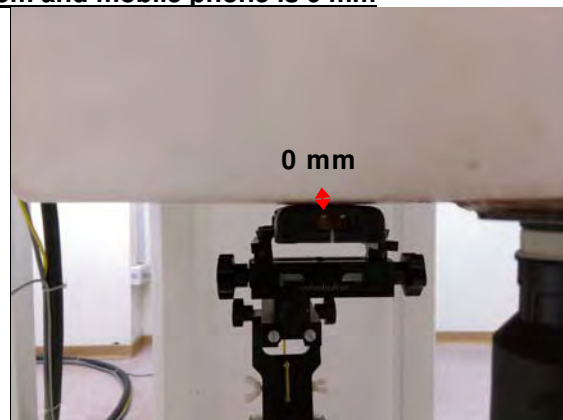


Fig.10 EUT Bottom side to flat phantom


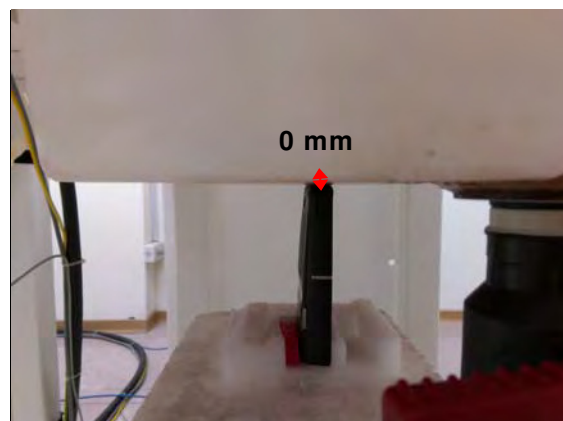


Fig.11 EUT Front side to flat phantom

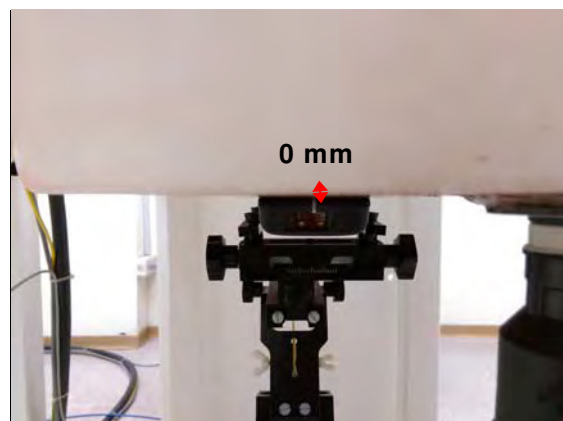

Hand - distance between flat phantom and mobile phone is 0 mm



Fig.12 EUT Left side to flat phantom


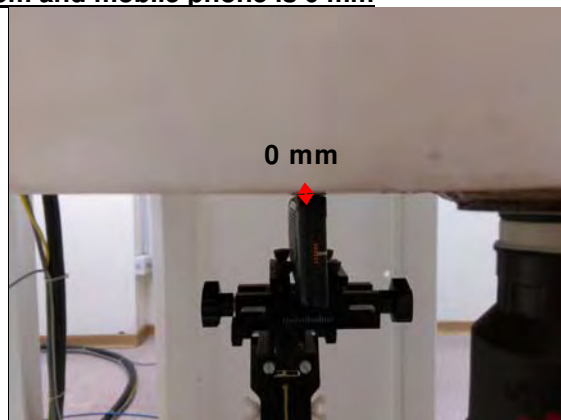


Fig.13 EUT Right side to flat phantom



Fig.14 EUT Top side to flat phantom

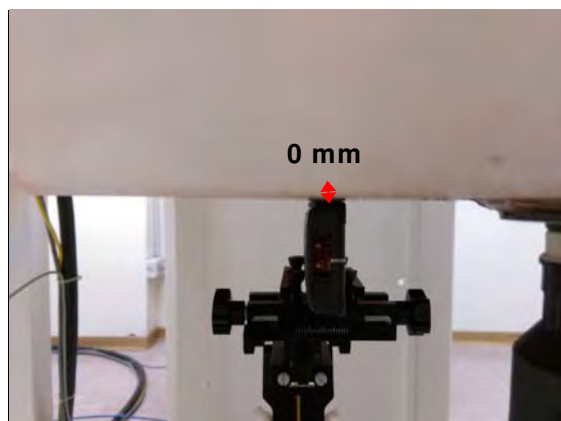

12. Photographs of the EUT



Fig.15 Front view of EUT



Fig.16 Back view of EUT



**Fig.17 Back view of EUT with battery3200
(Model No:Standard BTDL1)**



**Fig.18 Back view of EUT with battery6400
(Model No:Extended BTDL1)**



Fig.19 battery3200 (Model No:Standard BTDL1)



Fig.20 battery6400 (Model No:Extended BTDL1)

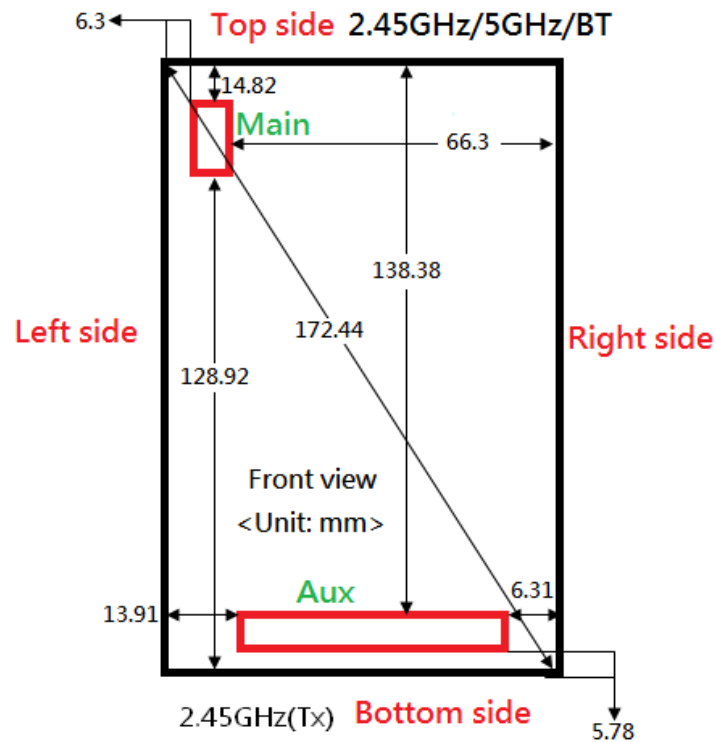


Fig.21 Antenna position of EUT

- End of Report -