

Date: 2025-07-21

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_250721 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.77$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(7.32, 7.48, 7.18); Calibrated: 2024-08-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.25 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.29 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

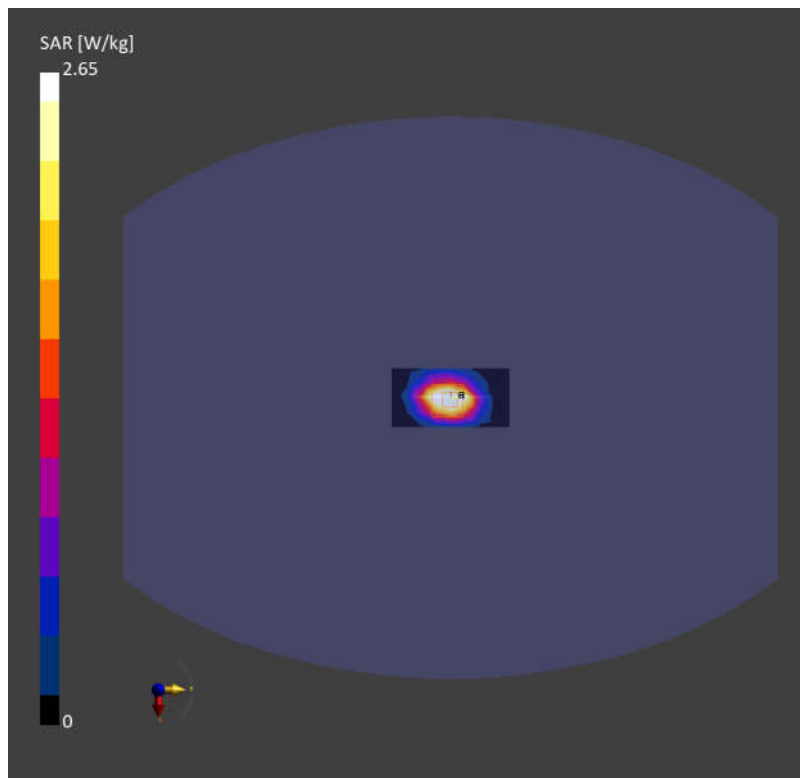

Date: 2025-08-16

System Check_Head_2450MHz**DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_250816 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.76$ S/m; $\epsilon_r = 39.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.61, 7.54, 7.66); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.25 W/kg;


Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

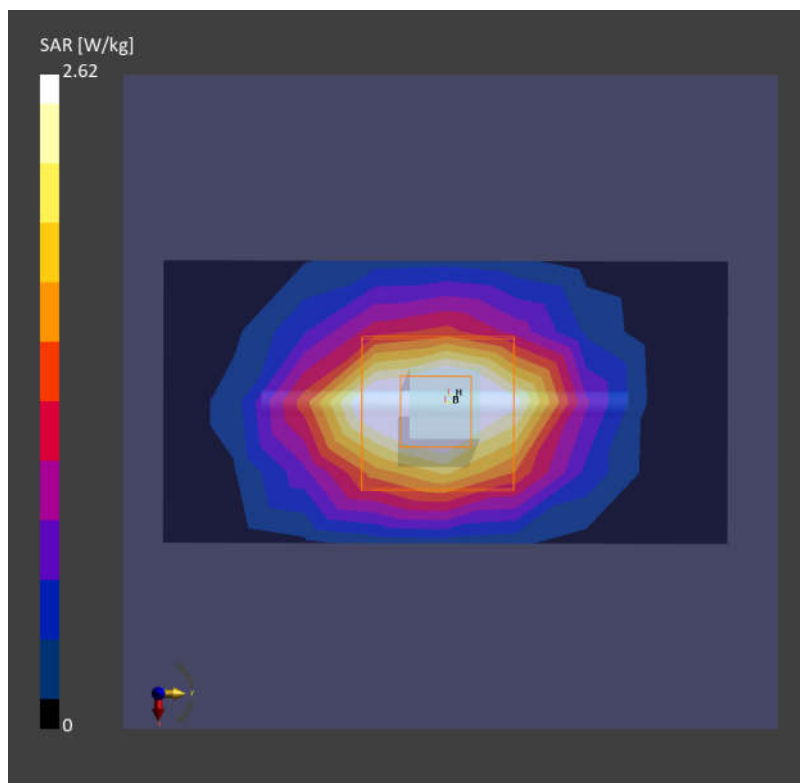

Date: 2025-07-24

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250_250724 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.67$ S/m; $\epsilon_r = 36.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(6.05, 6.18, 5.93); Calibrated: 2024-08-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.71 W/kg; SAR (10g) = 1.11 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.86 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 66.1 %

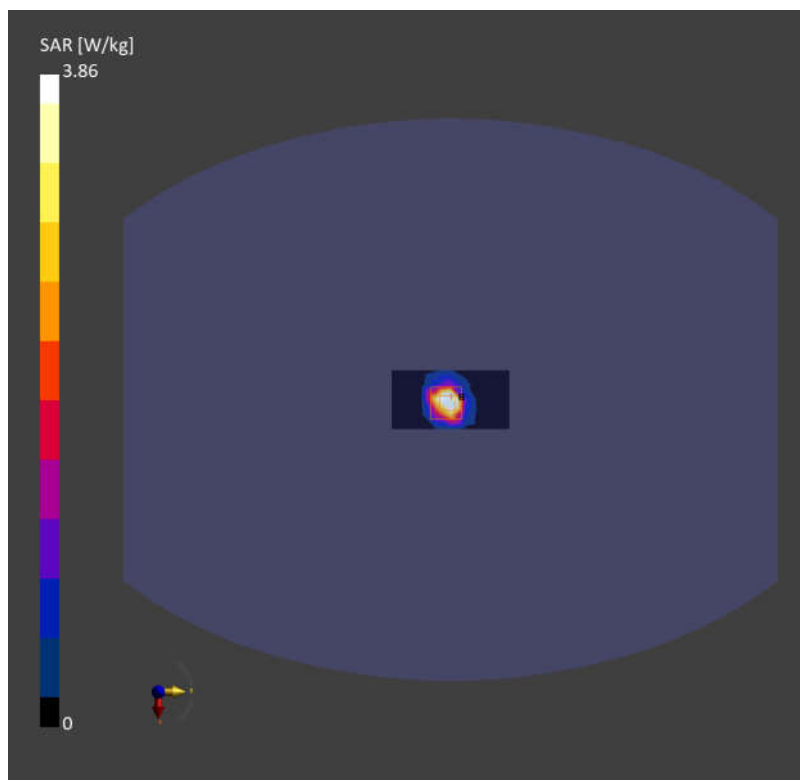

Date: 2025-08-19

System Check_Head_5250MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1

Medium: HSL_5250_250819 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.66$ S/m; $\epsilon_r = 36.5$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.92, 5.86, 5.95); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.59 W/kg; SAR (10g) = 1.07 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 3.85 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 66.1 %

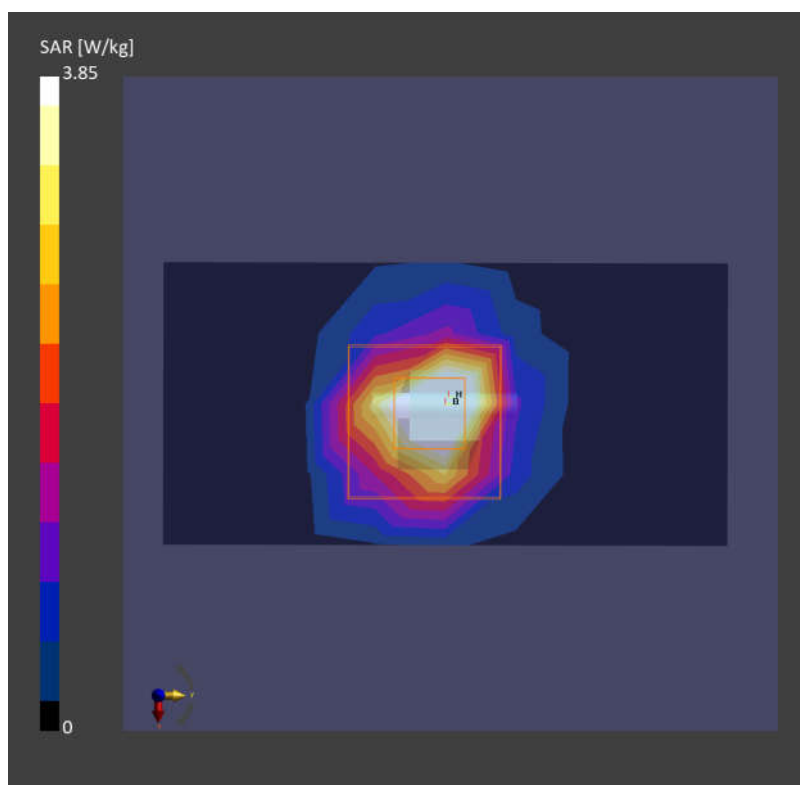

Date: 2025-07-27

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_250727 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.02$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(5.4, 5.52, 5.3); Calibrated: 2024-08-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.05 W/kg; SAR (10g) = 1.20 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 4.27 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.3 %

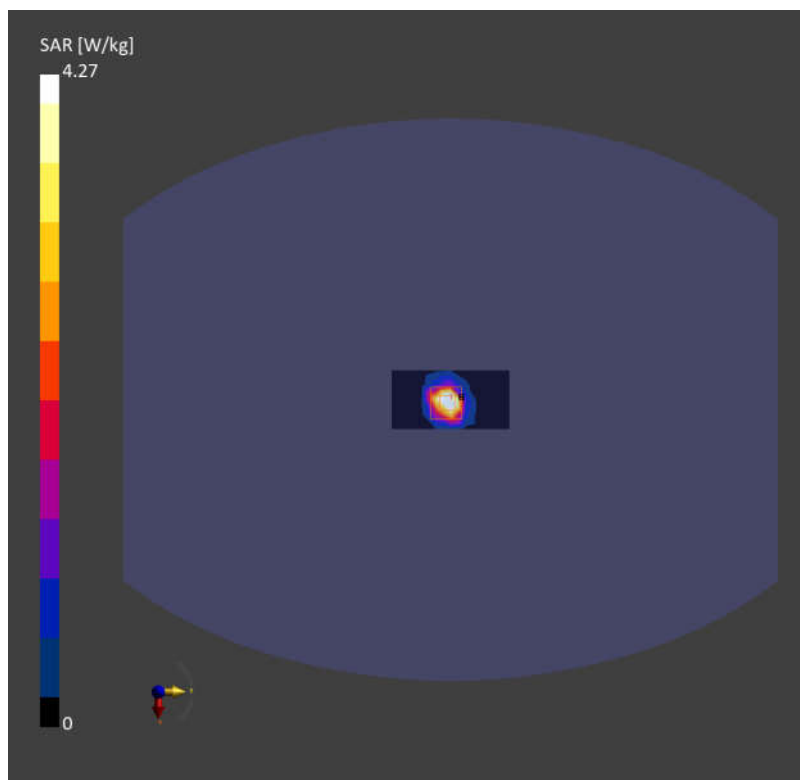

Date: 2025-08-21

System Check_Head_5600MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600_250821 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.06$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.48, 5.43, 5.51); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.95 W/kg; SAR (10g) = 1.17 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 4.31 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.3 %

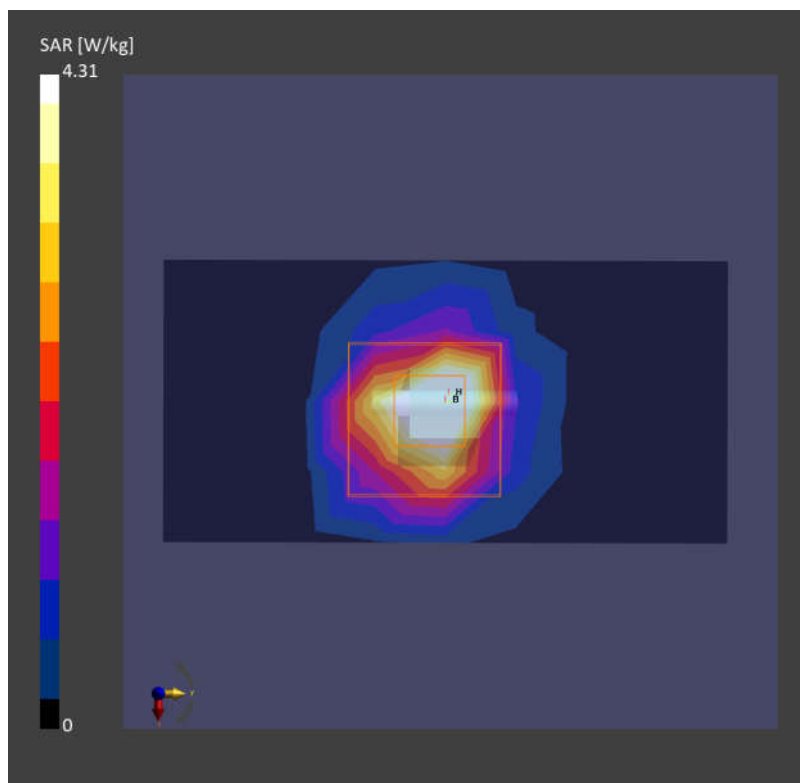

Date: 2025-07-29

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5750_250729 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.13$ S/m; $\epsilon_r = 35.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7630; ConvF(5.55, 5.67, 5.44); Calibrated: 2024-08-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.60 W/kg; SAR (10g) = 1.06 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.11 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.6 %

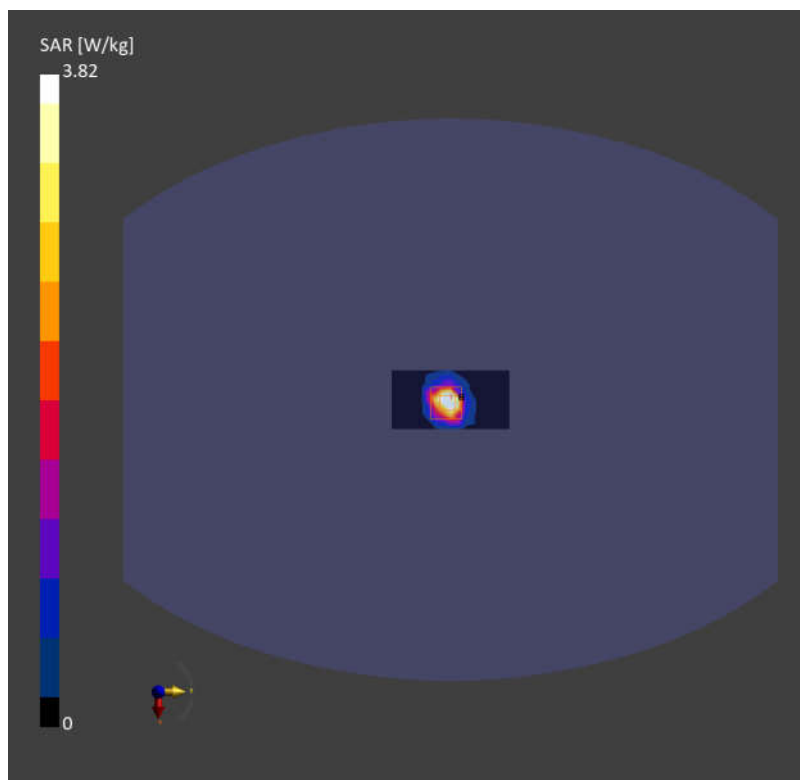

Date: 2025-08-25

System Check_Head_5750MHz**DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1

Medium: HSL_5750_250825 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.23$ S/m; $\epsilon_r = 35.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(5.57, 5.52, 5.6); Calibrated: 2025-07-01
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1338; Calibrated: 2025-03-18
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.55 W/kg; SAR (10g) = 1.04 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm
mm x 1.4 mm

Power Drift = -0.04 dB

SAR (1g) = 3.90 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 60.6 %

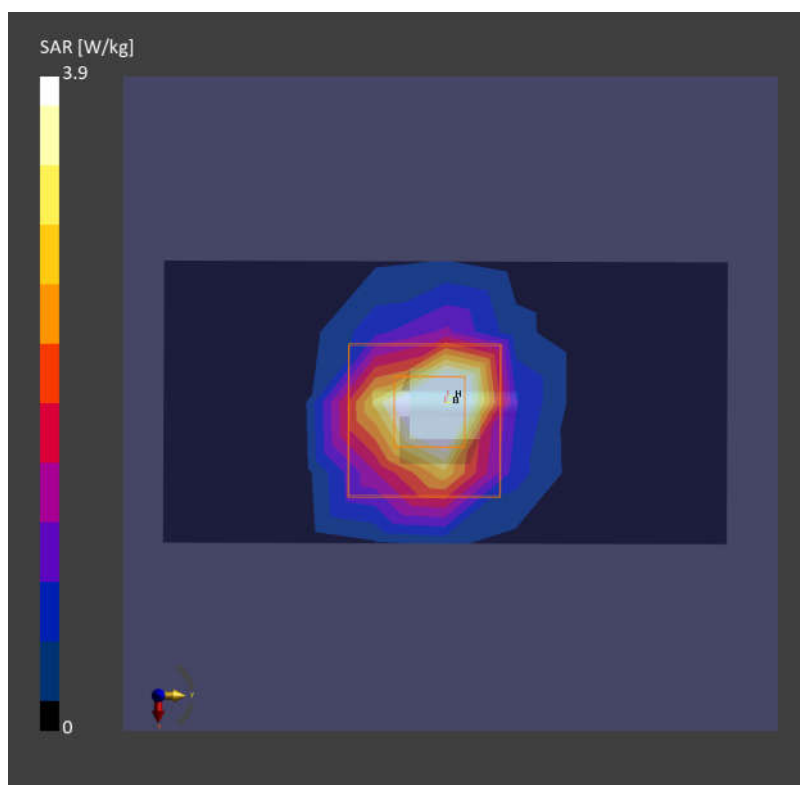

Date: 2025-08-02

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6500_250802 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.10$ S/m; $\epsilon_r = 34.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.34, 6.3, 5.44); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1650; Calibrated: 2024-11-25
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 13.7 W/kg; SAR (10g) = 2.93 W/kg;

Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm
x 1.4 mm


Power Drift = -0.03 dB

SAR (1g) = 15.2 W/kg; SAR (10g) = 2.98 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 56.5 %

psAPD (4.0cm2, sq) = 71.6 [W/m2]

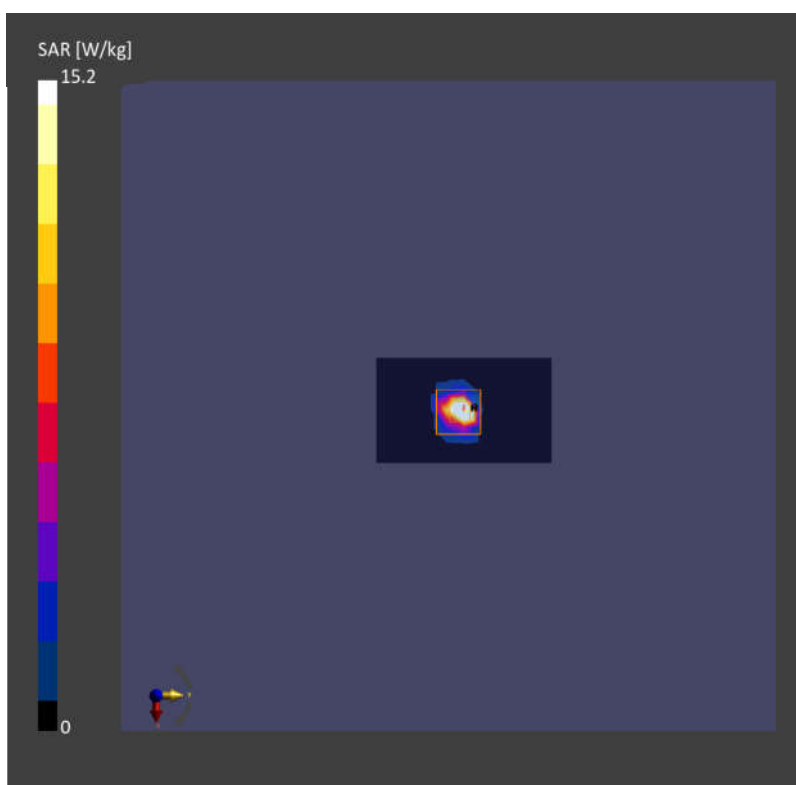

Date: 2025-08-28

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6500_250828 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.10$ S/m; $\epsilon_r = 34.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.34, 6.3, 5.44); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 13.7 W/kg; SAR (10g) = 2.93 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 15.4 W/kg; SAR (10g) = 2.85 W/kg

Smallest distance from peaks to all points 3 dB below = 4.8 mm

Ratio of SAR at M2 to SAR at M1 = 56.5 %

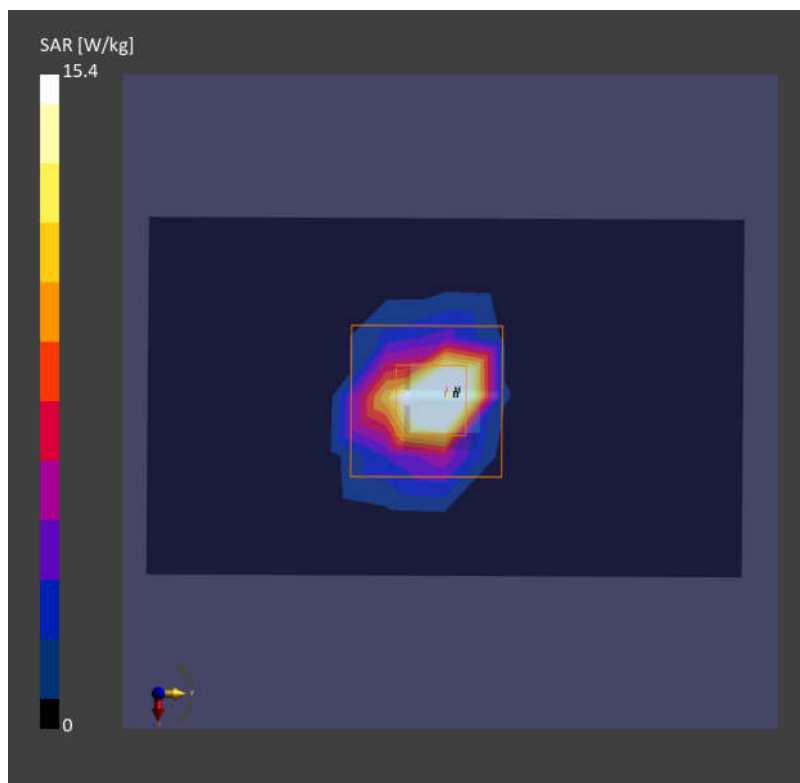psAPD (4.0cm², sq) = 70.9 [W/m²]

Date: 2025-09-12

System Check_Head_6500MHz**DUT: D6.5GHzV2 - SN1026**

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6500MHz_250912 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.07$ S/m; $\epsilon_r = 34.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.34, 6.3, 5.44); Calibrated: 2025-05-22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1691; Calibrated: 2025-06-04
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2135; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Pin=50mW/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 10.7 W/kg; SAR (10g) = 2.35 W/kg;


Pin=50mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.11 dB

SAR (1g) = 15.2 W/kg; SAR (10g) = 2.81 W/kg

Smallest distance from peaks to all points 3 dB below = 4.9 mm

Ratio of SAR at M2 to SAR at M1 = 51.0 %

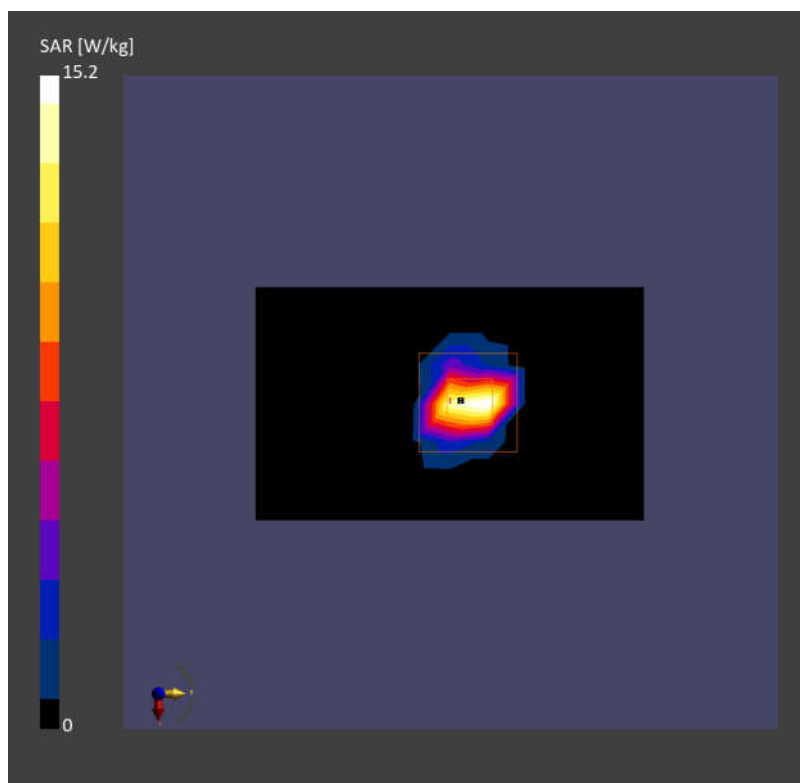psAPD (4.0cm², sq) = 67.0 [W/m²]

Measurement Report for Source 10G, FRONT, Validation band, CW, Channel 10000 (10000.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]
Source 10G,	100.0 x 100.0 x 105.0

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor
5G	FRONT, 10.00	Validation band	CW, 0--	10000.0, 10000	1.0

Hardware Setup

Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave - 1065	Air -	EUmmWV4 - SN9553_F1-55GHz, 2024-11-15	DAE4 Sn1650, 2024-11-25

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.125 x 0.125
Sensor Surface [mm]	10.0
MAIA	N/A

Measurement Results

Scan Type	5G Scan
Date	2025-08-05
Avg. Area [cm ²]	4.00
psPDn+ [W/m ²]	99.8
psPDtot+ [W/m ²]	100
psPDmod+ [W/m ²]	104
E _{max} [V/m]	242
Power Drift [dB]	0.03

