

Date: 2026/2/5

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 41.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(7.28, 6.99, 6.98); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 12.7 W/kg; SAR (10g) = 5.99 W/kg;


Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 12.7 W/kg; SAR (10g) = 5.96 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.4 %

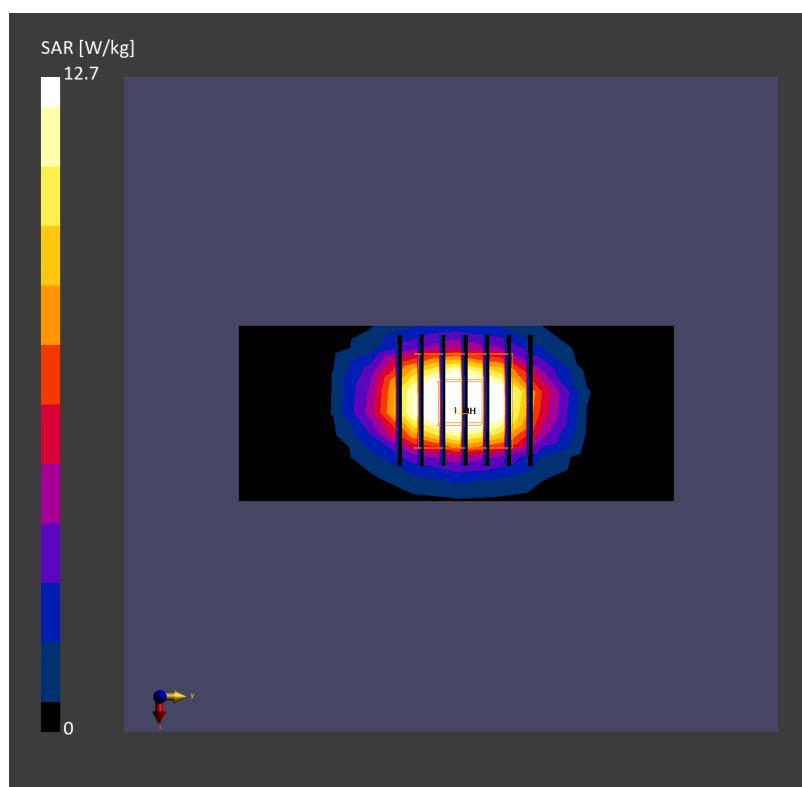

Date: 2026/2/6

System Check_5600MHz**DUT:D5GHzV2-SN:1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.00$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7930; ConvF(5.27, 5.06, 5.05); Calibrated: 2025/7/21
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1664; Calibrated: 2025/7/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm

SAR (1g) = 7.78 W/kg; SAR (10g) = 2.26 W/kg;

Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 8.18 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.4 %

