

Date: 2026-08-19

System Check_2450MHz**DUT: D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450MHz_260819 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 39.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8, 7.92, 7.79); Calibrated: 2026-06-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0-


Pin=250 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 13.2 W/kg; SAR (10g) = 6.25 W/kg;**Pin=250 mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.11 dB

SAR (1g) = 12.6 W/kg; SAR (10g) = 5.91 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.0 %

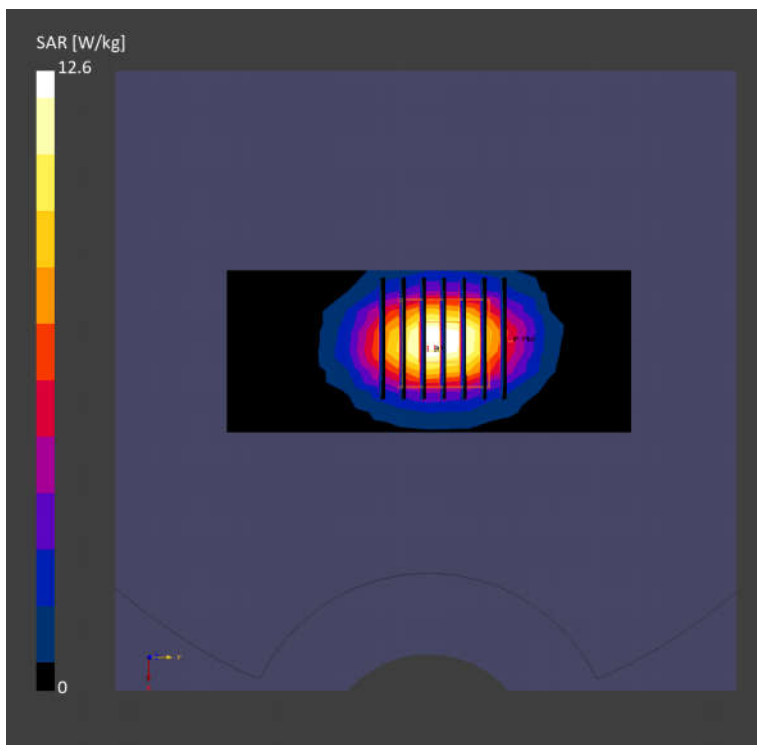

Date: 2026-08-19

System Check_5600MHz**DUT: D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL_5600MHz_260819 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.11$ S/m; $\epsilon_r = 35.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.4, 5.34, 5.25); Calibrated: 2026-06-30
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2025-11-28
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 18.0.0.7250
- UID: CW, 0-

Pin=100 mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
SAR (1g) = 8.11 W/kg; SAR (10g) = 2.44 W/kg;**Pin=100 mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 8.79 W/kg; SAR (10g) = 2.48 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 60.1 %

