

Date: 2025-03-13

**System Check\_Head\_2450MHz****DUT: D2450V2 - SN1095**

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used:  $f = 2450.000$  MHz;  $\sigma = 1.77$  S/m;  $\epsilon_r = 39.3$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN7774; ConvF(6.08, 6.63, 6.23); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: 16.4.0.5005

**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 10.0mm

SAR (1g) = 2.64 W/kg; SAR (10g) = 1.25 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0mm x 5.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 2.84 W/kg; SAR (10g) = 1.31 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.3 %

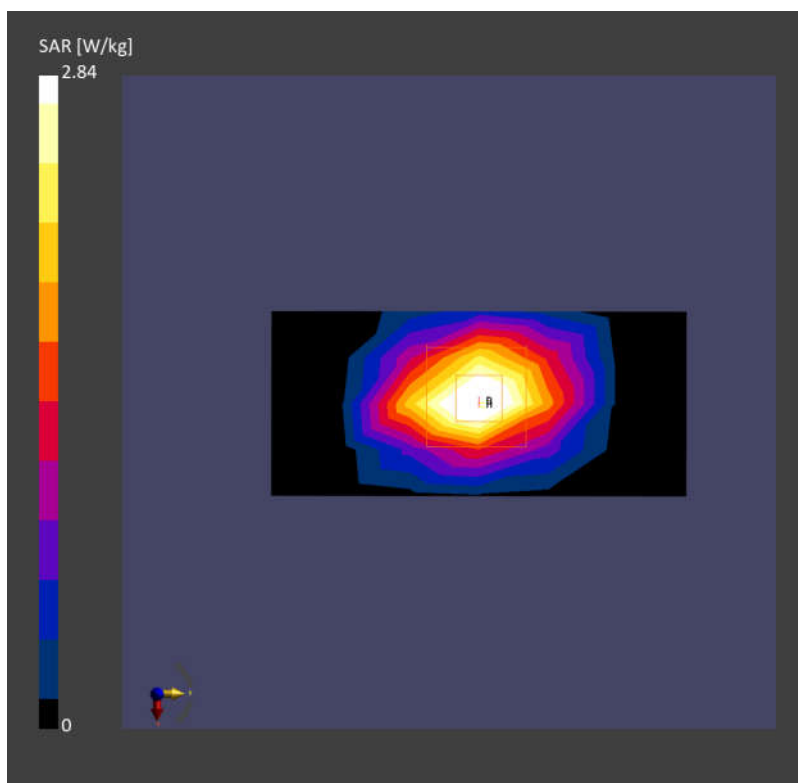

Date: 2025-03-14

**System Check\_Head\_5250MHz****DUT: D5GHzV2 - SN1113**


Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 5250.000$  MHz;  $\sigma = 4.74$  S/m;  $\epsilon_r = 35.9$   
Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN7774; ConvF(4.32, 4.72, 4.38); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: 16.4.0.5005

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0mm  
SAR (1g) = 4.47 W/kg; SAR (10g) = 1.33 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0mm x 4.0 mm x 1.4 mm  
Power Drift = -0.05 dB  
SAR (1g) = 4.37 W/kg; SAR (10g) = 1.24 W/kg  
Smallest distance from peaks to all points 3 dB below = 6.9 mm  
Ratio of SAR at M2 to SAR at M1 = 69.8 %

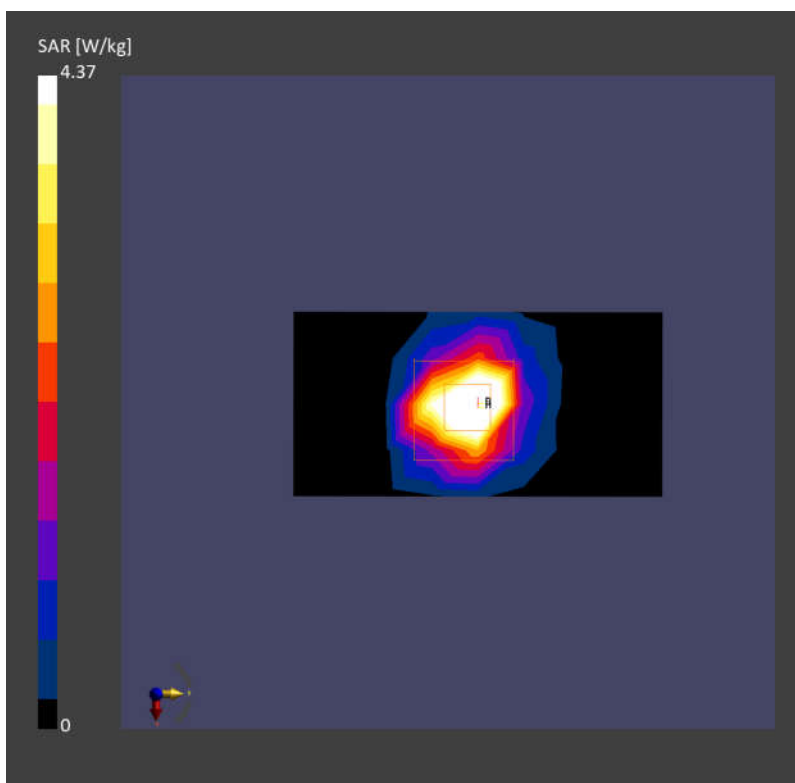

Date: 2025-03-15

**System Check\_Head\_5600MHz****DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used:  $f = 5600.000$  MHz;  $\sigma = 5.16$  S/m;  $\epsilon_r = 35.3$ 

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN7774; ConvF(3.87, 4.18, 3.91); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: 16.4.0.5005

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0mm

SAR (1g) = 4.61 W/kg; SAR (10g) = 1.35 W/kg;


**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.44 W/kg; SAR (10g) = 1.26 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 66.2 %

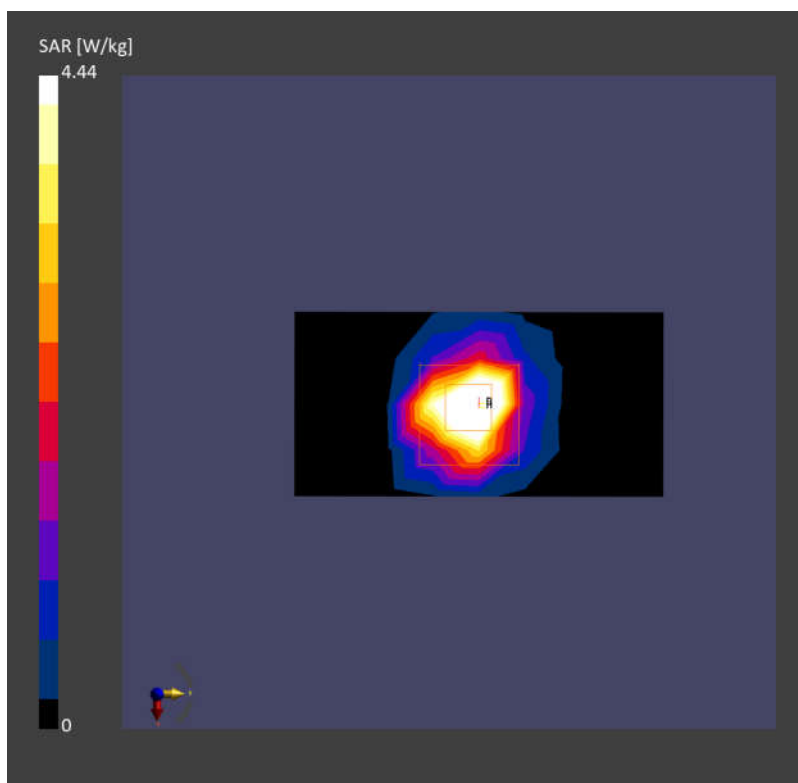

Date: 2025-03-16

**System Check\_Head\_5750MHz****DUT: D5GHzV2 - SN1113**

Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 5750.000$  MHz;  $\sigma = 5.34$  S/m;  $\epsilon_r = 35.0$   
Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN7774; ConvF(3.91, 4.24, 3.96); Calibrated: 2024-06-27
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2024-05-23
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2074; Section: Flat
- Measurement Software: 16.4.0.5005

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0mm  
SAR (1g) = 4.38 W/kg; SAR (10g) = 1.30 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0mm x 4.0 mm x 1.4 mm  
Power Drift = -0.04 dB  
SAR (1g) = 4.26 W/kg; SAR (10g) = 1.11 W/kg  
Smallest distance from peaks to all points 3 dB below = 7.4 mm  
Ratio of SAR at M2 to SAR at M1 = 65.4 %

