

Date: 2025-11-04

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.912$ S/m; $\epsilon_r = 42.1$


Ambient Temperature: 23.5°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.53, 10.34, 10.38); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 210.0 mm): Measurement Grid: 15.0 mm x 15.0 mm
SAR (1g) = 2.35 W/kg; SAR (10g) = 1.59 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.21 W/kg; SAR (10g) = 1.39 W/kg
Smallest distance from peaks to all points 3 dB below = 20.1 mm
Ratio of SAR at M2 to SAR at M1 = 85.5 %

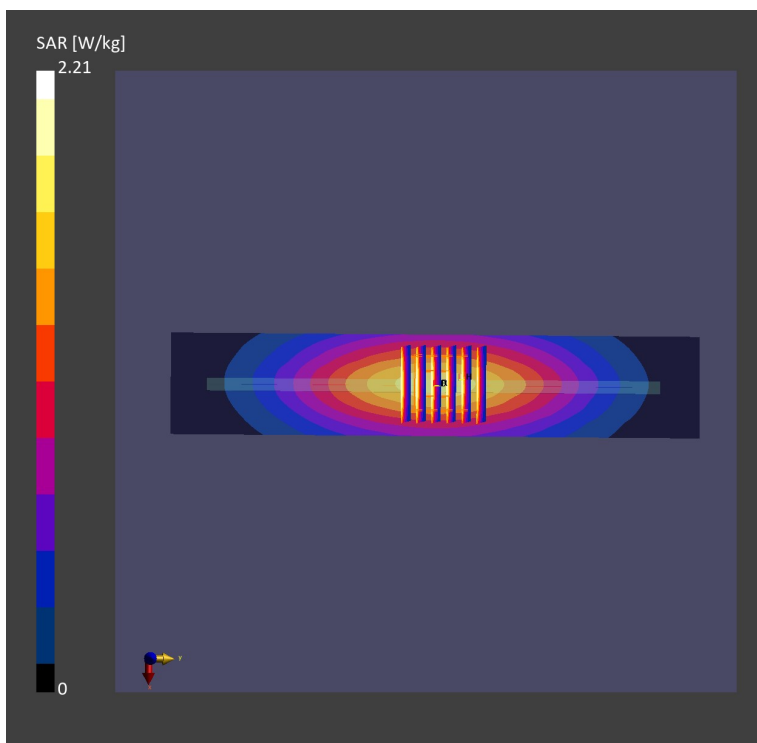

Date: 2025-11-04

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.934$ S/m; $\epsilon_r = 41.5$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(10.23, 10.04, 10.08); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (36.0 mm x 210.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 2.57 W/kg; SAR (10g) = 1.65 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.08 dB

SAR (1g) = 2.35 W/kg; SAR (10g) = 1.43 W/kg

Smallest distance from peaks to all points 3 dB below = 16.5 mm

Ratio of SAR at M2 to SAR at M1 = 87.4 %

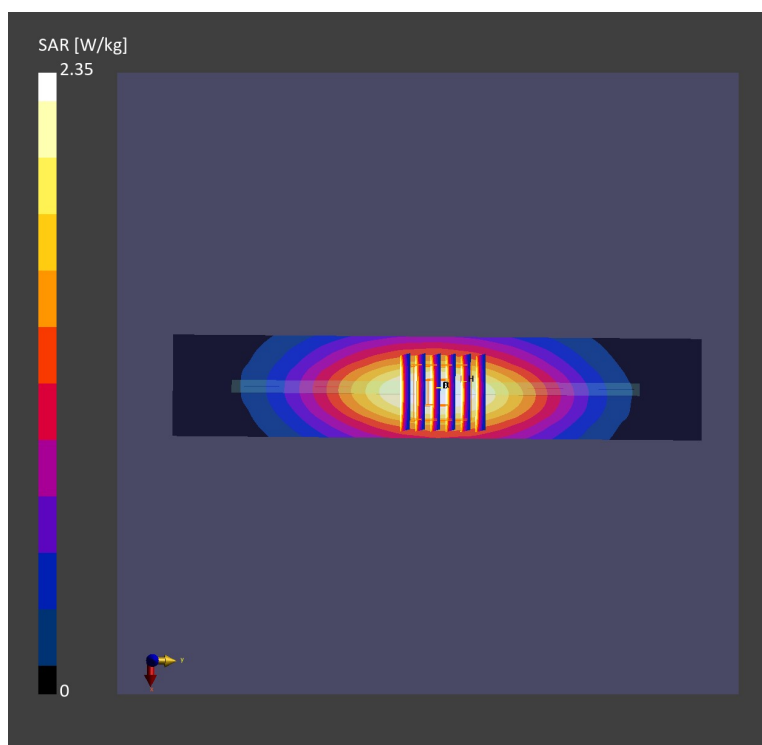

Date: 2025-11-05

System Check_1750MHz**DUT:D1750V2-SN:1090**

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 41.2$

Ambient Temperature: 23.8°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.61, 8.45, 8.49); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 9.77 W/kg; SAR (10g) = 5.13 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.14 dB

SAR (1g) = 8.93 W/kg; SAR (10g) = 4.99 W/kg

Smallest distance from peaks to all points 3 dB below = 10.2 mm

Ratio of SAR at M2 to SAR at M1 = 84.8 %

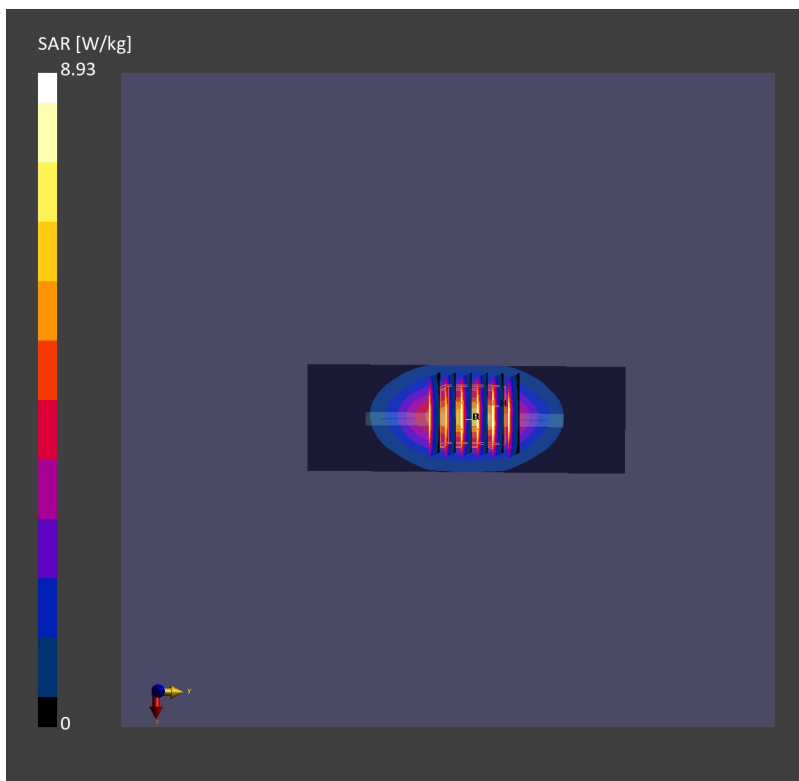

Date: 2025-11-05

System Check_1900MHz**DUT:D1900V2-SN:5d182**


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 39.5$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(8.33, 8.18, 8.21); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 15.0 mm x 15.0 mm
SAR (1g) = 10.7 W/kg; SAR (10g) = 5.51 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 10.1 W/kg; SAR (10g) = 5.32 W/kg
Smallest distance from peaks to all points 3 dB below = 9.9 mm
Ratio of SAR at M2 to SAR at M1 = 81.6 %

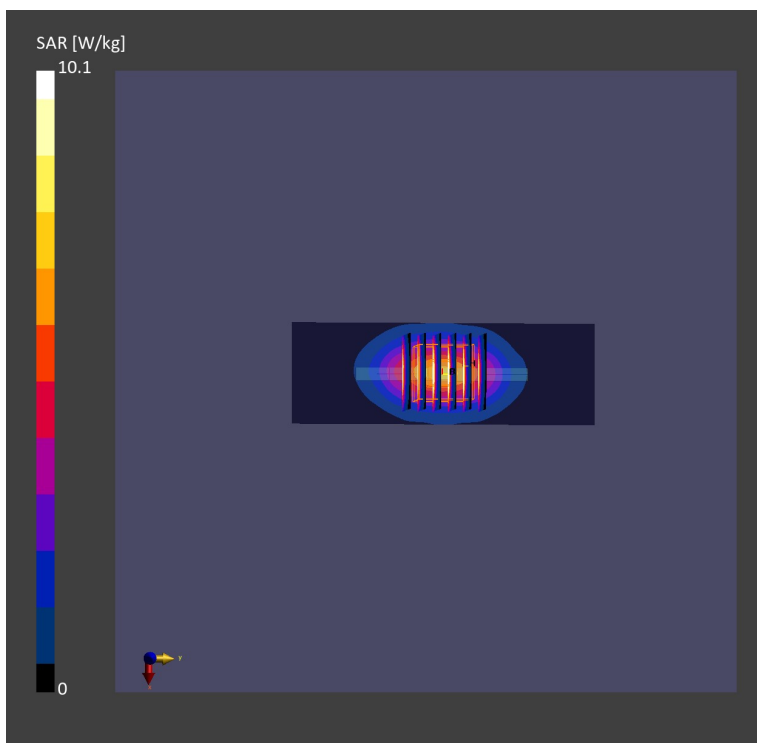

Date: 2025-12-03

System Check_2450MHz**DUT:D2450V2-SN:1095**

Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 39.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(7.87, 7.72, 7.76); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 14.5 W/kg; SAR (10g) = 6.44 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.07 dB

SAR (1g) = 13.1 W/kg; SAR (10g) = 6.17 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 83.5 %

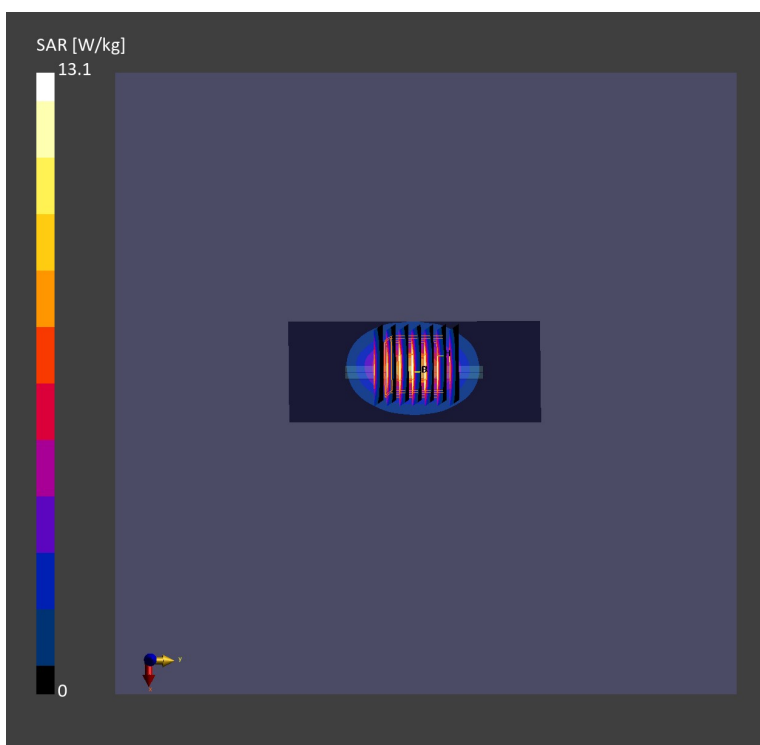

Date: 2025-12-08

System Check_5250MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.51$ S/m; $\epsilon_r = 34.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(6.08, 5.97, 6.0); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.61 W/kg; SAR (10g) = 2.27 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 8.11 W/kg; SAR (10g) = 2.15 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 65.5 %

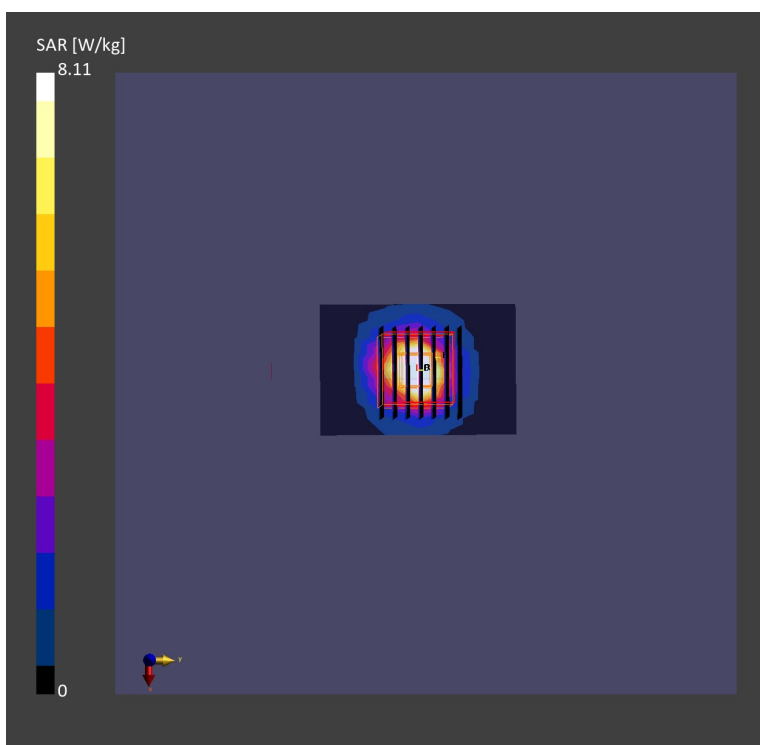

Date: 2025-12-08

System Check_5600MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 4.85$ S/m; $\epsilon_r = 34.3$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.54, 5.44, 5.47); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.87 W/kg; SAR (10g) = 2.26 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.15 dB

SAR (1g) = 8.79 W/kg; SAR (10g) = 2.31 W/kg

Smallest distance from peaks to all points 3 dB below = 7.8 mm

Ratio of SAR at M2 to SAR at M1 = 61.8 %

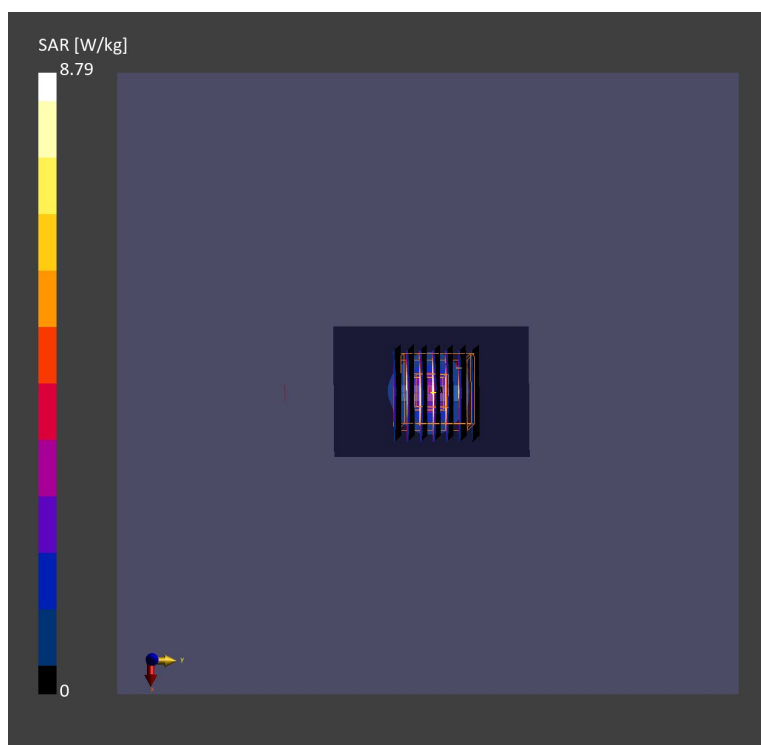

Date: 2025-12-09

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 34.0$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(5.52, 5.42, 5.44); Calibrated: 2025-06-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V8.0 (Left); Type: QD OVA 004 AA; Serial: 2131
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 7.55 W/kg; SAR (10g) = 2.23 W/kg;


Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.16 dB

SAR (1g) = 8.25 W/kg; SAR (10g) = 2.21 W/kg

Smallest distance from peaks to all points 3 dB below = 8.8 mm

Ratio of SAR at M2 to SAR at M1 = 61.5 %

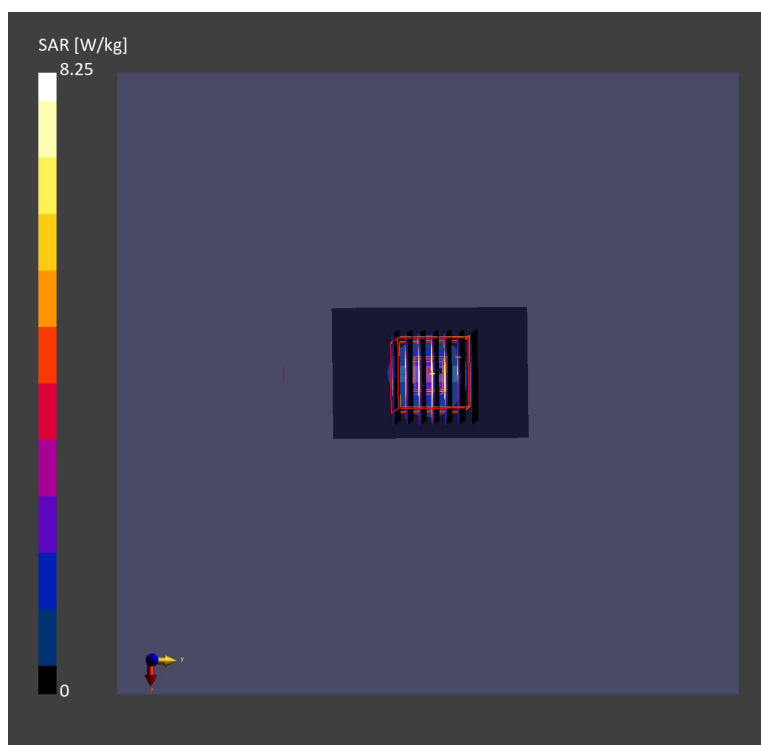

Date: 2025-11-06

System Check_13MHz**DUT: CLA-13 - SN:1023**

Communication System: CW; Frequency: 13.000 MHz; Duty Cycle: 1:1

Medium: Head Simulating Liquid Medium parameters used: $f = 13.000$ MHz; $\sigma = 0.739$ S/m; $\epsilon_r = 54.5$

Ambient Temperature: 23.7°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7641; ConvF(18.57, 19.41, 16.88); Calibrated: 2025-6-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1326; Calibrated: 2025-07-11
- Phantom: ELI V5.0 (20deg probe tilt); Serial: 1233; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=1000mW/Area Scan (40.0 mm x 90.0 mm): Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.565 W/kg; SAR (10g) = 0.359 W/kg;

Pin=1000mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 0.578 W/kg; SAR (10g) = 0.365 W/kg

Smallest distance from peaks to all points 3 dB below = 15.1 mm

Ratio of SAR at M2 to SAR at M1 = 77.5 %

