


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

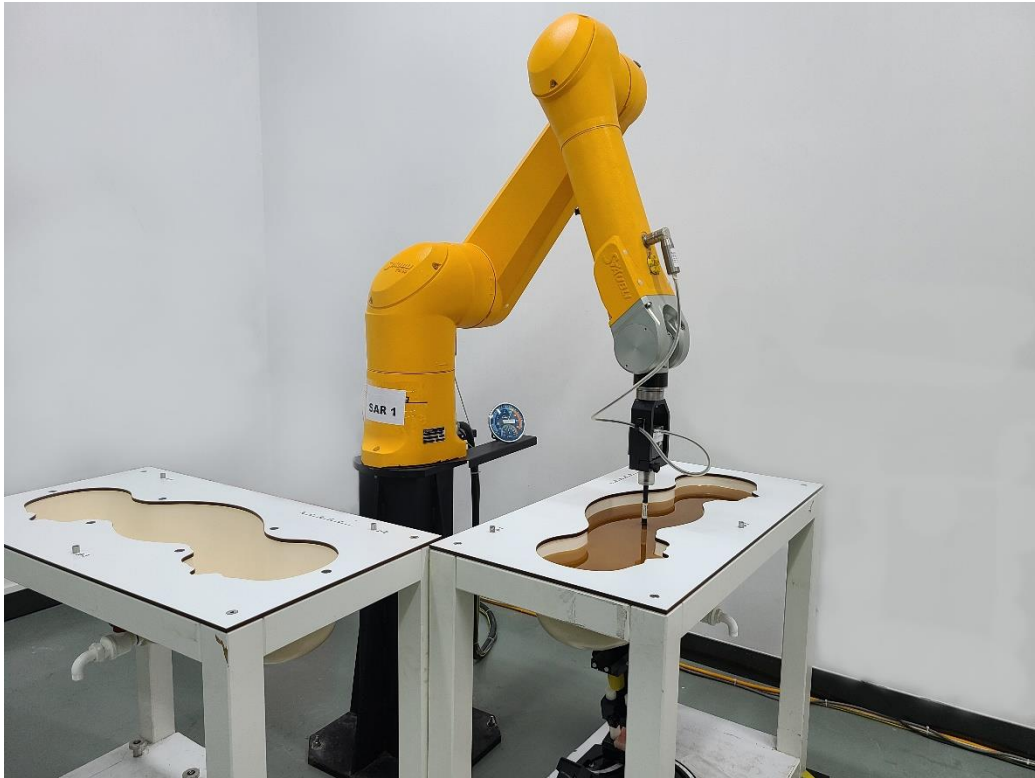

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the liquid level reaching approximately the 10 cm mark. The container has a blue outer rim and a white inner lining.	NA

3. Photographs of EUT test position



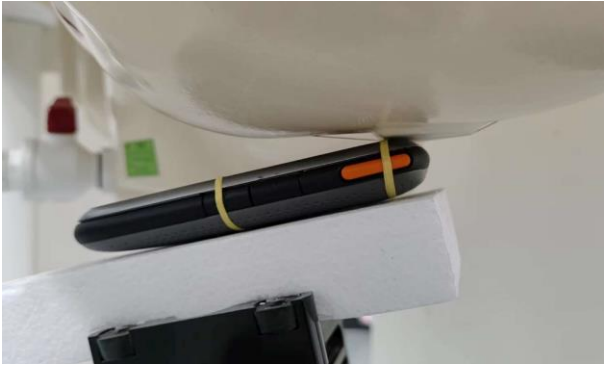
Photo 2: Left cheek	Photo 3: Left tilted
	
Photo 4: Right cheek	Photo 5: Right tilted
	
Photo 6: Front side 10mm	Photo 7: Back side 10mm
	

Photo 8: Left side 10mm	Photo 9: Right side 10mm
	
Photo 10: Top side 10mm	Photo 11: Bottom side 10mm
	

4. EUT Constructional Details

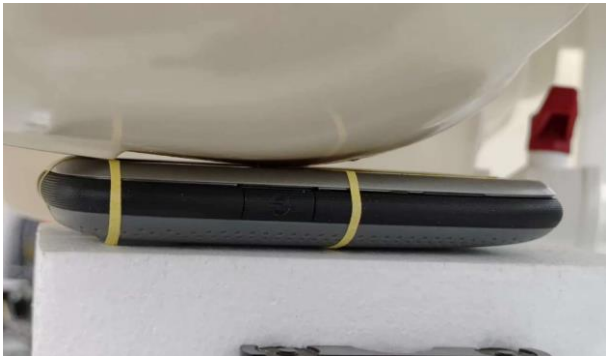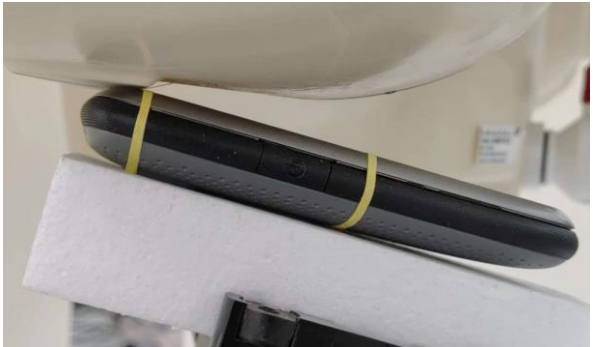