

APPENDIX**12. Photographs of Test Setup**

Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid (Head & Body)

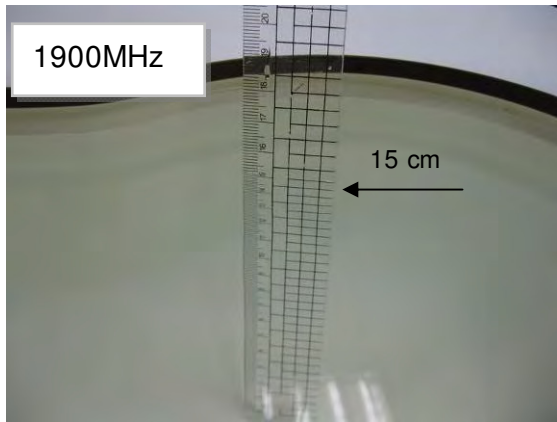


Fig.2.1

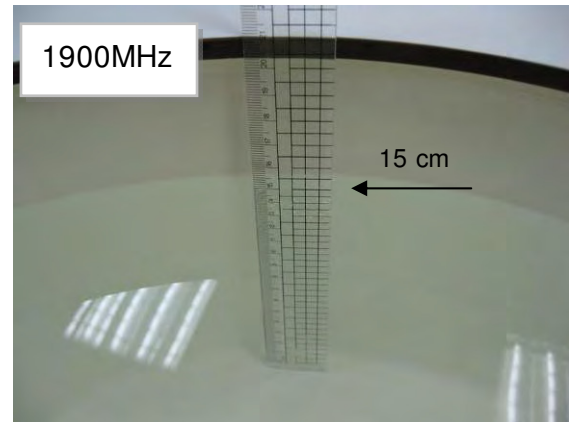


Fig.2.2

Head Mode

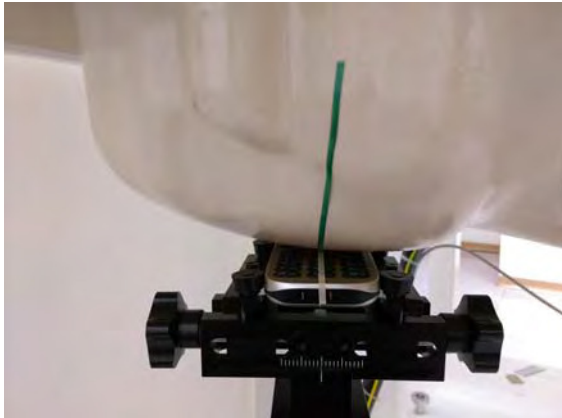


Fig.3 Right Head Section / Cheek-Touch Position

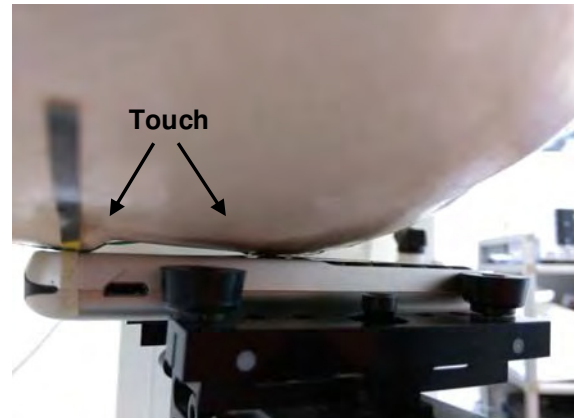


Fig.4 Right Head Section / Ear-Tilt Position(15°)



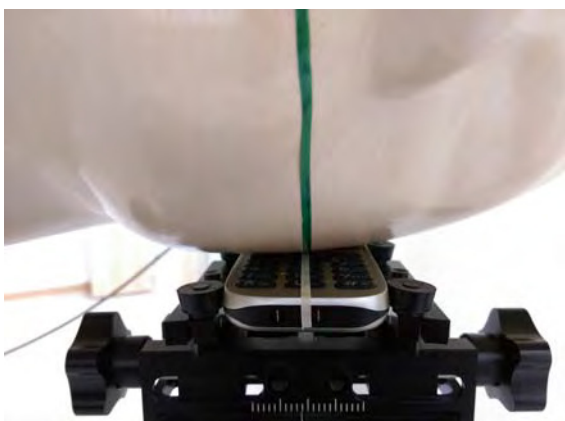


Fig.5 Left Head Section / Cheek-Touch Position

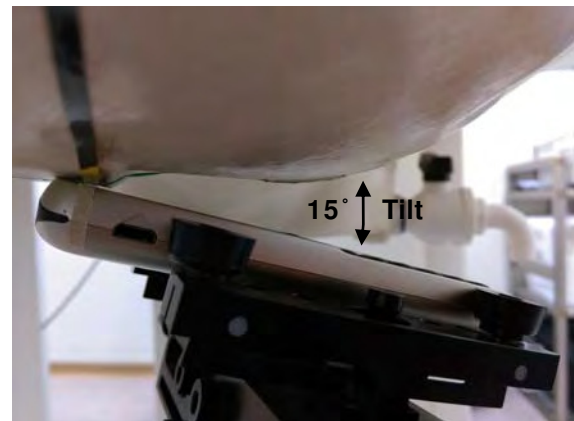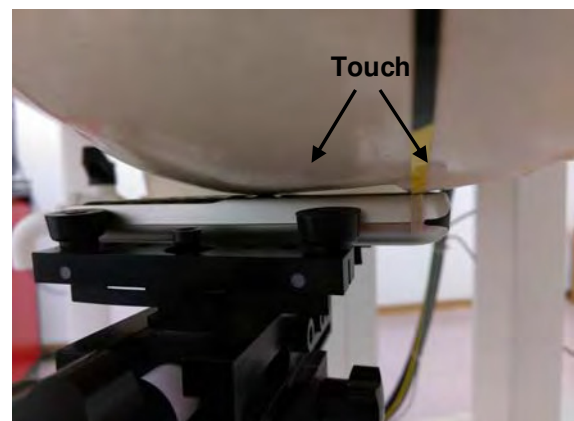

Head Mode

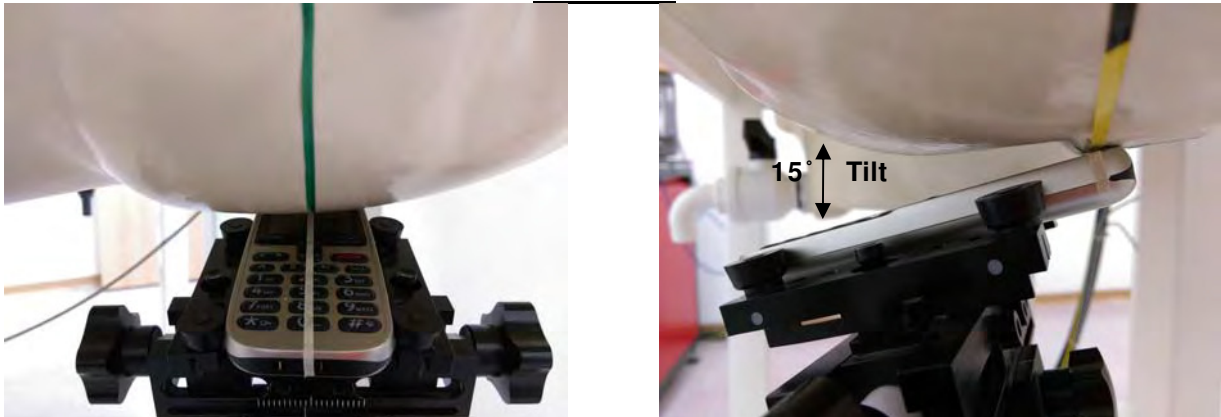


Fig.6 Left Head Section / Ear-Tilt Position(15°)

Body-worn - distance between flat phantom and mobile phone is 10 mm



Fig.7 EUT Front side to flat phantom

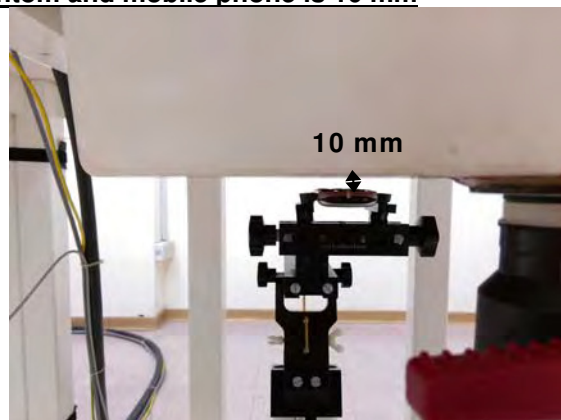


Fig.8 EUT Back side to flat phantom


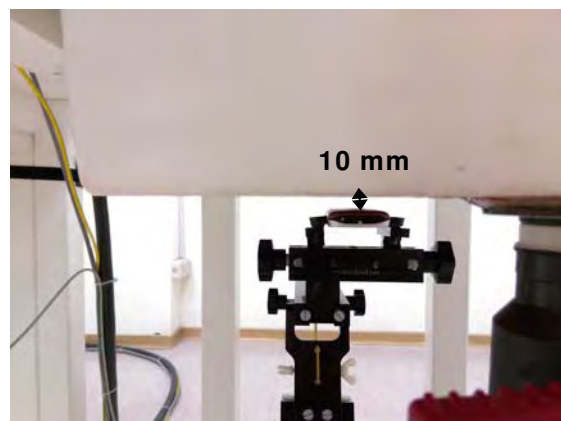


Fig.9 EUT Back side with headset to flat phantom

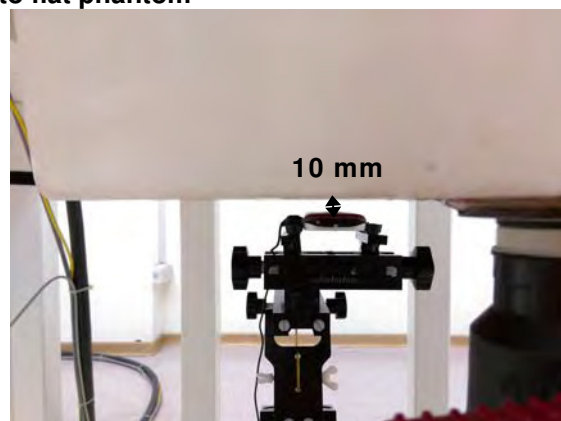

13. Photographs of the EUT



Fig.10 Front view of EUT



Fig.11 Back view of EUT



Fig.12 Headset



Fig.12 2nd Headset

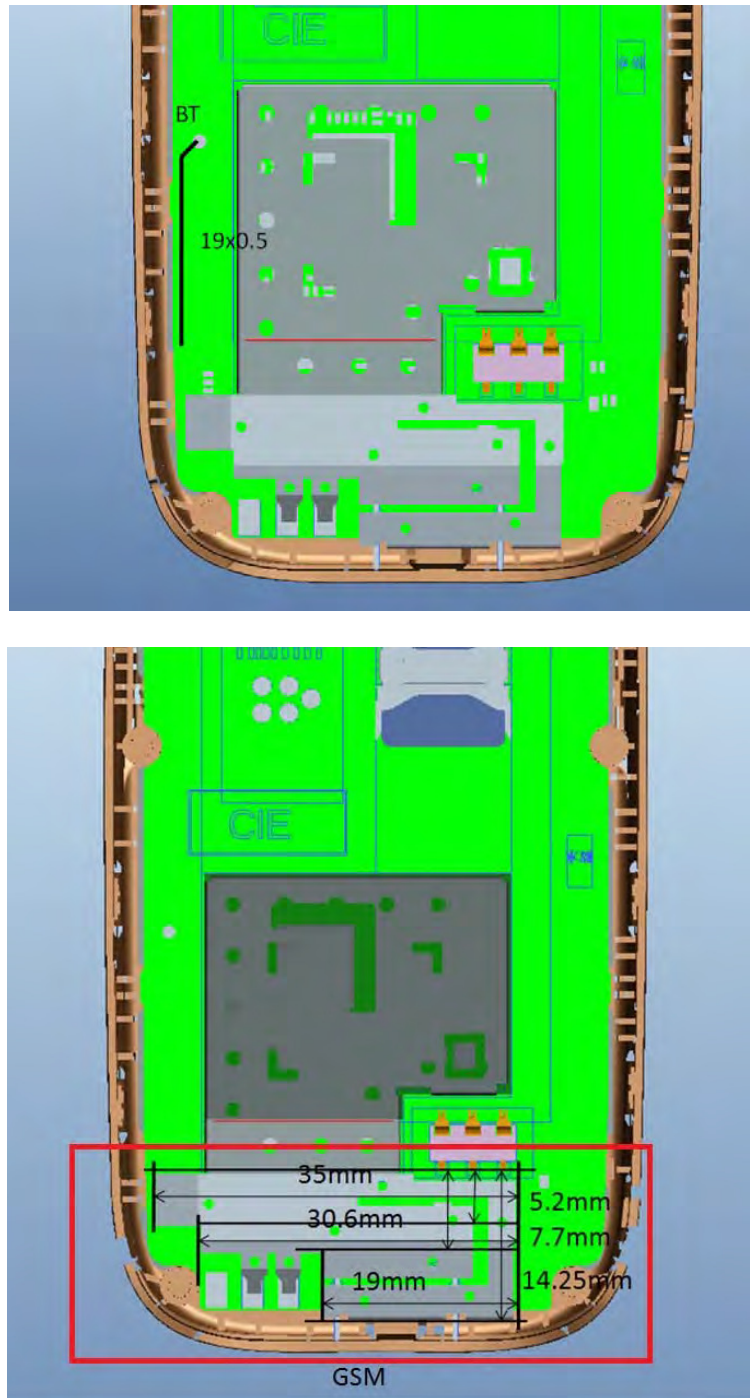


Fig.13 Antenna position of EUT

- End of Report -