




Roche Diabetes Care Inc Accu-Chek Guide Me Blood Glucose Meter 2444MHz
 Theta = 0, Phi = 0

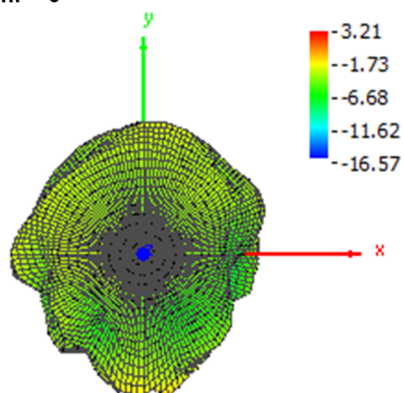


Theta = 180, Phi = 0

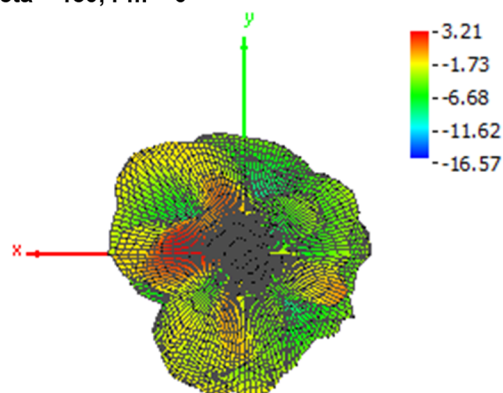


Theta = 90, Phi = 0

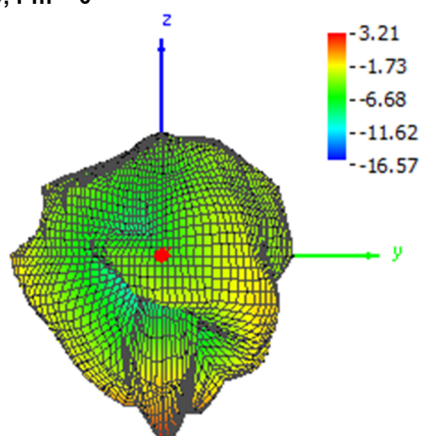


Theta = 90, Phi = 180

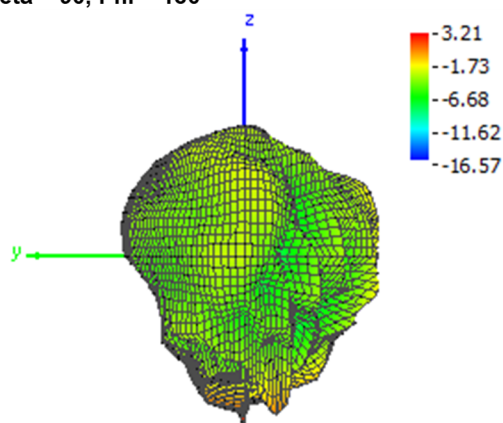


Theta = 90, Phi = 270

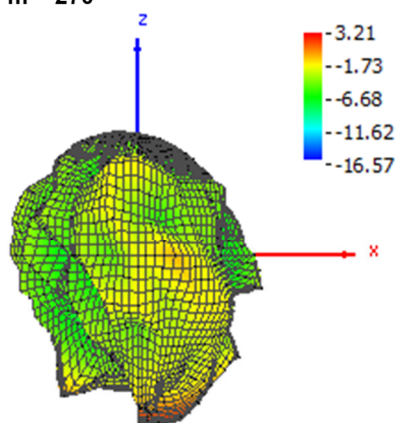


Theta = 90, Phi = 90

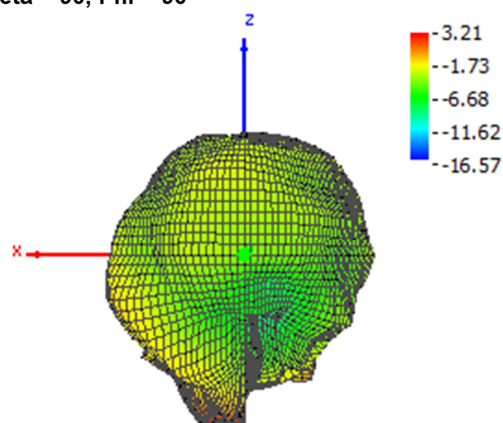


Roche Diabetes Care Inc Accu-Chek Guide Me Blood Glucose Meter 2480MHz
 Theta = 0, Phi = 0

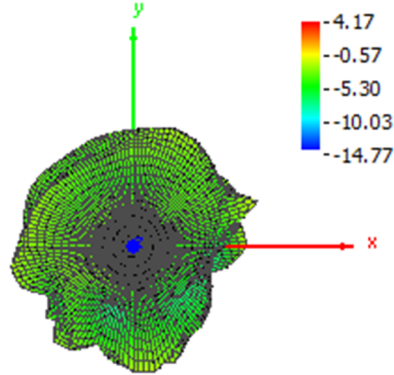


Theta = 180, Phi = 0

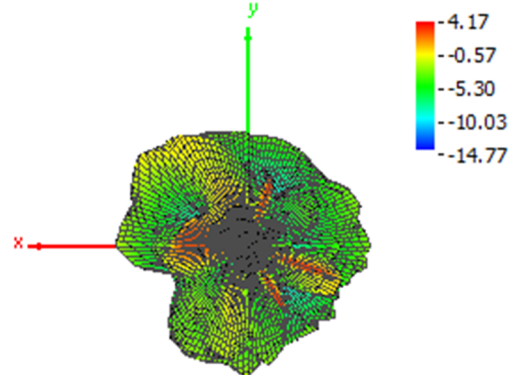


Theta = 90, Phi = 0

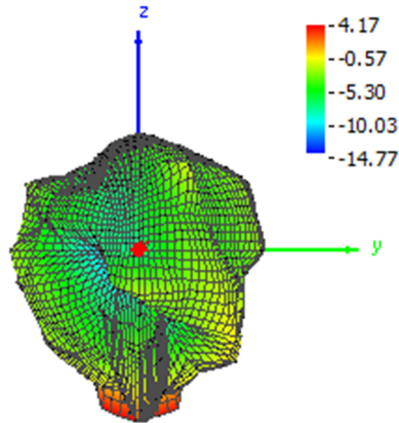


Theta = 90, Phi = 180

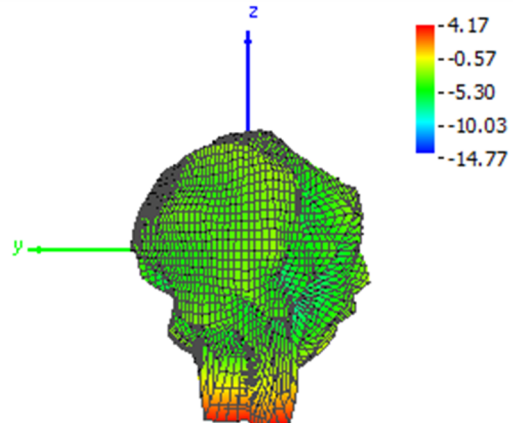

Theta = 90, Phi = 270

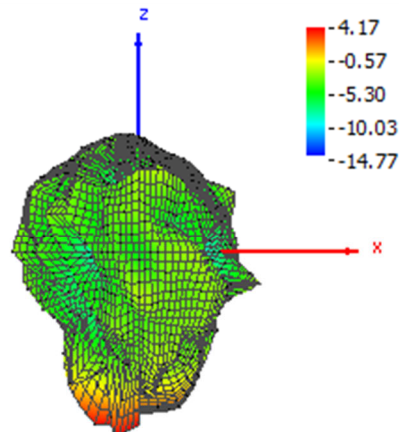



Theta = 90, Phi = 90

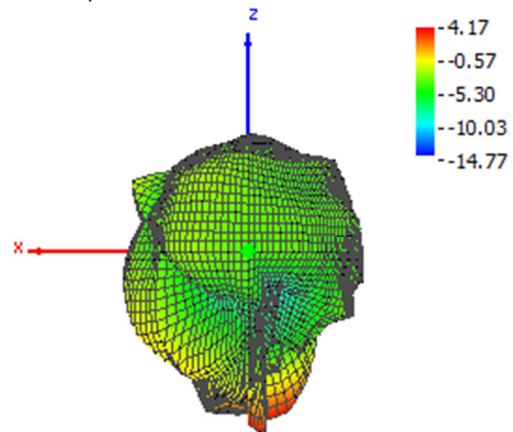

8.2. 2D TRP- Free Space

XY-plane

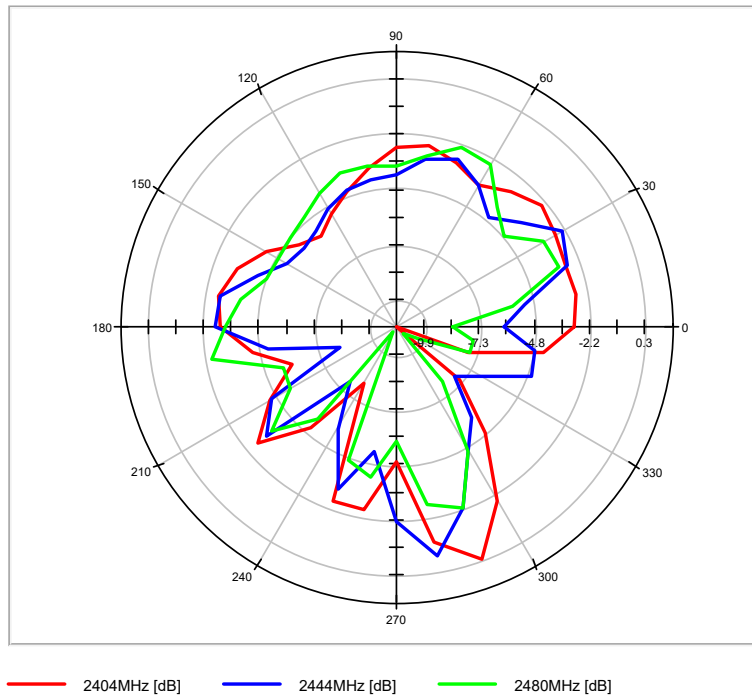

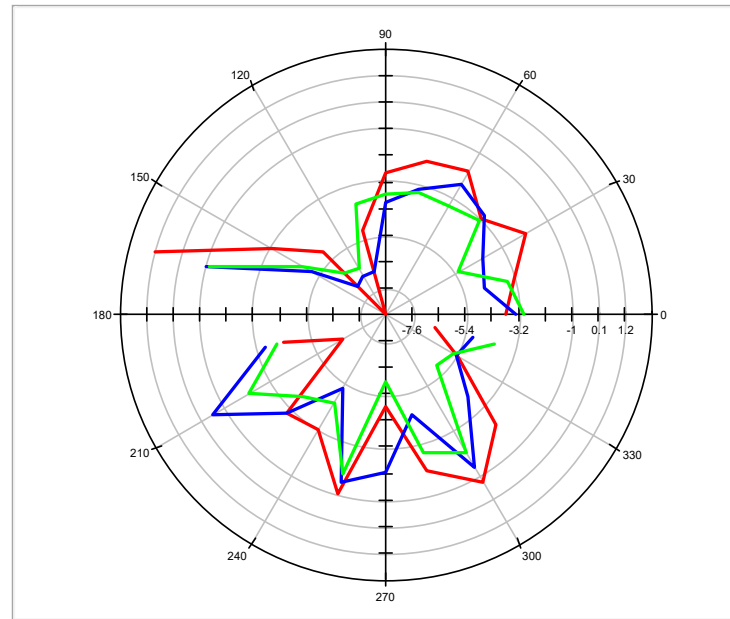

— 2404MHz [dB] — 2444MHz [dB] — 2480MHz [dB]

End of Report