



8.1. 3D TRP- Free Space

Roche Diabetes Care Inc Accu-Chek Instant Blood Glucose Meter 980mmol/L 2404MHz


Theta = 0, Phi = 0

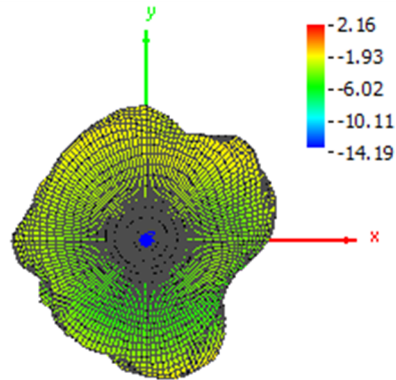


Theta = 180, Phi = 0

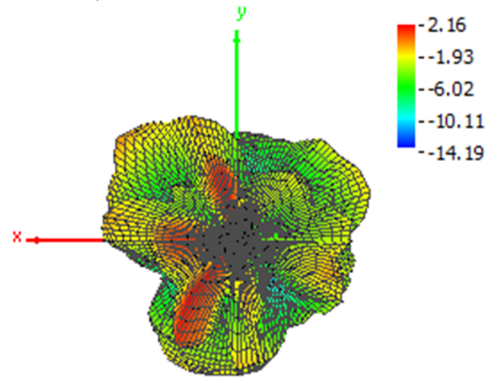


Theta = 90, Phi = 0

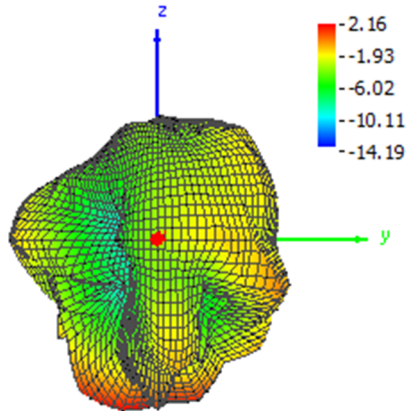


Theta = 90, Phi = 180

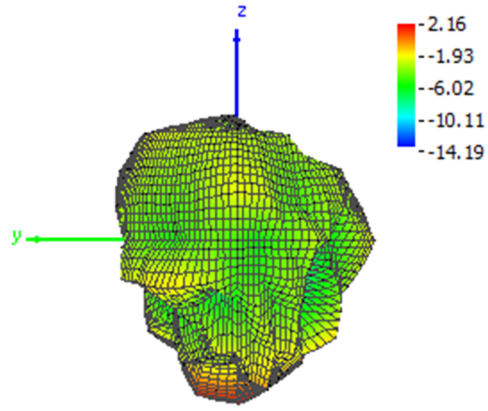


Theta = 90, Phi = 270

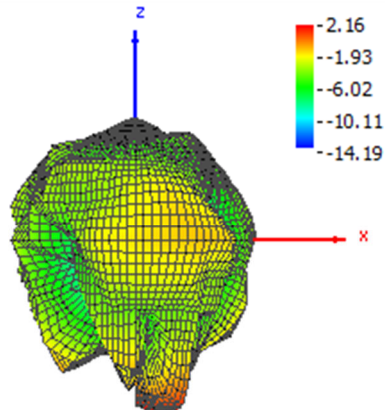


Theta = 90, Phi = 90

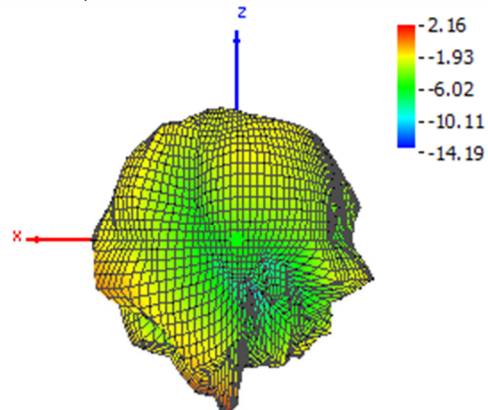


Roche Diabetes Care Inc Accu-Chek Instant Blood Glucose Meter 980mmol/L 2444MHz
 Theta = 0, Phi = 0

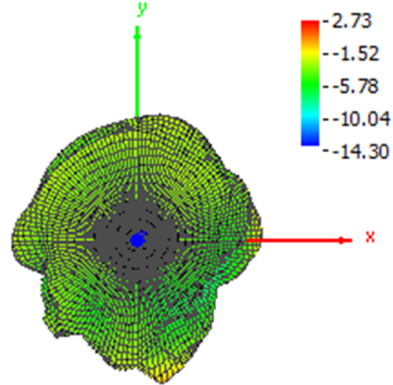


Theta = 180, Phi = 0

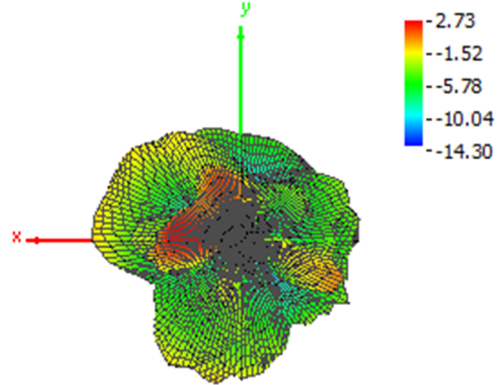


Theta = 90, Phi = 0

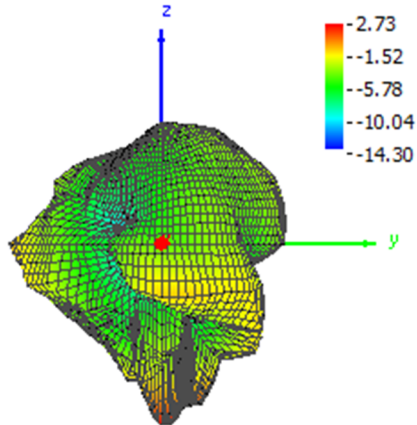

Theta = 90, Phi = 180

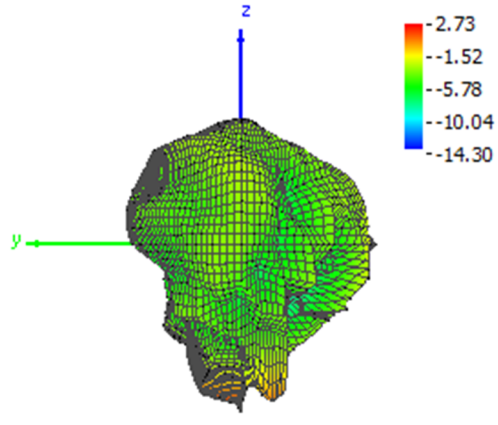

Theta = 90, Phi = 270

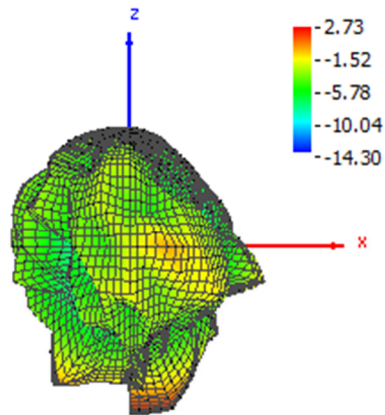

Theta = 90, Phi = 90

