



Roche Diabetes Care Inc Accu-Chek Instant Blood Glucose Meter 980mmol/L 2480MHz


Theta = 0, Phi = 0

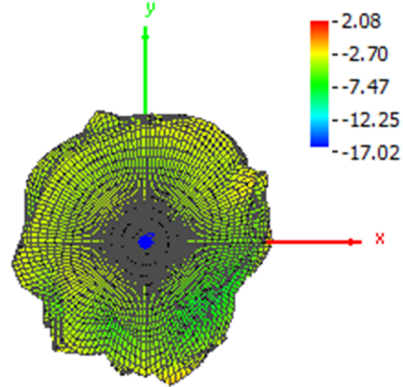


Theta = 180, Phi = 0

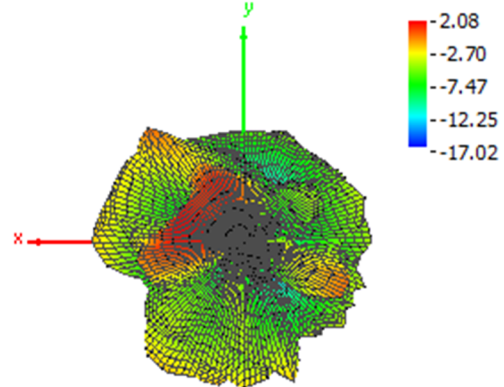


Theta = 90, Phi = 0

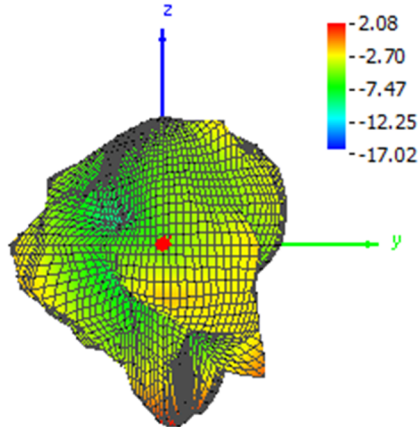


Theta = 90, Phi = 180

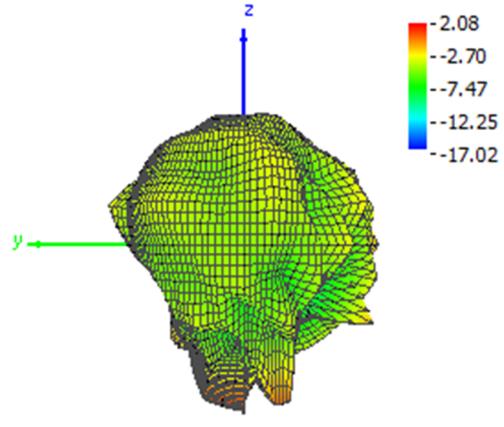


Theta = 90, Phi = 270

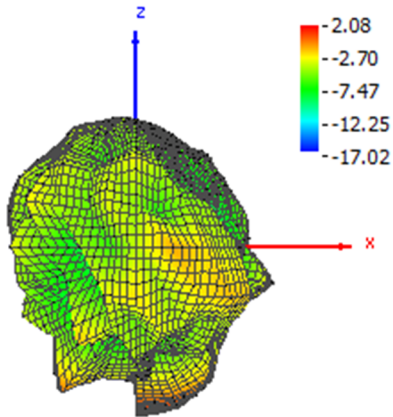

Theta = 90, Phi = 90

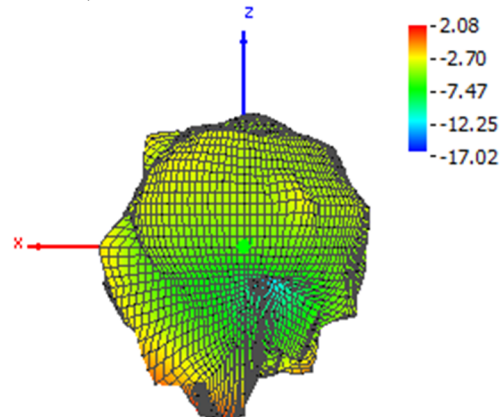

YZ_Plane

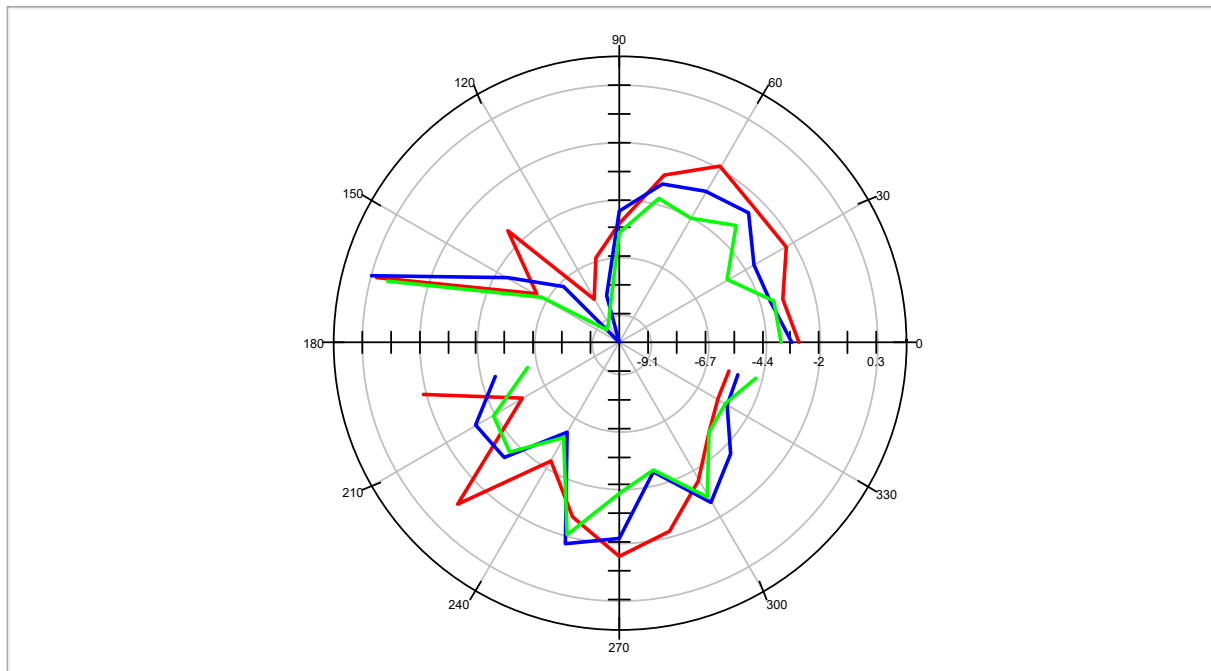

— 2404MHz [dB] — 2444MHz [dB] — 2480MHz [dB]

End of Report