


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

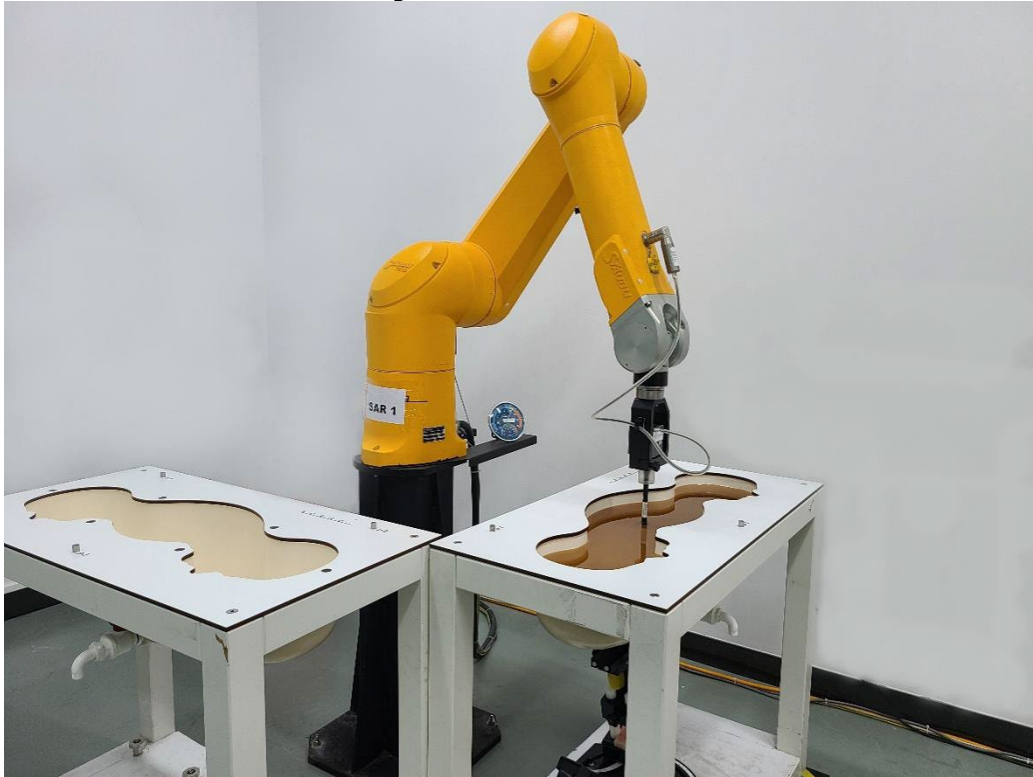

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

Photo 2: Left Cheek

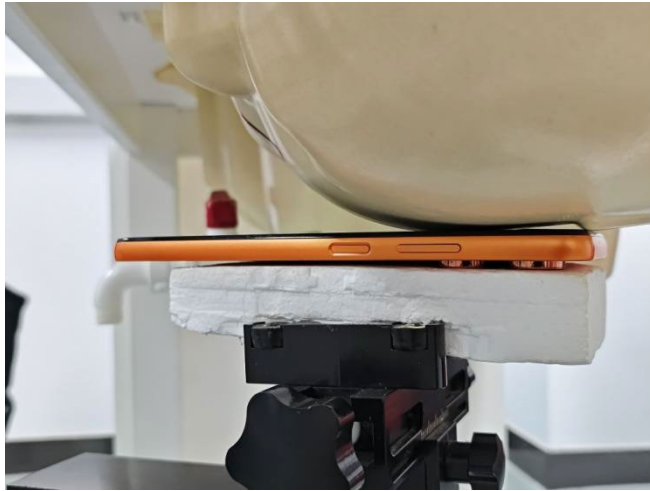


Photo 3: Left Tilted



Photo 4: Right Cheek

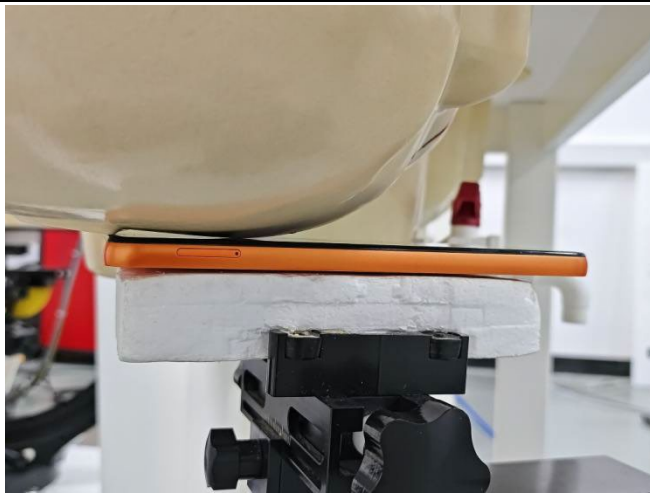


Photo 5: Right Tilted



Photo 6: Front Side 15mm



Photo 7: Back Side 15mm



Photo 8: Front Side 10mm



Photo 9: Back Side 10mm



Photo 10: Left Side 10mm



Photo 11: Right Side 10mm



Photo 12: Top Side 10mm

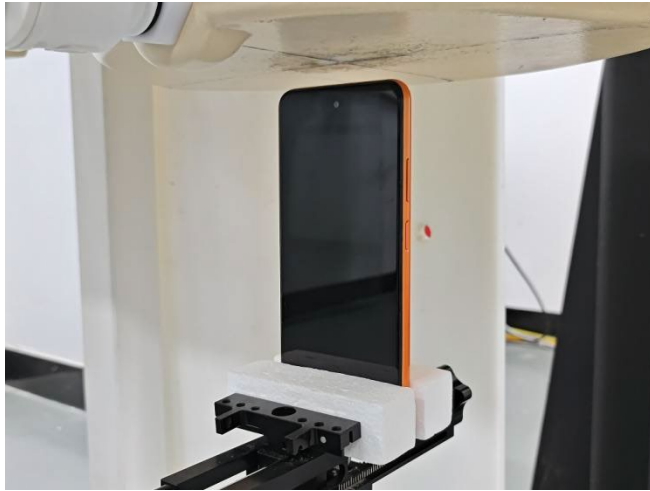


Photo 13: Bottom Side 10mm

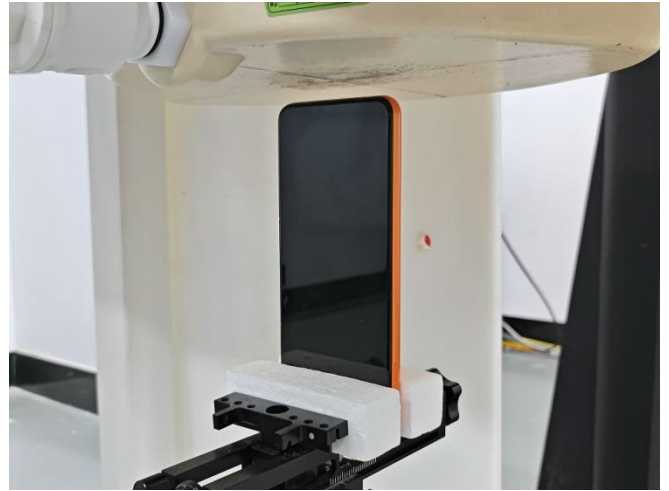


Photo 14: Front Side 0mm



Photo 15: Back Side 0mm



Photo 16: Left Side 0mm

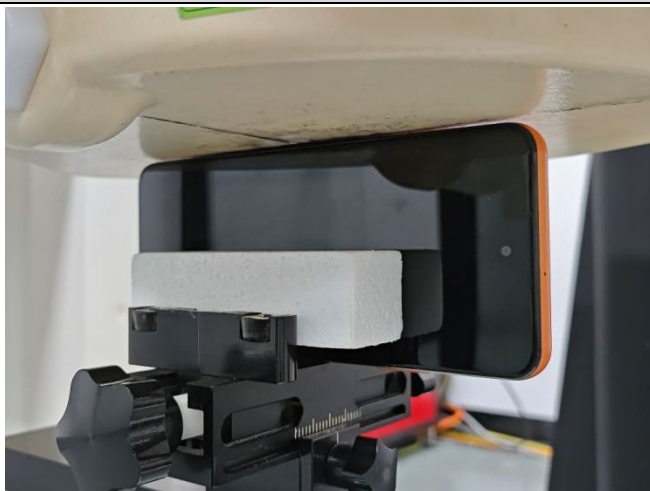


Photo 17: Right Side 0mm



Photo 18: Bottom Side 0mm



Photo 19: Top Side 0mm



Photo 20: Front Side 0mm for NFC



Photo 21: Back Side 0mm for NFC

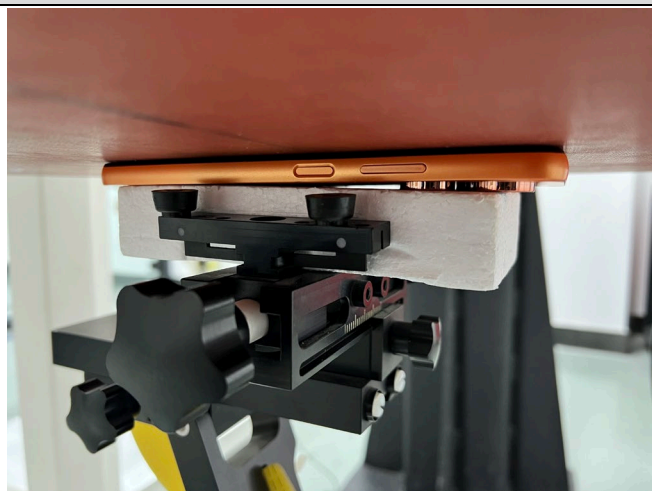


Photo 22: Left Side 0mm for NFC

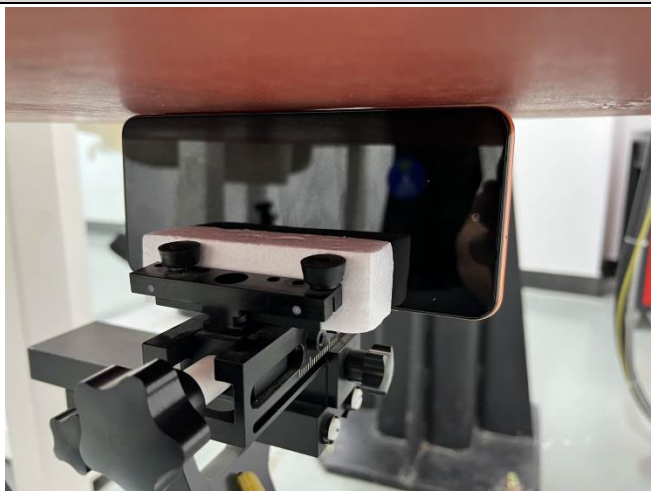


Photo 23: Right Side 0mm for NFC



Photo 24: Bottom Side 0mm for NFC


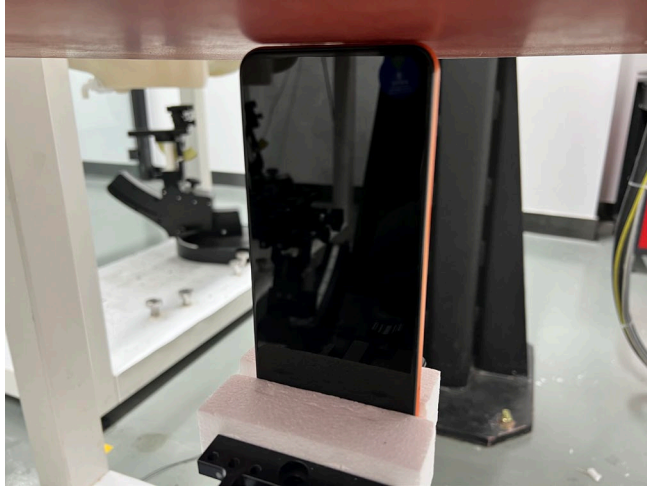


Photo 25: Top Side 0mm for NFC



4. EUT Constructional Details

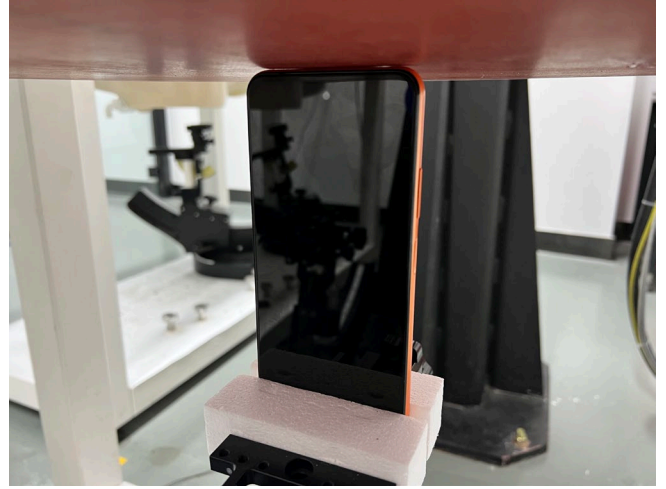