In Collaboration with
s p e a g
CALIBRATION LABORATORY

CAICT

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn http://www.caic.ac.cn

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5250MHz

Impedance, transformed to feed point	47.0Ω- 2.60jΩ
Return Loss	- 27.8dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	49.8Ω+ 3.05jΩ
Return Loss	- 30.3dB

Antenna Parameters with Head TSL at 5750MHz

Impedance, transformed to feed point	51.9Ω+ 0.96jΩ
Return Loss	- 33.5dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.101 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG

In Collaboration with
s p e a g
CALIBRATION LABORATORY

CAICT

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn http://www.caic.ac.cn

DASY5 Validation Report for Head TSL Date: 2023-08-23

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1245

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Medium parameters used: f = 5250 MHz; σ = 4.627 S/m; ε_r = 35.17; ρ = 1000 kg/m^3

Medium parameters used: f = 5600 MHz; σ = 5 S/m; ε_r = 34.58; ρ = 1000 kg/m^3

Medium parameters used: f = 5750 MHz; σ = 5.162 S/m; ε_r = 34.36; ρ = 1000 kg/m^3

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN3617; ConvF(5.5, 5.5, 5.5) @ 5250 MHz; ConvF(5.01, 5.01, 5.01) @ 5600 MHz; ConvF(5.15, 5.15, 5.15) @ 5750 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.63 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 31.2 W/kg

SAR(1 g) = 7.84 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.4%

Maximum value of SAR (measured) = 18.5 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.43 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 35.6 W/kg

SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.3 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.4%

Maximum value of SAR (measured) = 19.7 W/kg

In Collaboration with
s p e a g
CALIBRATION LABORATORY

CAICT

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn http://www.caic.ac.cn

Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 61.00 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 36.0 W/kg
SAR(1 g) = 7.83 W/kg; SAR(10 g) = 2.19 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 61%
Maximum value of SAR (measured) = 19.8 W/kg

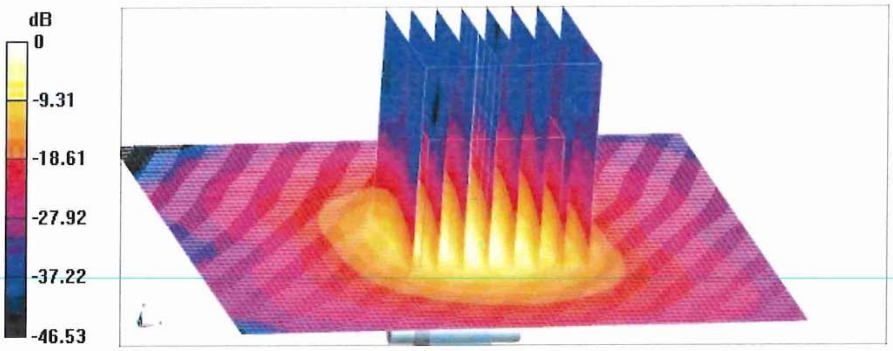

0 dB = 19.8 W/kg = 12.97 dBW/kg

In Collaboration with
s p e a g
CALIBRATION LABORATORY

CAICT

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2117
E-mail: emf@caict.ac.cn http://www.caic.ac.cn

Impedance Measurement Plot for Head TSL

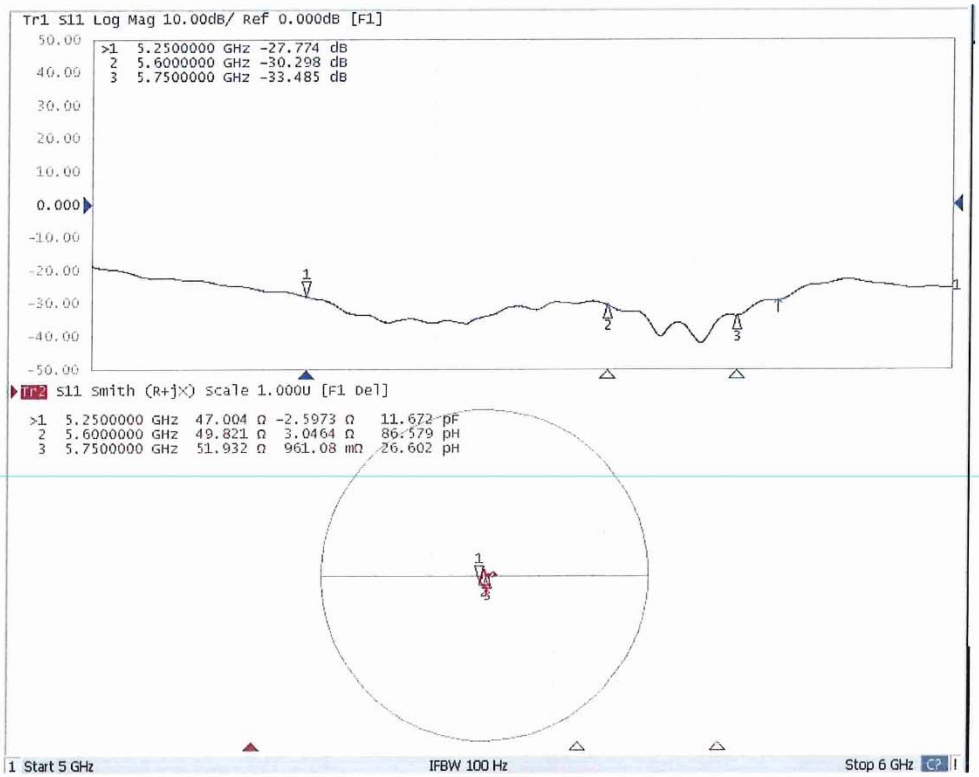

D5GHzV2 - SN:1245 Extended Dipole Calibrations

Per FCC KDB 865664 D01, calibration intervals of up to 3 years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements.

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20 dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from calibration date.

D5GHzV2-SN:1245						
5250MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-27.774	/	47.004	/	-2.5973	/
2024/8/20	-25.515	-8.13	51.281	4.277	1.8032	4.4005
5600MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-30.298	/	49.821	/	3.0464	/
2024/8/20	-33.499	10.57	50.527	0.706	2.0683	-0.9781
5750MHz Head						
Date of Measurement	Return Loss (dB)	Delta (%)	Real Impedence(Ω)	Delta (Ω)	Imaginary Impedence(Ω)	Delta (Ω)
2023/8/23	-33.485	/	51.932	/	0.9611	/
2024/8/20	-29.979	-10.47	47.897	-4.035	2.2950	1.3339

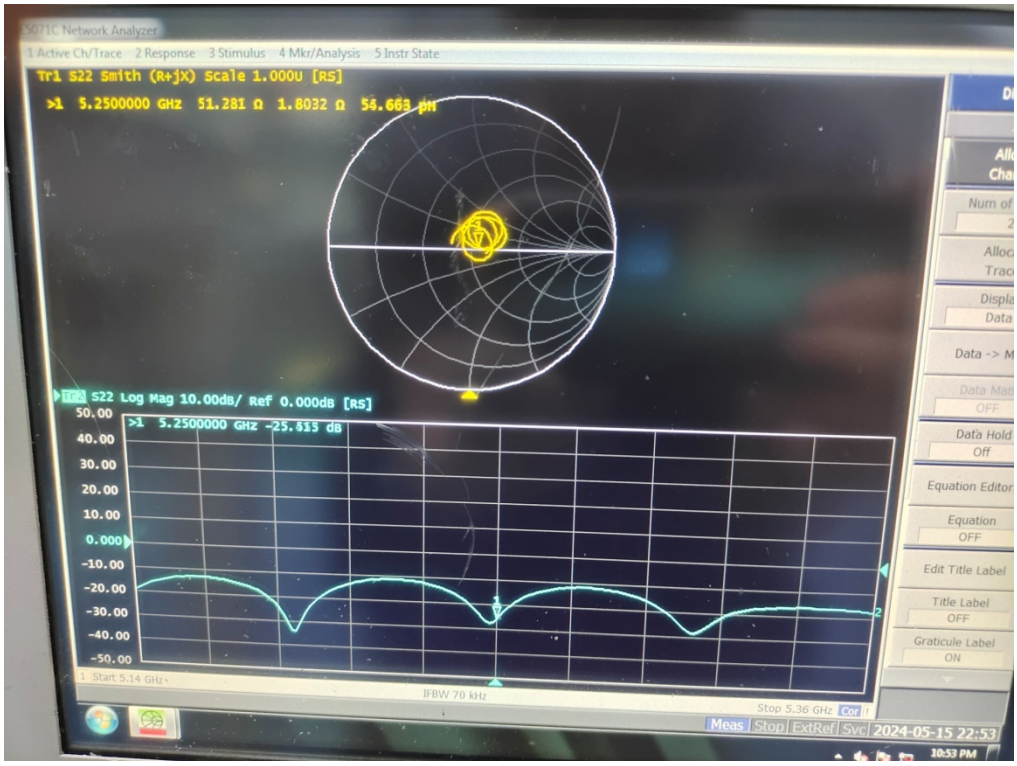
E5071C Network Analyzer
1 Active Ch/Trace 2 Response 3 Stimulus 4 Mkr/Analysis 5 Instr State
Tr1 S22 Smith (R+jX) Scale 1.000U [RS]
>1 5.2500000 GHz 51.281 Ω 1.8032 Ω 54.663 pH
S22 Log Mag 10.00dB/ Ref 0.000dB [RS]
>1 5.2500000 GHz -25.415 dB
50.00
40.00
30.00
20.00
10.00
0.000
-10.00
-20.00
-30.00
-40.00
-50.00
Start 5.14 GHz
IFBW 70 kHz
Stop 5.36 GHz
Meas Stop ExtRef Svc 2024-05-15 22:53
Allocate Channels
Num of Traces
Allocate Traces
Display Data
Data -> Mem
Data Math OFF
Data Hold Off
Equation Editor
Equation OFF
Edit Title Label
Title Label OFF
Graticule Label ON

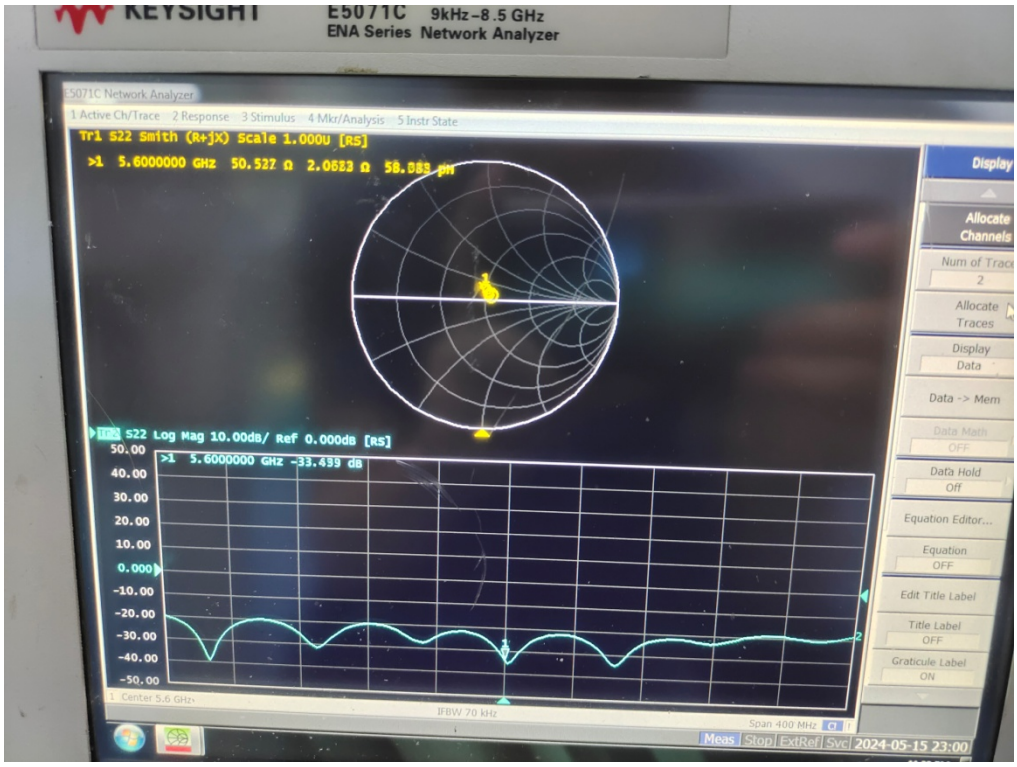
KEYSIGHT
E5071C 9kHz–8.5 GHz
ENA Series Network Analyzer
E5071C Network Analyzer
1 Active Ch/Trace 2 Response 3 Stimulus 4 Mkr/Analysis 5 Instr State
Tr1 S22 Smith (R+jX) Scale 1.000U [RS]
>1 5.6000000 GHz 50.527 Ω 2.0583 Ω 58.083 pH
S22 Log Mag 10.00dB/ Ref 0.000dB [RS]
>1 5.6000000 GHz -33.439 dB
50.00
40.00
30.00
20.00
10.00
0.000
-10.00
-20.00
-30.00
-40.00
-50.00
Center 5.6 GHz
IFBW 70 kHz
Span 400 MHz
Meas Stop ExtRef Svc 2024-05-15 23:00
Display
Allocate Channels
Num of Traces
Allocate Traces
Display Data
Data -> Mem
Data Math OFF
Data Hold Off
Equation Editor...
Equation OFF
Edit Title Label
Title Label OFF
Graticule Label ON

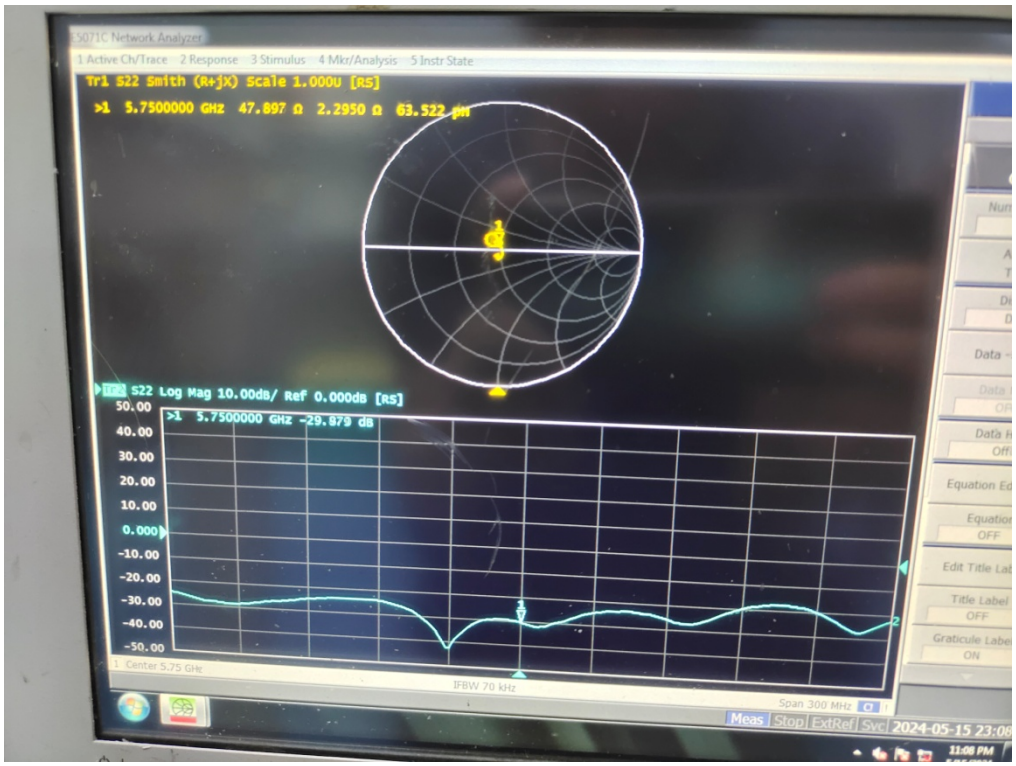

	Name	Signature
Calibrated By:	Karl Gong	Karl Gong