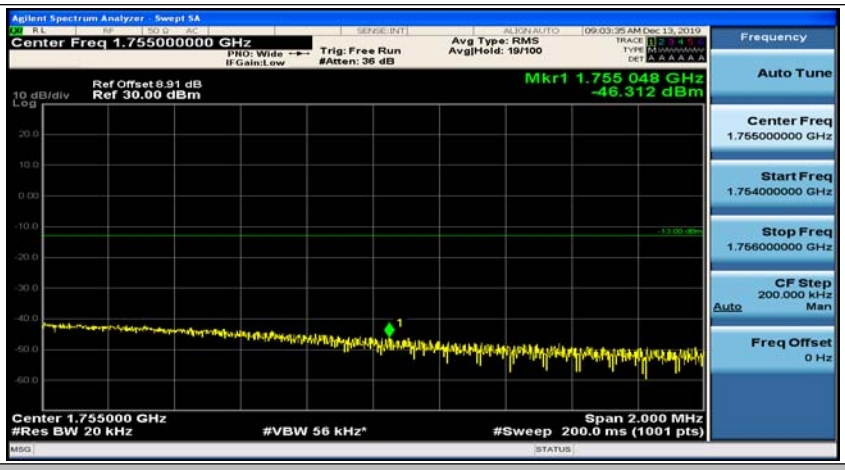

(Channel Bandwidth:20 MHz)_HCH_16QAM_1RB#99

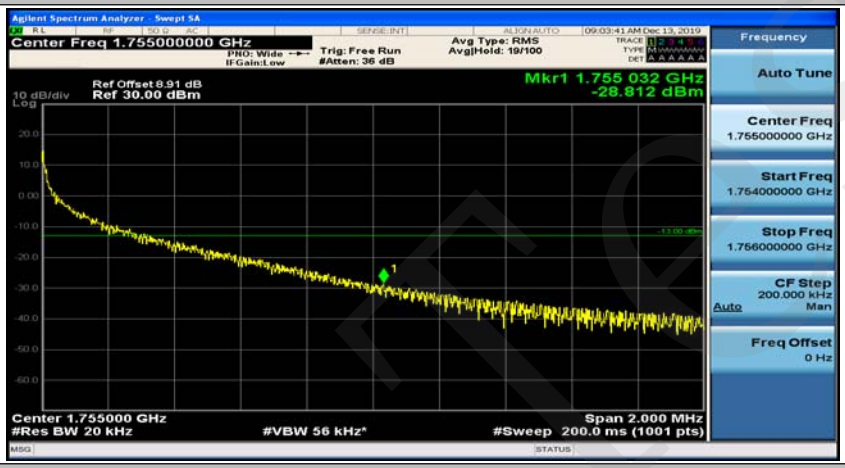

(Channel Bandwidth:20 MHz)_HCH_16QAM_50RB#0

(Channel Bandwidth:20 MHz)_HCH_16QAM_50RB#25

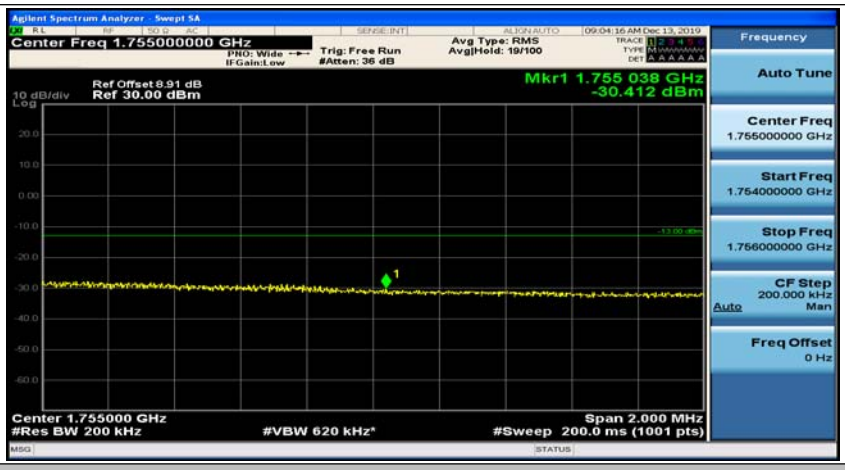

(Channel Bandwidth:20 MHz)_HCH_16QAM_50RB#50

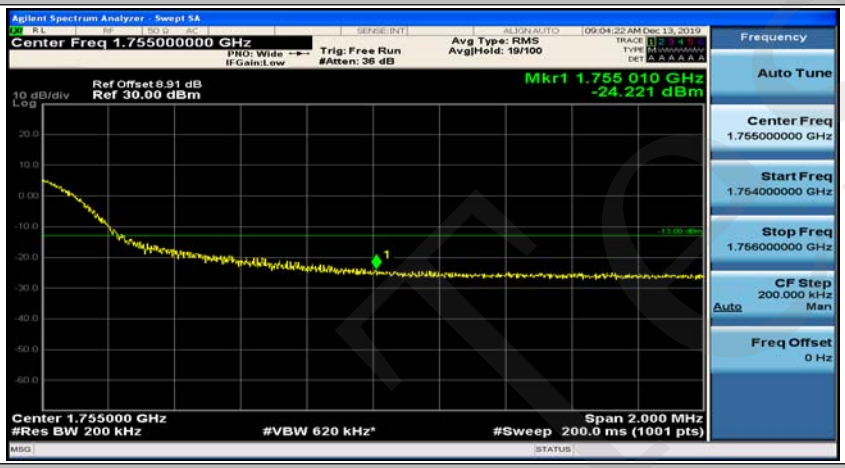

(Channel Bandwidth:20 MHz)_HCH_16QAM_100RB#0

Appendix E: Conducted Spurious Emission

Test Graphs

Channel Bandwidth: 1.4 MHz

(Channel Bandwidth: 1.4 MHz)_LCH_QPSK_1RB#0

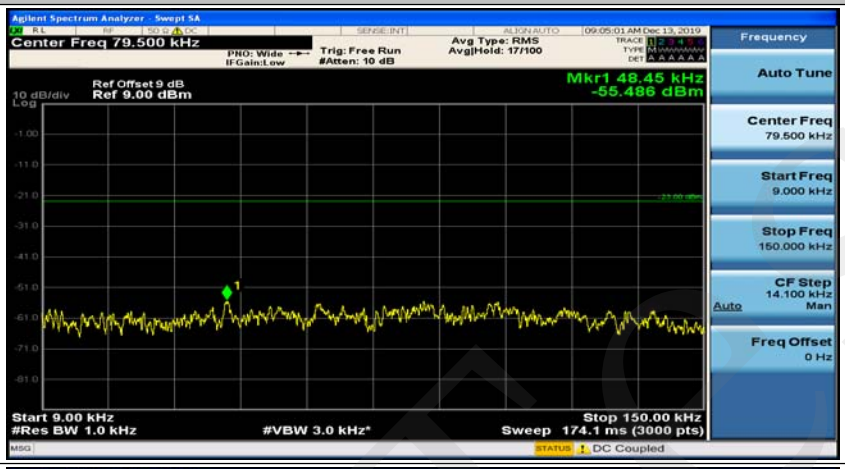

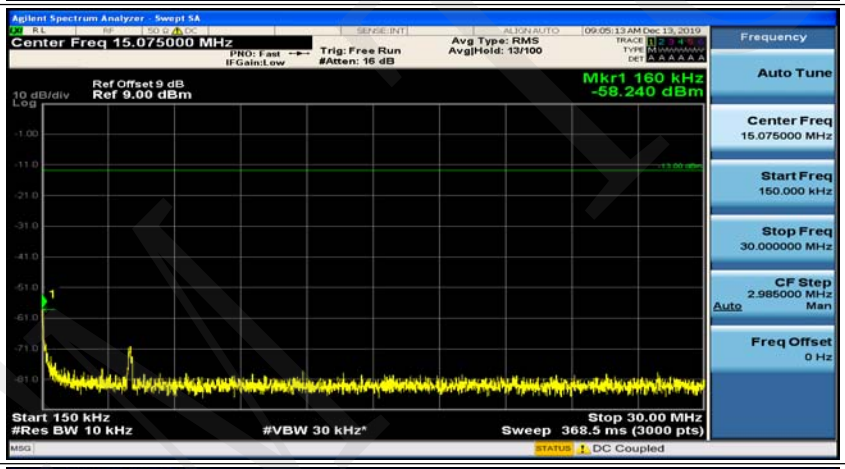

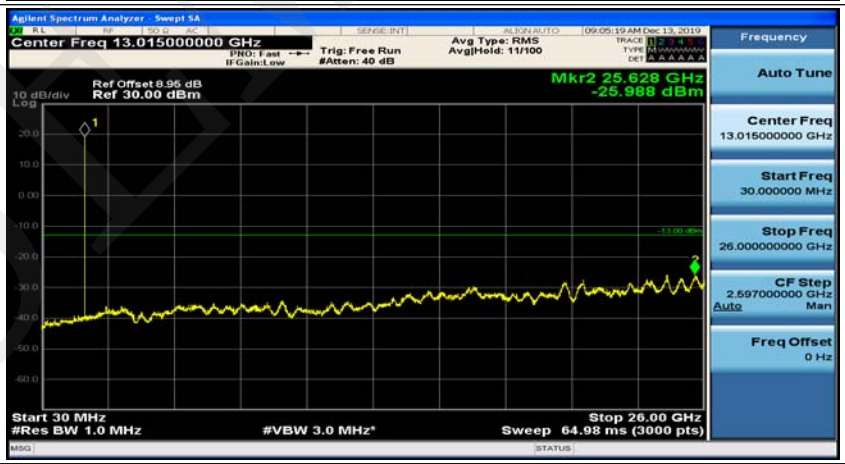

(Channel Bandwidth: 1.4 MHz)_LCH_QPSK_1RB#3

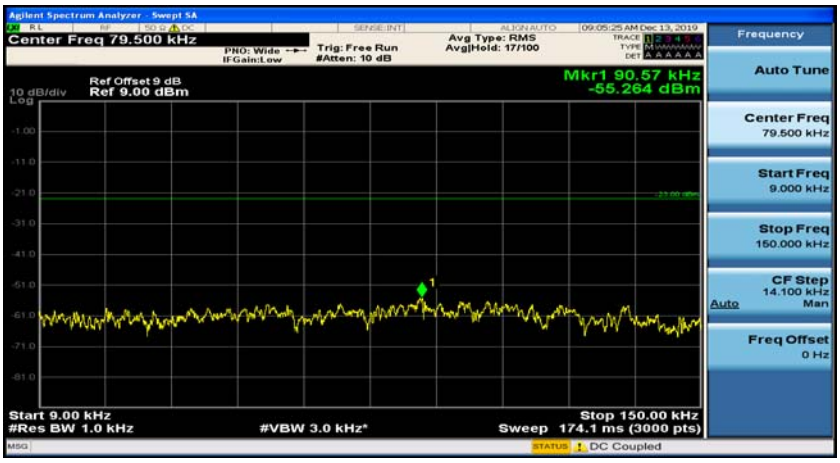

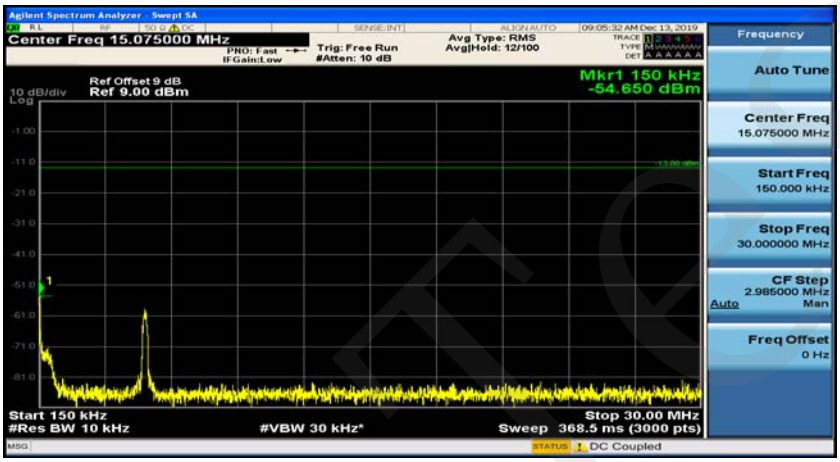

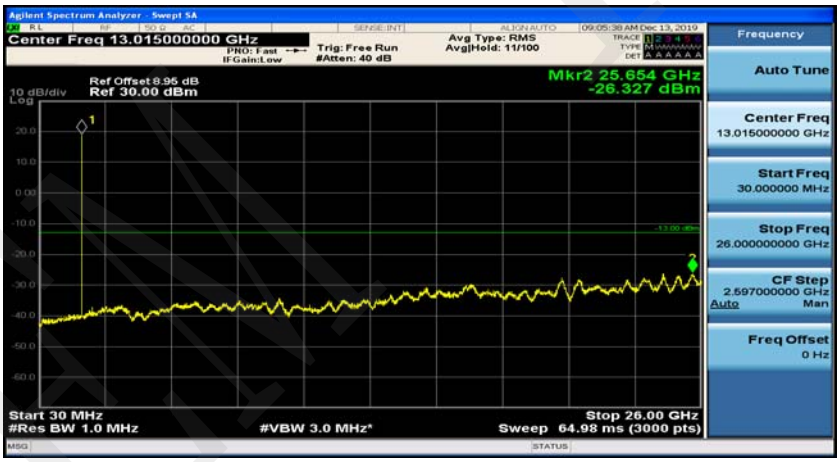

(Channel Bandwidth: 1.4 MHz)_LCH_QPSK_1RB#5

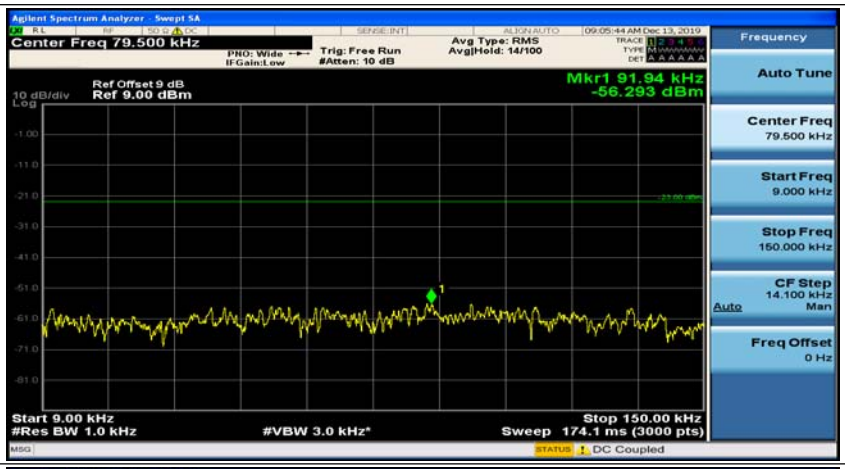
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 14/100
09:05:44 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 91.94 kHz
-56.293 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

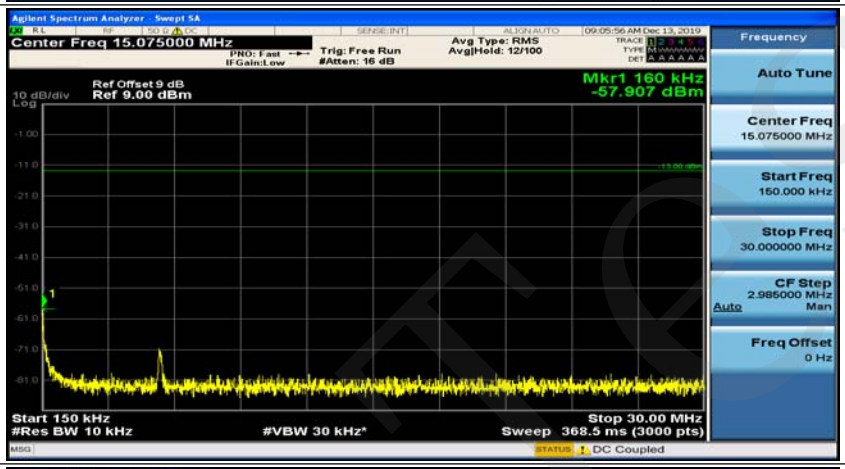
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:05:56 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-57.907 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:06:02 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.628 GHz
-26.568 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_MCH_QPSK_1RB#0

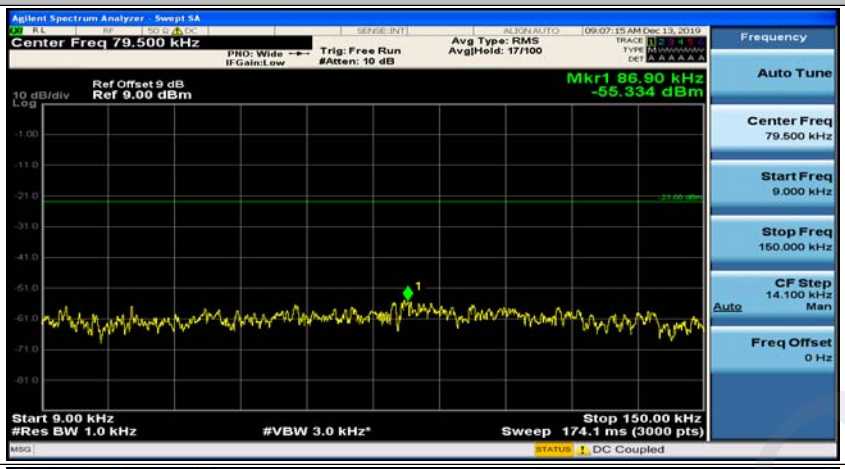

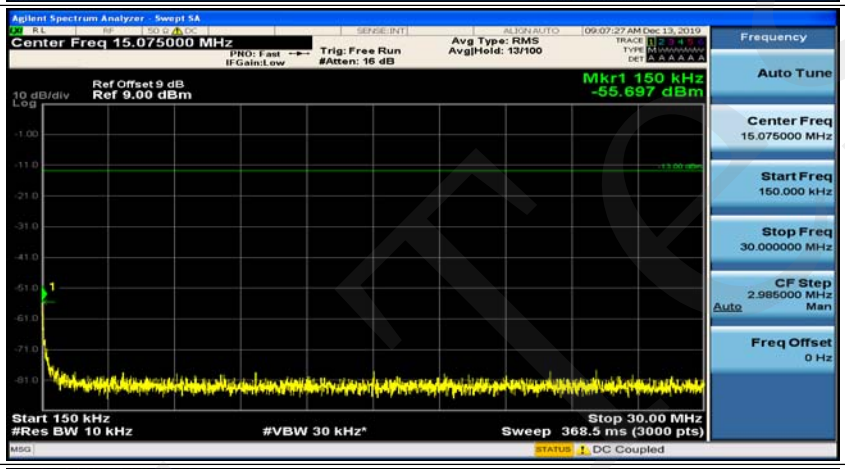

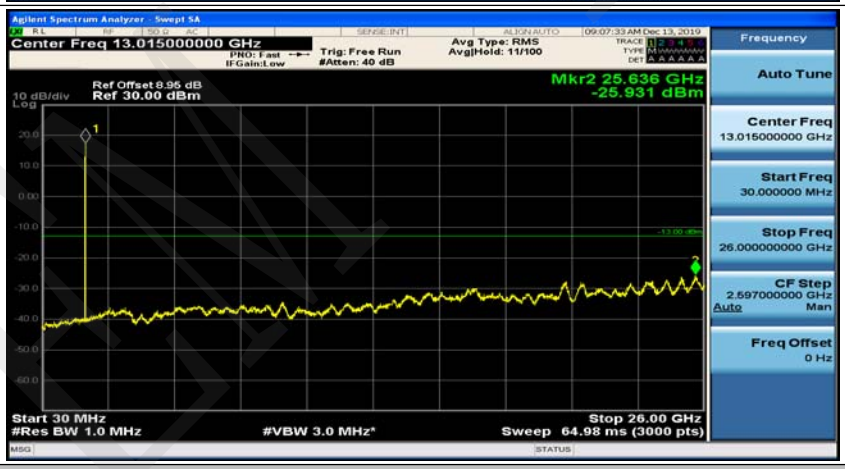

(Channel Bandwidth: 1.4 MHz)_MCH_QPSK_1RB#3

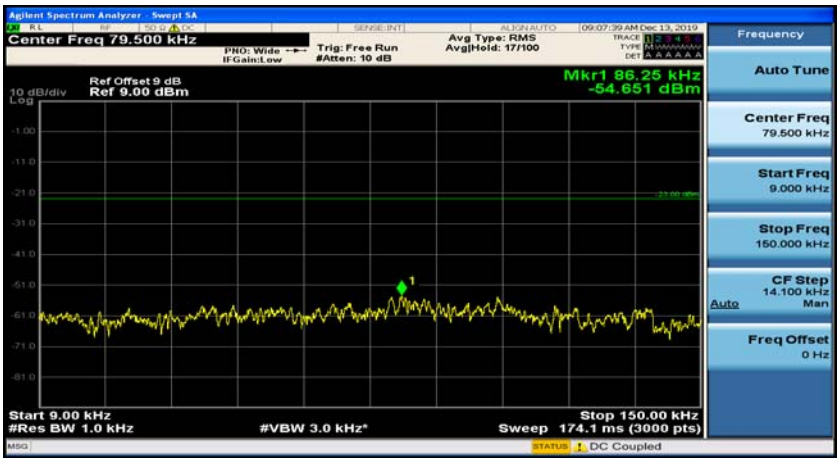

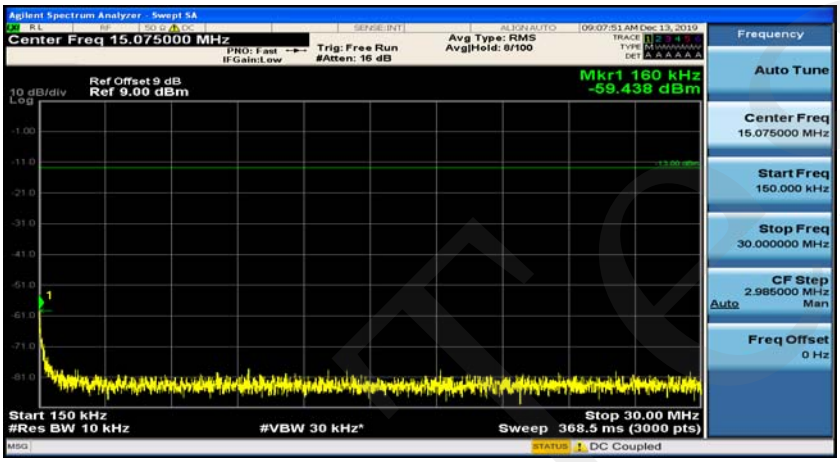

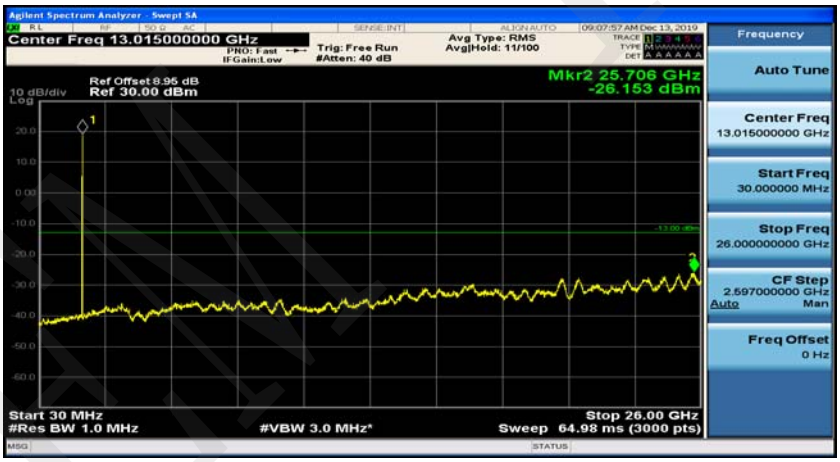

(Channel Bandwidth: 1.4 MHz)_MCH_QPSK_1RB#5

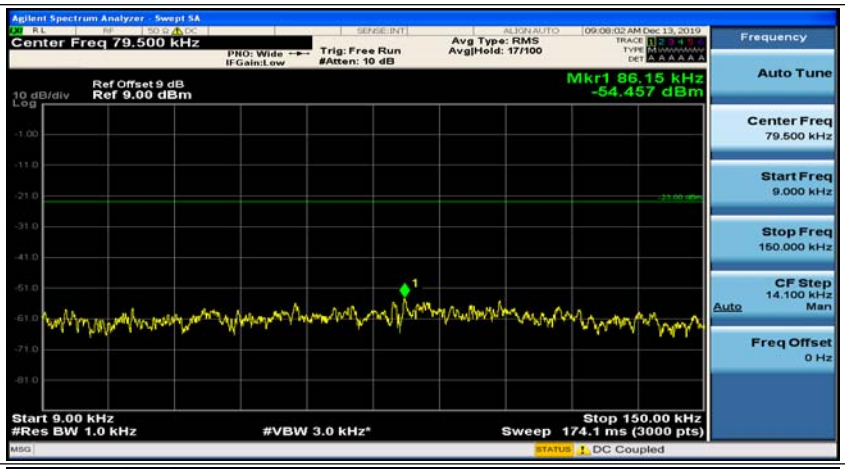
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:08:02 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 86.15 kHz
-54.457 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

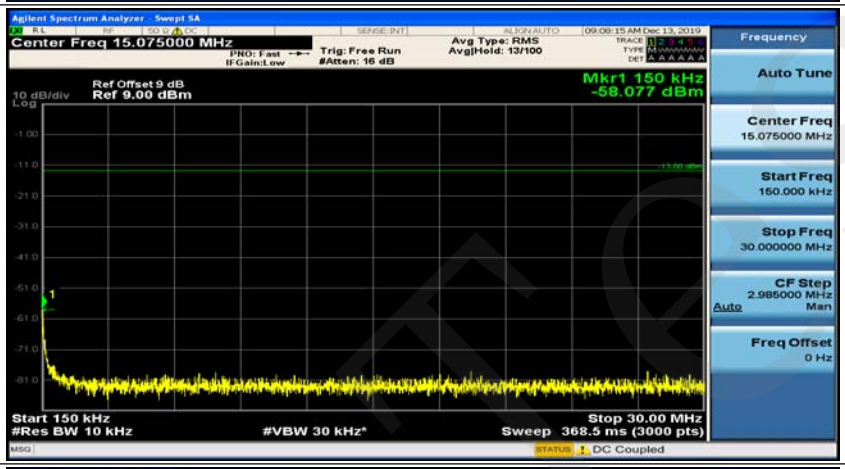
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 13/100
09:08:15 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-58.077 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:08:21 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.619 GHz
-26.252 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_HCH_QPSK_1RB#0

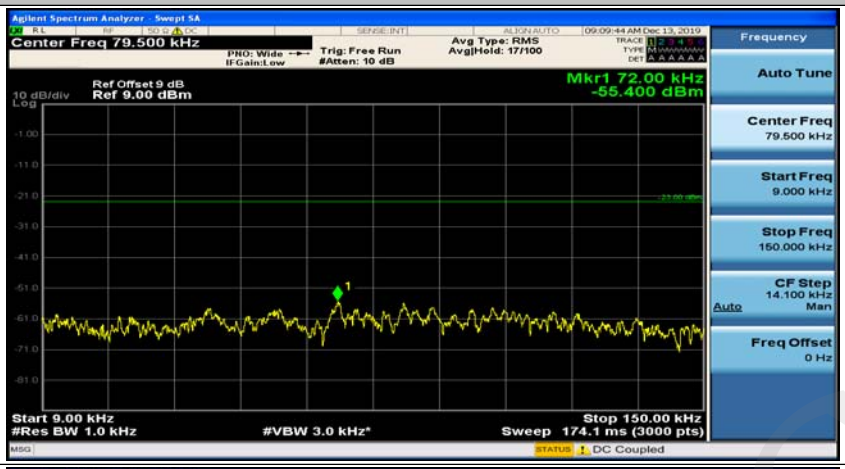

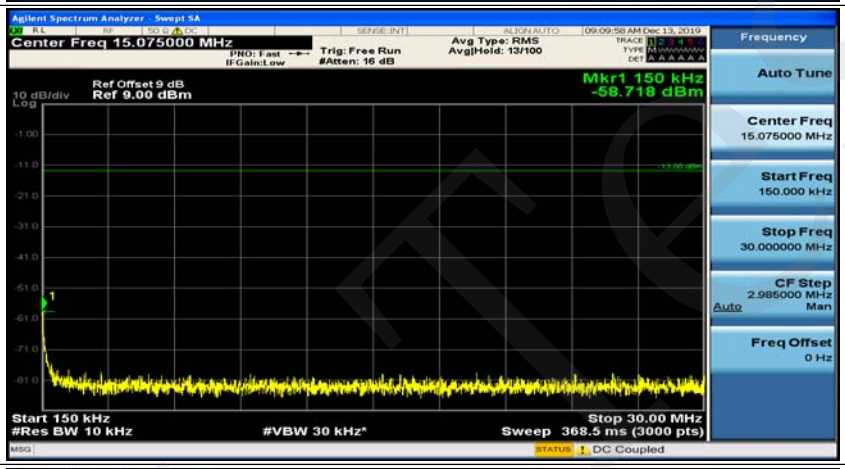

(Channel Bandwidth: 1.4 MHz)_HCH_QPSK_1RB#3

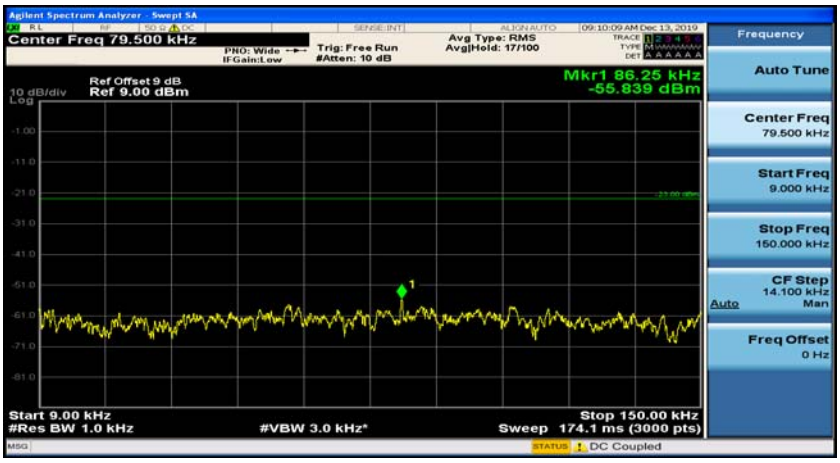

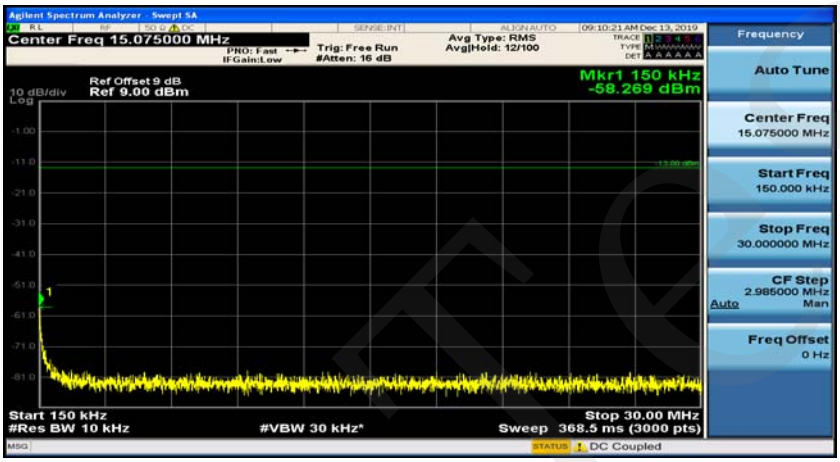

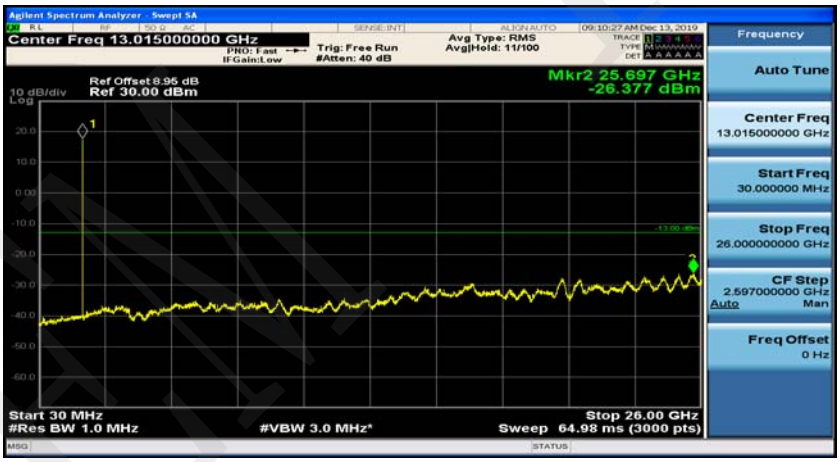

(Channel Bandwidth: 1.4 MHz)_HCH_QPSK_1RB#5

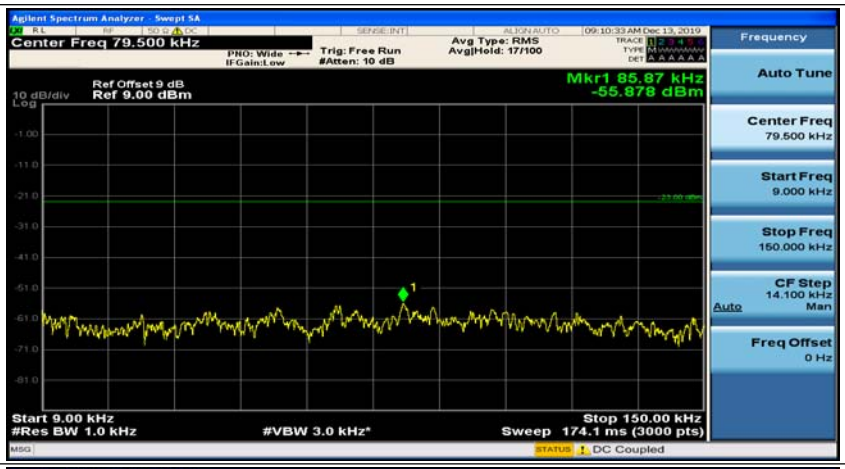
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:10:33 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 85.87 kHz
-55.878 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

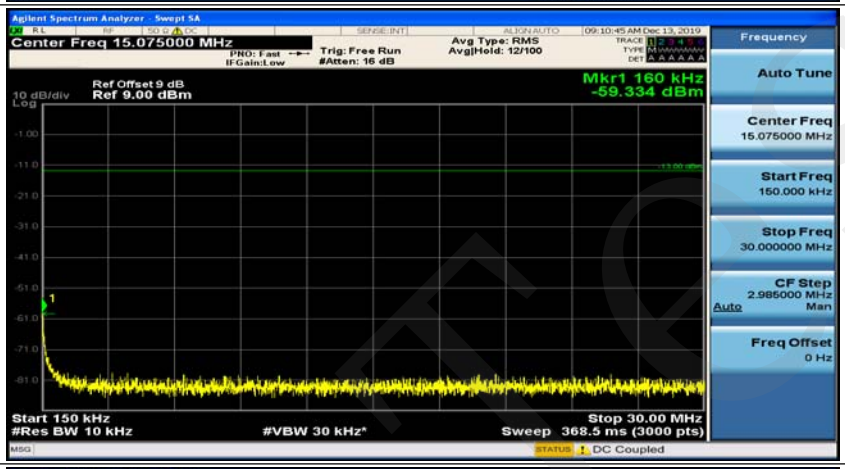
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:10:45 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-59.334 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

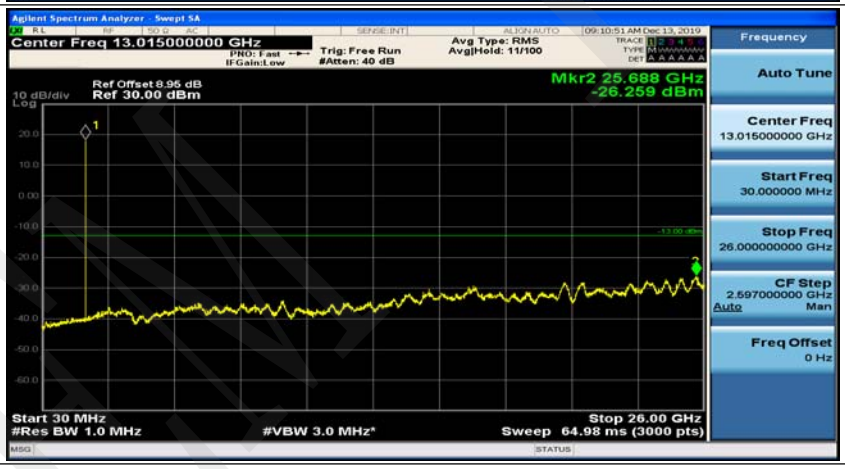
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:10:51 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.688 GHz
-26.259 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_LCH_16QAM_1RB#0

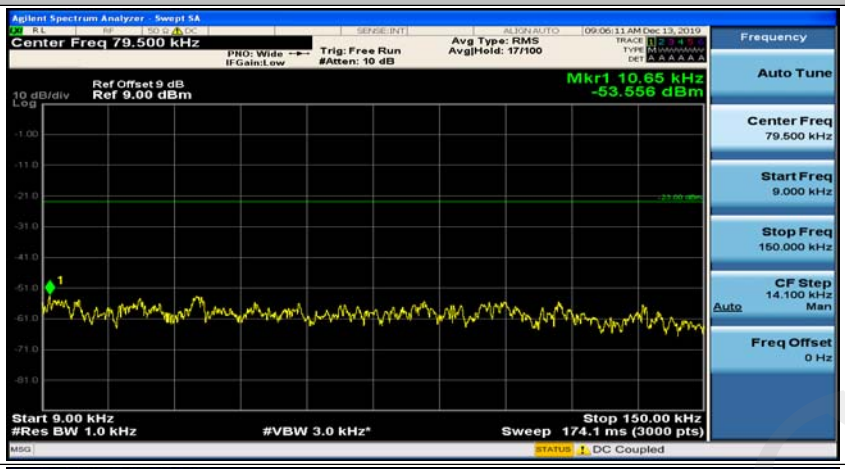

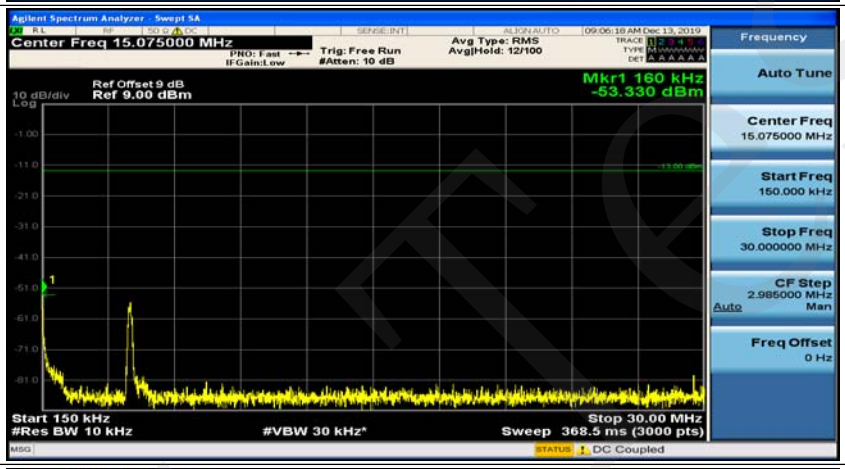

(Channel Bandwidth: 1.4 MHz)_LCH_16QAM_1RB#3

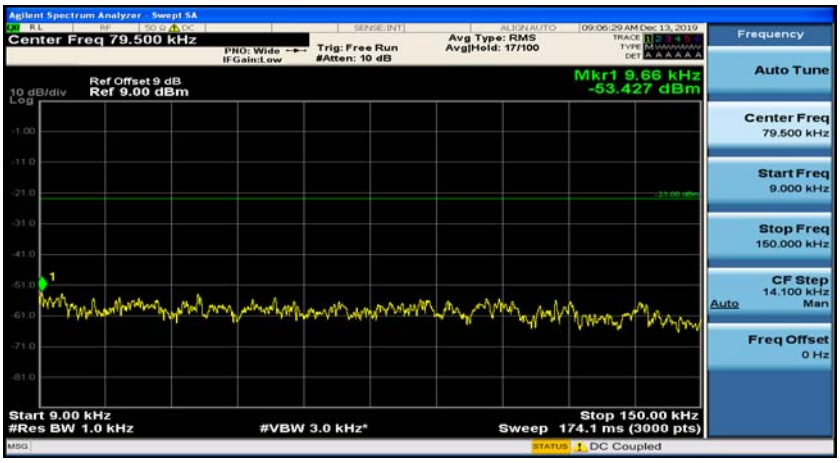

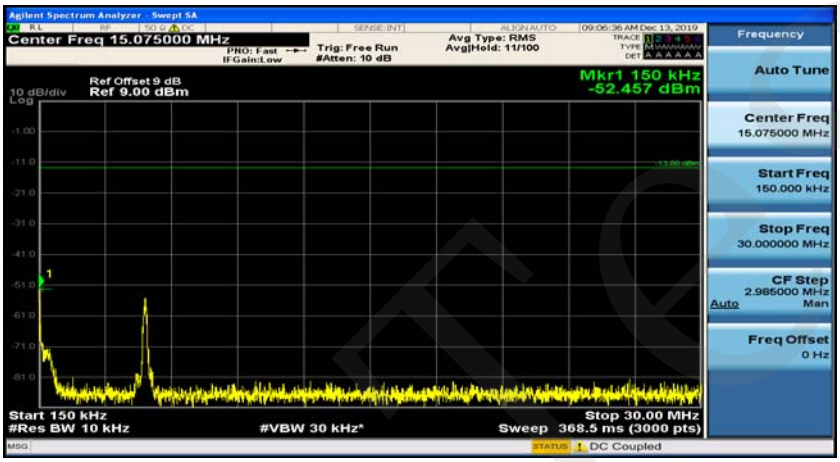

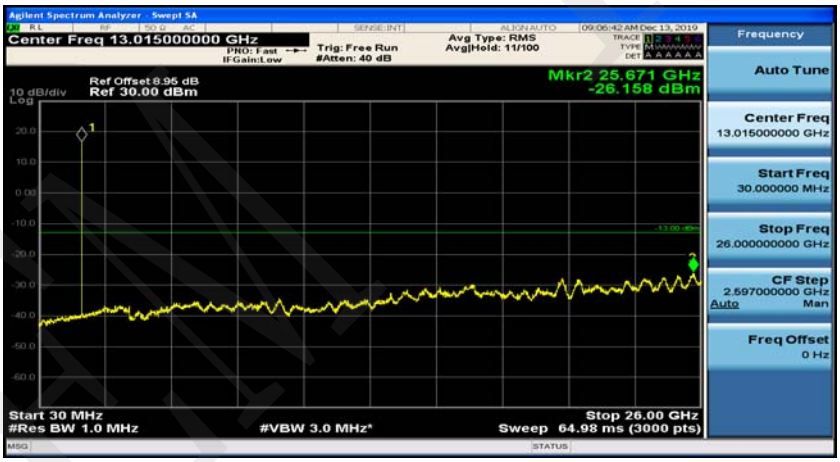

(Channel Bandwidth: 1.4 MHz)_LCH_16QAM_1RB#5

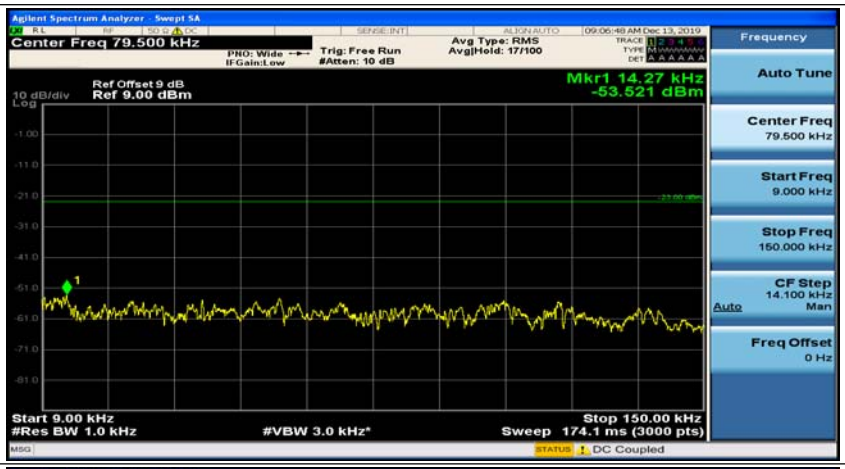
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 14.27 kHz
-53.521 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

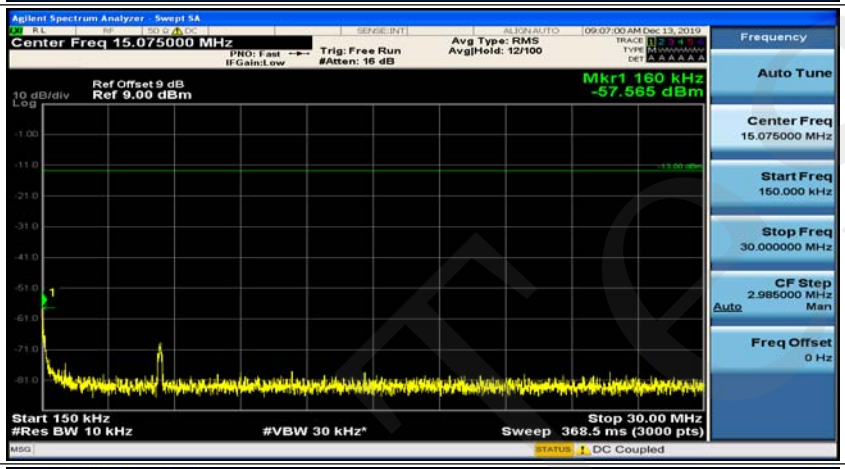
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-57.565 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

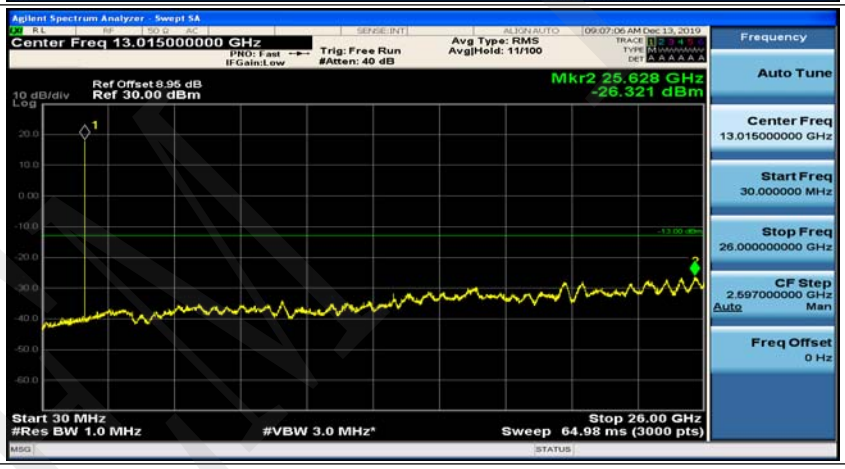
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.628 GHz
-26.321 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_MCH_16QAM_1RB#0

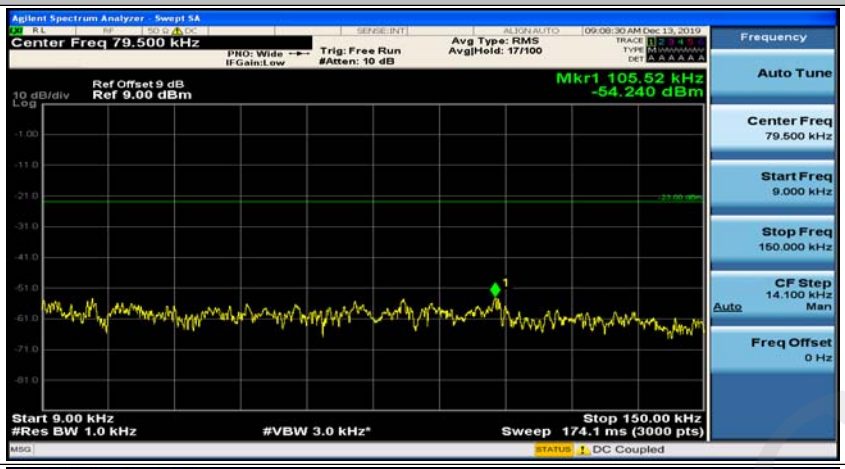

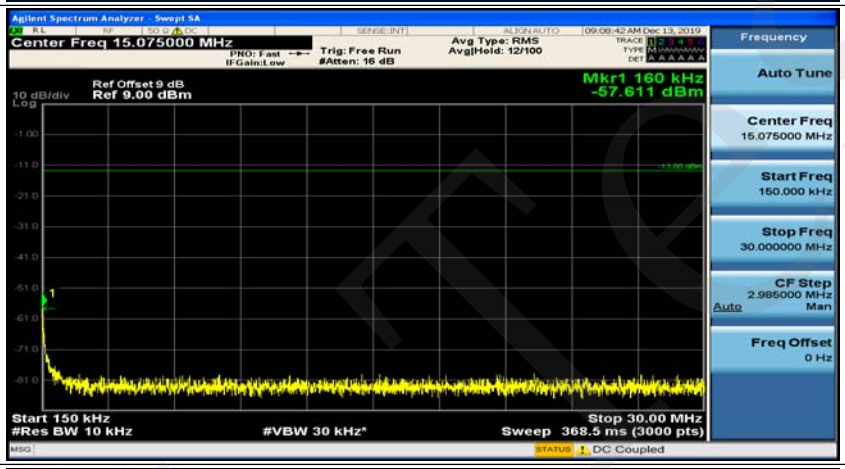

(Channel Bandwidth: 1.4 MHz)_MCH_16QAM_1RB#3

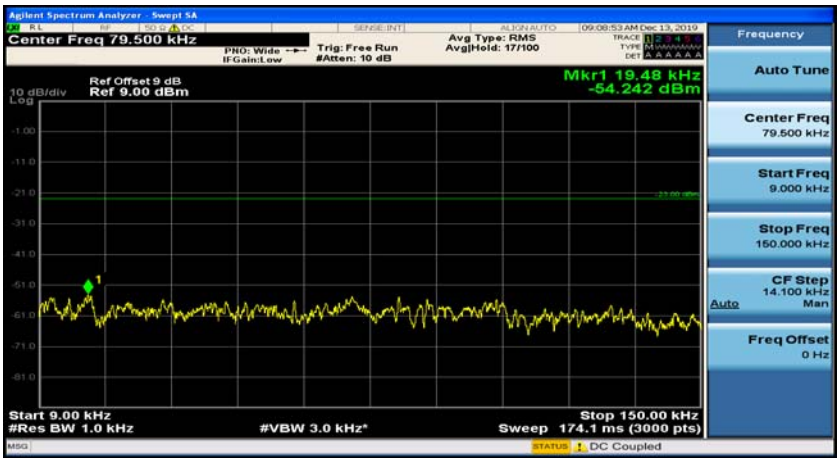

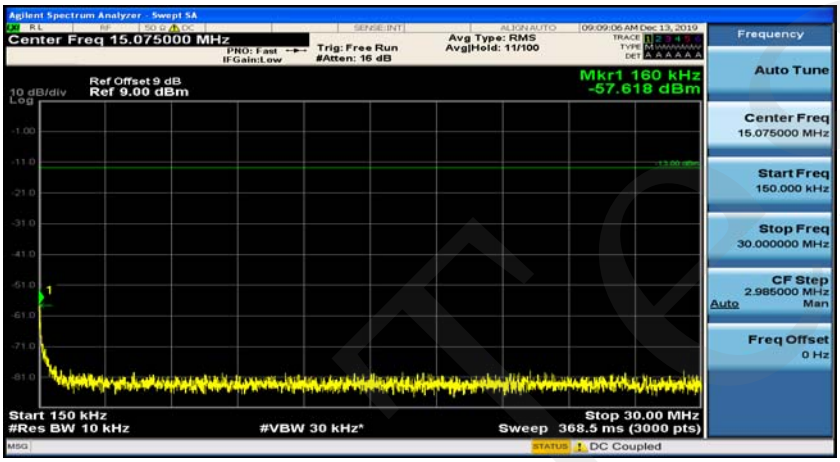

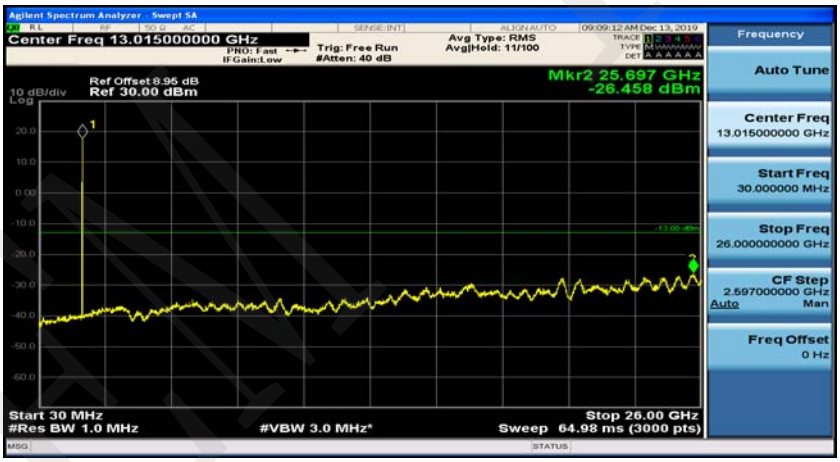

(Channel Bandwidth: 1.4 MHz)_MCH_16QAM_1RB#5

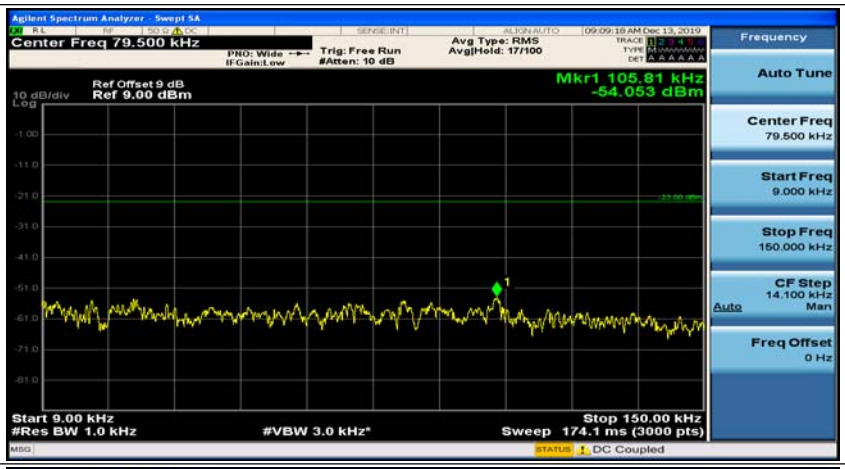
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:09:18 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 105.81 kHz
-54.053 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

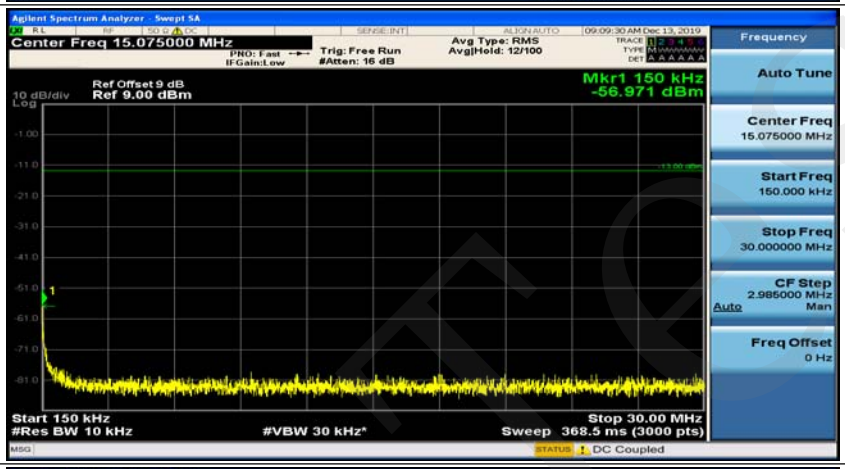
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:09:30 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-56.971 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

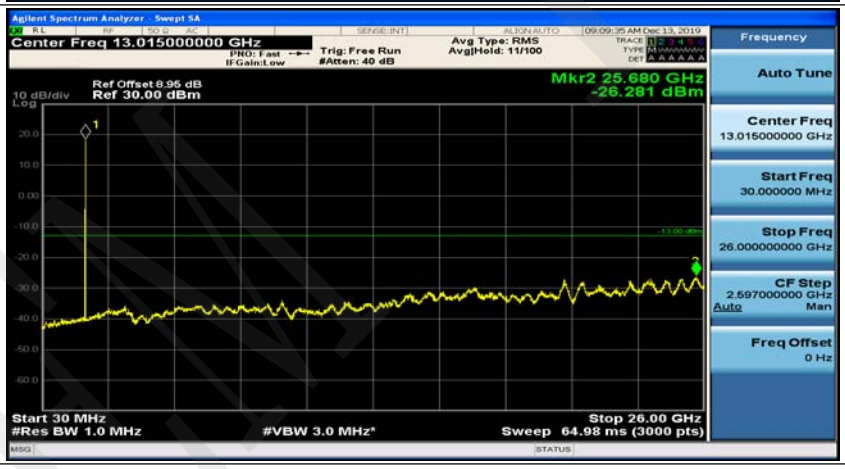
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:09:35 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.680 GHz
-26.281 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 1.4 MHz)_HCH_16QAM_1RB#0

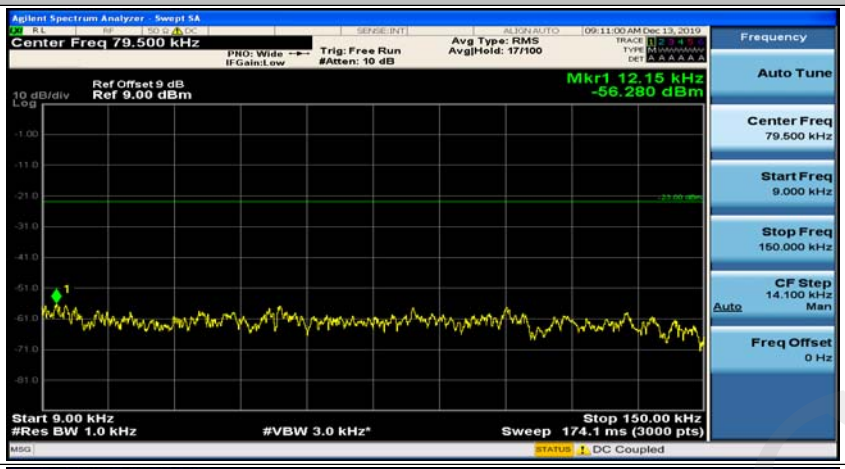

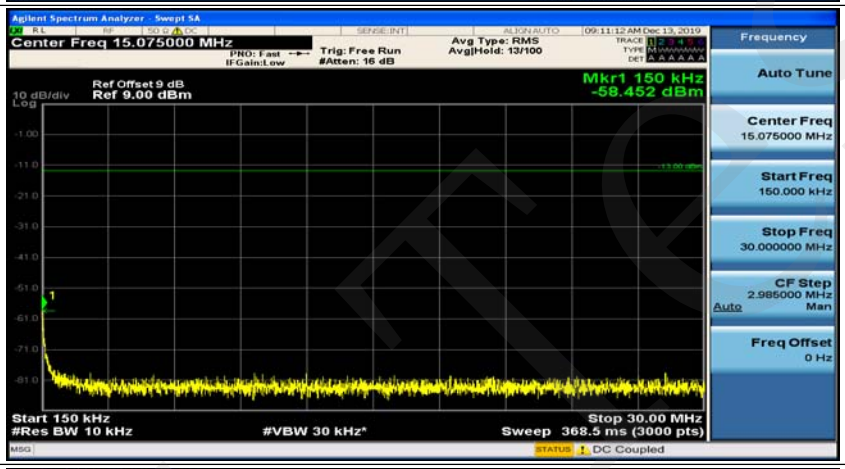

(Channel Bandwidth: 1.4 MHz)_HCH_16QAM_1RB#3

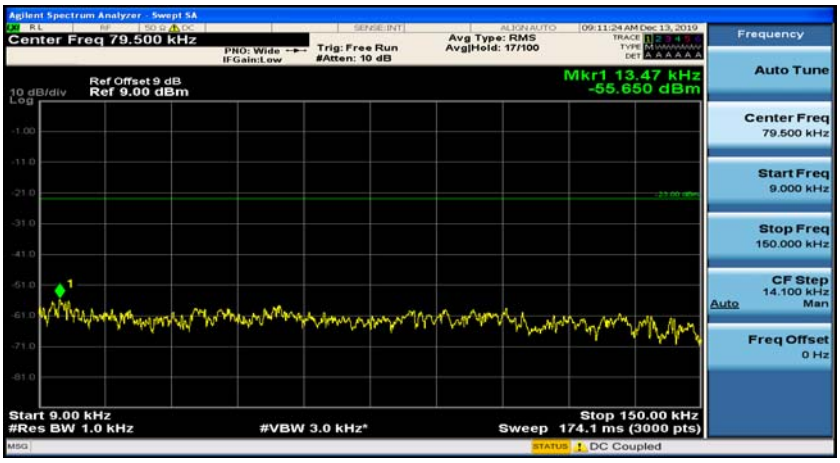

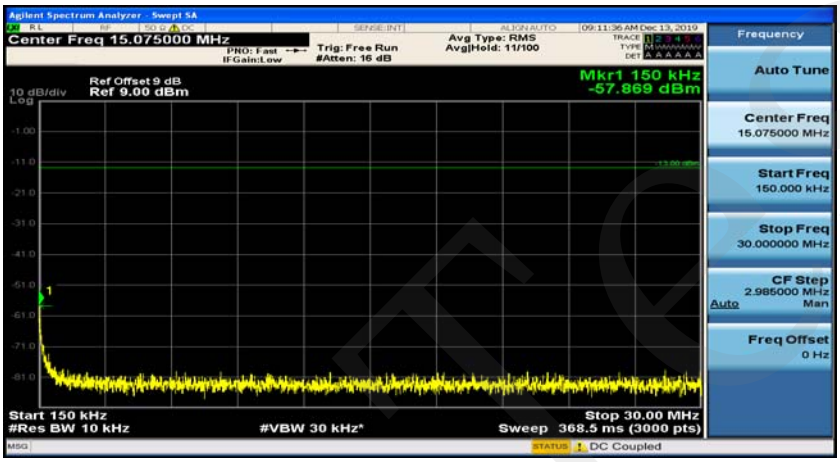

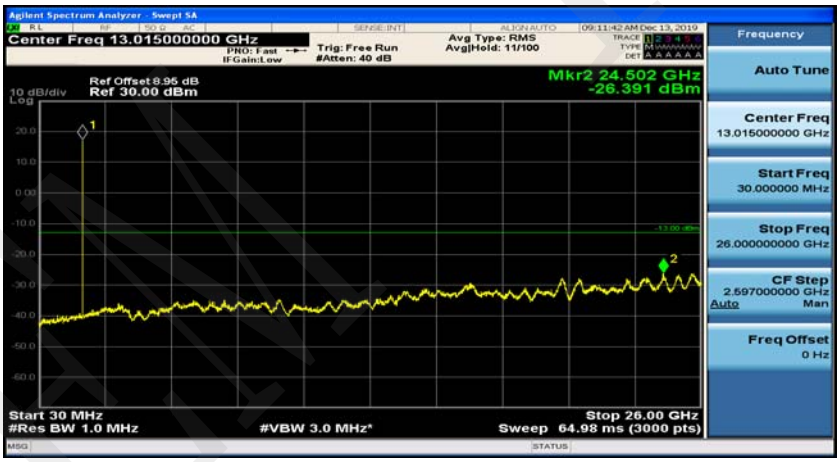

(Channel Bandwidth: 1.4 MHz)_HCH_16QAM_1RB#5

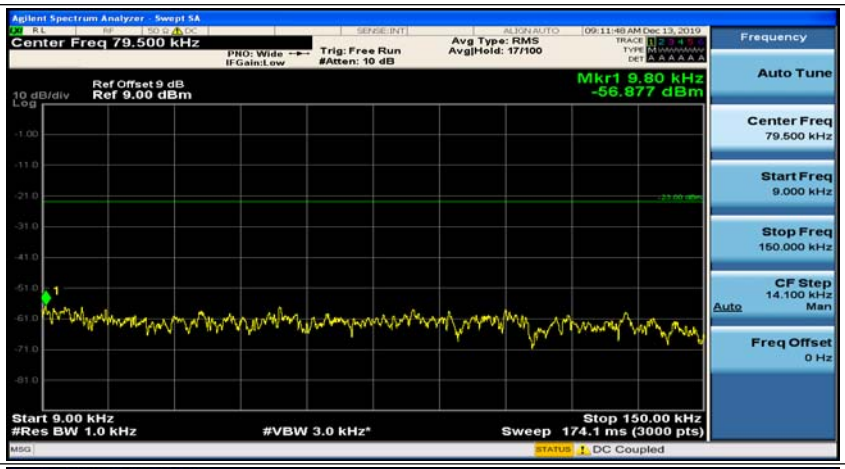
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 9.80 kHz
-56.877 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

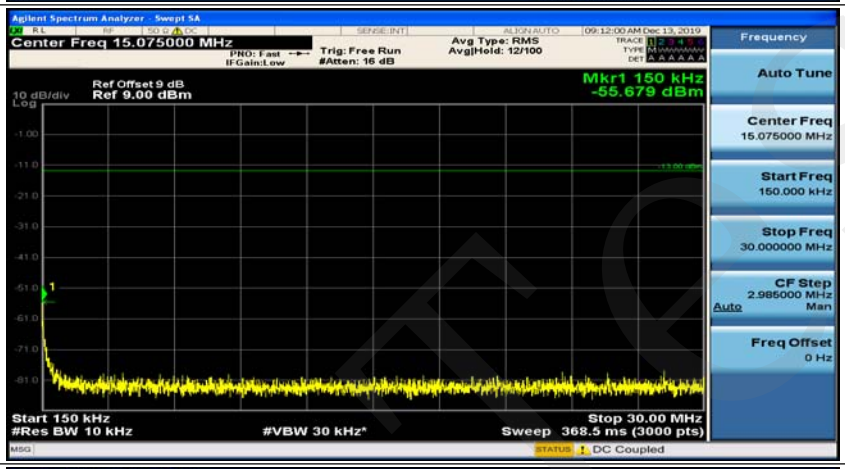
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-55.679 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.602 GHz
-26.367 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 3 MHz

(Channel Bandwidth: 3 MHz)_LCH_QPSK_1RB#0

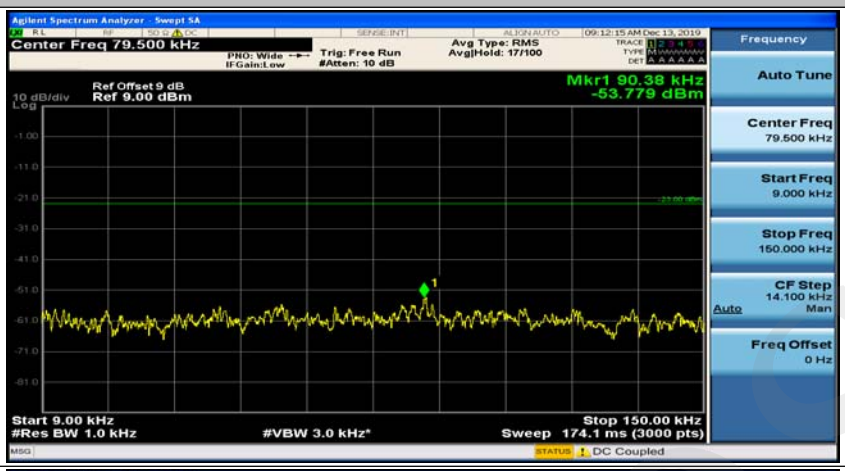

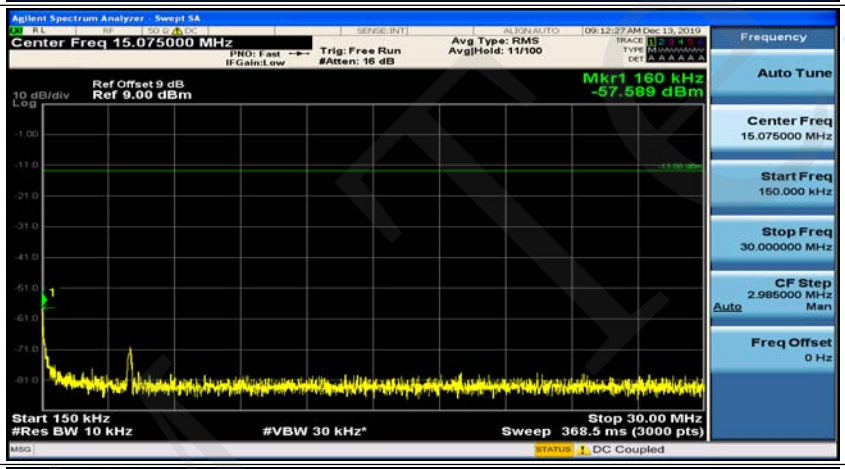

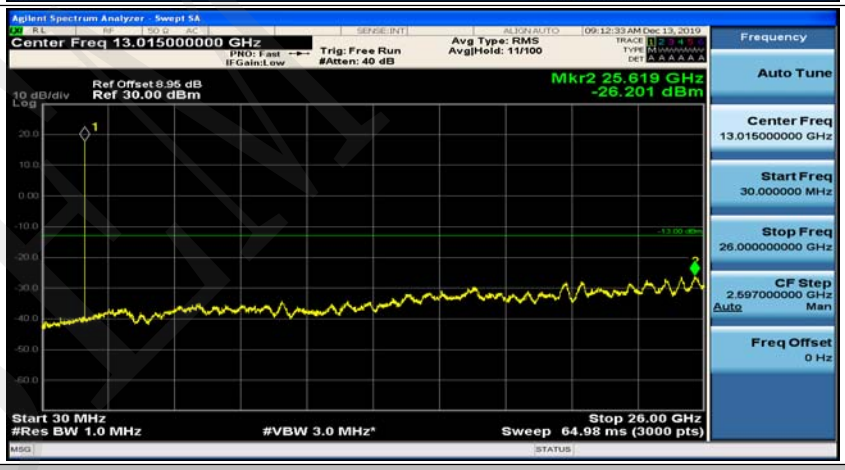

(Channel Bandwidth: 3 MHz)_LCH_QPSK_1RB#7

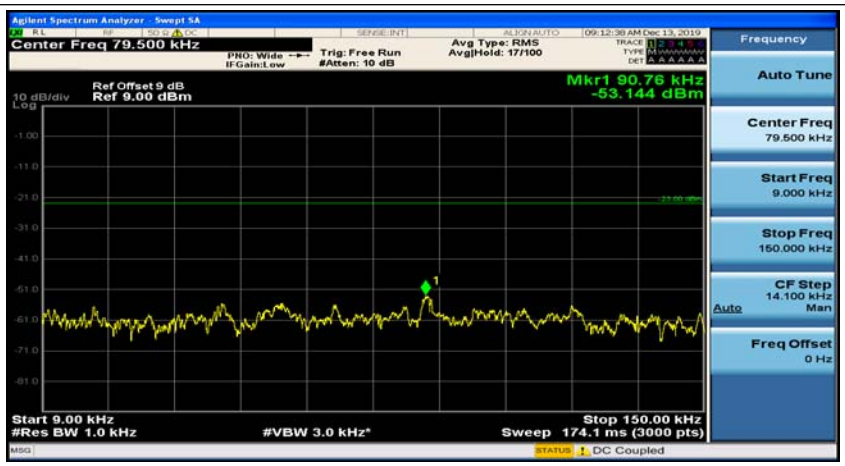
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:12:38 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 90.76 kHz
-53.144 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

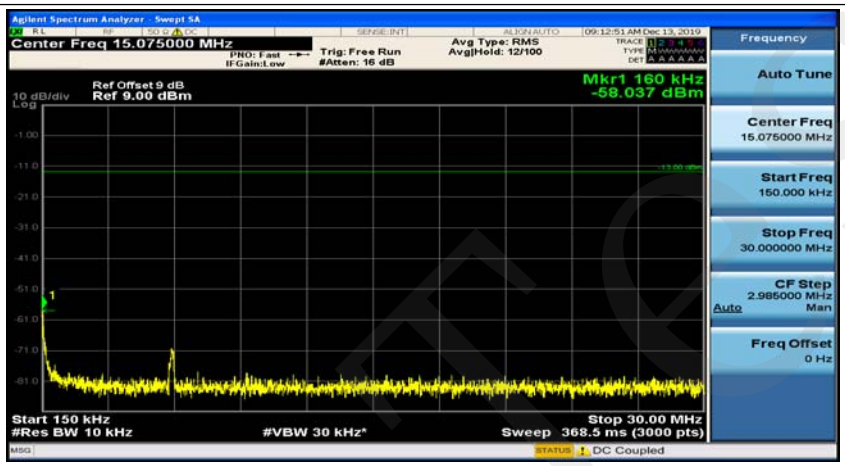
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:12:51 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.037 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

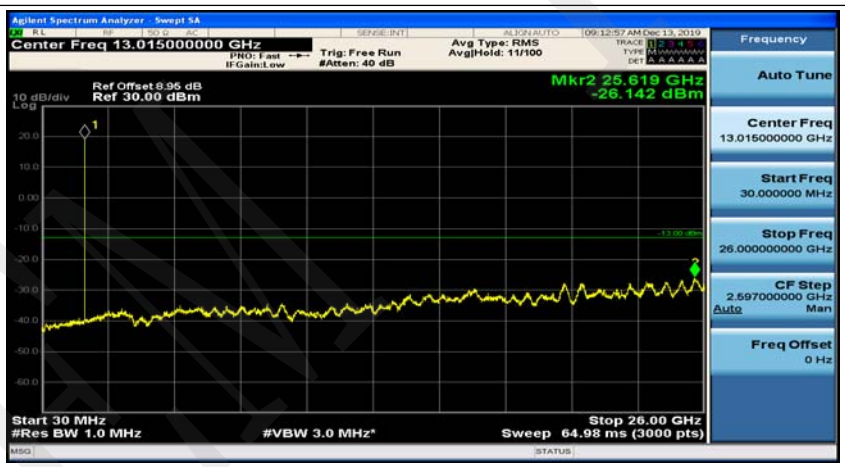
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:12:57 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.619 GHz
-26.142 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_MCH_QPSK_1RB#0

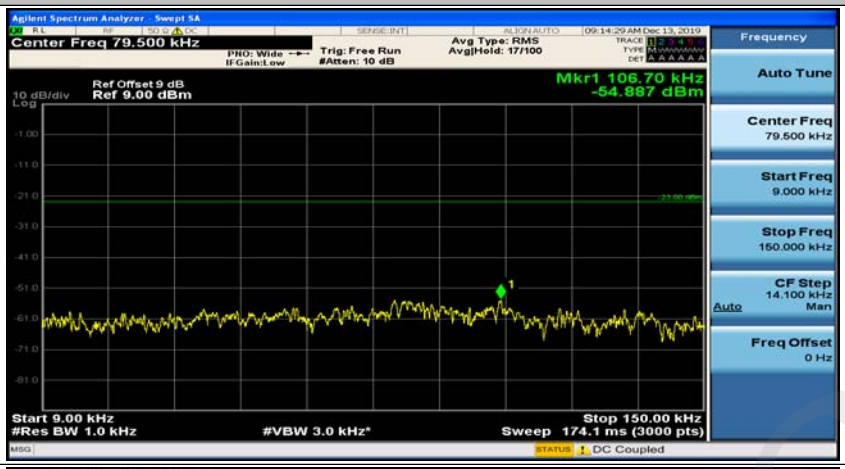

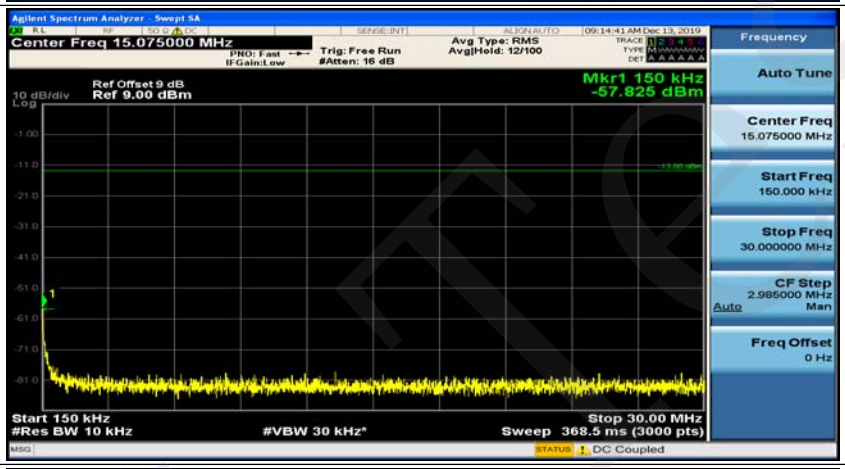

(Channel Bandwidth: 3 MHz)_MCH_QPSK_1RB#7

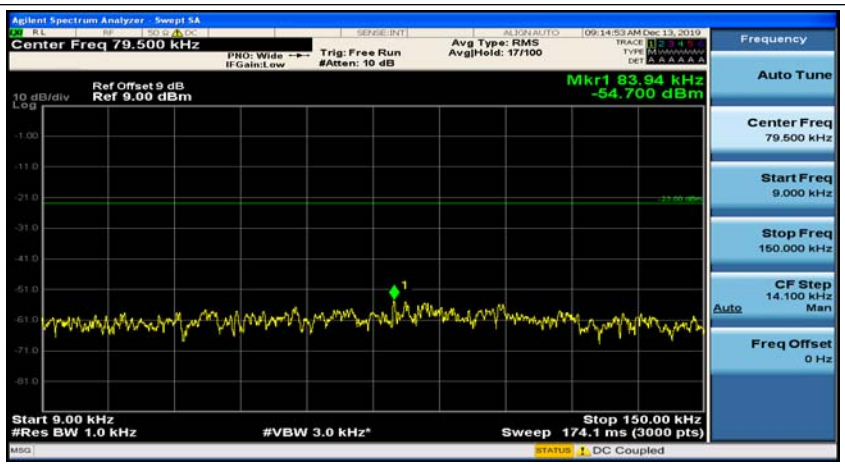
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:14:53 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 83.94 kHz
-54.700 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

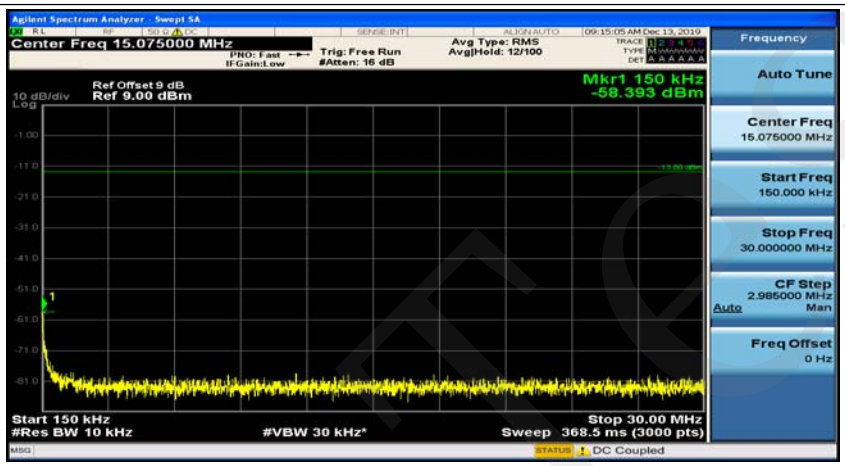
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:15:05 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-58.393 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:15:11 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.610 GHz
-26.605 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_HCH_QPSK_1RB#0

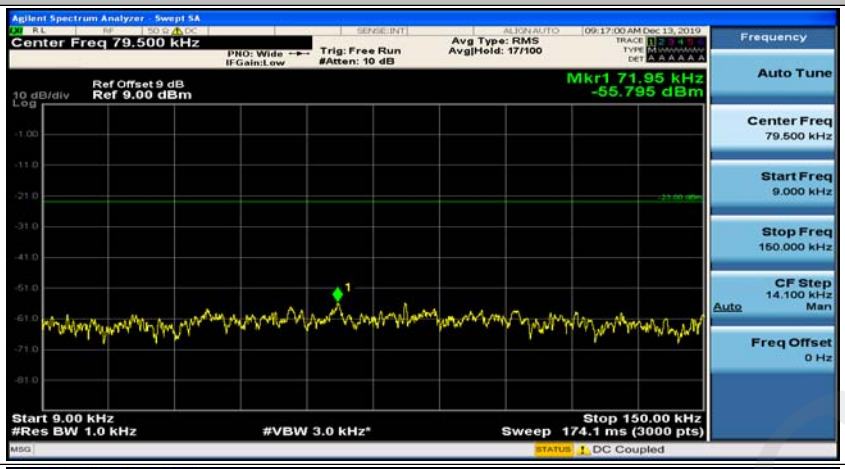

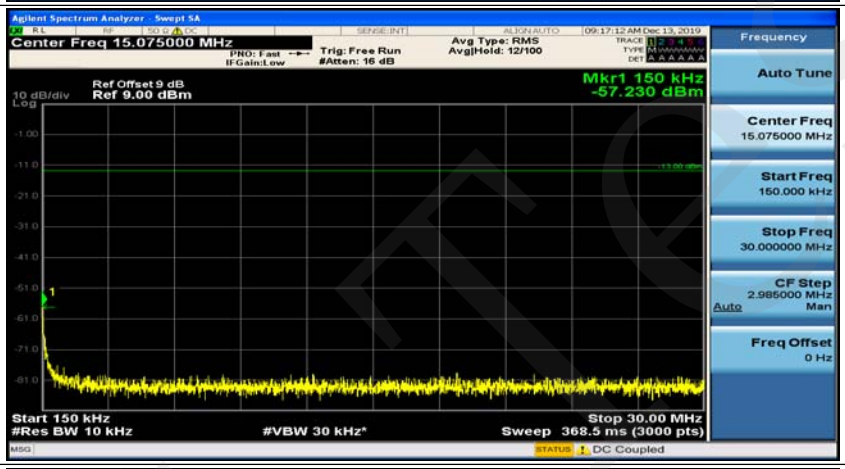

(Channel Bandwidth: 3 MHz)_HCH_QPSK_1RB#7

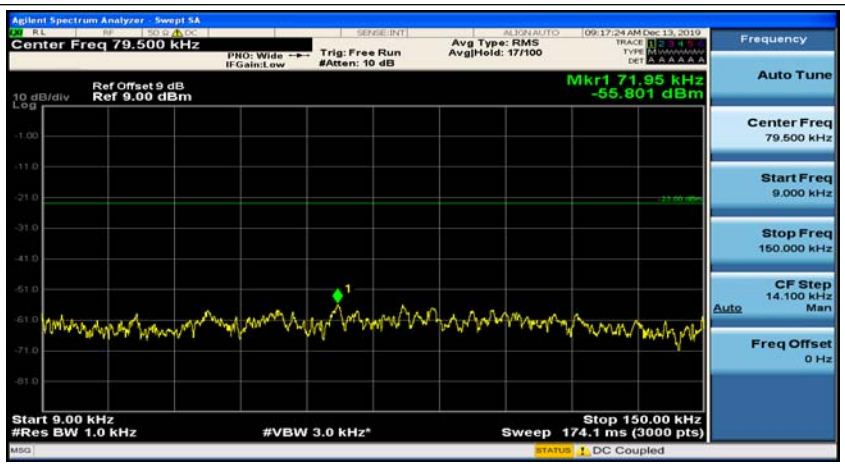
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:17:24 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 71.95 kHz
-55.801 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

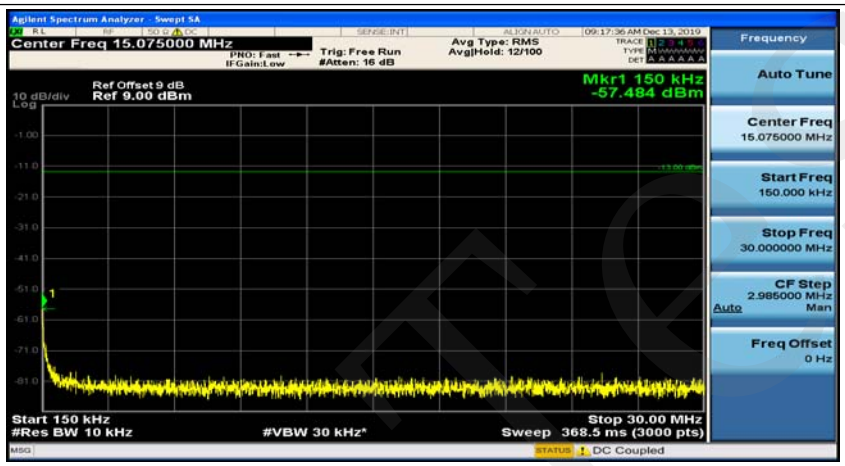
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:17:36 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.484 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

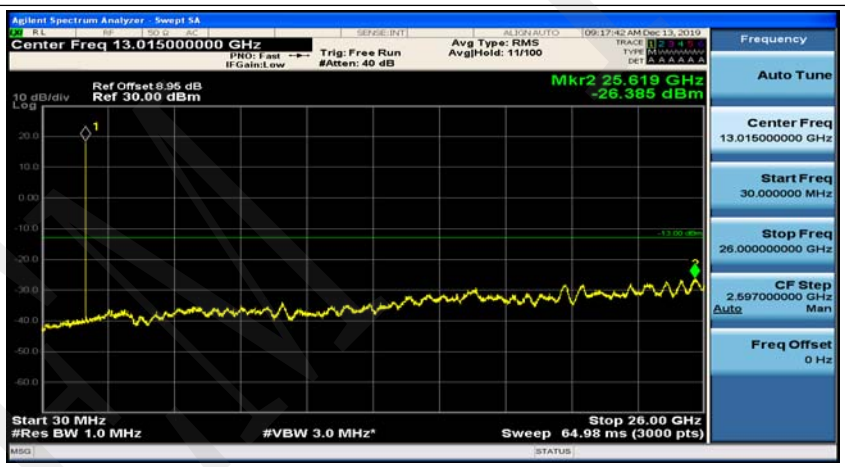
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:17:42 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.619 GHz
-26.385 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_LCH_16QAM_1RB#0

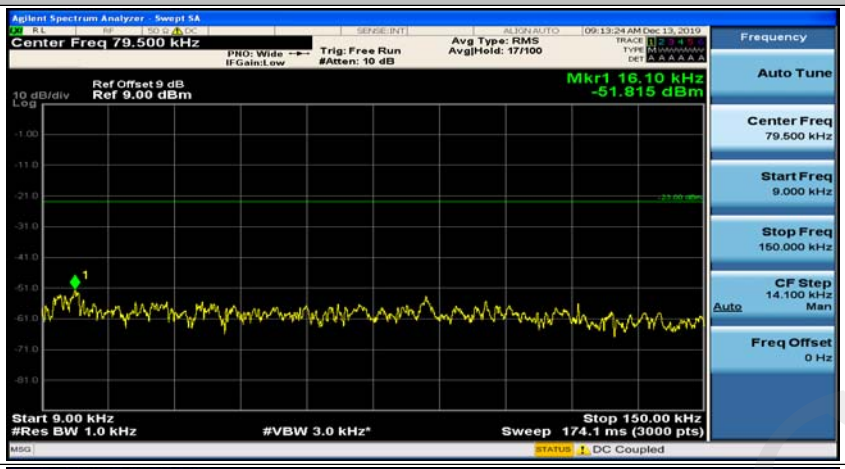

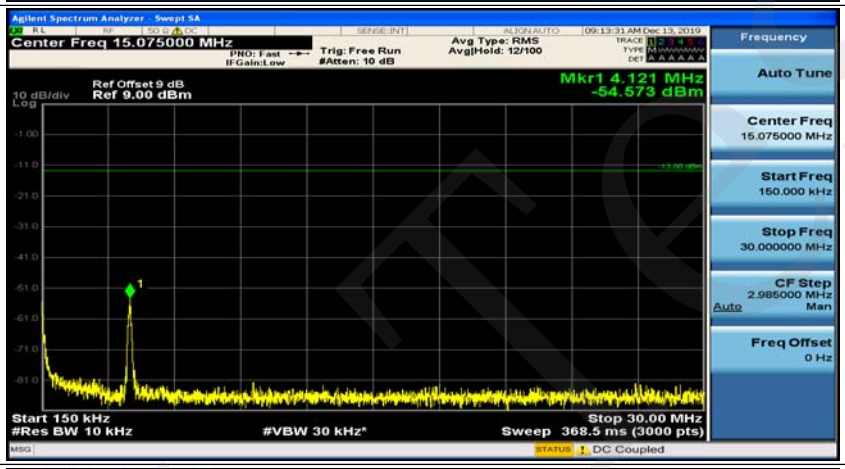

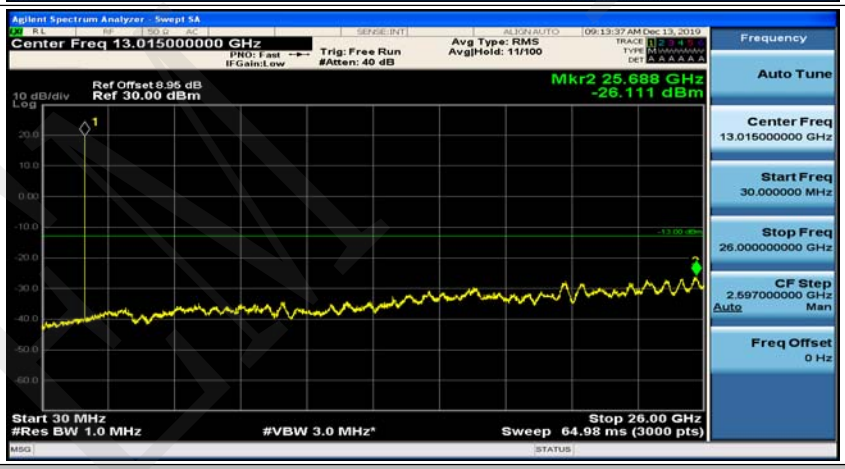

(Channel Bandwidth: 3 MHz)_LCH_16QAM_1RB#7

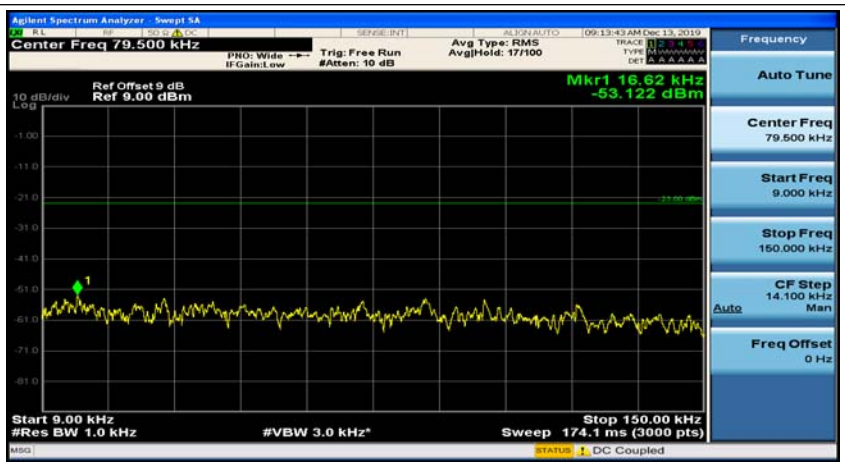
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:13:43 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 16.62 kHz
-53.122 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 79.500 kHz
Start Freq 9.000 kHz
Stop Freq 150.000 kHz
CF Step 14.100 kHz
Auto Man
Freq Offset 0 Hz

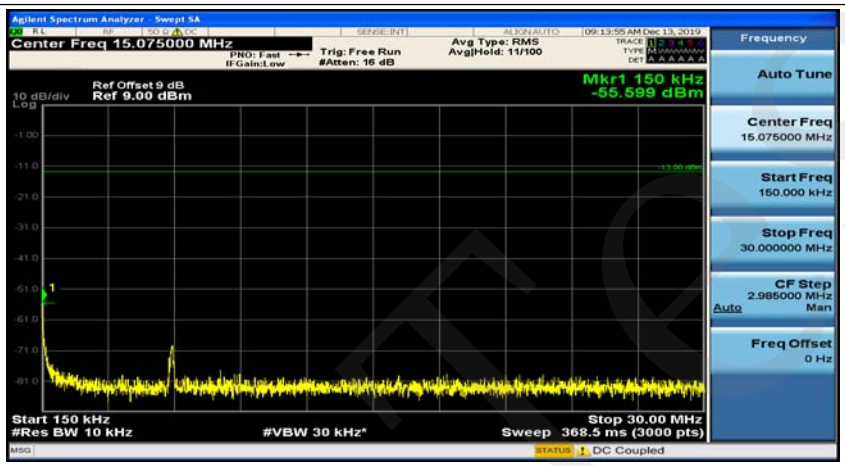
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 11/100
09:13:55 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-55.599 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq 15.075000 MHz
Start Freq 150.000 kHz
Stop Freq 30.000000 MHz
CF Step 2.985000 MHz
Auto Man
Freq Offset 0 Hz

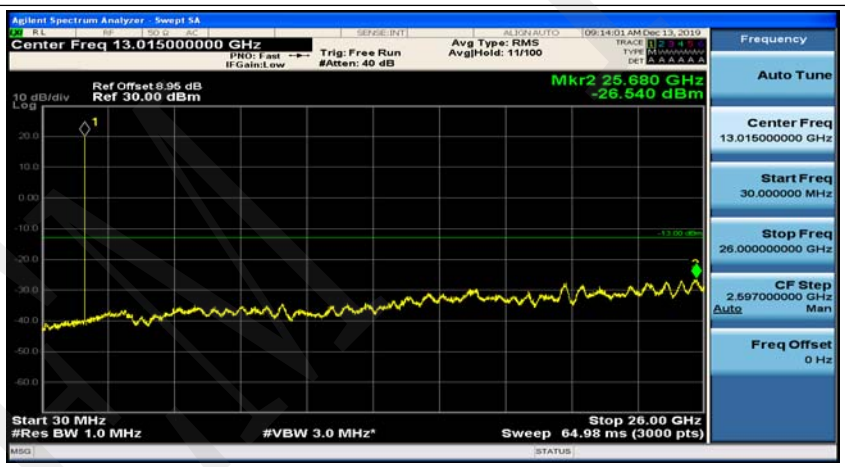
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:14:01 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.680 GHz
-26.540 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq 13.015000000 GHz
Start Freq 30.000000 MHz
Stop Freq 26.000000000 GHz
CF Step 2.597000000 GHz
Auto Man
Freq Offset 0 Hz

(Channel Bandwidth: 3 MHz)_MCH_16QAM_1RB#0

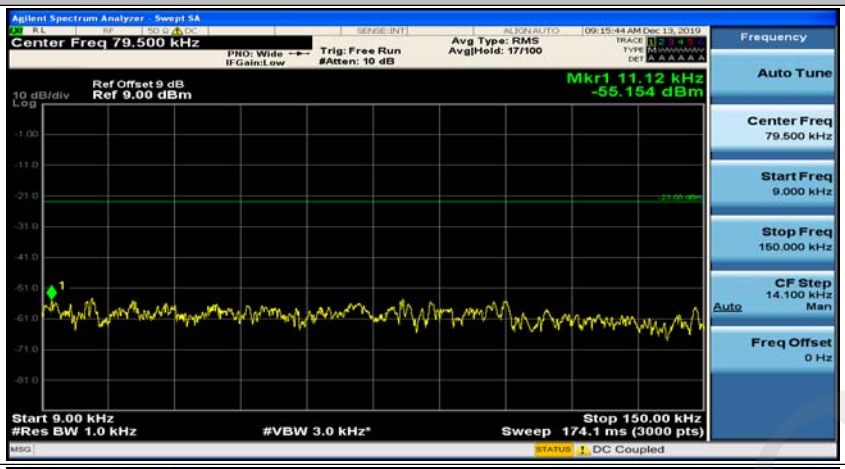

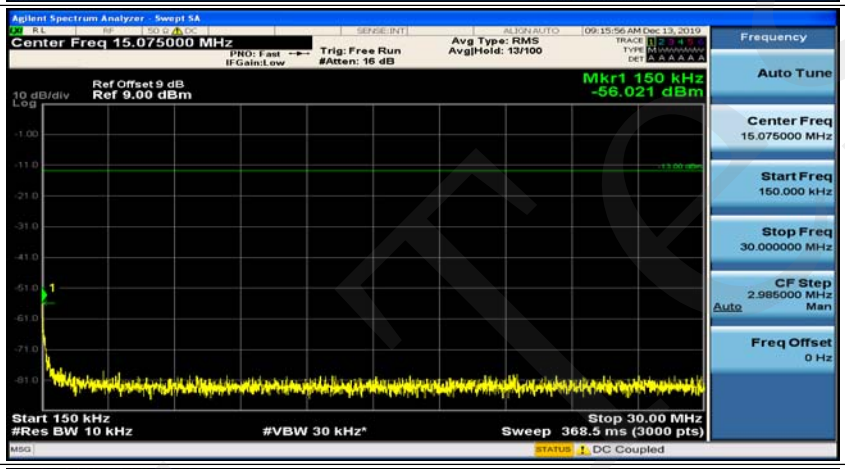

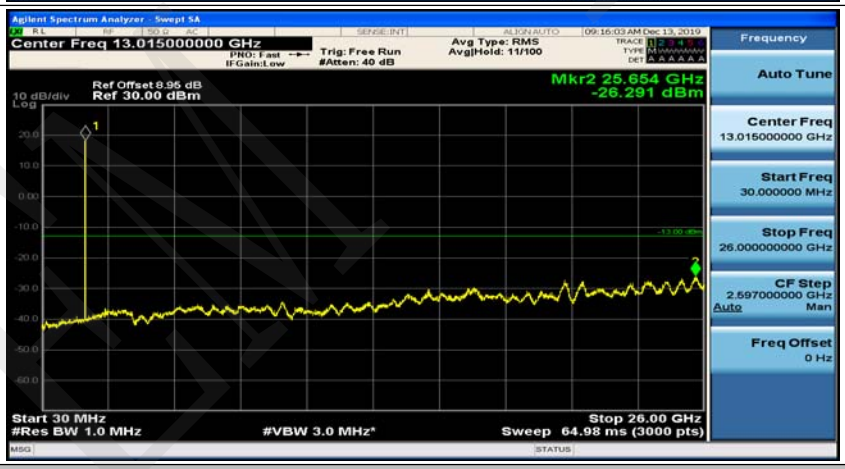

(Channel Bandwidth: 3 MHz)_MCH_16QAM_1RB#7

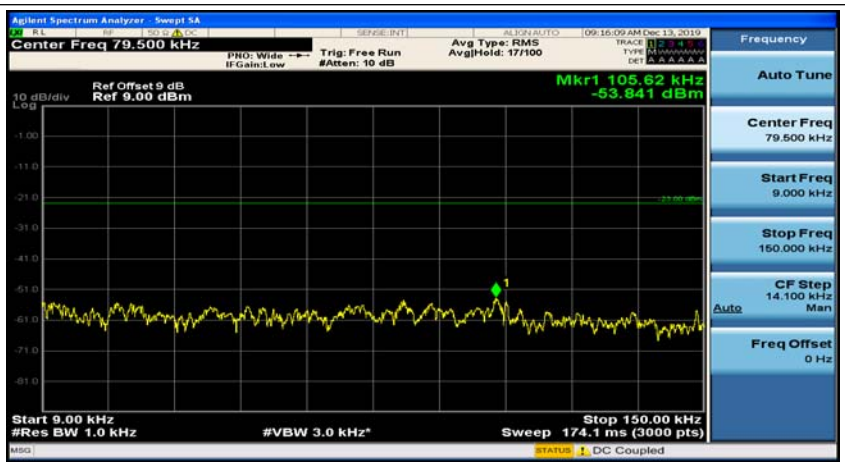
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:16:09 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 105.62 kHz
-53.841 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

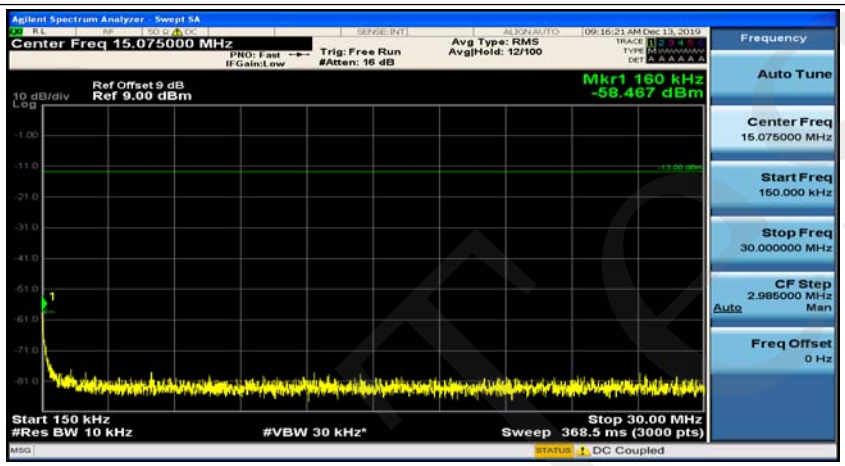
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:16:21 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 160 kHz
-58.467 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:16:27 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.706 GHz
-26.001 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 3 MHz)_HCH_16QAM_1RB#0

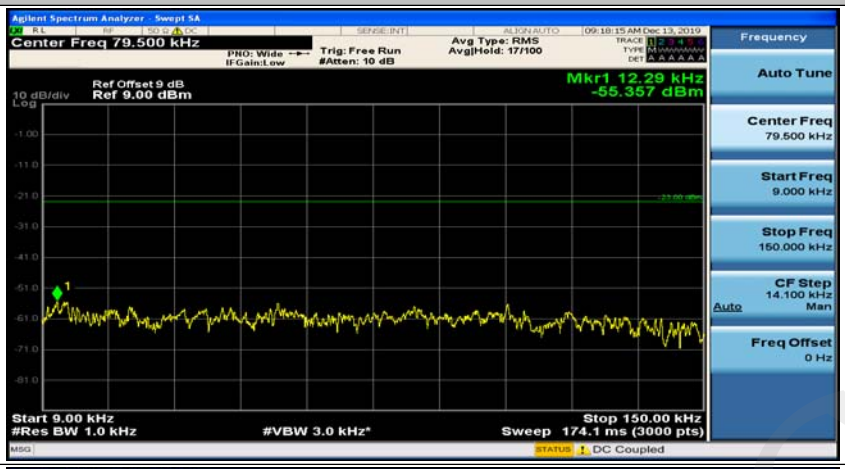

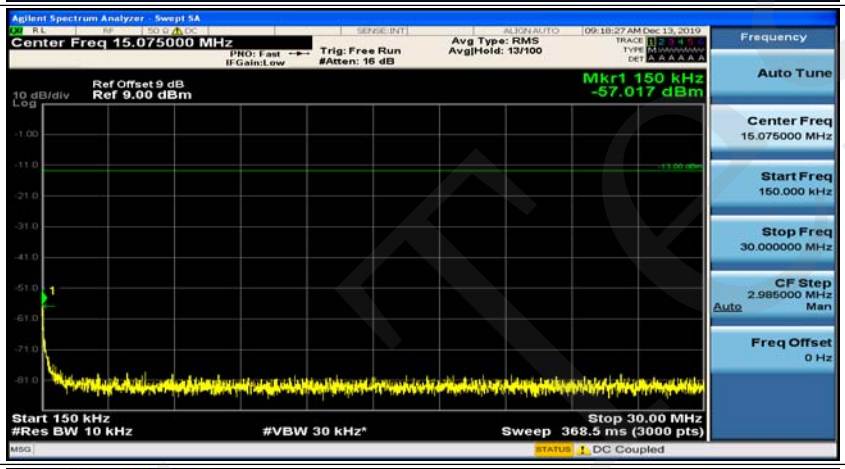

(Channel Bandwidth: 3 MHz)_HCH_16QAM_1RB#7

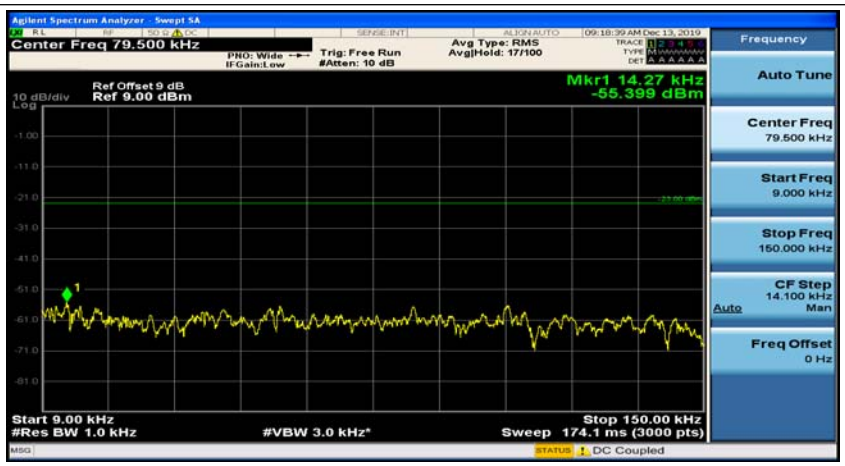
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:18:39 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 14.27 kHz
-55.399 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

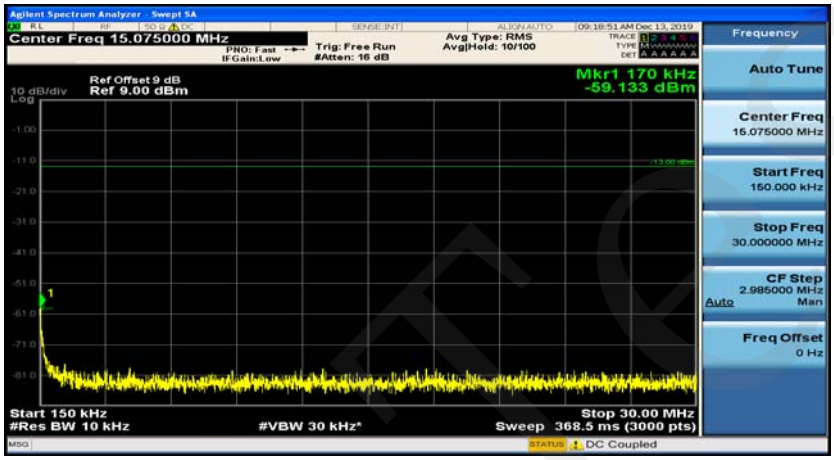
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 10/100
09:18:51 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 170 kHz
-59.133 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 10/100
09:18:56 AM Dec 13, 2019
Ref Offset 8.96 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.732 GHz
-26.195 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

Channel Bandwidth: 5 MHz

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#0

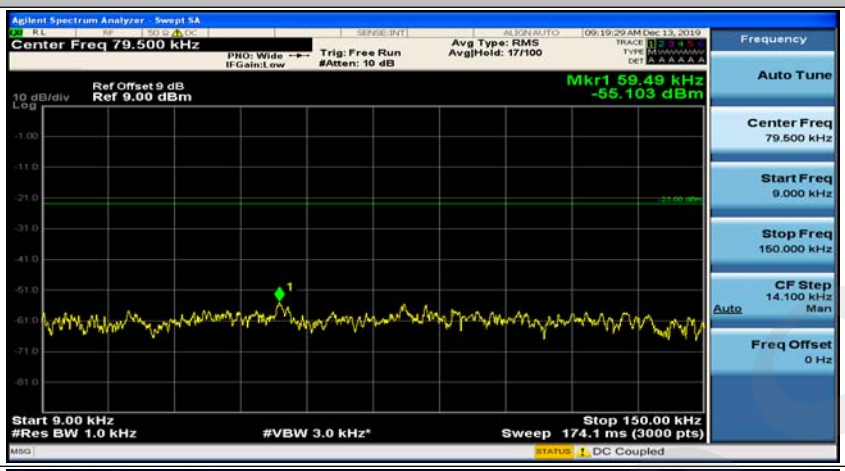

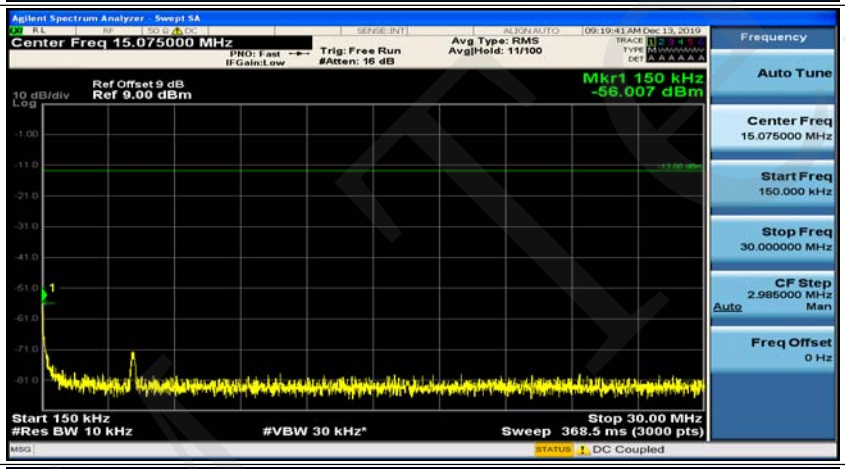

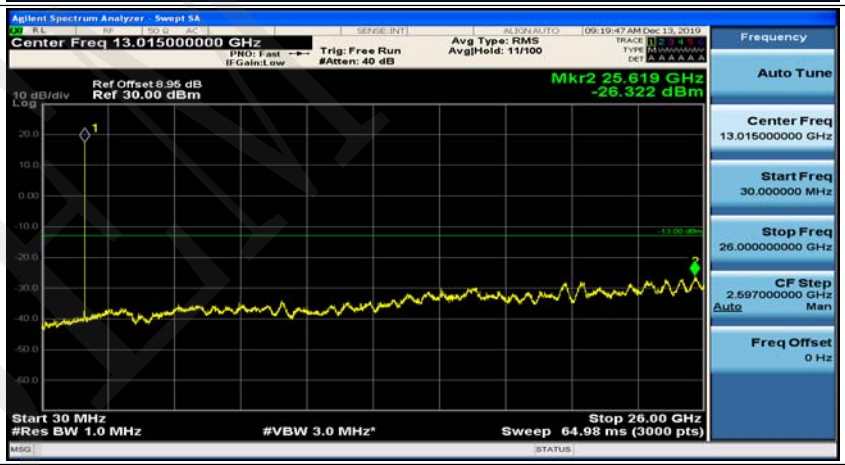

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#12

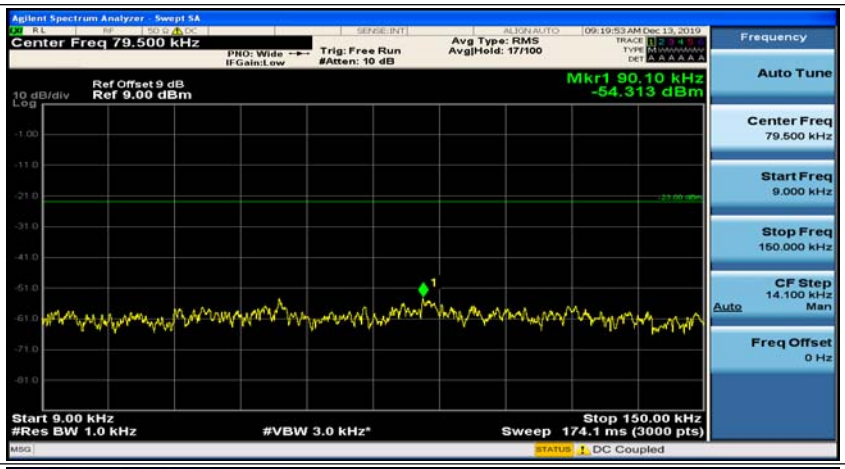

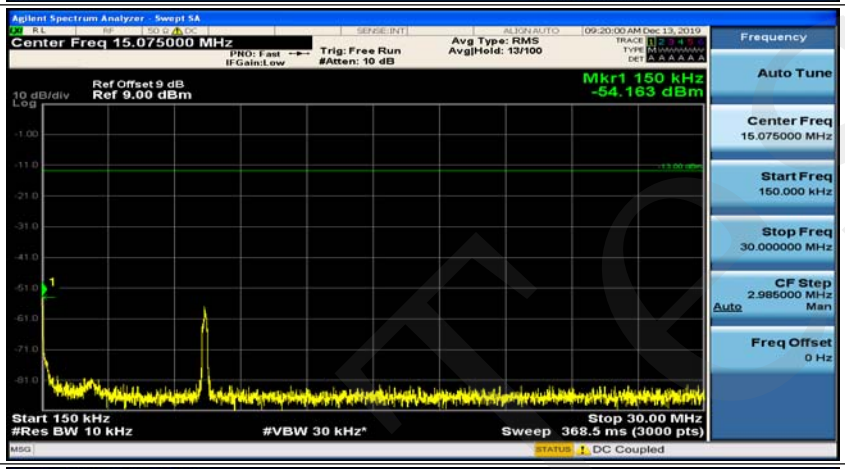

(Channel Bandwidth: 5 MHz)_LCH_QPSK_1RB#24

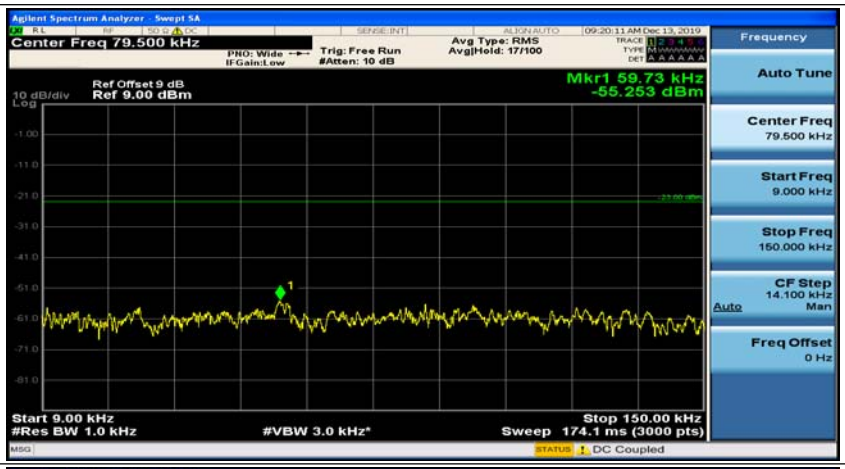
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:20:11 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 59.73 kHz
-55.253 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

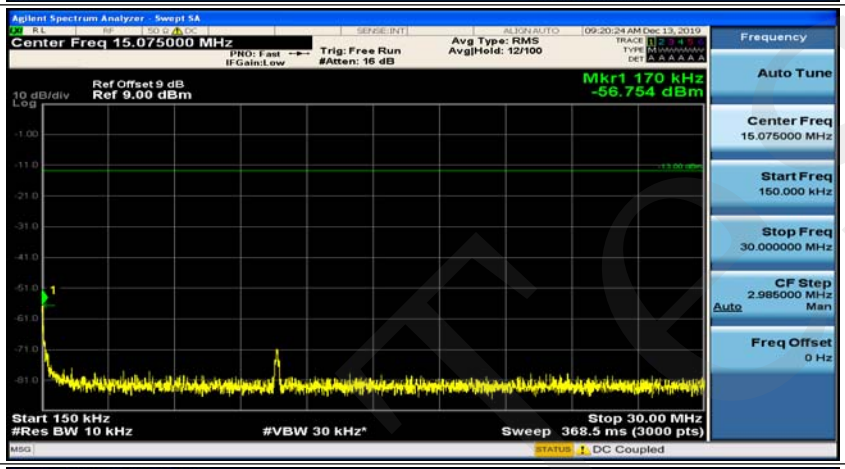
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:20:24 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 170 kHz
-56.754 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

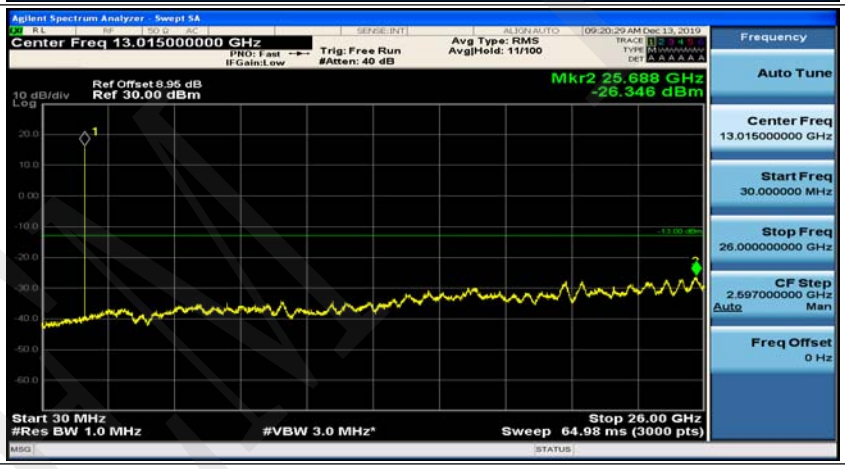
Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:20:29 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.688 GHz
-26.346 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#0

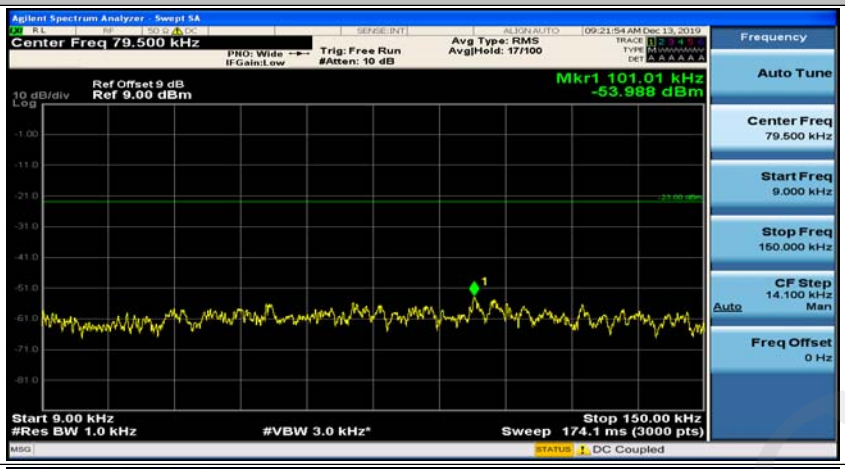

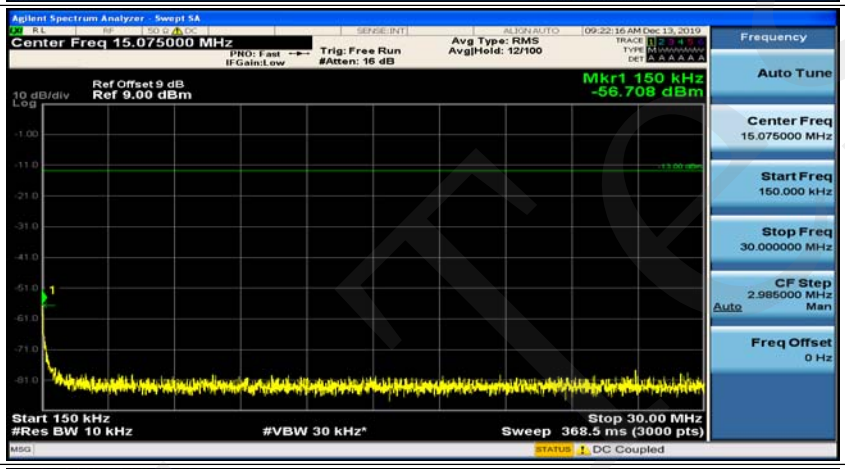

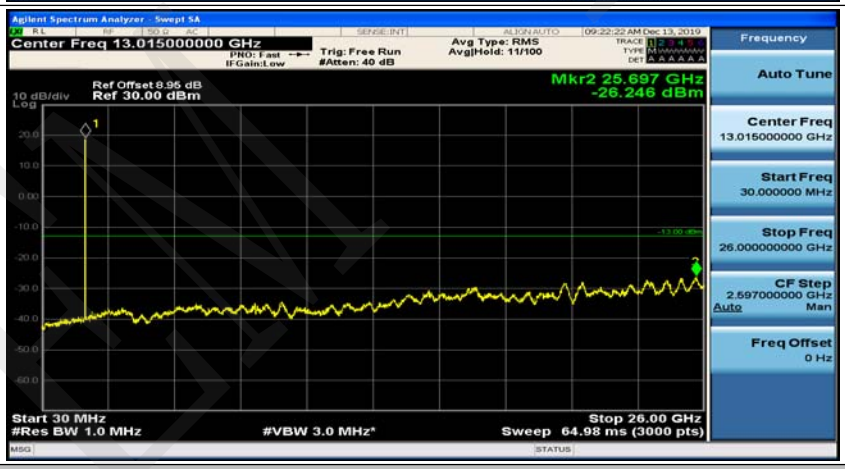

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#12

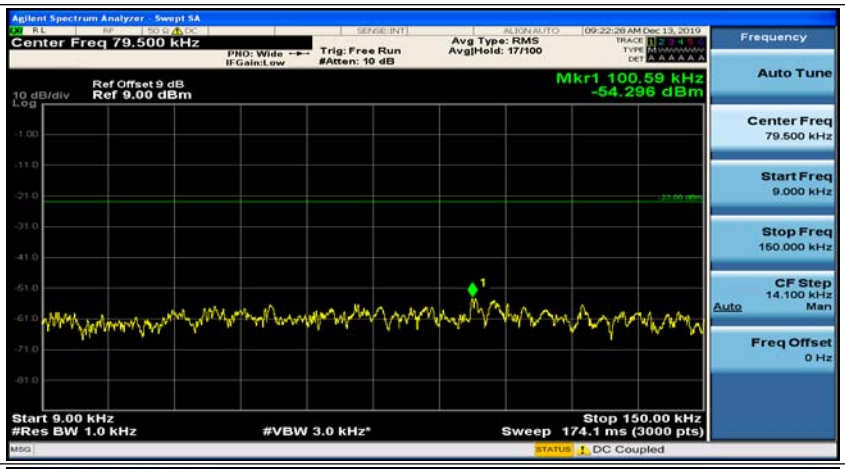

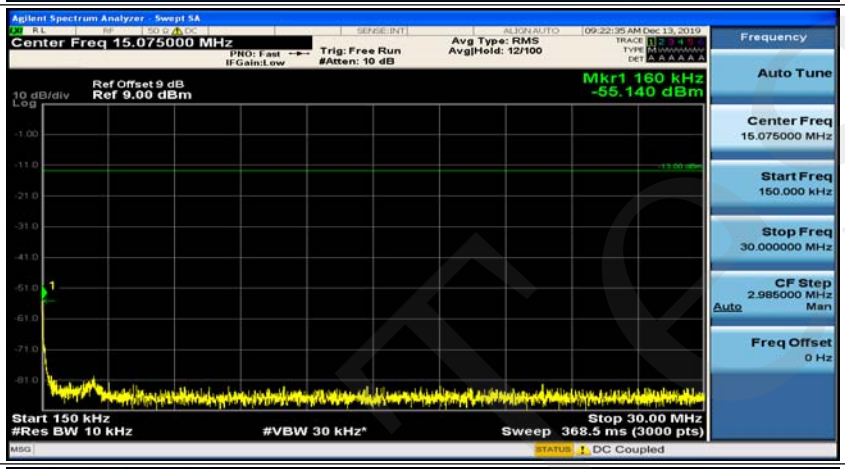

(Channel Bandwidth: 5 MHz)_MCH_QPSK_1RB#24

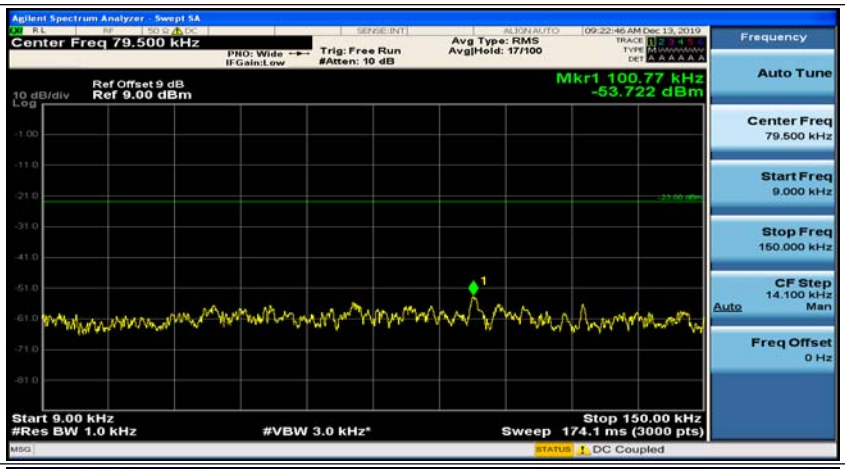
Agilent Spectrum Analyzer - Swept SA
Center Freq 79.500 kHz
PNO: Wide
IFGain:Low
Trig: Free Run
#Atten: 10 dB
Avg Type: RMS
Avg|Hold: 17/100
09:22:46 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 100.77 kHz
-53.722 dBm
Start 9.00 kHz
#Res BW 1.0 kHz
#VBW 3.0 kHz*
Stop 150.00 kHz
Sweep 174.1 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
79.500 kHz
Start Freq
9.000 kHz
Stop Freq
150.000 kHz
CF Step
14.100 kHz
Auto
Man
Freq Offset
0 Hz

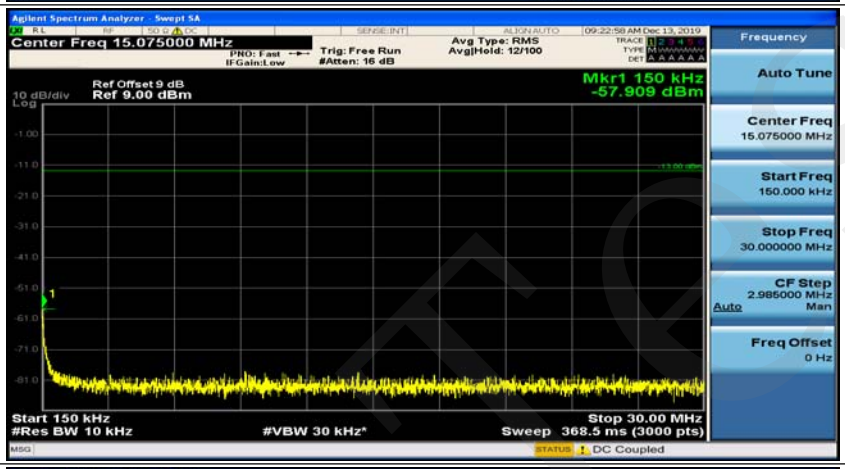
Agilent Spectrum Analyzer - Swept SA
Center Freq 15.075000 MHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 16 dB
Avg Type: RMS
Avg|Hold: 12/100
09:22:58 AM Dec 13, 2019
Ref Offset 9 dB
10 dB/div
Ref 9.00 dBm
Mkr1 150 kHz
-57.909 dBm
Start 150 kHz
#Res BW 10 kHz
#VBW 30 kHz*
Stop 30.00 MHz
Sweep 368.5 ms (3000 pts)
DC Coupled
Frequency
Auto Tune
Center Freq
15.075000 MHz
Start Freq
150.000 kHz
Stop Freq
30.000000 MHz
CF Step
2.985000 MHz
Auto
Man
Freq Offset
0 Hz

Agilent Spectrum Analyzer - Swept SA
Center Freq 13.015000000 GHz
PNO: Fast
IFGain:Low
Trig: Free Run
#Atten: 40 dB
Avg Type: RMS
Avg|Hold: 11/100
09:23:04 AM Dec 13, 2019
Ref Offset 8.95 dB
10 dB/div
Ref 30.00 dBm
Mkr2 25.645 GHz
-26.256 dBm
Start 30 MHz
#Res BW 1.0 MHz
#VBW 3.0 MHz*
Stop 26.00 GHz
Sweep 64.98 ms (3000 pts)
Frequency
Auto Tune
Center Freq
13.015000000 GHz
Start Freq
30.000000 MHz
Stop Freq
26.000000000 GHz
CF Step
2.597000000 GHz
Auto
Man
Freq Offset
0 Hz