

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V17.0.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Frequency	5200 MHz $\pm$ 1 MHz 5300 MHz $\pm$ 1 MHz 5600 MHz $\pm$ 1 MHz 5800 MHz $\pm$ 1 MHz	

Head TSL parameters at 5200MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.6 $\pm$ 6 %	4.63 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5200MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	20 dBm input power	7.67 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.5 W/kg $\pm$ 24 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	20 dBm input power	2.76 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg $\pm$ 24 % (k=2)

Head TSL parameters at 5300MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.4 $\pm$ 6 %	4.74 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5300MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	20 dBm input power	7.98 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.5 W/kg $\pm$ 24 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	20 dBm input power	2.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.5 W/kg $\pm$ 24 % (k=2)

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Head TSL parameters at 5600MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	5.06 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5600MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	20 dBm input power	8.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.1 W/kg ± 24 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	20 dBm input power	2.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.1 W/kg ± 24 % (k=2)

Head TSL parameters at 5800MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.6 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

SAR result with Head TSL at 5800MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	20 dBm input power	7.89 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	78.6 W/kg ± 24 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	20 dBm input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24 % (k=2)



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	47.7Ω- 1.84jΩ
Return Loss	- 30.4dB

Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	46.9Ω+ 0.06jΩ
Return Loss	- 29.8dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	52.7Ω+ 4.29jΩ
Return Loss	- 26.2dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	53.4Ω+ 1.95jΩ
Return Loss	- 28.4dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.099 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL
Test Laboratory: CTTL, Beijing, China

Date: 2026-02-05

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN 1371	5200	HSL	20

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat	10	CW,	5200	5.52	4.63	35.6


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL5G	EX3DV4 - SN7307, 2025-05-27	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

Zoom Scan		Zoom Scan	
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.67
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.16
Sensor Surface [mm]	1.4	Power Drift [dB]	0.07
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.4	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	62.8
Scan Method	Measured	Dist 3dB Peak [mm]	7.2

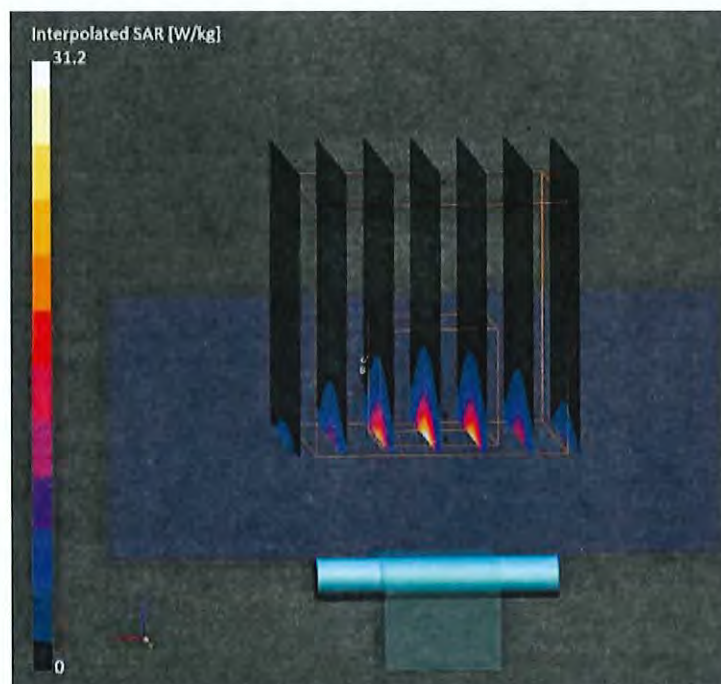



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Date: 2026-02-06

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN 1371	5300	HSL	20

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat	10	CW,	5300	5.34	4.74	35.4


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL5G	EX3DV4 - SN7307, 2025-05-27	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.98
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.26
Sensor Surface [mm]	1.4	Power Drift [dB]	0.02
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.4	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	61.6
Scan Method	Measured	Dist 3dB Peak [mm]	7.2

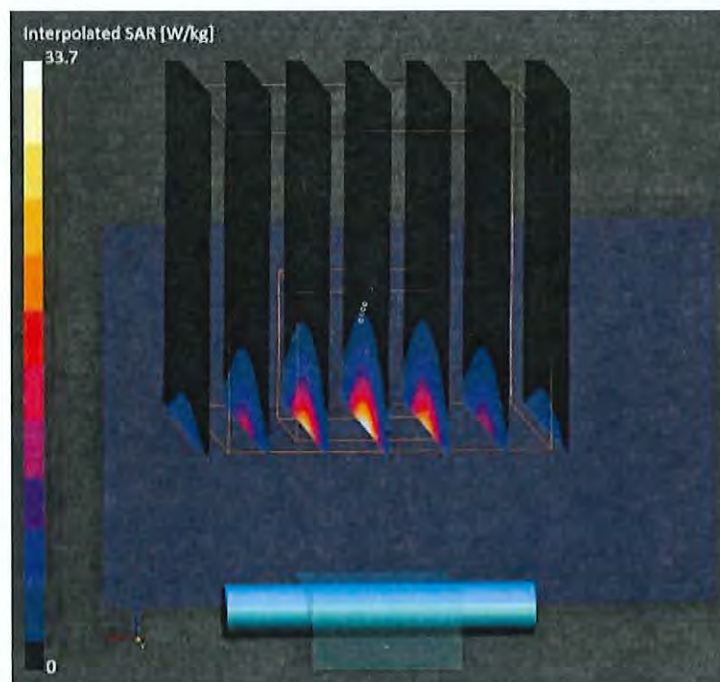



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Date: 2026-02-06

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN 1371	5600	HSL	20

Exposure Conditions

Phantom	Position, Test	Band Group,	Frequency	Conversion	TSL Cond.	TSL
Section, TSL	Distance [mm]	UID	[MHz]	Factor	[S/m]	Permittivity
Flat	10	CW,	5600	4.95	5.06	34.8


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL5G	EX3DV4 - SN7307, 2025-05-27	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

Zoom Scan		Zoom Scan	
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	8.24
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.32
Sensor Surface [mm]	1.4	Power Drift [dB]	-0.03
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.4	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	59.5
Scan Method	Measured	Dist 3dB Peak [mm]	7.4

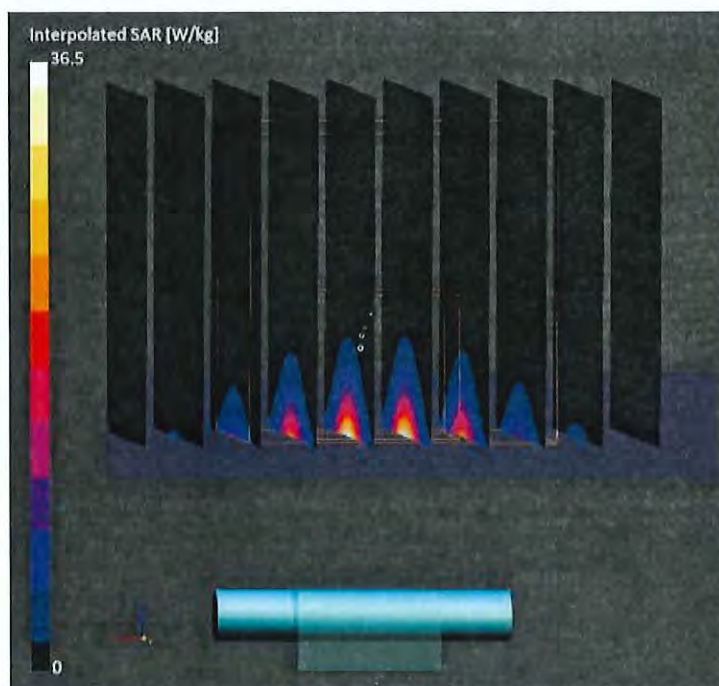



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

DASY6 Validation Report for Head TSL

Date: 2026-02-09

Test Laboratory: CTTL, Beijing, China

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 – SN 1371	5800	HSL	20

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat	10	CW,	5800	5.03	5.25	34.6


Hardware Setup

Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL5G	EX3DV4 - SN7307, 2025-05-27	DAE4 Sn1588, 2025-08-29

Scan Setup

Measurement Results

Zoom Scan		Zoom Scan	
Grid Extents [mm]	22.0×22.0×22.0	psSAR1g [W/kg]	7.89
Grid Steps [mm]	4.0×4.0×1.4	psSAR10g [W/kg]	2.22
Sensor Surface [mm]	1.4	Power Drift [dB]	0.02
Graded Grid	Yes	Power Scaling	Disabled
Grading Ratio	1.4	Scaling Factor [dB]	
MAIA	N/A	TSL Correction	No correction
Surface Detection	VMS + 6p	M2/M1 [%]	57.0
Scan Method	Measured	Dist 3dB Peak [mm]	6.9

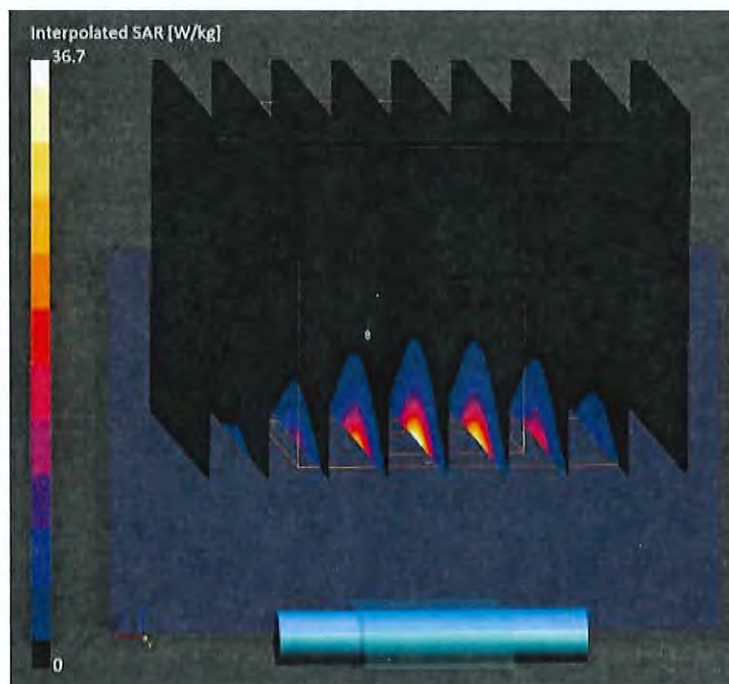



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2711
E-mail: emf@caict.ac.cn <http://www.caict.ac.cn>

Impedance Measurement Plot for Head TSL

