




Appendix I

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

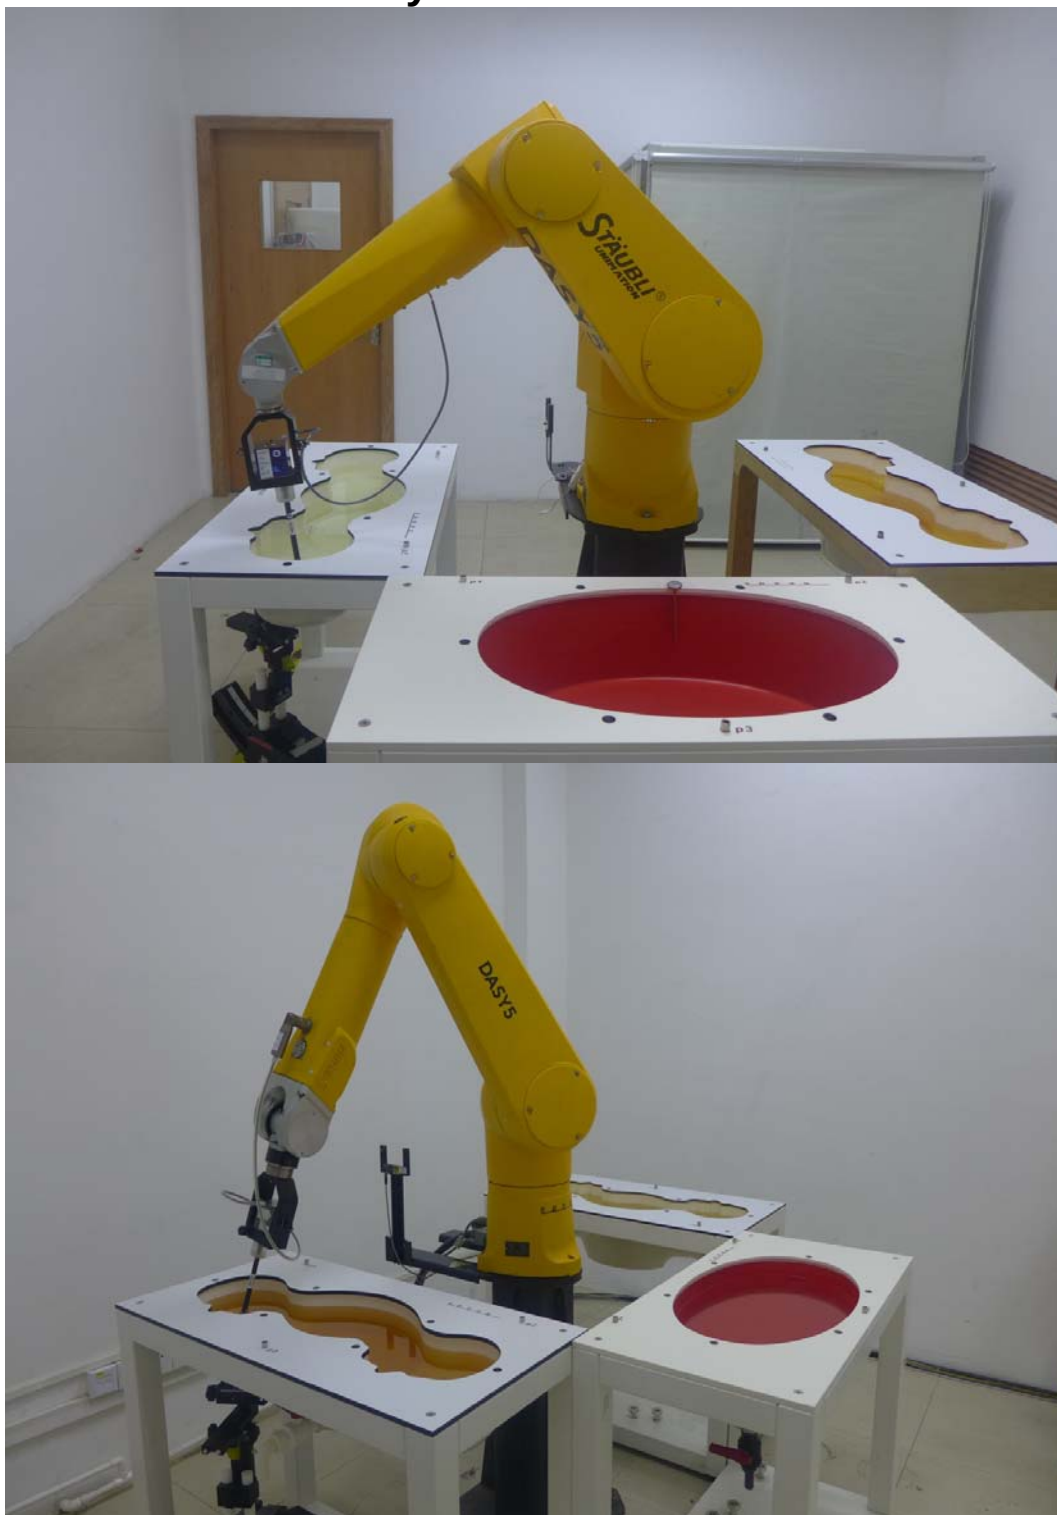

2. Photographs of Tissue Simulate Liquid

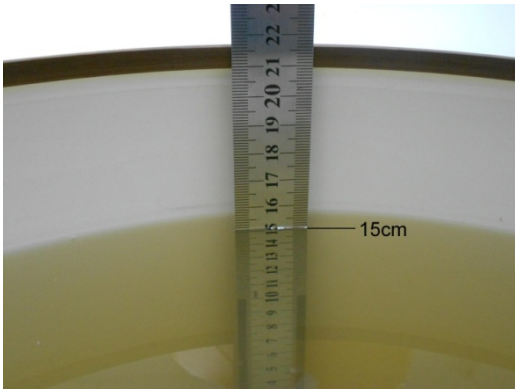
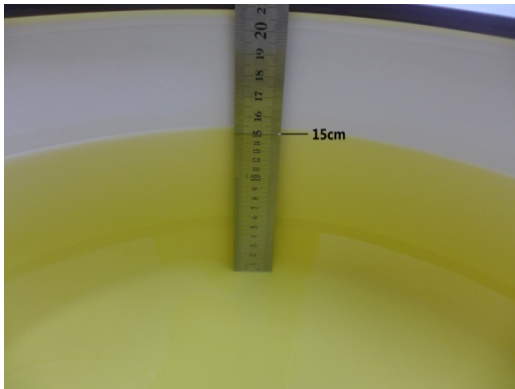
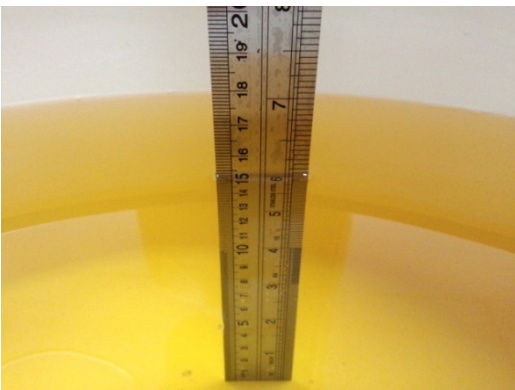
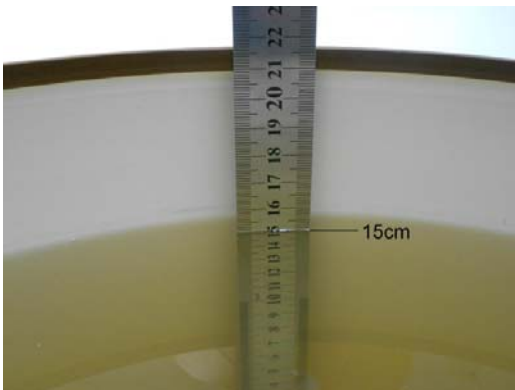
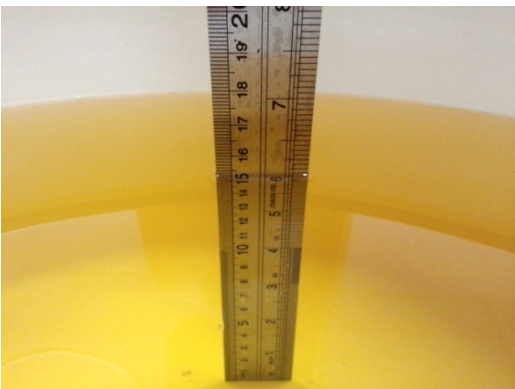
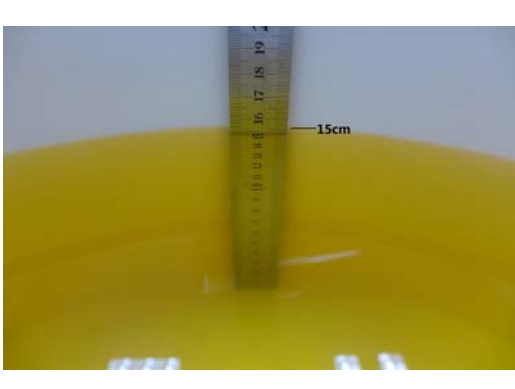
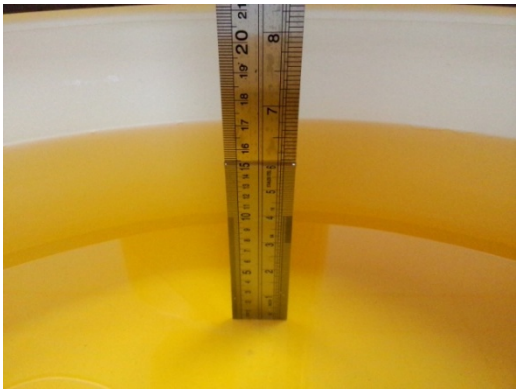
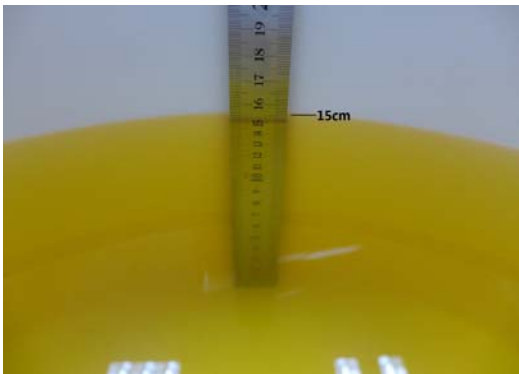
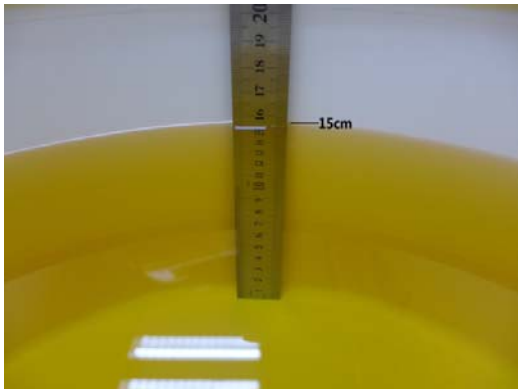
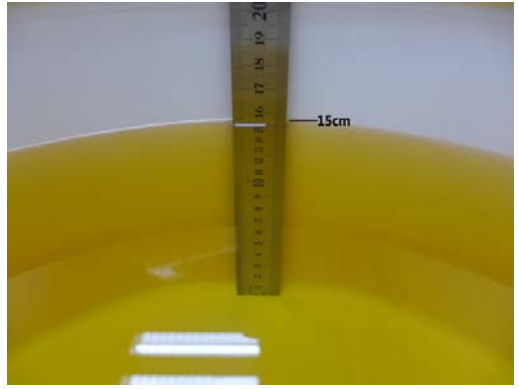
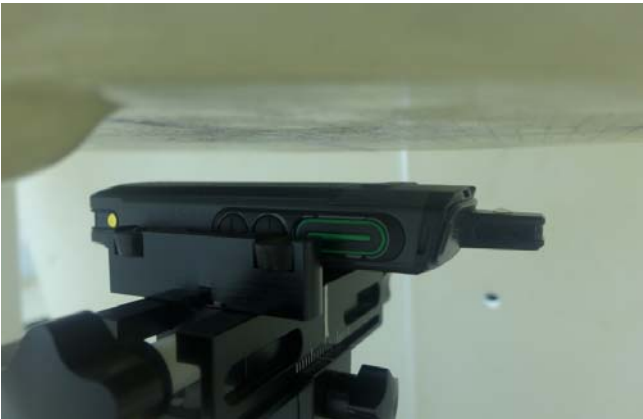
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	
Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
	

Photo 7: Tissue Simulant Liquid for Head 1900	Photo 8: Tissue Simulant Liquid for Body 1900
	
Photo 9: Tissue Simulant Liquid for Head 2450	Photo 10: Tissue Simulant Liquid for Body 2450
	
Photo 11: Tissue Simulant Liquid for Head 2600	Photo 12: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position

Photo 13: Front side 10mm	Photo 14: Front side 15mm
	
Photo 15: Back side 15mm	Photo 16: Back splint 0mm
	

4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
	
Photo 19: Back View	NA
	NA