



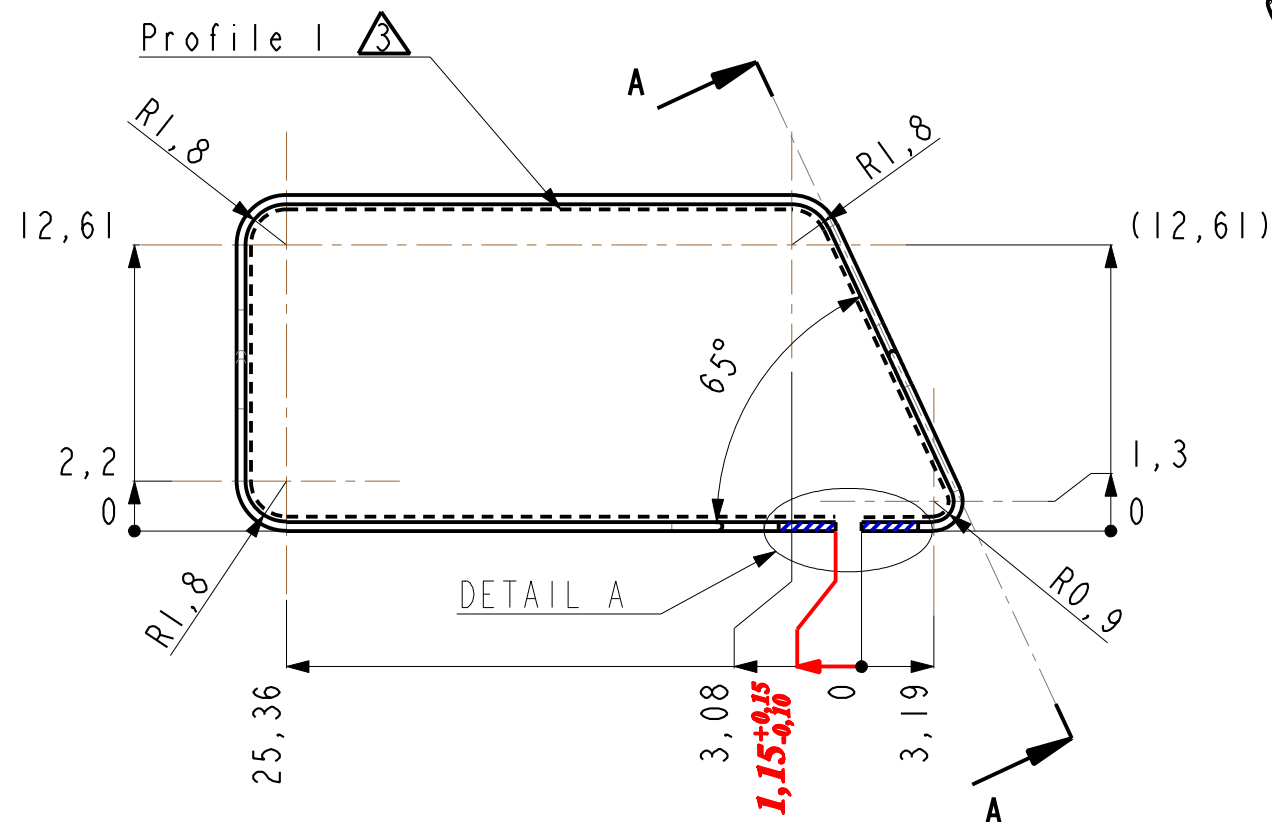


1 The antenna shall be gold plated everywhere unless otherwise specified.
Gold plate according to ASTM B488-11, Type I, Code C, Class 5.0.
Plating thickness: min 5µm , max 11µm.

③ Dimensional control of the antenna (profile 1, 2 , 3 and 4) will be realized after final molding in the header.
When visually inspected in molded header, antenna needs to remain located by antenna supports.



5 Supplier shall provide as annex of the header CoC the used bare wire CoC with the indication of the wire dimensions and tolerances for each shipped lot.

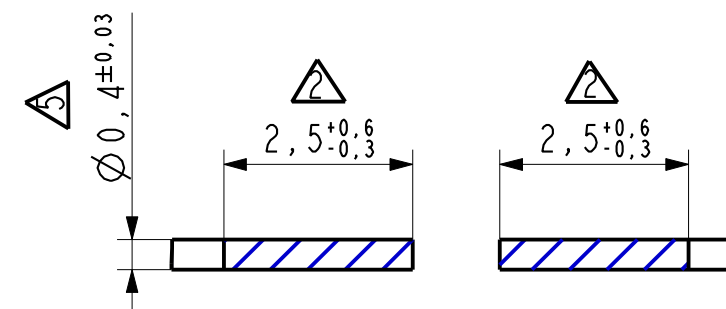

DETAIL A
SCALE 10:1

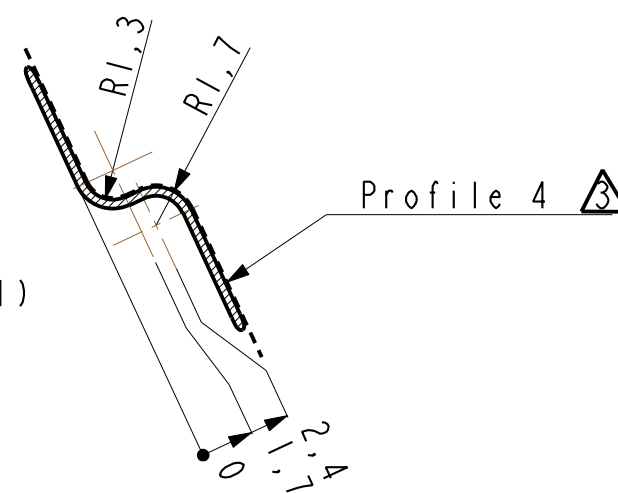

SECTION A - A

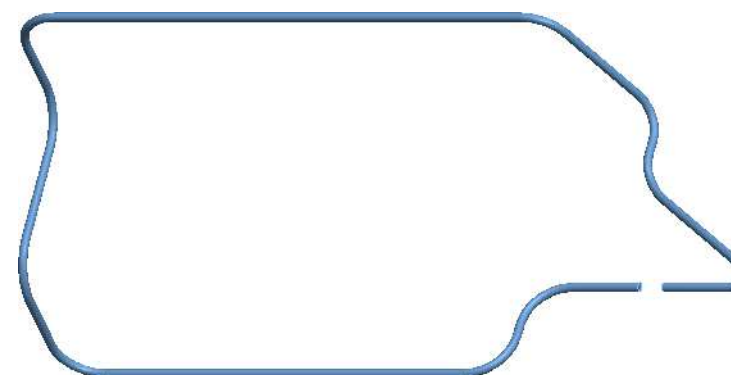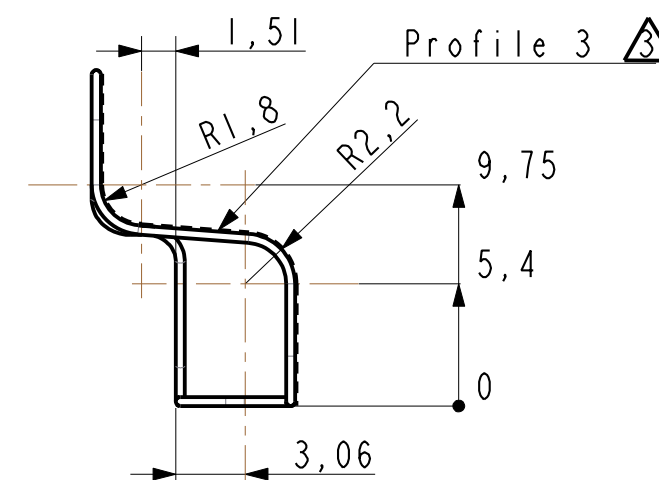

FF00892A

A 02/04/15 AM020564		B ..16/06/2016 AM021651		D	E	F	G
MATERIAL : SMCS711; ASTM B488-11				REMARKS : For dimension modified, the text must be : Bold, Italic and in Red Color. ex : 2.66±0.05			
OVERALL TOLERANCES :±0,1 mm ANGLES :±2°				☒ numbering for CRM use only.			
CARDIAC RHYTHM MANAGEMENT				RF Antenna DF4/IS4			
 SORING GROUP AT THE HEART OF MEDICAL TECHNOLOGY				Mechanical Studies and Development (MSD)			
PREPARED BY: A.Lombardi	CHECKED BY: L.Di Maio	APPROVED BY: R.Cicerone	Scale 3:1 	A3	GA25		B
DATE 17-May-16	DATE	DATE					I / I