

BEHIND THE EARS HEARING AIDS

Operating instructions

- lewi R
- risa R



Specific function

audifon hearing aids are wearable air conduction hearing aids, used to compensate for hearing loss of the wearer by recording, processing and emitting an amplified sound signal. The hearing aids are available with different amplifications and output sound levels, to compensate for light to severe hearing loss. These hearing aids are not suitable for children under 36 months of age.

It is additionally possible to activate the tinnitus module integrated in the hearing aid to treat chronic, persistent tinnitus (a ringing sound in the ears).

The hearing aids are designed for a lifespan of 6 years.

 Hearing aids need to be fitted individually by a hearing care professional or ENT doctor. Diagnostics and the prescription of hearing aids are the task of an ENT doctor.

CONTENTS

1	INTRODUCTION	5
2	YOUR HEARING AID	6
2.1	Type	6
2.2	Overview	6
2.3	Batteries	7
2.3.1	Note on the battery	8
2.3.2	Low battery warning	9
3	OPERATION RISA R, LEWI R	10
3.1	Construction	10
3.2	Inserting battery	11
3.3	Removing battery	12
3.4	Switching hearing aids on and off	13
3.5	Inserting and removing hearing aids	14
3.5.1	Inserting hearing aids	14
3.5.2	Removing hearing aids	15
3.6	Volume and program selection	16
3.6.1	Binaural synchronisation	16
3.6.2	Multifunctional rocker switch	17
3.6.3	Volume selection	18
3.6.4	Selecting the hearing programs	19
4	TINNITUS COMBI INSTRUMENT	21
4.1	Start-up	21
5	WIRELESS FUNCTIONALITY / BLUETOOTH CONNECTIVITY	22
5.1	Using hearing aids with iOS devices	22
5.1.1	Pairing hearing aids with the iOS device / iPhone	22
5.1.2	Operating hearing aids with an iOS device / iPhone	23
5.1.3	Operation via the menu <i>MFI Hearing Devices</i>	24
5.1.4	Operation via the quick start menu	24
5.2	Pairing hearing aids with an Android device	25

5.3	Using hearing aids with the MULTISTREAMER PRO	26
5.3.1	Pairing hearing aids with the MULTISTREAMER PRO	26
5.3.2	Pairing your smartphone with the MULTISTREAMER PRO	26
5.4	Flight mode	27
6	ACCESSORIES	28
6.1	Compatibility	29
7	CARE INSTRUCTIONS	30
7.1	General	31
7.2	Cleaning and care of Behind-The-Ear hearing aids with an external receiver	33
	Changing the earwax protection filter	33
7.3	Drying hearing aids	32
8	DEALING WITH PROBLEMS	35
9	SAFETY INSTRUCTIONS	36
9.1	Important warnings	36
9.2	Notes on product safety	38
10	SIDE EFFECTS	41
11	OPERATING CONDITIONS	42
12	TRANSPORT AND STORAGE CONDITIONS	43
13	ENVIRONMENTALLY FRIENDLY DISPOSAL	44
14	OTHER INFORMATION	45
14.1	EU Declaration of conformity	45
14.2	FCC Statement	46
15	SERVICE	46
16	KEY TO SYMBOLS	49

WARRANTY CARD

1 INTRODUCTION

Congratulations on the purchase of your new audifon hearing aids. Your hearing care professional has set this for your individual requirements. These instructions are therefore intended to help you use your audifon hearing aids properly.

Please read through the following operating and care instructions carefully to avoid malfunctions and faults. If you follow the instructions, your hearing aids will prove an invaluable help in day-to-day communication with your surroundings and other people.

The specific model of your hearing aids is shown on the sticker on the packaging, on the warranty card or printed on the hearing aids themselves.

Please take note of the following:

Your hearing aid will not make your hearing normal again, nor will it prevent or improve any physical hearing loss. If you fail to wear your hearing aid regularly, you will not benefit fully from it. Use of a hearing aid only accounts for part of your hearing ability and may need to be supplemented by auditory training and instruction in lip reading.

If you have any further questions, please contact your hearing care professional.

2 YOUR HEARING AID

2.1 Type

Your hearing aids are behind-the-ear hearing aids with an external receiver. The receiver is located directly in your ear.

2.2 Technical features

Model	Battery				Amplification in dB (peak)			Indication range
	Size	Average Service life (zinc air) in hours						
		HE S	HE M	HE P	HE S	HE M	HE P	
Iewi R	312	100	90	80	45	56	67	Minor to severe hearing loss
risa R	312	100	90	80	45	56	67	Minor to severe hearing loss

The detailed acoustic data for your hearing aid can be found in a separate data specification. This and further information are available from your hearing care professional or www.audifon.com.

2.3 Batteries

To start your hearing aids first insert a battery in the battery compartment.

Make sure you only use zinc air batteries. Please follow the instructions on the battery packaging. For the exact type of battery in your hearing aid please see the overview table.

Always switch your hearing aid off after use. Remove the battery if your instruments are out of use for long periods, to avoid damage.

2.3.1 Note on the battery

A zinc air battery is used to supply the power for your hearing aids. This type of battery is only activated when oxygen comes through the air holes into the button cell and the chemical reaction is started. During production, the air holes are sealed with a protective strip. This means that the battery remains fresh until use, and it lasts longer when it is sealed. Removing the protective strip allows oxygen to enter and the chemical reaction is activated.

Important notes:

- ⚠ Refitting the strip when the battery is not in use will not extend its service life.
- ⚠ Your batteries should be stored at room temperature. Avoid keeping them in hot places or rooms with high humidity (e.g. bathroom). Storage in a cooled location is not necessary.
- ⚠ Never carry batteries loose in a trouser pocket or a purse. Metal objects like coins or keys could cause batteries to short-circuit.
- ⚠ Old batteries may contain hazardous substances or heavy metals that pollute the environment and harm health. Batteries are recycled as they contain valuable raw materials such as iron, zinc, manganese or nickel. Old batteries should not be placed in household waste. Consumers are bound to dispose of batteries at a collection point provided by the local authority or sales outlet. After use you can also return the batteries in the appropriate containers at the premises of your hearing care professional for free.

2.3.2 Low battery warning


An audible signal indicates the end of the battery life (approx. 30 minutes before the end of the battery's life).

3 OPERATION – LEWI R, RISA R

3.1 Construction

The hearing aids consist of the following elements:

- ① Receiver module
- ② Dome
- ③ Concha clip (optional)
- ④ Microphone inlets
- ⑤ Rocker switch
- ⑥ Battery compartment / ON/OFF switch

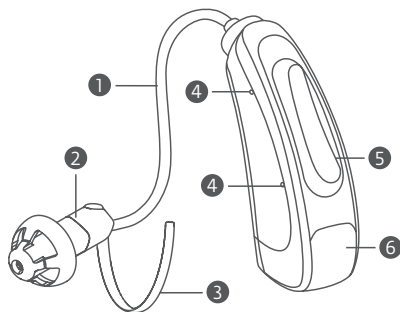

☞ The hearing aids have side markings at the receiver module
blue = left, red = right


☞ Your hearing aids may differ from the illustrations.

3.2 Inserting battery




Remove a battery from its packaging.

If the battery has a protective film, remove and wait a few minutes before inserting the battery.



Open the battery compartment carefully with your finger nail at the opening edge and swing it right out.



Then insert the battery in the battery compartment. Make sure the (+) symbol on the battery matches the (+) symbol on the battery compartment.

☞ Please do not open the battery compartment any wider than shown here. This might damage the device.

⚠ **NOTE:** Do not force the battery into the battery compartment. If it does not fit, check whether you are inserting it correctly and that it is the correct type of battery (see Section 2.2).

3.3 Removing battery



Open the battery compartment carefully with your finger nail at the opening edge and swing it right out.

Then remove the battery from the battery compartment.


 Please do not open the battery compartment any wider than shown in Section 3.2. This might damage the device.

3.4 Switching hearing aids on and off

Your hearing aids are switched on and off via the battery compartment.

Switching on

Close the battery compartment securely with a battery inserted by moving it past the catch of the OFF position into the casing.




You will feel the battery compartment clicking into place as you close it.

The hearing aids are now switched on. After a preset delay and a start-up jingle, the first program will activate and the hearing aids are ready for use.

Switching off

To switch off, open the battery compartment carefully with your fingernail at the opening edge and swing it out to the first catch position.




This is the OFF position.

If the devices will be out of use for a long time, open the battery compartment fully and remove the battery.

3.5 Inserting and removing hearing aids

3.5.1 Inserting the hearing aids

Place the hearing aids behind your ear.

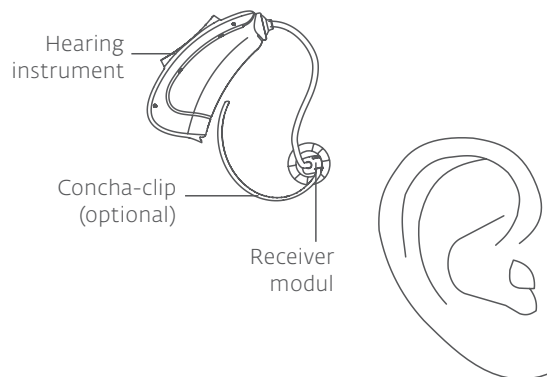

 The hearing aids have markings for the sides:
blue = left, red = right

Slide the receiver unit carefully into your ear canal.
Rotate slightly until it is positioned properly.

Open and close your mouth to avoid air being trapped
in the ear canal.



The optional Concha-Clip helps improve the fit of the receiver unit in the ear. To position the Concha-Clip, bend slightly and place the Concha-Clip carefully in the outer part of your ear.

Switch the hearing aid on by closing the battery compartment securely.

 **Caution: Risk of injury!**
Always wear the receiver module with its dome or ear adapter and check that it is positioned securely on the tube.

3.5.2 Removing hearing aids

Lift your hearing aid and slide carefully over the outer part of your ear. Carefully pull the tube with the receiver unit out of the ear canal. Switch the hearing aid off by moving the battery compartment to the OFF position.

 **Warning: Risk of injury!**
In very rare cases the dome may remain in the ear canal on removal. Should this happen, please contact your doctor or hearing care professional at once.
Please do not try to remove the dome yourself.

3.6 Volume and program selection

3.6.1 Binaural synchronisation


If you have had two hearing aids of the same type adjusted by your hearing care professional, they are synchronised as a pair. You can tell this, because after your devices have been switched on, the pairing melody plays in both hearing aids.

After the hearing aids have been paired, all settings made in one device are also written to the second device. The tones and melodies are played in both hearing aids with a slight delay.

If the connection is broken, you do not need to take action. The devices renew the connection quickly for themselves. You can tell this, because after your devices have been switched on, the pairing melody plays in both hearing aids.

If this does not work once, please restart both hearing aids.

3.6.2 Multifunctional rocker switch




Your hearing aids feature a multifunctional rocker switch for controlling the volume and selecting the different programs.

The multi-function rocker switch can be activated by pressing the top (+) and bottom end (-).

- **Volume control**
To control the volume, press the multi-function rocker switch briefly on the top or bottom button (also see 3.6.3).
- **Program selector switch**
To change the program, press the multi-function rocker switch briefly on the top or bottom button (also see 3.6.4).
- **Volume control and program selector switch combined**
To control the volume, press the multi-function rocker switch briefly on the top or bottom button; to change the program hold the switch down for approx. 1 second (see also 3.6.3 and 3.6.4).

3.6.3 Volume selection



The volume can be adjusted in steps using the multi-function rocker switch. Briefly pressing the top end of the switch increases the volume, while briefly pressing the bottom end reduces the volume.

When you switch your devices on, they will be at the volume set for you. You can only increase or reduce the volume in steps. Each time you press the switch, you will hear audible confirmation.

Once you have reached the upper or lower volume limit, you will hear a clear signal.

 Volume control and program selection are optional functions. Your hearing care professional will set your hearing aids to your individual requirements.

3.6.4 Selecting the hearing programs


Multifunctional rocker switch

Your hearing care professional will have adjusted your hearing aids to various hearing situations with you and assigned them to specific hearing programs.

The multi-function rocker switch allows you to swap between the hearing programs..

To do so, simply hold down one end of the multi-function rocker switch until you hear audible confirmation of the change in program with a tone. After you have released the multi-function rocker switch, the melody for the selected program is played. The number of signals indicates the number of the program selected. You can move through the hearing situations up or down. Your hearing care professional has set the number of selectable programs for your individual requirements.

Program change sequence*:



 Volume control and program selection are optional functions. Your hearing care professional will set your hearing aids to your individual requirements.

Hearing program	Description of setting
1	_____
2	_____
3	_____
4	_____

4 TINNITUS COMBI INSTRUMENTT

Combi hearing aids from audifon play an effective part in tinnitus therapy.

These instruments are designed to accustom you to your tinnitus and/or hyperacusis and will help correct disorders of the audiological system, compensate for tinnitus and improve existing hyperacusis.

Your hearing care professional will have adjusted the combi hearing aids to your individual hearing situation with you.



Warning: Damage to hearing!

The maximum volume of the tinnitus combi instrument lies in a range that can lead to hearing loss according to OSHA regulations. The tinnitus combi instrument should not be used for longer than eight (8) hours, at a sound pressure level (SPL) of less than 90 dB SPL. At a higher sound pressure, the device should not be used for more than two (2) hours daily. Under no circumstances should the tinnitus combi instrument be used with a volume that is not appropriate for the user.

4.1 Start-up

Information on operating devices with active tinnitus modules can be found in Section 3 of these operating instructions.

5 WIRELESS FUNCTIONALITY / BLUETOOTH CONNECTIVITY

5.1 Using hearing aids with iOS devices

5.1.1 Pairing hearing aids with the iOS device / iPhone

To be able to use your hearing aids via your iOS device, you have to pair it with your iOS device. This is how the hearing aids and the iOS device communicate with each other. Please follow the instructions to successfully pair the hearing aids.

1. Press the settings icon on your iOS device.
2. In the Settings menu go to: General → Accessibility → MFi Hearing Devices under the hearing category
3. If the Bluetooth function is still deactivated on this screen, activate Bluetooth. While the iOS device is looking for hearing aids, open and close the battery compartments of your hearing aids (this puts the hearing aids into pairing mode).
4. Among the devices now displayed, the device name of your hearing aids appears, created based on your first names. If this does not happen within 5-7 seconds, press the upper left edge of the screen to go back to <Accessibility> and open MFi Hearing Devices again.
5. After your hearing aids are displayed, select these from the list, to connect the devices with the iOS device.

6. Two pairing requests appear – one for each hearing aid. Select Pair to make a final connection. Both requests can be delayed by a couple of seconds.

7. Pairing is now complete.

5.1.2 Operating hearing aids with an iOS device / iPhone

Your made-for-iPhone hearing aid is equipped for operation with an iPhone, iPad or iPod Touch.

To use your hearing aid with an iOS device, pair the hearing aid as described in Section 5.1.1.

There are two ways for you to operate your hearing aids with your iOS device:

1. Via the menu MFi Hearing Devices
2. Via the quick start menu of the iOS device

In both menus you have access to set

1. The microphone volume
2. The desired hearing program
3. The listening function via your iOS device, with which the audio signals from the microphone of the iOS device are transmitted directly to your hearing aids.

5.1.3 Operation via the menu MFi Hearing Devices

Navigate to the sub-menu MFi Hearing Devices.

You can find this under

- Settings**
- **General**
- **Accessibility**
- **MFi Hearing Devices**

Your connected hearing aids are displayed here. Select the connected hearing aids via Connected, to reach the hearing aid settings.

5.1.4 Operation via the quick start menu

Press the home button three times. The MFi Hearing Devices menu opens.

If you require support for pairing or using the devices listed above with your hearing aid, please contact your hearing care professional.

For further operating functions, let your hearing care professional explain to you about the related free app.

5.2 Pairing hearing aids with an Android device

To be able to use your hearing aids via your Android device, you have to pair it with your Android device. This is how the hearing aids and the Android device communicate with each other. Please follow the instructions to successfully pair the hearing aids.

1. Press the settings icon.
2. Select Bluetooth.
3. Change the settings in On, if Bluetooth is switched off. Open and close the battery compartment of the hearing systems. This lets you transfer the hearing systems into pairing mode.
4. Under Paired devices you can see your first name, followed by Hearing Aid, if the hearing systems were detected. If the name does not appear on the list of paired devices within 5–7 seconds, press the Accessibility Icon in the top left corner, then on hearing aids.
5. The right hearing system appears on the list once, as does the left hearing system. Both list entries must be clicked for pairing.
6. Pairing is complete.

5.3 Using hearing aids with the MULTISTREAMER PRO

To use your hearing aids with an Android device, a TV or other devices that have an AUX output, you can get the MULTISTREAMER PRO accessory from your hearing care professional.

5.3.1 Pairing hearing aids with the MULTISTREAMER PRO

When you purchased your MULTISTREAMER PRO from your hearing care professional, you connected your hearing aids to the MULTISTREAMER PRO for the first time with them. This means that the initialisation of the connection is completed.

From now on you can connect your hearing aids automatically to your MULTISTREAMER PRO. To do this, just switch on your MULTISTREAMER PRO and then (within 180 seconds) your hearing aid(s).

5.3.2 Pairing your smartphone with the MULTISTREAMER PRO

Switch on the MULTISTREAMER PRO. Then press the multifunction button for 5 seconds. The LED changes to red then flashing blue. Refresh the Bluetooth menu in your smartphone. The MULTISTREAMER PRO is displayed in the selection. Select the device, and select Pair. The MULTISTREAMER PRO is paired with your smartphone.

For further operating functions see the operating instructions of the MULTISTREAMER PRO, included with your MULTISTREAMER PRO.

5.4 Flight mode

When you enter an aeroplane or areas where transmission of wireless signals is forbidden, you must switch off the wireless functions of your electronic devices.



For this reason, please put your hearing aids in flight mode in these situations, or if in doubt speak to trained personnel.

To switch your hearing aid to flight mode, please press the multifunction rocker switch up for 5 seconds. All wireless functions of your hearing aids are now switched off.

If you switch the hearing aids off and on again, all functions are reactivated.

6 ACCESSORIES

The hearing aids of the lewi and risa families have the following accessories, which you can obtain from your hearing care professional. You can download the audifon app for free in the corresponding platforms. For more information, please contact your hearing care professional.

Accessories	Description
audifon App	smart-phone App for remote control of your hearing aids
multistreamer pro	audio streamer to enhance the functionality of your hearing aids
UniTip Soundshell	Individual earmold for your hearing aids
UniTip Domes	Universal ear pieces for use with your hearing aids
UniTip receiver unit S-M-P	Receiver unit is used to deliver the amplified sound into the ear canal
Concha Clip	Concha clip fixes the UniTip receiver unit in the ear canal
CeruStop Filter	Small filter that protects the earphone from blockage and should be replaced regularly
audifit Software from Version 5.8	Fitting software that the hearing aid specialist uses to fit the hearing aids for you

6.1 Compatibility with smart-phones

The hearing aids of the families lewi and risa are compatible with common smart-phones, which have Bluetooth version 4.0 or higher, if necessary, the accessory product MULTISTREAMER PRO be necessary for an audio transmission (eg Android operating system of the smart-phone).

For a list of the lewi and risa family of hearing aids and audifon app compatible smart-phones, tablets, etc., visit:

www.audifon.com

7 CARE INSTRUCTIONS

7.1 General

audifon hearing aids will improve your hearing ability as well as your quality of life. To ensure your hearing aids function perfectly and so make hearing a pleasant experience for years to come, audifon offers special care products designed to enable optimum cleaning of your devices.

Protect your hearing aids against moisture (e.g. showers, sweat, rain), and take your hearing aids out before using hairspray or similar cosmetic products.

We also recommend that you carry out daily care on your hearing aids, as the devices are exposed to moisture and dust through intended use, even if they are handled with care. Whatever type of hearing aid you use: Every one is in direct contact with the skin. This produces perspiration, which may damage your hearing aid in the long term unless dried on a daily basis. audifon's behind-the-ear hearing aids are coated with a water-repellent finish, known as the nanoShield, to prevent any damage from moisture.

Wearing a hearing aid or a receiver unit in the ear canal will always involve soiling with earwax. For this reason we recommend regular cleaning. Earwax can build up at the sound outlets, particularly with hearing aids with an external receiver, and so affect sound quality.

Should your hearing aid still not function correctly despite regular care, call on your hearing care professional. Do not try under any circumstances to repair your hearing aid yourself.

7.2 Cleaning and care of Behind-The-Ear hearing aids with an external receiver

Hearing aids with an external receiver have special requirements in terms of cleaning and care. Please proceed as follows:

To clean your hearing aids on the outside, either use an audifon pro care Cleaning-Tissue or a dry, lint-free cloth which you have moistened with the audifon pro care Cleaning-Spray. Rub your hearing aid carefully with a tissue or cloth. This will remove soiling and residues of earwax quickly and easily. When handling the external receiver, please take special care. Make sure that moisture does not get into the microphone inlets of the hearing aid.


Changing the earwax protection filter

Hearing aids with an external receiver feature protection filters to prevent earwax being deposited inside the receiver. It is necessary to regularly change the filter to ensure your hearing aids function perfectly. To replace the filter, proceed as follows:



First remove the dome from the receiver module and clean it.

Remove the changing tool from the filter dispenser and put the black side on the filter.



Pull out the filter with a gentle turning motion.

Turn the changing tool. At the other end of the changing tool is a new filter.



Press the new filter with the changing tool into the filter opening of the hearing aid until it clicks into place.

Then simply pull the changing tool out and dispose of it.

7.3 Drying hearing aids

Your hearing aids should be dried after use at the end of the day and above all after cleaning. If you take care of your hearing aids by drying them carefully, this will significantly increase their service life. There are two ways of doing this. If you have an audifon drying station of the type dry star UV 2 or dry go, use this for drying. Take note of the individual product instructions for further details. Alternatively, you can dry your hearing aids in the audifon pro care Drying-Tub with an audifon Drying-Capsule.

dry star UV 2

The audifon dry star UV 2 will dry your tinnitus instruments gently yet thoroughly thanks to the constant circulation of uniformly warm air inside the casing. At the same time, the UVC radiation used here will kill 99.9% of all common bacteria.

The audifon dry star UV 2 is not only automatic but also consumes very little power, switching itself off at the end of the drying program. The drying station is simple to operate using a single sensor button.



dry go

The audifon dry go is the perfect solution for drying your devices when on trips or out and about. Once connected, for example to the USB port on your laptop, the drying program can be conveniently started at the touch of a single button. A flow of warm air inside the audifon dry go will then dry your devices reliably. The drying station switches off automatically at the end of the drying program.



8 DEALING WITH PROBLEMS

If you experience any malfunctions when using your hearing aids, this does not necessarily mean that they are faulty. Therefore first check your hearing aid to make sure that:

- the hearing aid is switched on (see „Switching on and off“ Section 3.4),
- the battery is not weak or flat,
- the volume is not at the lowest setting (increase the volume slightly if necessary),
- the right program has been set (change program if necessary),
- the receiver unit / earwax protection system is not blocked.

If this does not eliminate the fault, consult your hearing care professional, who will be pleased to help you.

ⓘ Note: Malfunctions!

Despite their EMC-compatible design, your devices may be subject to interference from other electrical equipment. In this case move away from the source of interference.

9 SAFETY INSTRUCTIONS

9.1 Important warnings

Warning: Risk of suffocation!

Batteries, hearing aids and other small parts can be swallowed. Keep such parts out of the reach of children under 36 month, the mentally disabled and pets. Should a battery, hearing aid or other small parts be accidentally swallowed, please consult a doctor immediately

Warning: Risk of injury!

In very rare cases the dome may remain in the ear canal on removal. Should this happen, please contact your doctor or hearing care professional at once. Please do not try to remove the dome yourself.

Warning: Damage to hearing!

The maximum volume of the tinnitus combi instrument lies in a range that can lead to hearing loss according to OSHA regulations. The tinnitus combi instrument should not be used for longer than eight (8) hours, at a sound pressure level (SPL) of less than 90 dB SPL. At a higher sound pressure, the device should not be used for more than two (2) hours daily. Under no circumstances should the tinnitus combi instrument be used with a volume that is not appropriate for the user.

Warning: Risk of explosion!

Do not use hearing aids in environments where there is a risk of explosion (e.g. in mines or industrial plants subject to such risk).

Warning: Risk of injury!

Hearing aids are adjusted to the individual hearing loss of each wearer and should therefore only be used by this person.

If the hearing aid is worn by other persons, this may harm their hearing.

Warning: Risk of injury!

Please only use genuine consumables specified by the manufacturer (dome, tubing, etc.) and accessories. Unauthorised changes or modifications that have not been explicitly approved may in the worst-case scenario result in injury.

Warning: Interference with active and inactive implants!

If you have an active or inactive implant (e.g. defibrillator, pacemaker), follow the implant manufacturer's instructions regarding use of mobile devices. In case of malfunctions, stop using your hearing aid and contact your doctor or the implant manufacturer.

If you have an active brain implant, ask your doctor or the implant manufacturer for a risk analysis..

Caution: Risk of injury!

Always wear your receiver module with its dome or made-to-measure ear mould.

Warning: Radio communications in rooms

Before making a connection between radio communications and the hearing aids, you should check whether use of radio communications is restricted in the room/area.

9.2 Notes on product safety

ⓘ **Note: Damage to hearing aid!**

Hearing aids are susceptible to impact, So avoid any hard knocks (e.g. by dropping them).

ⓘ **Note:**

To avoid damage to your hearing aids, do not wear them in the following situations:

- when swimming, in the shower or bath
- when washing or blow-drying your hair
- when using hair spray, perfume, aftershave or body lotion
- during high-frequency heat therapy treatment
- when it is very hot or raining heavily

Should your hearing aid become damp, remove the battery and dry the hearing aid in one of the drying containers specified by the manufacturer. Do not dry your hearing aid in the microwave under any circumstances.

ⓘ **Note: Damage to hearing aid!**

No changes may be made to the hearing aids unless they are made directly by the manufacturer.

ⓘ **Hinweis: Beschädigung des Hörgerätes!**

Do not force the battery into the battery compartment. If it does not fit, check whether you are inserting it correctly and that it is the correct type of battery.

ⓘ **Note: Leaking batteries can damage your hearing aid!**

If you are not going to use your hearing aid for a long time, remove the battery to increase its service life, to avoid battery leakage and to prevent corrosion to the battery contacts.

ⓘ **Note: Strong radiation can damage hearing aids!**

Make sure you take out your hearing aids if you are undergoing a CT or MRI scan, other magnetic field-based examinations or radiotherapy.

ⓘ **Note: Damage to hearing aid!**

Never leave your hearing aid in the sun, near a naked flame or in a hot vehicle. Otherwise your hearing aids might become damaged.

ⓘ **Note: Damage to hearing aid!**

Never try to change the shape of your hearing aid, ear mould or tubing yourself. Otherwise your hearing aids might become damaged.

ⓘ **Note: Malfunctions!**

Despite their EMC-compatible design, your devices may be subject to interference from other electrical equipment. In this case move away from the source of interference.

ⓘ **Note: Interference with electronic devices!**

If you are in an environment where use of electronic or wireless devices is restricted, check if your hearing aids must be turned off.

❗ **Note: User age!**

The hearing aids are not intended for children under 36 months.

❗ **Reporting serious incidents!**

All serious incidents related to the product that occur should be reported to the manufacturer and to the responsible authorities in the member state in which the user and/or the patient are registered.

10 SIDE EFFECTS

Please consult your doctor or hearing care professional at once if you notice the following symptoms:

- Sensation of a foreign body
- Build-up of earwax
- Skin irritation
- Dizziness
- Vomiting
- Headache
- Pain in or behind the ear
- a subjective deterioration in your hearing or an increase in the tinnitus level

Good health practice requires a medical evaluation by a licensed physician (preferably a physician specializing in ear diseases) before recommending a hearing aid to a person with a hearing loss. Licensed physicians specializing in ear diseases are often referred to as otolaryngologists, otologists or otorhinolaryngologists. The purpose of the medical evaluation is to ensure that all medically treatable conditions that may affect hearing are identified and treated before the hearing aid is purchased.

11 OPERATING CONDITIONS

- Relative humidity between 10% and 90%
- Operating temperature between 0 °C and 40 °C
- Air pressure between 500 hPa and 1100 hPa

12 TRANSPORT AND STORAGE CONDITIONS

- Relative humidity between 10% and 60%
- Storage temperature between -20 °C and 60 °C
- Remove battery for storage
- Store away from magnetic fields

13 ENVIRONMENTALLY FRIENDLY DISPOSAL

Old hearing aids and batteries must not be disposed of with your household waste. Please return old hearing aids and batteries to your hearing care professional for environmentally friendly disposal. This is the person to contact in the disposal chain for electronic waste.



14 OTHER INFORMATION

14.1 EU Declaration of conformity

audifon hereby declares that the hearing aids lewi R and risa R comply with the following directives:
93/42/EEC for medical devices
2011/65/EU RoHs for the reduction of hazardous substances

The declaration of conformity is available for inspection at

audifon GmbH & Co. KG
Werner-von-Siemens-Straße 2
99625 Kölleda
and at **www.audifon.com**

15 SERVICE

Arrange for your hearing aids to be checked regularly by a hearing care professional.

14.2 FCC Statement



Federal Communications Commission Statement

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

NOTE:

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Date

Hearing care professional

Date

Hearing care professional

Date

Hearing care professional

Arrange for your hearing aids to be checked regularly by a hearing care professional.

Date

Hearing care professional

Date

Hearing care professional

Date

Hearing care professional

16 KEY TO SYMBOLS

-  Indicates a situation that may result in serious, moderate or minor injury
-  Indicates possible damage to property
-  Additional information for better understanding
-  Manufacturer of the device
-  Please do not dispose of hearing aids with your household waste.
-  Read and observe the directions in the operating instructions. It contains important warnings and information about safety precautions.
-  Restrict humidity
-  Restrict temperatures
-  This is a medical product.
-  Item number
-  Serial number
-  Batch number

WARRANTY CARD

You have chosen high-quality hearing aids from audifon. Your hearing care professional offers _____ months warranty on our hearing aids from the date of purchase (date of invoice). The warranty covers defects in materials and manufacture. It does not cover batteries, chemical or electrochemical effects, wear and tear or mechanical damage due to improper handling. The right to claim under warranty is void if you or any unauthorised third persons carry out alterations or improper repairs. Therefore always follow the safety and care instructions. Proof of purchase must be provided as proof of warranty. The date of purchase and the serial number must be clearly visible. Warranty obligations will not result in an extension of the warranty period, nor will they initiate a new warranty period for the hearing aid. The warranty period for built-in spare parts ends at the same time as the warranty period for the whole hearing aid.

 The warranty period for built-in spare parts ends at the same time as the warranty period for the whole hearing aid.

Hearing aid type

Date of sale

Your hearing care professional

Signature

Stamp:

Name _____

Street No. _____

Town and postcode _____

Telephone _____

Date of issue _____

R

Type _____ Side _____

Serial number _____

Warranty _____ Batterie type _____

L

Type _____ Side _____

Serial number _____

Warranty _____ Batterie type _____

audifon



Head office

audifon GmbH & Co. KG
Werner-von-Siemens-Straße 2
99625 Kölleda
Deutschland

Telefon +49-3635-4056-590

Fax +49-3635-4056-589

contact@audifon.com

www.audifon.com

CE 0297

High-tech
made in Germany