




PLUG IN THE POWER SUPPLY AND RF WILL COME ON AT 13.56MHz

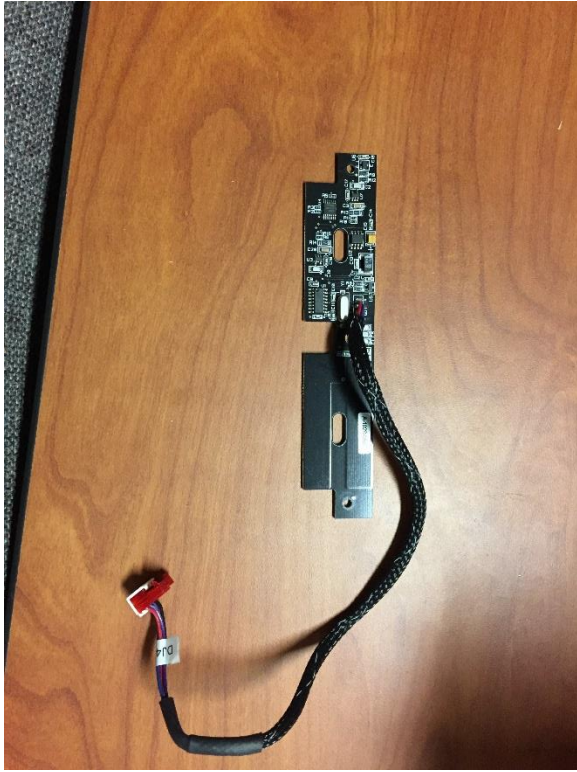


RFID Board – Actual EUT

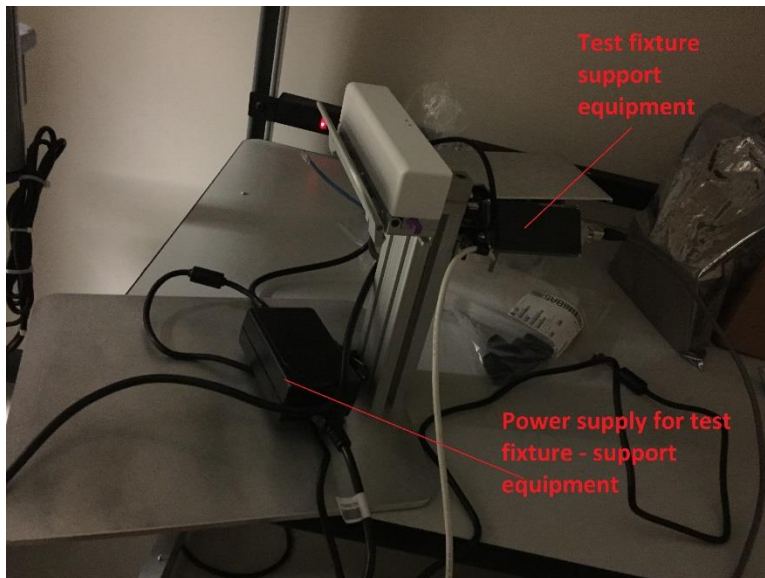

Board installed in test fixture

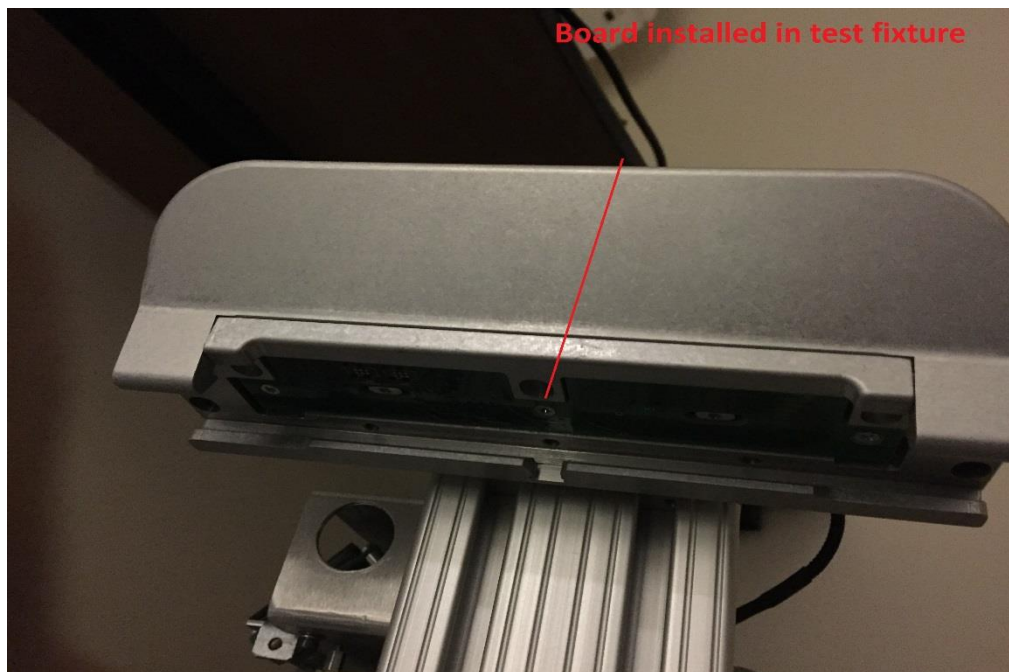

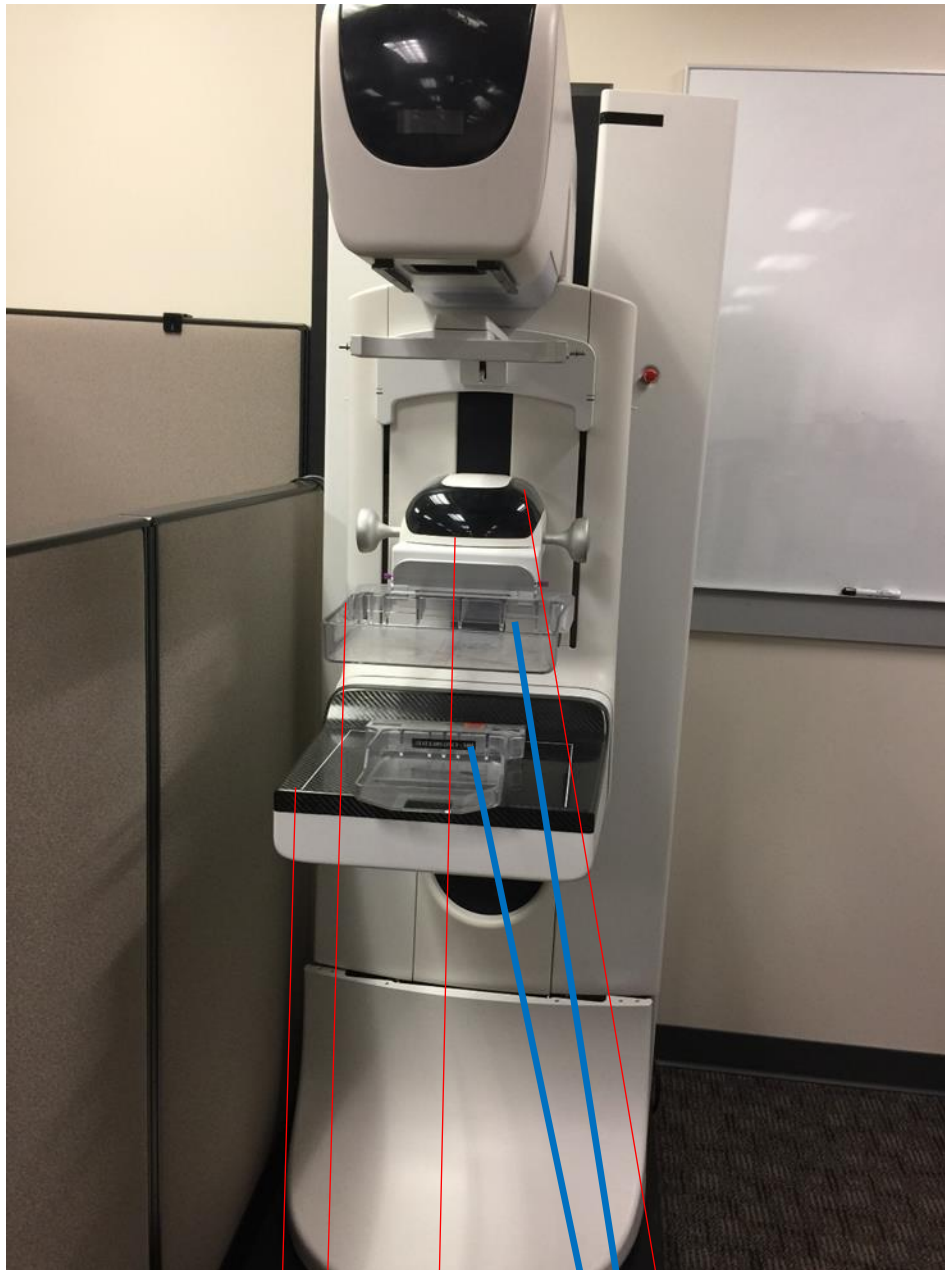


That is where
RFID board is
installed
Compression Paddle

Compression Device

Showing two paddles one attached to compression
device. RF Tag is installed in paddle for paddle
identification.

Breast platform

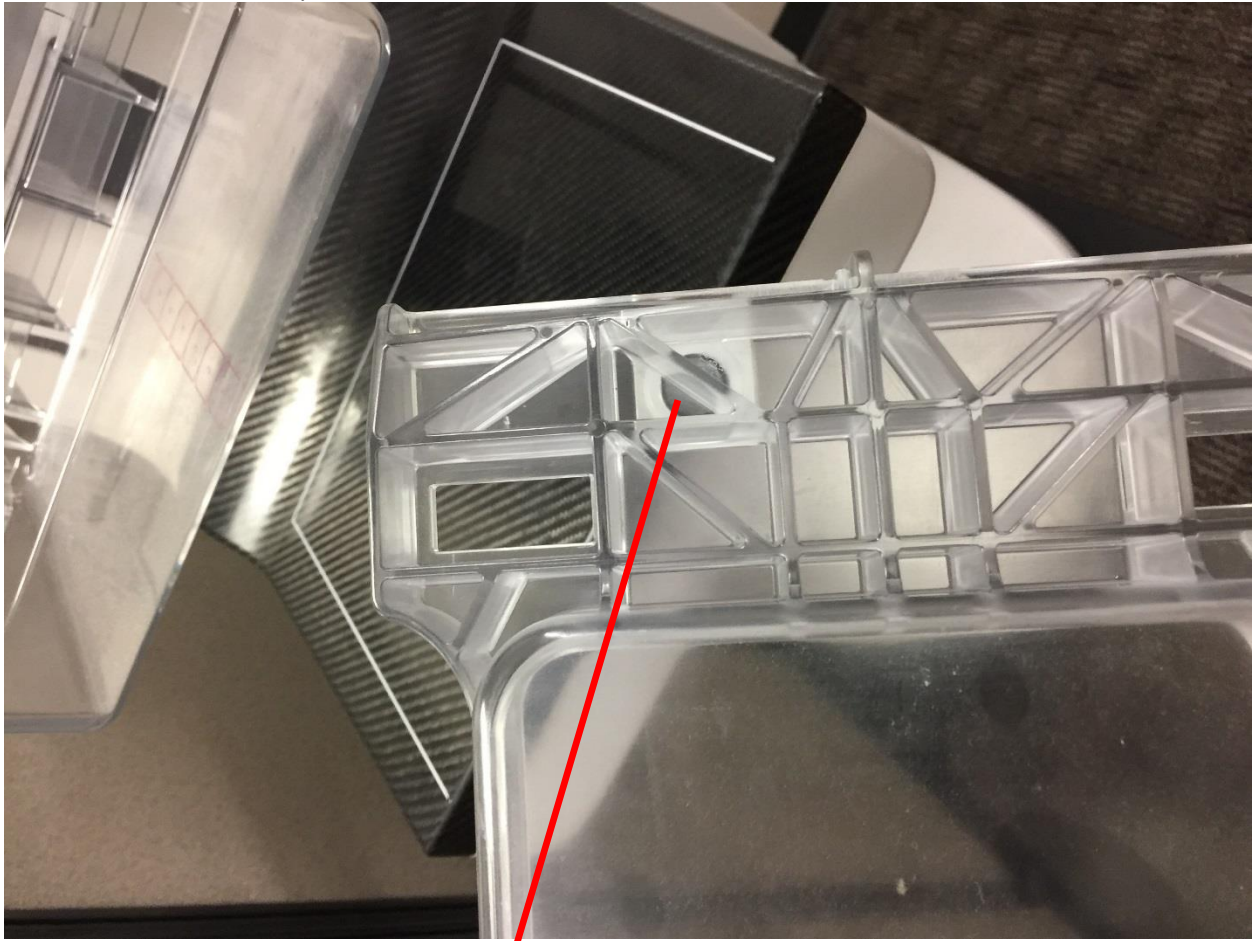

Round DOT is the RF tag in the paddle.

RFID is used to identify which paddle is used during X ray exam on a patient.