

D5GHzV2 - SN: 1262

January 17, 2025

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance	47.7 Ω – 2.7 j Ω
Return Loss	-28.7 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance	52.0 Ω + 0.7 j Ω
Return Loss	-33.6 dB

Antenna Parameters with Head TSL at 5750 MHz

Impedance	52.3 Ω + 2.6 j Ω
Return Loss	-29.3 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.194 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

D5GHzV2 - SN: 1262

January 17, 2025

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 - SN1262	5250	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		5250, 0	5.68	4.58	35.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2025-01-17	EX3DV4 - SN7349, 2025-01-10	DAE4lp Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2025-01-17
psSAR1g [W/Kg]	7.78
psSAR10g [W/Kg]	2.23
Power Drift [dB]	-0.09
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

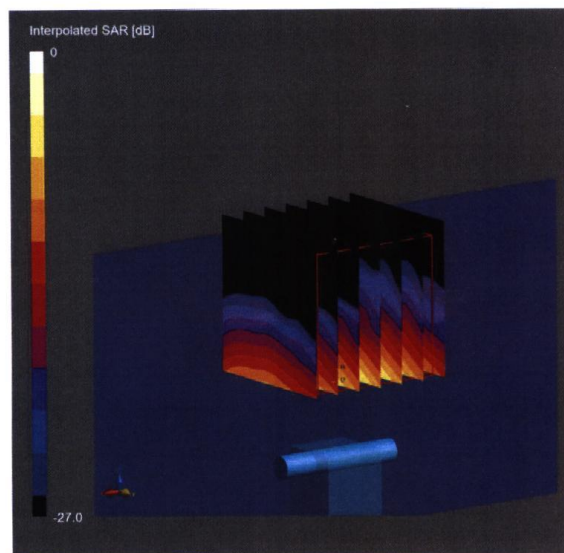

0 dB = 31.3 W/Kg

D5GHzV2 - SN: 1262

January 17, 2025

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 - SN1262	5600	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		5600, 0	5.21	4.96	35.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2025-01-17	EX3DV4 - SN7349, 2025-01-10	DAE4ip Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2025-01-17
psSAR1g [W/Kg]	8.12
psSAR10g [W/Kg]	2.34
Power Drift [dB]	-0.02
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative



0 dB = 35.1 W/Kg

Certificate No: D5GHzV2-1262_Jan25

Page 7 of 9

D5GHzV2 - SN: 1262

January 17, 2025

System Performance Check Report

Summary

Dipole	Frequency [MHz]	TSL	Power [dBm]
D5GHzV2 - SN1262	5750	HSL	20

Exposure Conditions

Phantom Section, TSL	Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat	10	CW, 0--		5750, 0	5.38	5.12	34.8

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center	HSL, 2025-01-17	EX3DV4 - SN7349, 2025-01-10	DAE4lp Sn1836, 2024-10-28

Scans Setup

	Zoom Scan
Grid Extents [mm]	22 x 22 x 22
Grid Steps [mm]	4.0 x 4.0 x 1.4
Sensor Surface [mm]	1.4
Graded Grid	Yes
Grading Ratio	1.4
MAIA	N/A
Surface Detection	VMS + 6p
Scan Method	Measured

Measurement Results

	Zoom Scan
Date	2025-01-17
psSAR1g [W/Kg]	7.61
psSAR10g [W/Kg]	2.17
Power Drift [dB]	-0.01
Power Scaling	Disabled
Scaling Factor [dB]	
TSL Correction	Positive / Negative

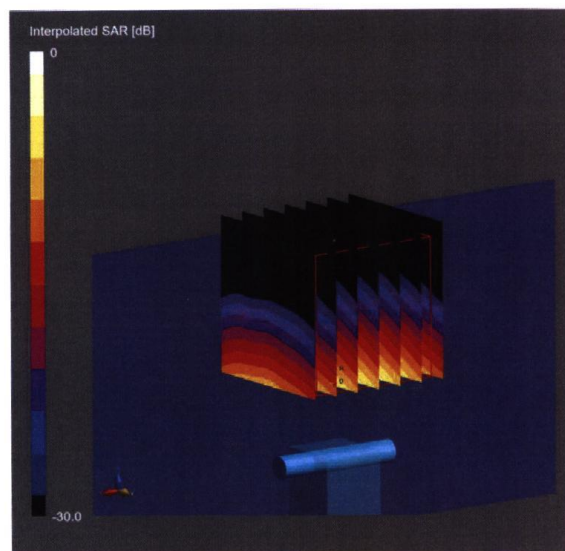


0 dB = 33.9 W/Kg

D5GHzV2 - SN: 1262

January 17, 2025

Impedance Measurement Plot for Head TSL

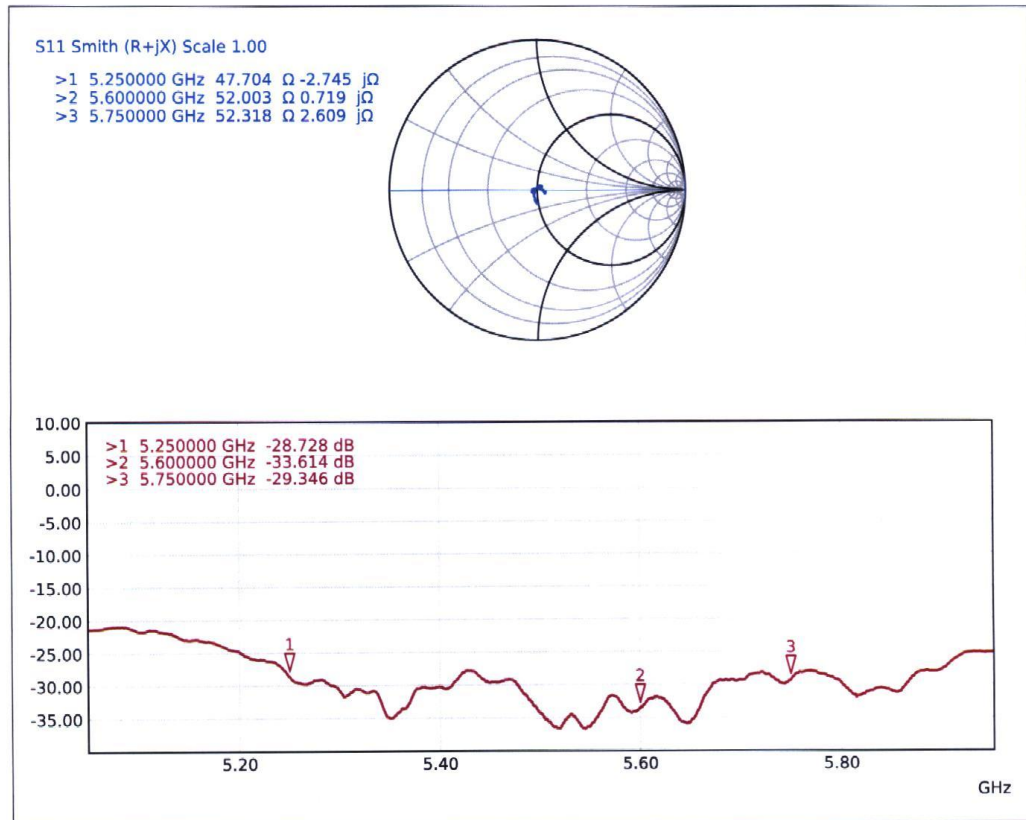

ANNEX I SAR Sensor Triggering Data Summary

ANT	Side	Distance
ANT2	Back (mm)	21
	Front(mm)	18
	Top(mm)	25
	Left (mm)	18
ANT1	Back (mm)	19
	Front(mm)	17
	Top(mm)	18
	Left (mm)	18
ANT3	Back (mm)	13
	Front(mm)	9
	Top(mm)	18
	Right (mm)	0

Per FCC KDB Publication 616217 D04v01r02, this device was tested by the manufacturer to determine the proximity sensor triggering distances for some positions. The measured output power within $\pm 5\text{mm}$ of the triggering points (or until touching the phantom) is included for front, rear and each applicable edge.

To ensure all production units are compliant it is necessary to test SAR at a distance 1mm less than the smallest distance from the device and SAR phantom (determined from these triggering tests according to the KDB 616217 D04v01r02) with the device at maximum output power without power reduction. These SAR tests are included in addition to the SAR tests for the device touching the SAR phantom, with reduced power.

Rear-Ant3

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	18	17	16	15	14	13	12	11	10	9	8
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	8	9	10	11	12	13	14	15	16	17	18
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Rear-Ant2

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	26	25	24	23	22	21	20	19	18	17	16
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	16	17	18	19	20	21	22	23	24	25	26
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Front/Left-Ant2

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	23	22	21	20	19	18	17	16	15	14	13
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	13	14	15	16	17	18	19	20	21	22	23
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Top/Left-Ant1

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	23	22	21	20	19	18	17	16	15	14	13
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	13	14	15	16	17	18	19	20	21	22	23
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Top -Ant3

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	23	22	21	20	19	18	17	16	15	14	13
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	13	14	15	16	17	18	19	20	21	22	23
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Rear-Ant1

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	23	22	21	20	19	18	17	16	15	14	13
Main antenna	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	13	14	15	16	17	18	19	20	21	22	23
Main antenna	Near	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far

Top-Ant2

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	29	28	27	26	25	24	23	22	21	20	19
Main antenna	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	20	21	22	23	24	25	26	27	28	29	30
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far

Front-Ant1

Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	23	22	21	20	19	18	17	16	15	14	13
Main antenna	Far	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near

Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	13	14	15	16	17	18	19	20	21	22	23
Main antenna	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far	Far

Front-Ant3


Moving device toward the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	14	13	12	11	10	9	8	7	6	5	4
Main antenna	Far	Far	Far	Far	Far	Near	Near	Near	Near	Near	Near


Moving device away from the phantom:

sensor near or far(KDB 616217 6.2.6)											
Distance [mm]	4	5	6	7	8	9	10	11	12	13	14
Main antenna	Near	Near	Near	Near	Near	Near	Far	Far	Far	Far	Far


Per FCC KDB Publication 616217 D04v01r02, the influence of table tilt angles to proximity sensor triggering is determined by positioning each edge that contains a transmitting antenna, perpendicular to the flat phantom, at the smallest sensor triggering test distance by rotating the device around the edge next to the phantom in $\leq 10^\circ$ increments until the tablet is $\pm 45^\circ$ or more from the vertical position at 0° .

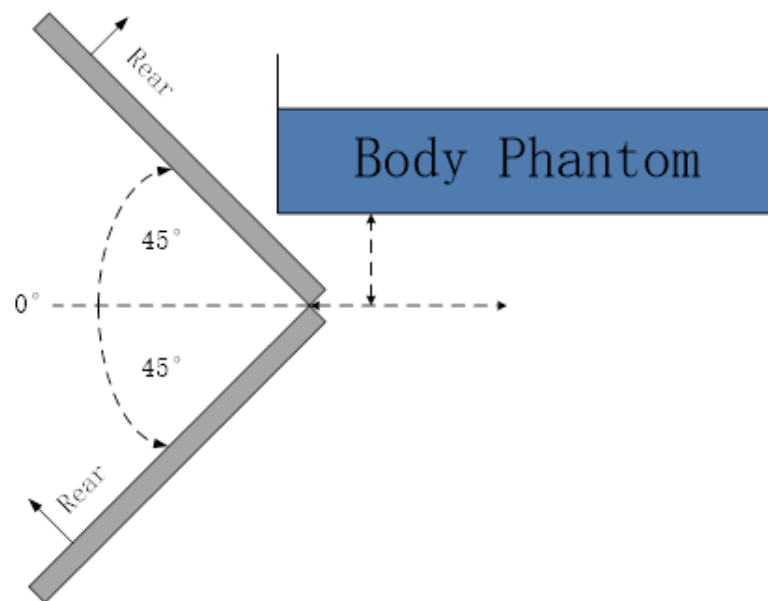

The front/rear evaluation

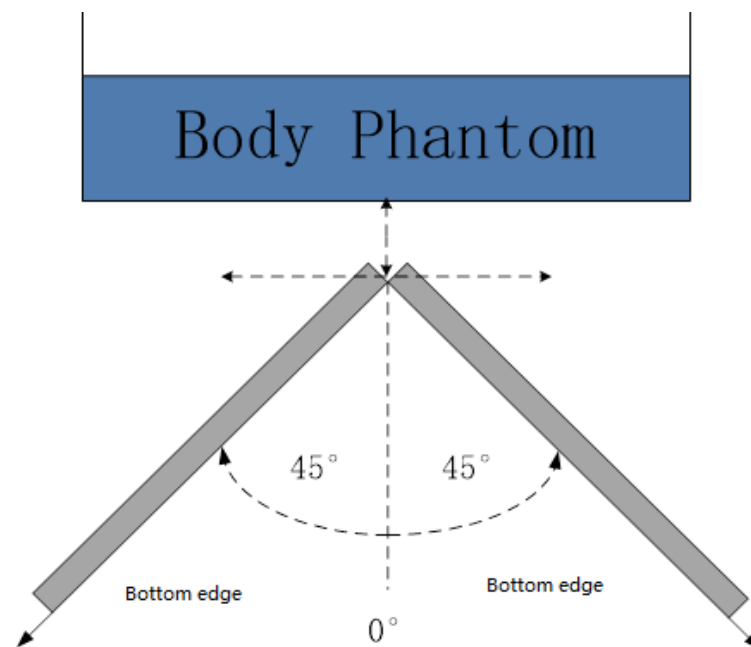

The top/bottom edge evaluation

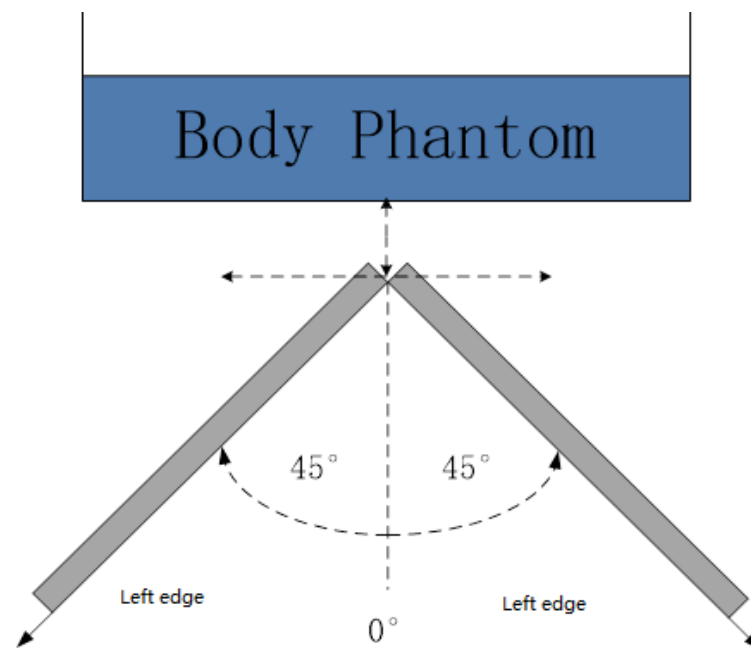

The left/right edge evaluation


Based on the above evaluation, we come to the conclusion that the sensor triggering is not released and normal maximum output power is not restored within the $\pm 45^\circ$ range at the smallest sensor triggering test distance declared by manufacturer.S

ANNEX J Extended Calibration SAR Dipole

If dipoles are verified in return loss ($< -20\text{dBm}$, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole D900V2– serial no.1d051

Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2024-07-09	-43.77	/	49.44	/	-0.31	/
2025-07-02	-38.80	11.35	49.52	-0.08	-1.04	0.73

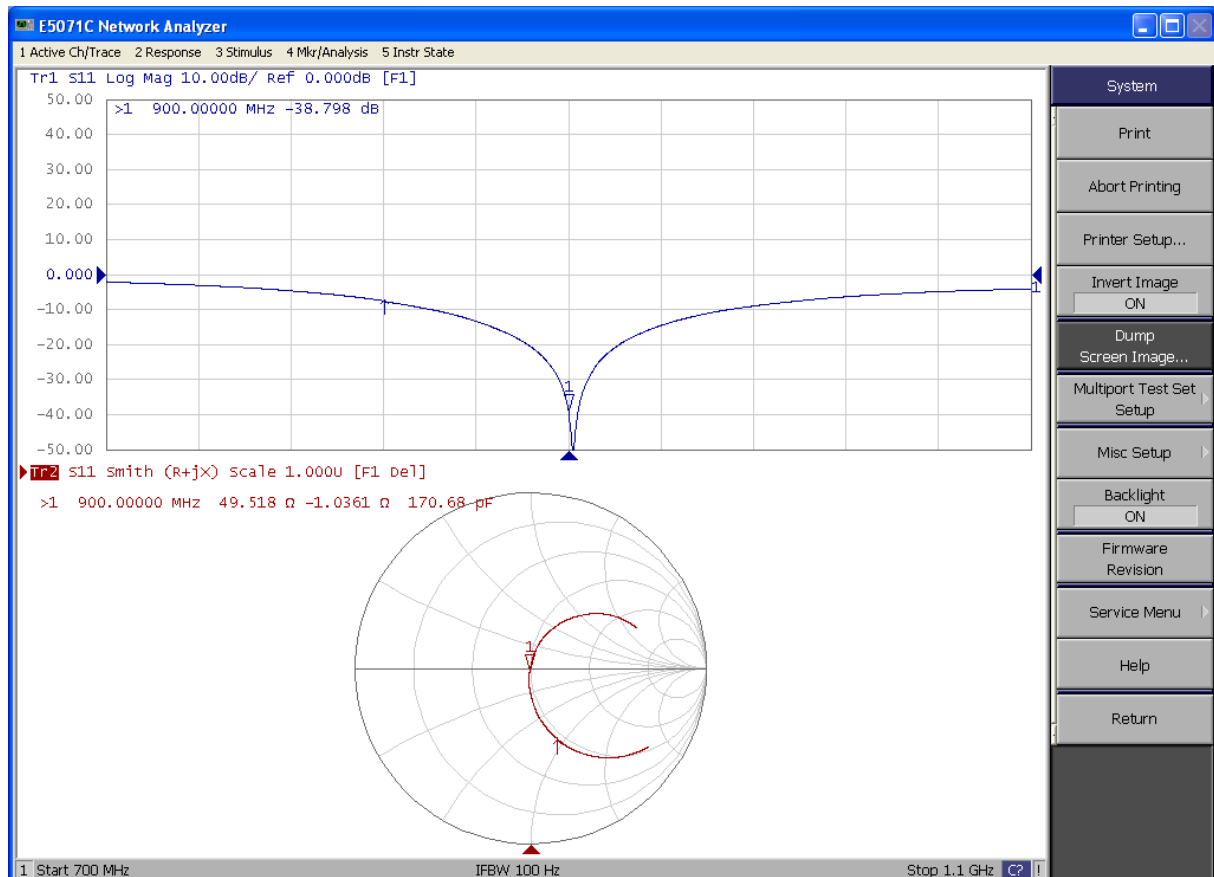

ANNEX K Accreditation Certificate



Accredited Laboratory

A2LA has accredited

TELECOMMUNICATION TECHNOLOGY LABS, CAICT

Beijing, People's Republic of China

for technical competence in the field of

Electrical Testing

This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017 *General requirements for the competence of testing and calibration laboratories*. This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).



Presented this 23rd day of July 2024.



Mr. Trace McInturf, Vice President, Accreditation Services
For the Accreditation Council
Certificate Number 7049.01
Valid to July 31, 2026

For the tests to which this accreditation applies, please refer to the laboratory's Electrical Scope of Accreditation.